

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061723\
 Data File : PD075860.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2023 17:15
 Operator : AR\AJ
 Sample : 03255-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMPOSIT-SB-24

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 22:04:48 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.768	32525797	16141381	15.269	14.878
28)	SA Decachlor...	9.090	7.913	47865253	19084903	18.894	19.518
Target Compounds							
11)	B alpha-Chl...	6.038	5.034	71477884	22743903	22.110	16.580 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061723\
Data File : PD075860.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2023 17:15
Operator : AR\AJ
Sample : 03255-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
COMPOSIT-SB-24

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 22:04:48 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

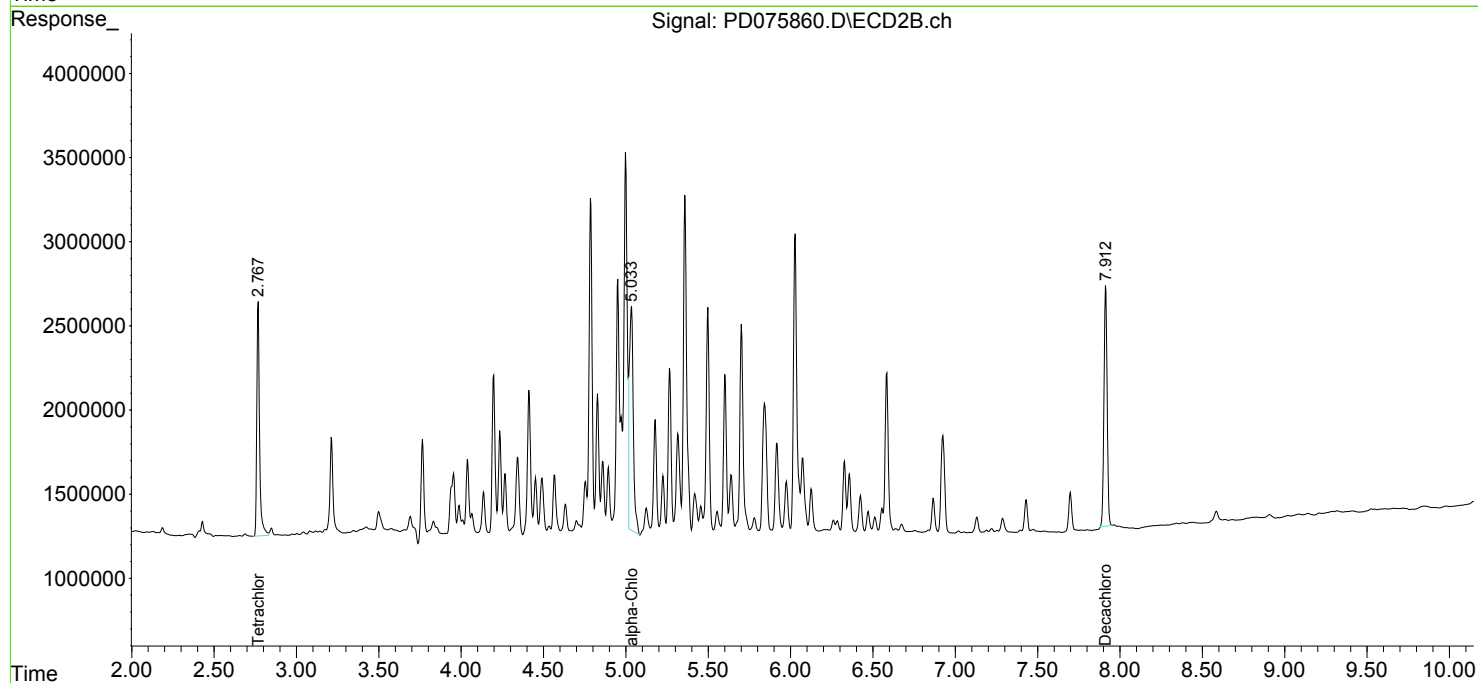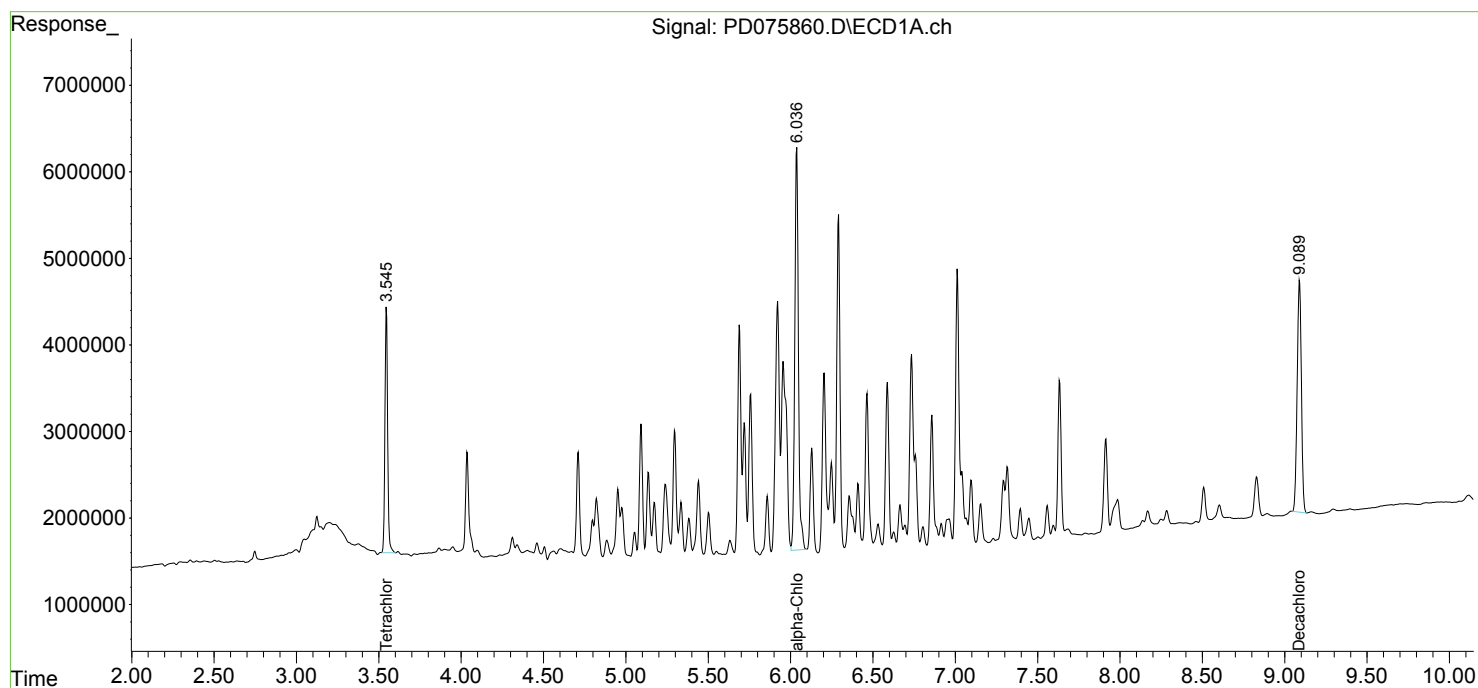


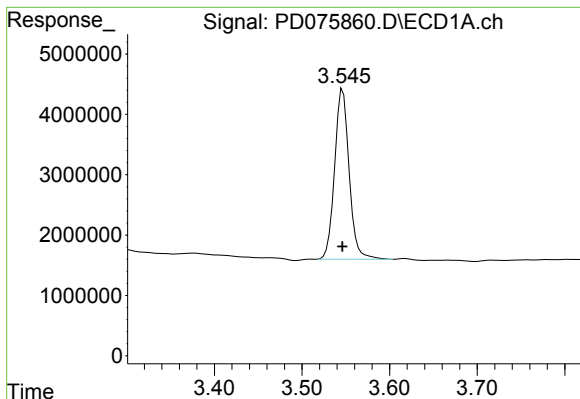

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 32525797
Conc: 15.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMPOSIT-SB-24

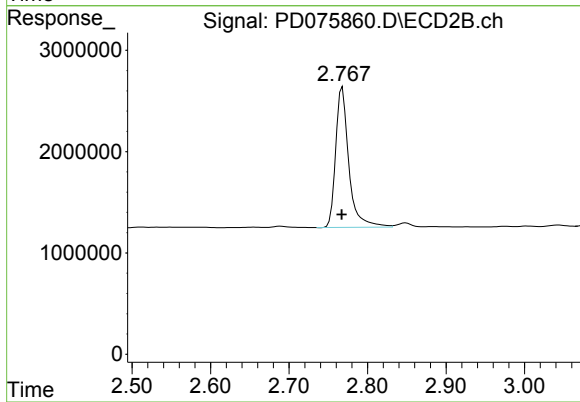


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: 0.000 min
Response: 16141381
Conc: 14.88 ng/ml

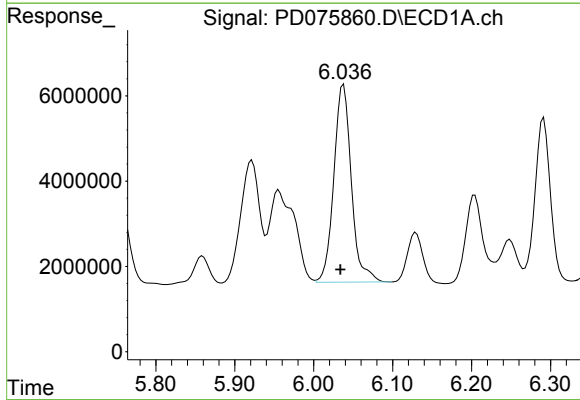


#11 alpha-Chlordane

R.T.: 6.038 min
Delta R.T.: 0.004 min
Response: 71477884
Conc: 22.11 ng/ml

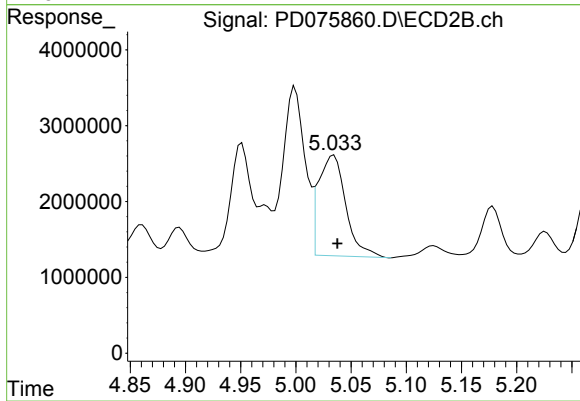

#11 alpha-Chlordane


R.T.: 5.034 min
Delta R.T.: -0.003 min
Response: 22743903
Conc: 16.58 ng/ml

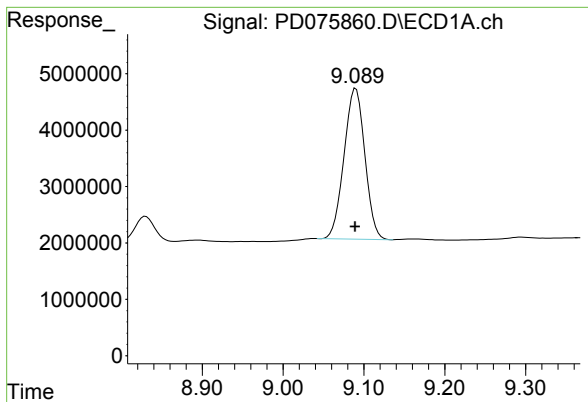

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.000 min
Response: 47865253
Conc: 18.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMPOSIT-SB-24

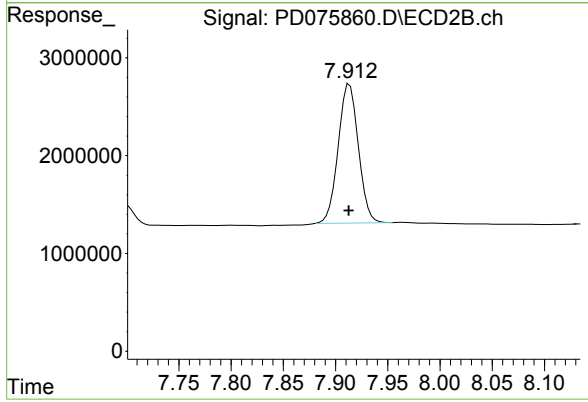

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 19084903
Conc: 19.52 ng/ml