

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061821\
 Data File : PD063893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 08:56
 Operator : AR\AJ
 Sample : PIBLK20
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 23:29:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.969	29649328	302.2E6	21.601	21.466
27)	SA Decachlor...	8.192	9.023	61412063	478.5E6	37.799	32.612
Target Compounds							
6)	B beta-BHC	4.367f	0.000	744409	0	0.800	N.D. #
7)	B delta-BHC	0.000	5.026	0	12501906	N.D.	0.567
8)	B Heptachlo...	0.000	5.850	0	1020920	N.D.	<MDL
16)	A 4,4'-DDD	0.000	6.752f	0	298855	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061821\
Data File : PD063893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 08:56
Operator : AR\AJ
Sample : PIBLK20
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 23:29:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

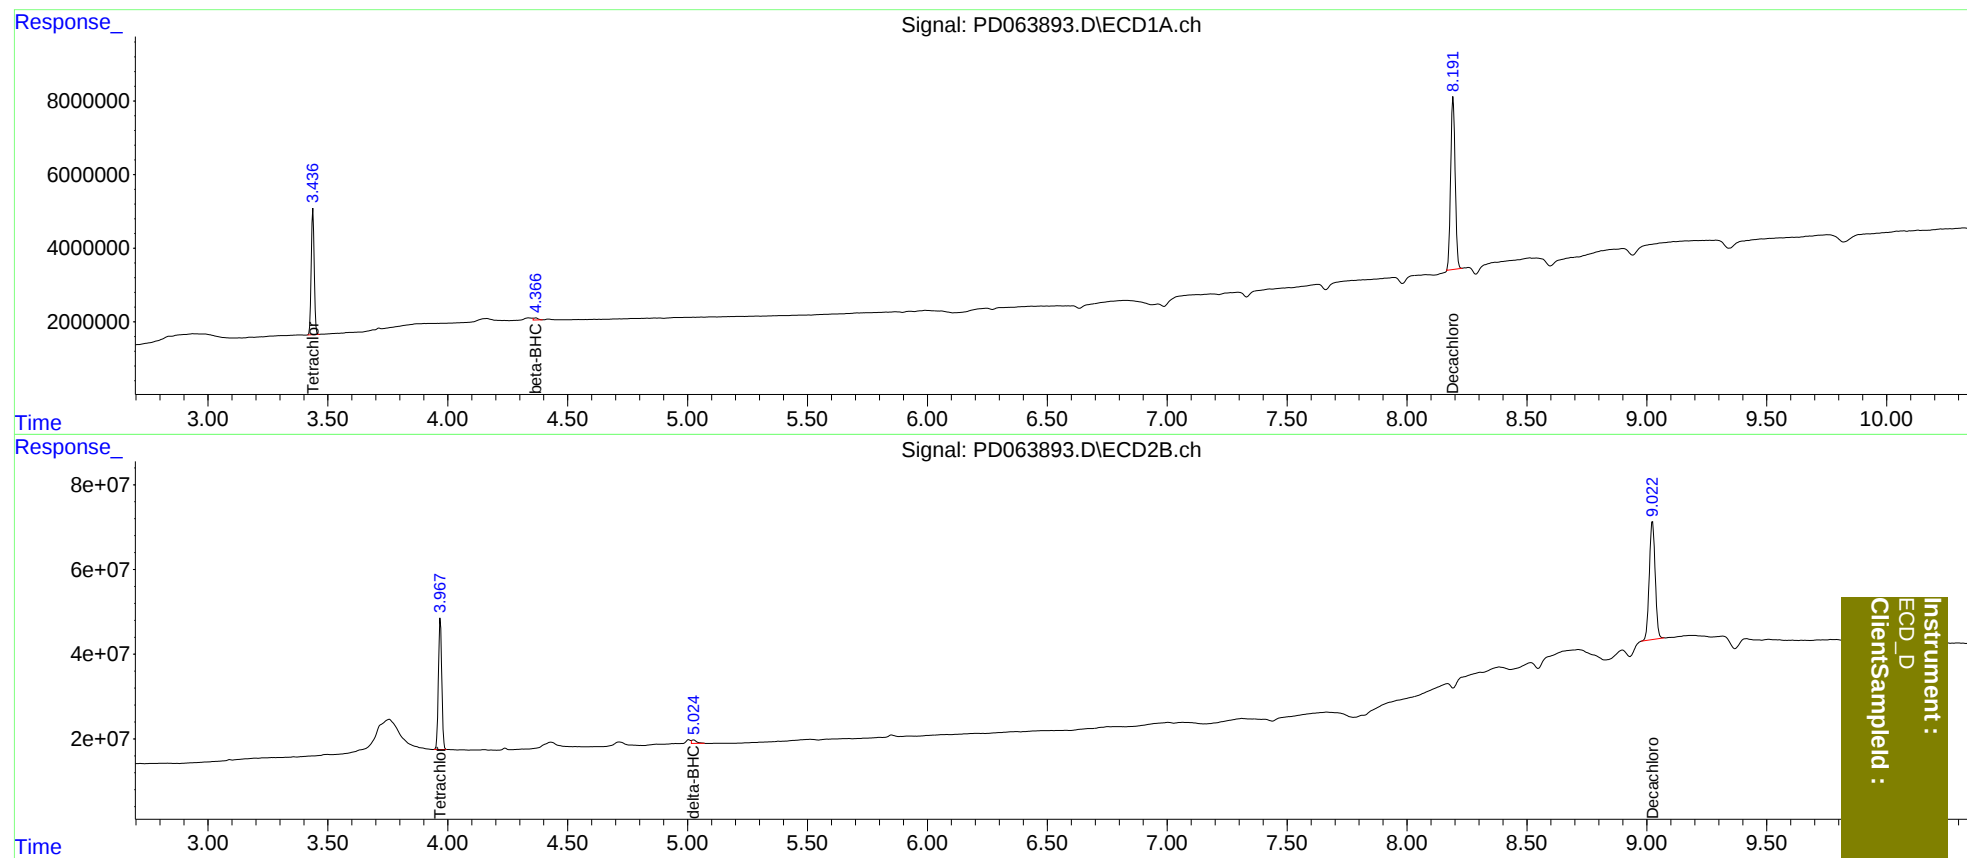


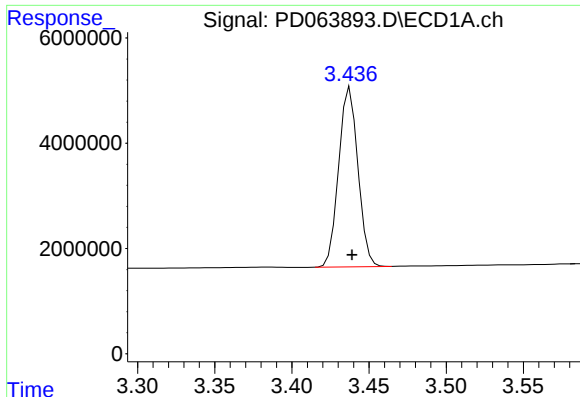

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.001 min
Response: 29649328
Conc: 21.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

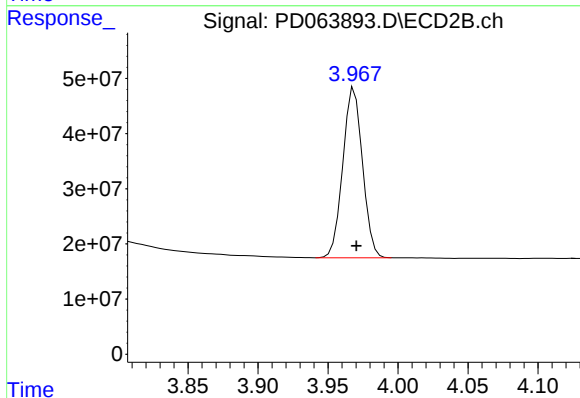


#1 Tetrachloro-m-xylene

R.T.: 3.969 min
Delta R.T.: -0.001 min
Response: 302173239
Conc: 21.47 ng/ml

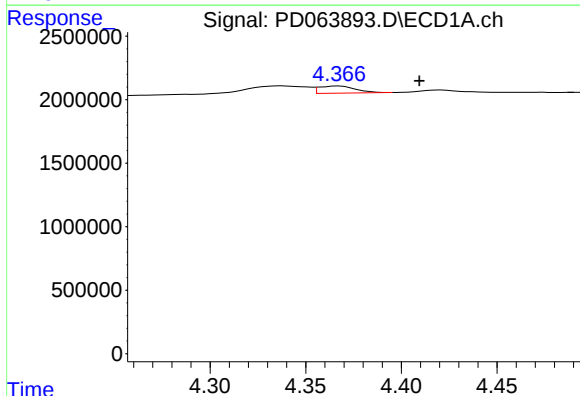


#6 beta-BHC

R.T.: 4.367 min
Delta R.T.: -0.042 min
Response: 744409
Conc: 0.80 ng/ml

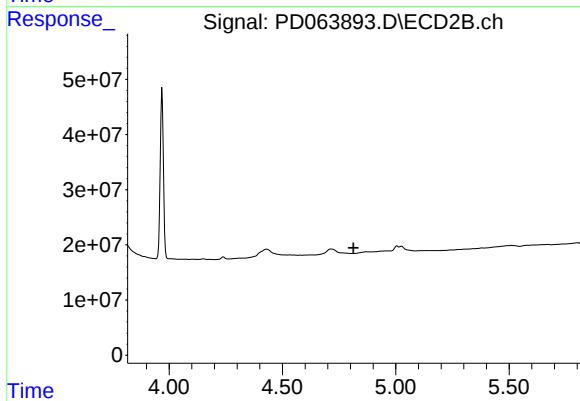

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.814 min
Response: 0
Conc: N.D.

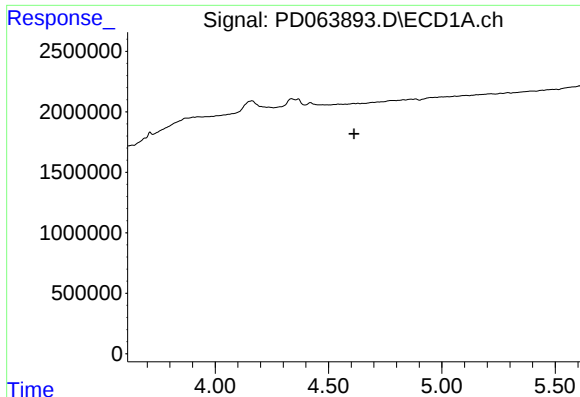

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.613 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

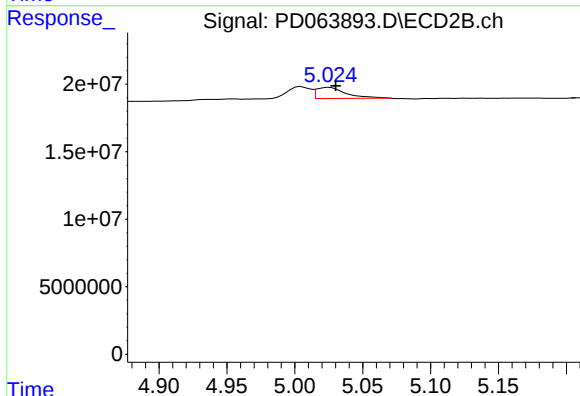


#7 delta-BHC

R.T.: 5.026 min
Delta R.T.: -0.005 min
Response: 12501906
Conc: 0.57 ng/ml

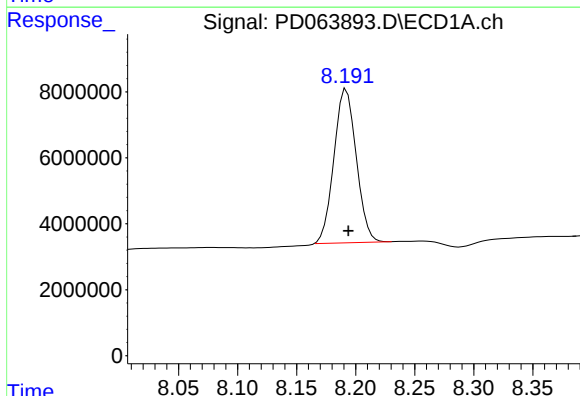

#27 Decachlorobiphenyl

R.T.: 8.192 min
Delta R.T.: -0.002 min
Response: 61412063
Conc: 37.80 ng/ml

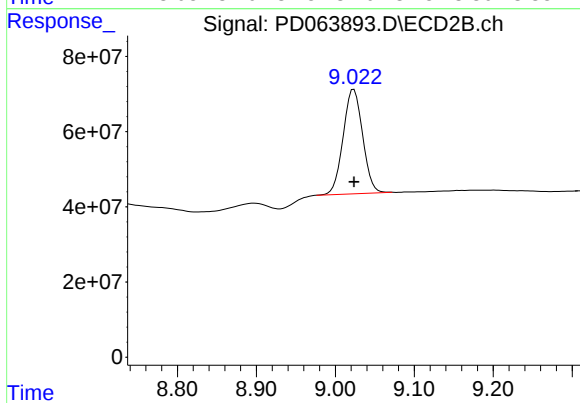

#27 Decachlorobiphenyl

R.T.: 9.023 min
Delta R.T.: 0.000 min
Response: 478509231
Conc: 32.61 ng/ml