

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061821\
 Data File : PD063897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 13:55
 Operator : AR\AJ
 Sample : M2649-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 23:30:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.970	13750323	144.3E6	10.018	10.252
27)	SA Decachlor...	8.194	9.025	22256703	192.2E6	13.699	13.102
Target Compounds							
2)	A alpha-BHC	0.000	4.330f	0	3332963	N.D.	0.151
3)	MA gamma-BHC...	4.163	0.000	1850045	0	0.919	N.D. #
6)	B beta-BHC	4.370f	4.782f	1347494	2735073	1.449	0.306 #
7)	B delta-BHC	0.000	5.025	0	32694294	N.D.	1.482
8)	B Heptachlo...	0.000	5.853	0	853595	N.D.	<MDL
9)	A Endosulfan I	0.000	6.204	0	2508042	N.D.	0.140
10)	B trans-Chl...	0.000	6.130f	0	2317537	N.D.	0.116
11)	B cis-Chlor...	0.000	6.149	0	4097567	N.D.	0.217
15)	B Endosulfa...	0.000	6.890	0	18521909	N.D.	1.224
19)	B Endosulfa...	6.659	0.000	11327693	0	7.888	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061821\
Data File : PD063897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 13:55
Operator : AR\AJ
Sample : M2649-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 23:30:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

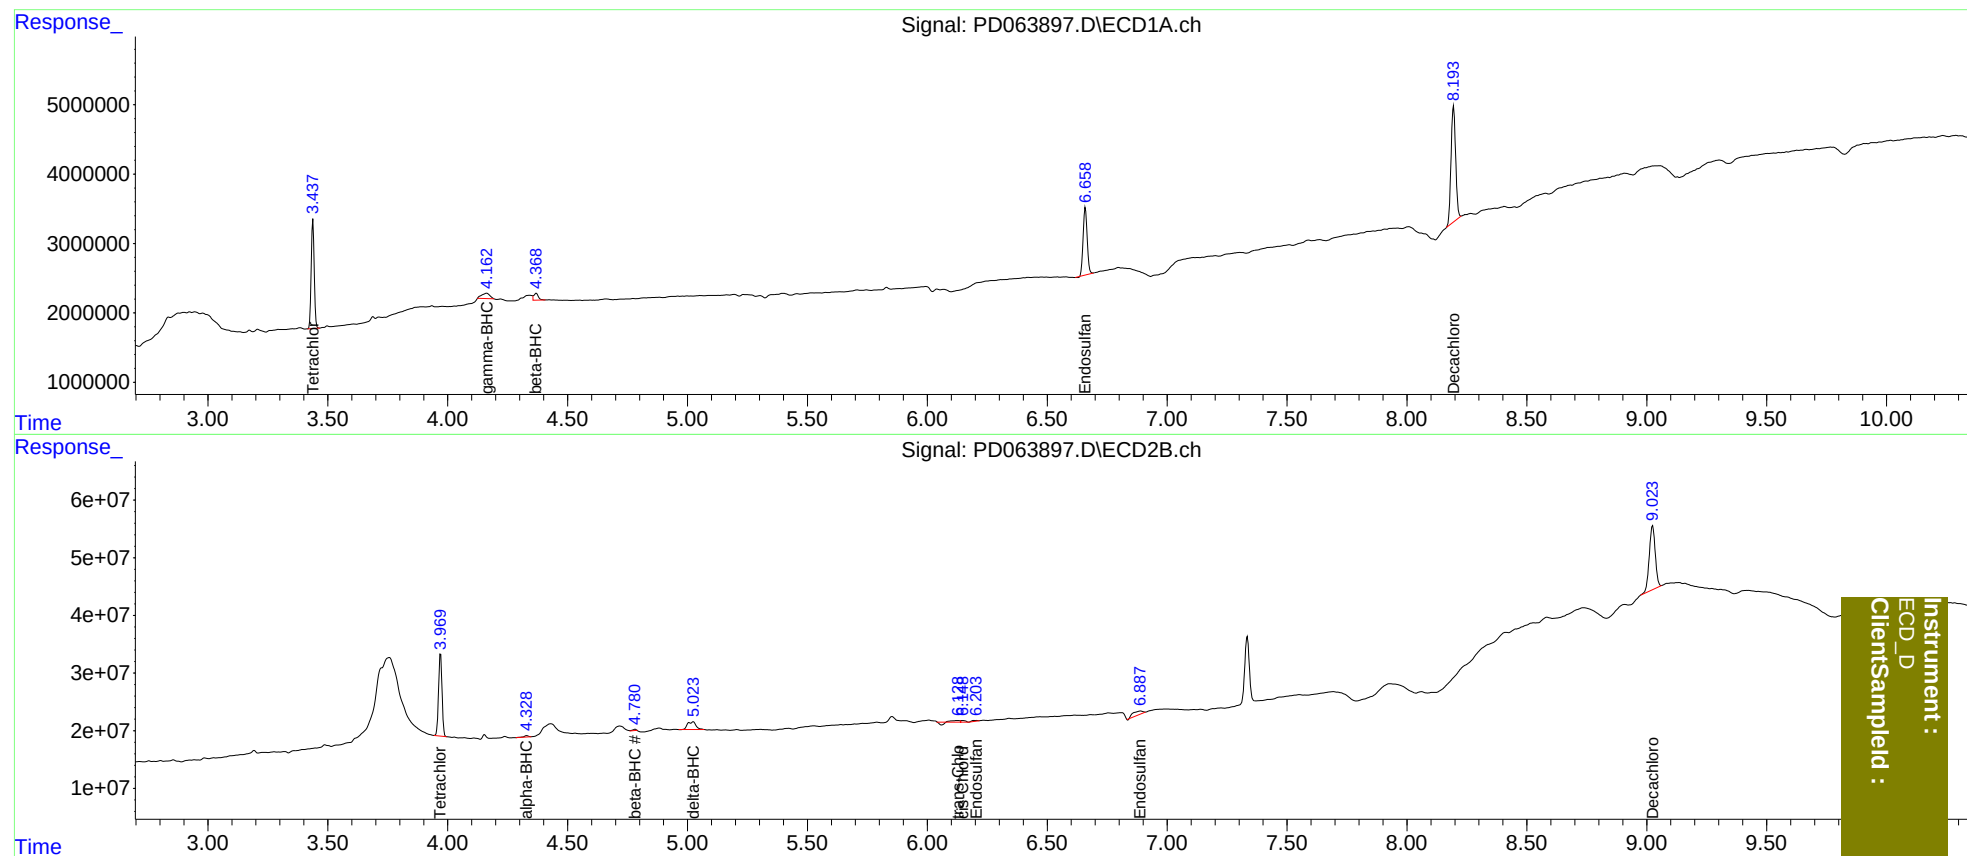


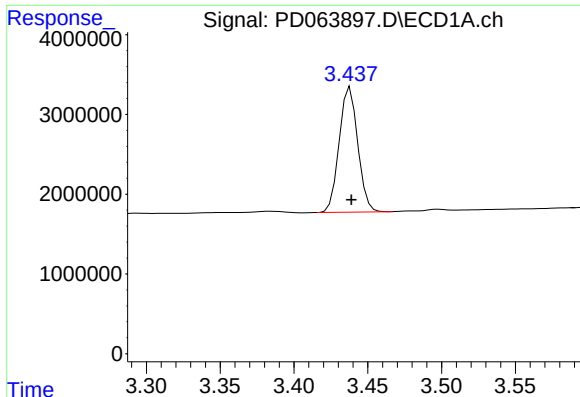

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: 0.000 min
Response: 13750323
Conc: 10.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

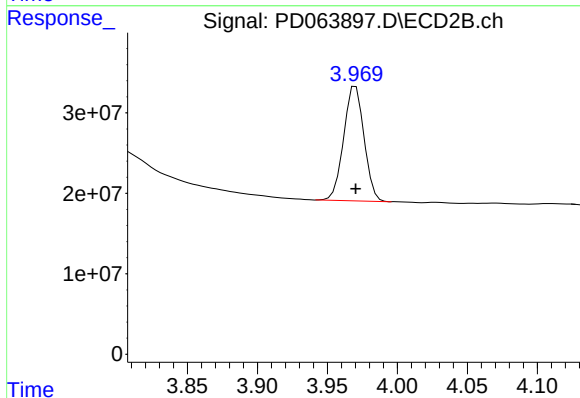


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 144313454
Conc: 10.25 ng/ml

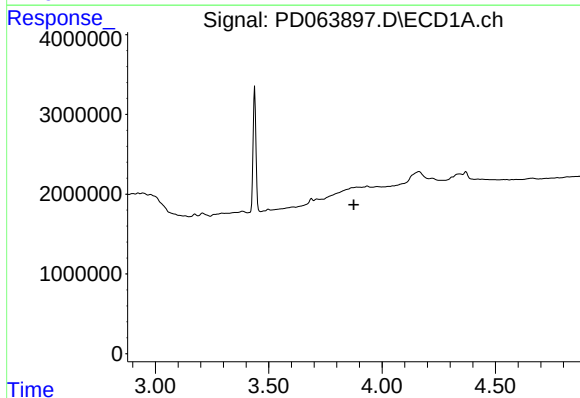


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.875 min
Response: 0
Conc: N.D.

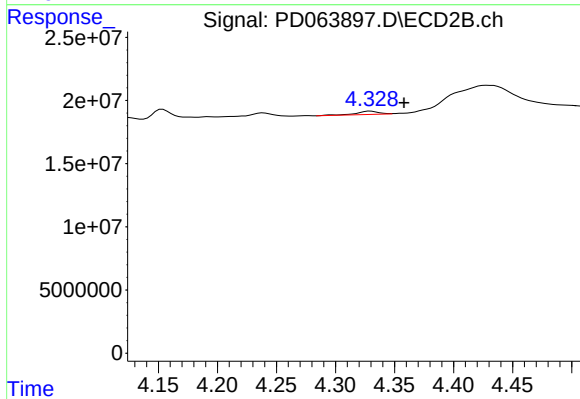

#2 alpha-BHC

R.T.: 4.330 min
Delta R.T.: -0.028 min
Response: 3332963
Conc: 0.15 ng/ml

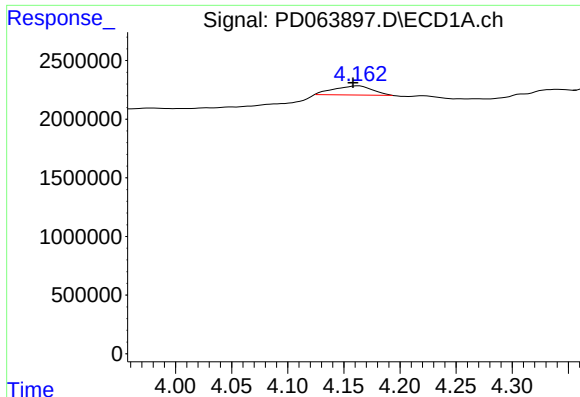

#3 gamma-BHC (Lindane)


R.T.: 4.163 min

Delta R.T.: 0.005 min

Response: 1850045

Conc: 0.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

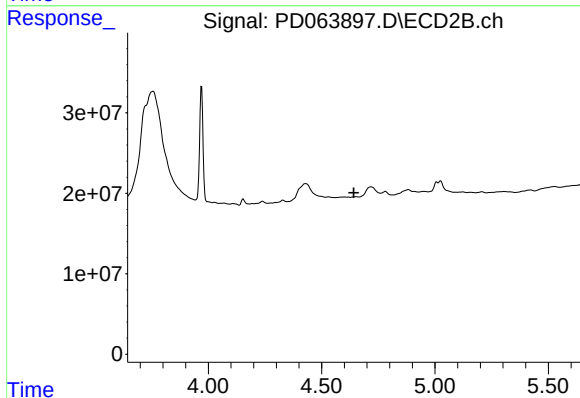


#3 gamma-BHC (Lindane)

R.T.: 0.000 min

Exp R.T. : 4.642 min

Response: 0

Conc: N.D.

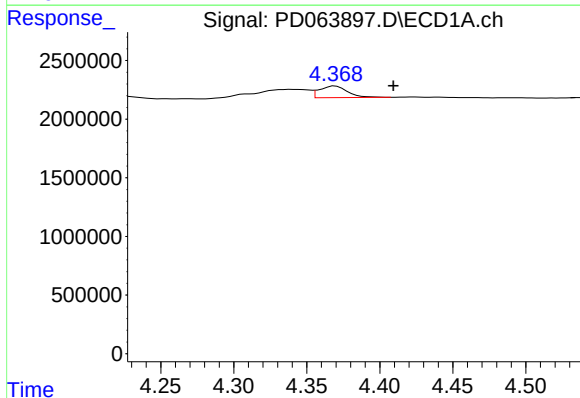


#6 beta-BHC

R.T.: 4.370 min

Delta R.T.: -0.040 min

Response: 1347494

Conc: 1.45 ng/ml

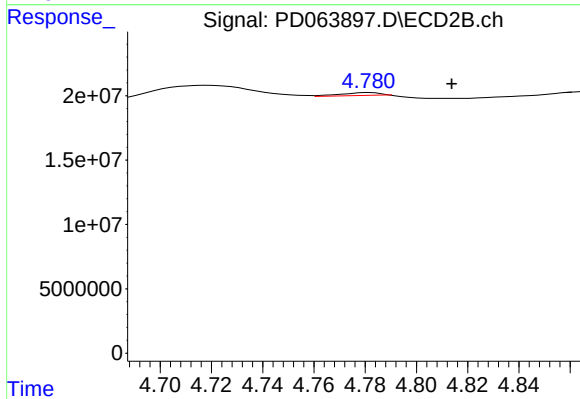


#6 beta-BHC

R.T.: 4.782 min

Delta R.T.: -0.032 min

Response: 2735073


Conc: 0.31 ng/ml

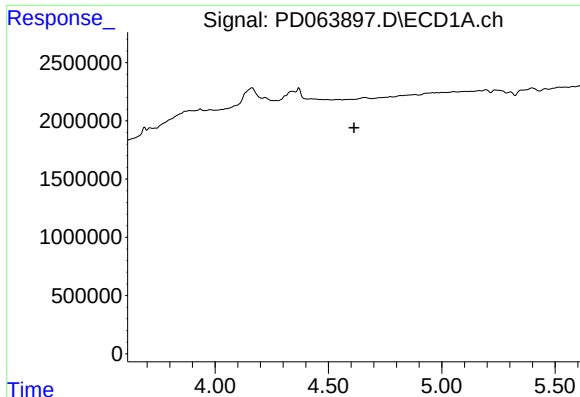

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.613 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

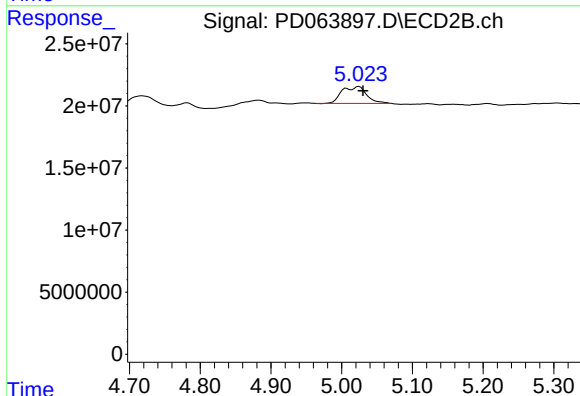


#7 delta-BHC

R.T.: 5.025 min
Delta R.T.: -0.005 min
Response: 32694294
Conc: 1.48 ng/ml

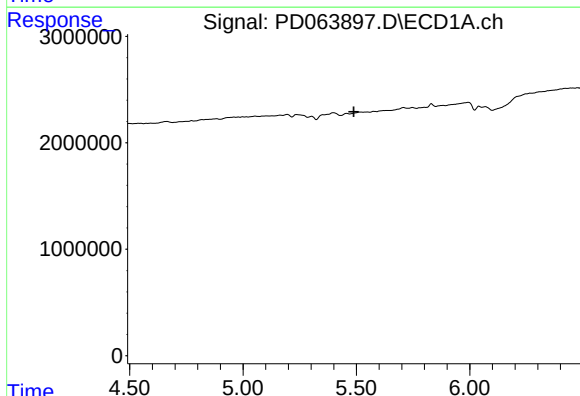


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.488 min
Response: 0
Conc: N.D.

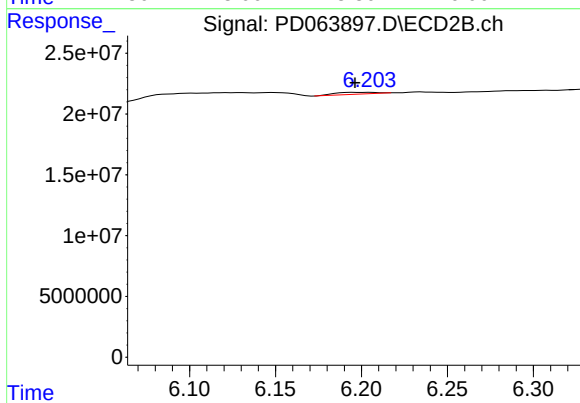

#9 Endosulfan I


R.T.: 6.204 min
Delta R.T.: 0.008 min
Response: 2508042
Conc: 0.14 ng/ml

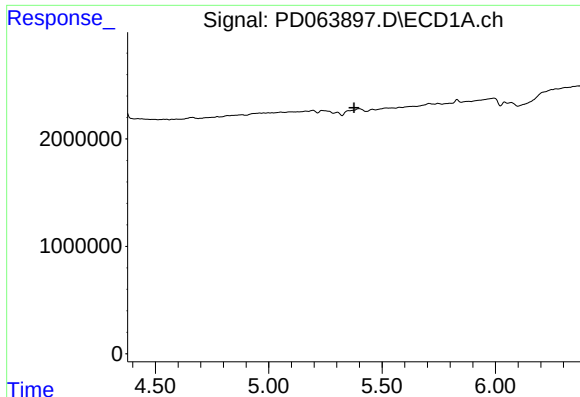

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

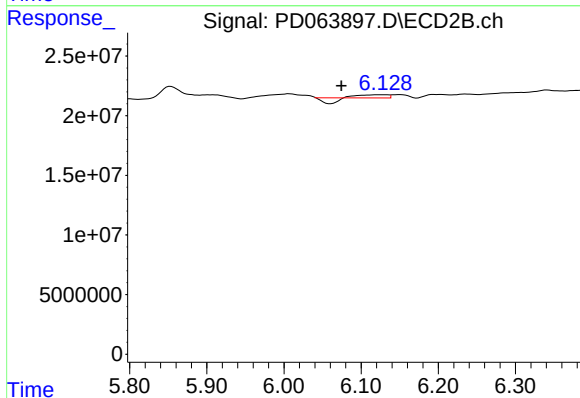


#10 trans-Chlordane

R.T.: 6.130 min
Delta R.T.: 0.055 min
Response: 2317537
Conc: 0.12 ng/ml

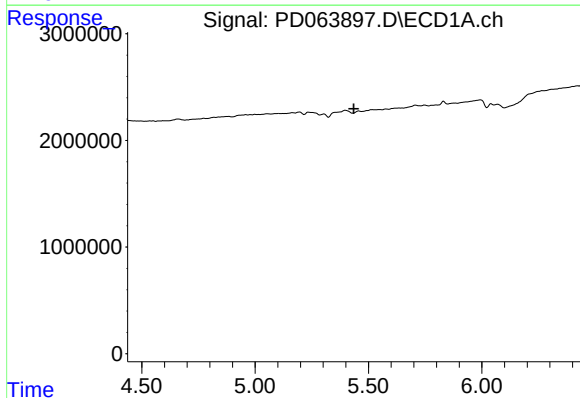


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.435 min
Response: 0
Conc: N.D.

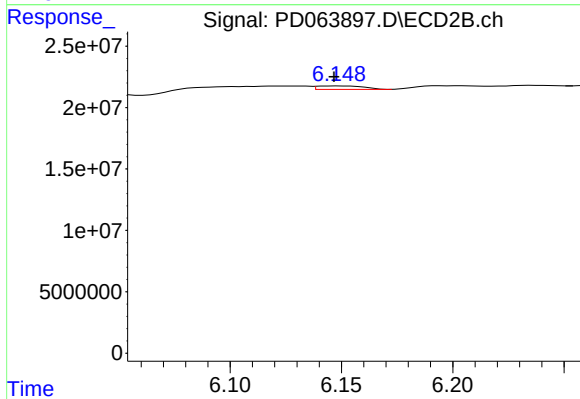

#11 cis-Chlordane


R.T.: 6.149 min
Delta R.T.: 0.002 min
Response: 4097567
Conc: 0.22 ng/ml

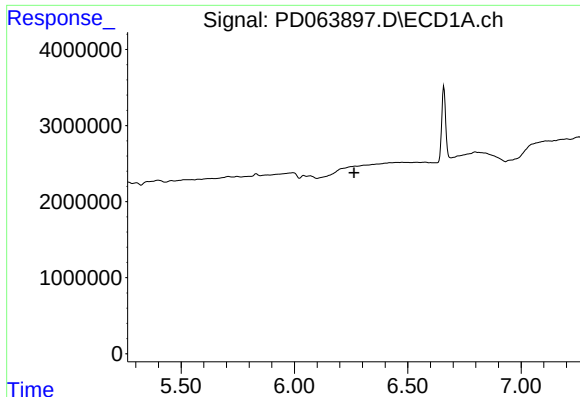

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.263 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

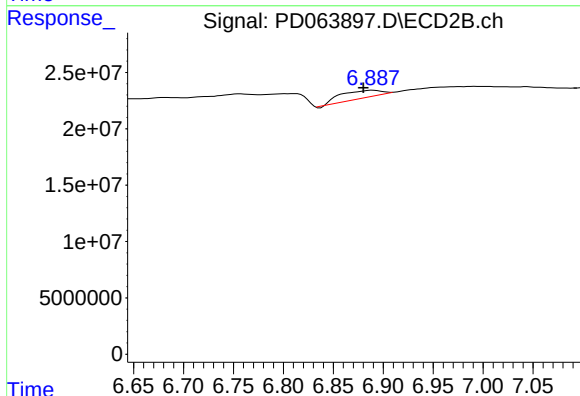


#15 Endosulfan II

R.T.: 6.890 min
Delta R.T.: 0.010 min
Response: 18521909
Conc: 1.22 ng/ml

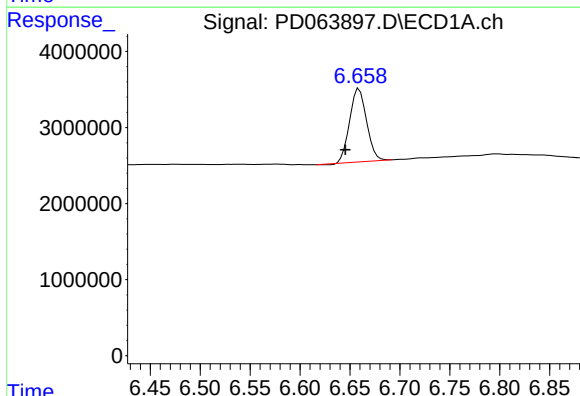


#19 Endosulfan Sulfate

R.T.: 6.659 min
Delta R.T.: 0.014 min
Response: 11327693
Conc: 7.89 ng/ml

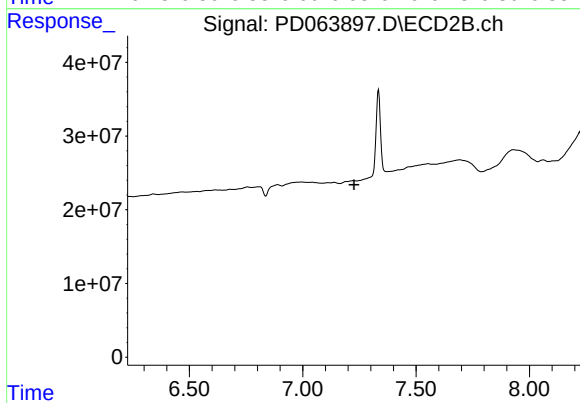

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.227 min
Response: 0
Conc: N.D.

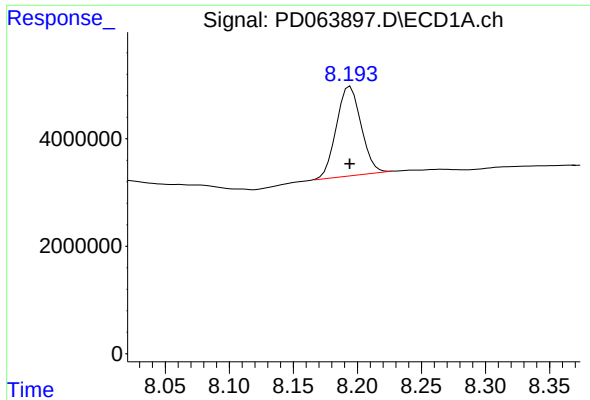

#27 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 22256703
Conc: 13.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

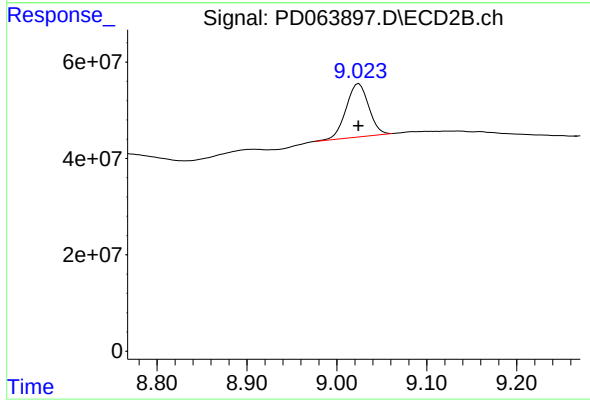

#27 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 192246834
Conc: 13.10 ng/ml