

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061821\
 Data File : PD063901.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 14:51
 Operator : AR\AJ
 Sample : PIBLK21
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 23:32:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.970	29175743	293.2E6	21.256	20.826
27)	SA Decachlor...	8.194	9.025	62563994	501.2E6	38.508	34.159
Target Compounds							
3)	MA gamma-BHC...	4.161	0.000	1262004	0	0.627	N.D. #
6)	B beta-BHC	4.368f	4.765f	801244	6465885	0.861	0.723
7)	B delta-BHC	0.000	5.025	0	7750486	N.D.	0.351
8)	B Heptachlo...	0.000	5.850	0	2948046	N.D.	0.148
9)	A Endosulfan I	0.000	6.194	0	1706743	N.D.	<MDL
10)	B trans-Chl...	0.000	6.025f	0	1254964	N.D.	<MDL
11)	B cis-Chlor...	0.000	6.194f	0	1706743	N.D.	<MDL
14)	MA Endrin	0.000	6.718f	0	1488806	N.D.	<MDL
15)	B Endosulfa...	0.000	6.912	0	8393790	N.D.	0.555
19)	B Endosulfa...	0.000	7.276f	0	11542363	N.D.	0.741
20)	A Methoxychlor	0.000	7.562	0	8168574	N.D.	1.132
26)	Toxaphene-5	0.000	7.562	0	8168574	N.D.	45.146

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061821\
Data File : PD063901.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 14:51
Operator : AR\AJ
Sample : PIBLK21
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 23:32:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

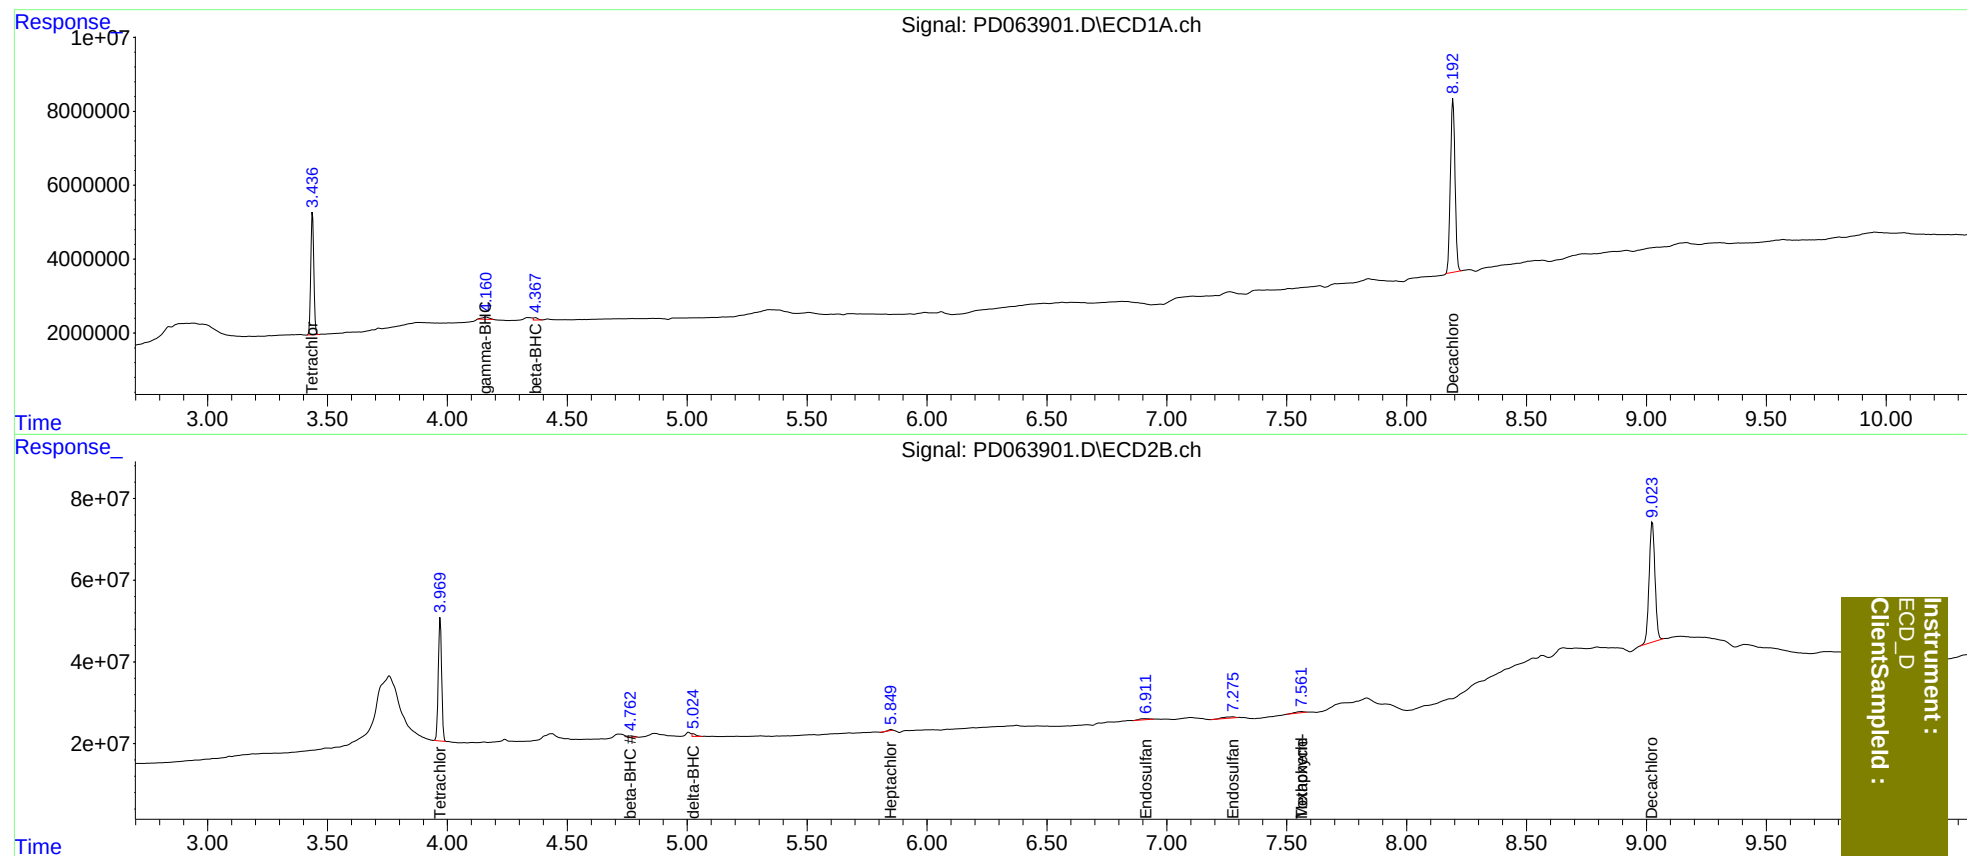


Instrument :
ECD_D
ClientSampled :

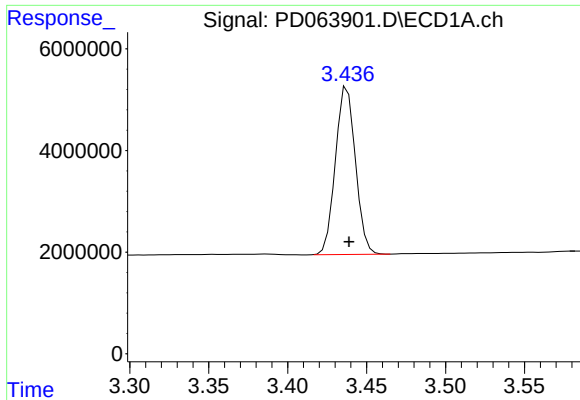

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: -0.001 min
Response: 29175743
Conc: 21.26 ng/ml

Instrument :
ECD_D
ClientSampleId :

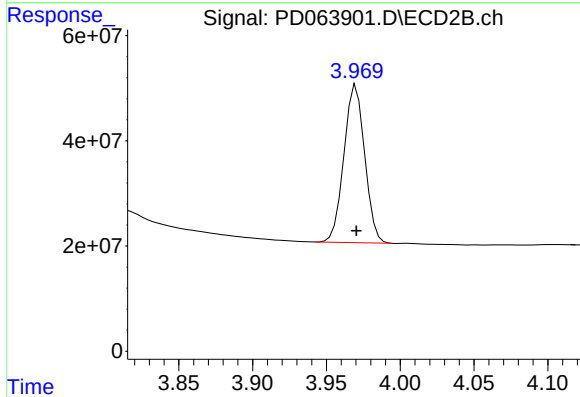


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 293161594
Conc: 20.83 ng/ml

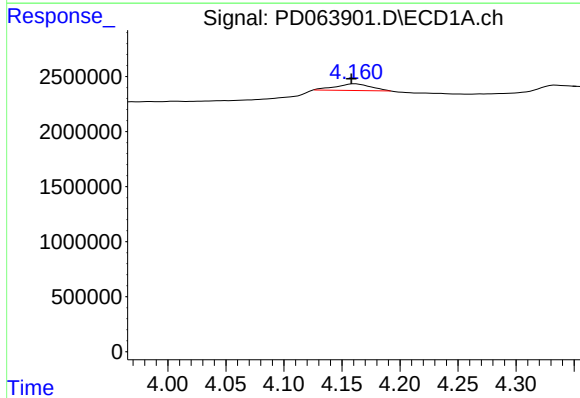


#3 gamma-BHC (Lindane)

R.T.: 4.161 min
Delta R.T.: 0.003 min
Response: 1262004
Conc: 0.63 ng/ml

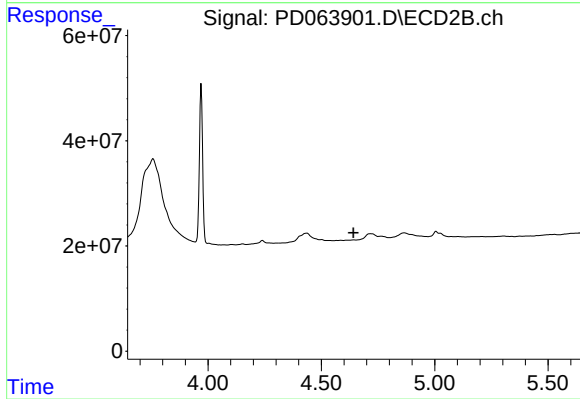

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.642 min
Response: 0
Conc: N.D.

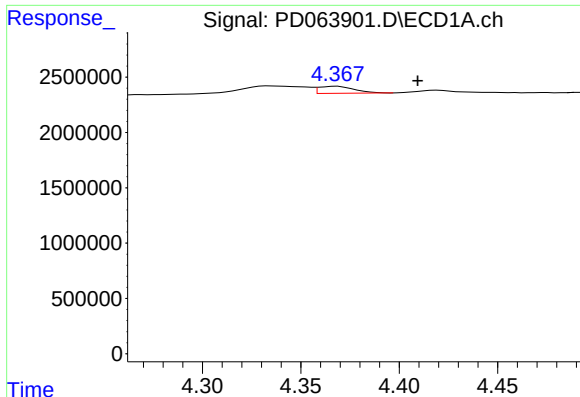

#6 beta-BHC


R.T.: 4.368 min
Delta R.T.: -0.041 min
Response: 801244
Conc: 0.86 ng/ml

Instrument :
ECD_D
ClientSampleId :

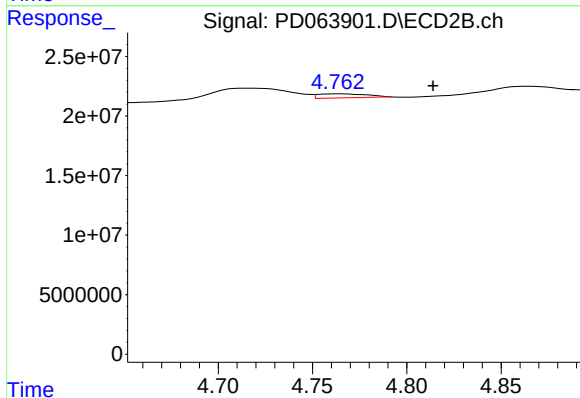


#6 beta-BHC

R.T.: 4.765 min
Delta R.T.: -0.049 min
Response: 6465885
Conc: 0.72 ng/ml

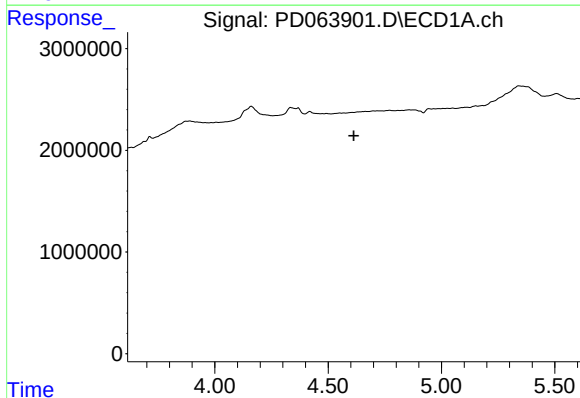


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.613 min
Response: 0
Conc: N.D.

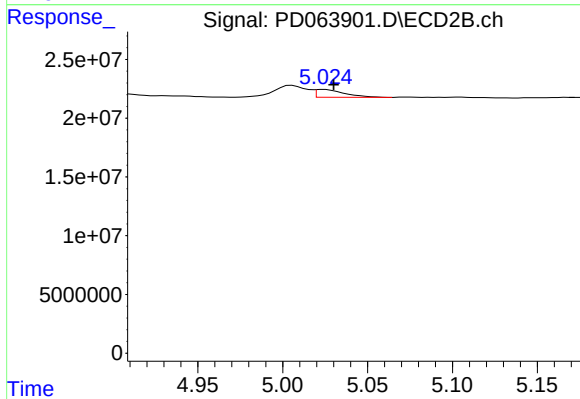

#7 delta-BHC


R.T.: 5.025 min
Delta R.T.: -0.005 min
Response: 7750486
Conc: 0.35 ng/ml

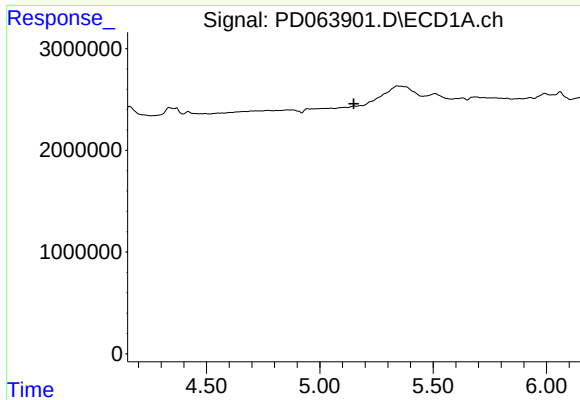

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.150 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

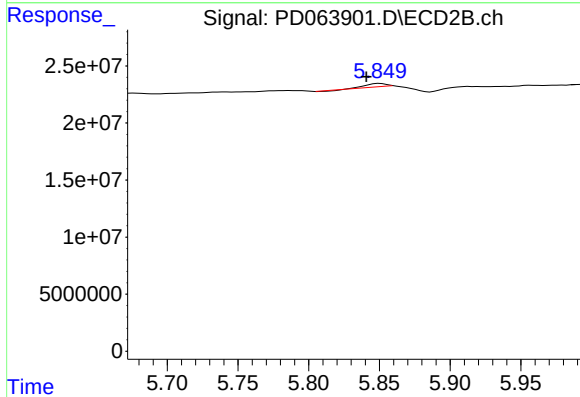


#8 Heptachlor epoxide

R.T.: 5.850 min
Delta R.T.: 0.010 min
Response: 2948046
Conc: 0.15 ng/ml

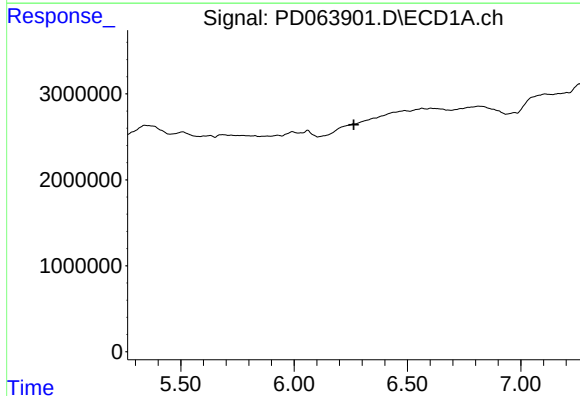


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.263 min
Response: 0
Conc: N.D.

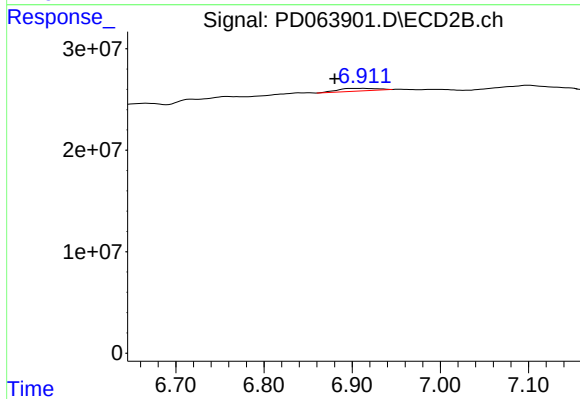

#15 Endosulfan II


R.T.: 6.912 min
Delta R.T.: 0.032 min
Response: 8393790
Conc: 0.55 ng/ml

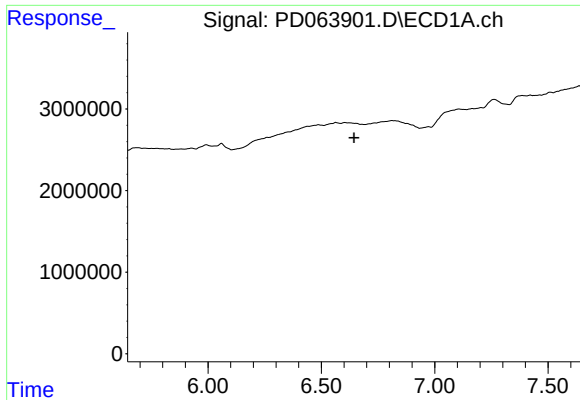

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.645 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

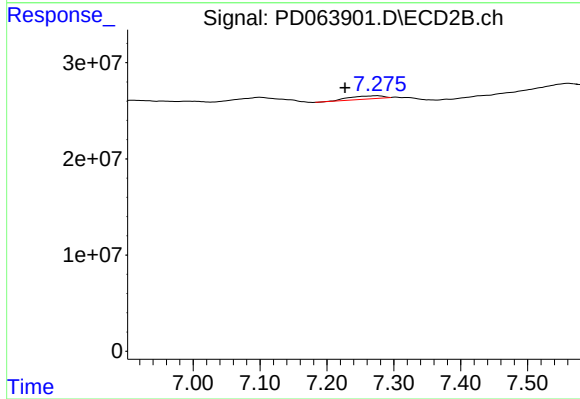


#19 Endosulfan Sulfate

R.T.: 7.276 min
Delta R.T.: 0.049 min
Response: 11542363
Conc: 0.74 ng/ml

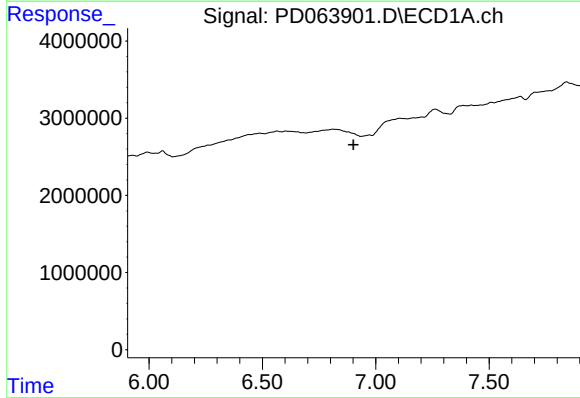


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.902 min
Response: 0
Conc: N.D.

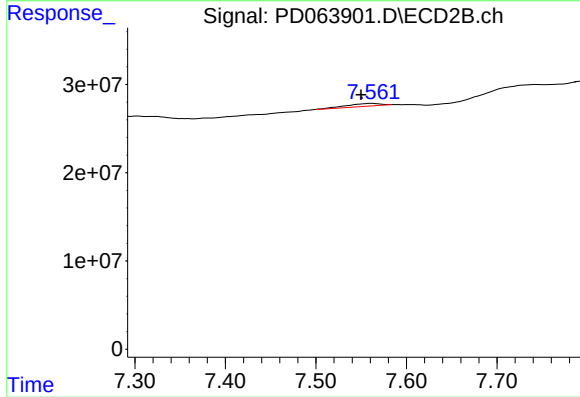

#20 Methoxychlor


R.T.: 7.562 min
Delta R.T.: 0.012 min
Response: 8168574
Conc: 1.13 ng/ml

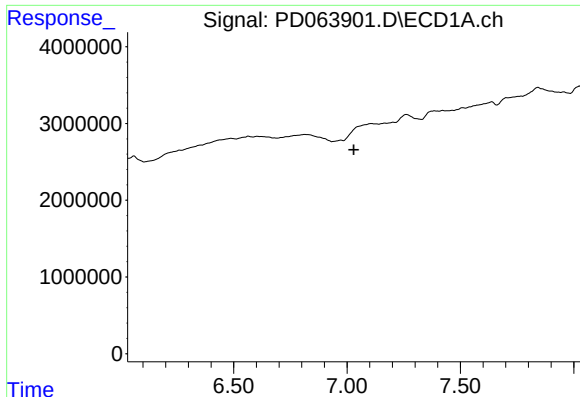

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T.: 7.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

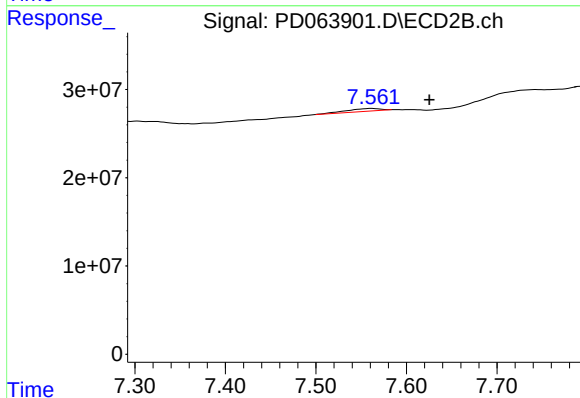


#26 Toxaphene-5

R.T.: 7.562 min
Delta R.T.: -0.064 min
Response: 8168574
Conc: 45.15 ng/ml

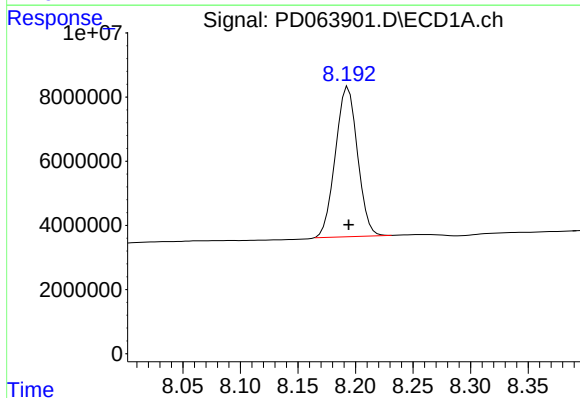

#27 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 62563994
Conc: 38.51 ng/ml

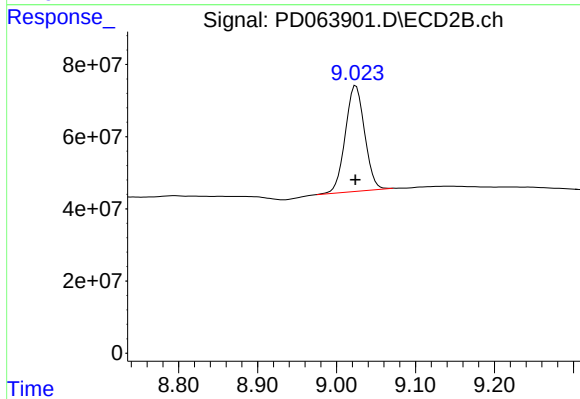

#27 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 501202822
Conc: 34.16 ng/ml