

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061821\
 Data File : PD063910.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 15:04
 Operator : AR\AJ
 Sample : INDA310
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3010

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 23:32:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.970	28839736	292.3E6	21.011	20.762
27)	SA Decachlor...	8.193	9.024	61062278	498.8E6	37.584	33.993
Target Compounds							
2)	A alpha-BHC	3.874	4.358	43010860	456.0E6	21.065	20.633
3)	MA gamma-BHC...	4.157	4.642	41562054	416.5E6	20.644	20.385
4)	MA Heptachlor	4.457	5.149	40146066	424.7E6	20.631	20.440
9)	A Endosulfan I	5.487	6.196	33639459	345.5E6	20.460	19.344
13)	MA Dieldrin	5.730	6.453	76740633	728.6E6	40.967	38.078
14)	MA Endrin	5.988	6.670	56883644	528.9E6	35.196	33.401
16)	A 4,4'-DDD	6.114	6.793	61308288	584.1E6	41.488	38.448
17)	MA 4,4'-DDT	6.354	7.092	60063723	537.6E6	39.562	34.976
20)	A Methoxychlor	6.902	7.550	166.7E6	1272.9E6	202.061	176.427

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061821\
Data File : PD063910.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 15:04
Operator : AR\AJ
Sample : INDA310
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 23:32:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

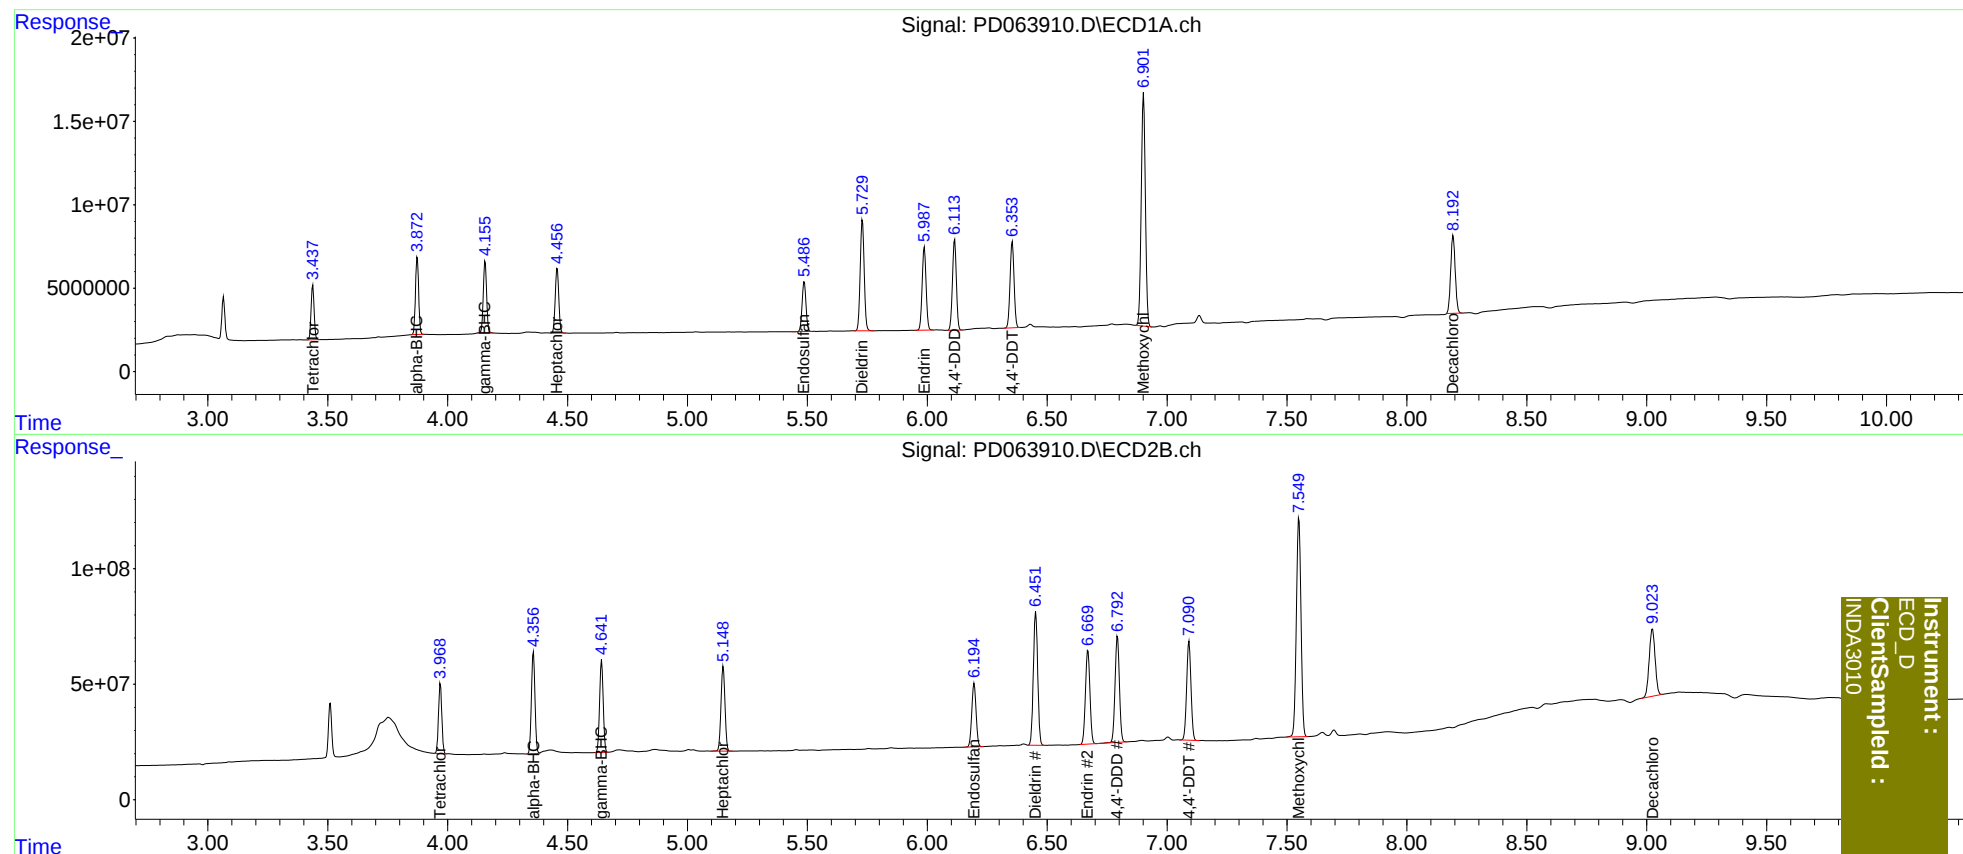

Instrument :
ECD_D
ClientSample :
INDA3010