

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061821\
 Data File : PD063904.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 13:41
 Operator : AR\AJ
 Sample : PB137170BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 23:30:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Instrument :
 ECD_D
 ClientSampleId :
 PLCS170

Manual Integrations
 APPROVED

Ankita
 6/21/2021 2:47:33 PM

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.970	29410254	283.9E6	21.426	20.168
2)	SA Decachlor...	8.195	9.025	62165670	500.9E6	38.263	34.135
Target Compounds							
2)	A alpha-BHC	3.872	4.356	13912583	113.7E6	6.814	5.145m
3)	MA gamma-BHC...	4.157	4.642	10935861	98899310	5.432	4.841
4)	MA Heptachlor	4.458	5.149	9447191	102.9E6	4.855	4.954
5)	MB Aldrin	4.706	5.454	9278669	97971421	4.940	4.760
6)	B beta-BHC	4.409	4.813	4644405	40329340	4.993	4.508
7)	B delta-BHC	4.612	5.029	9494984	160.6E6	4.865	7.282 #
8)	B Heptachlo...	5.149	5.839	8680091	126.3E6	4.934	6.344m#
9)	A Endosulfan I	5.488	6.196	8245830	90278047	5.015	5.055
10)	B trans-Chl...	5.375	6.073	9132040	94936792	4.995	4.764m
11)	B cis-Chlor...	5.434	6.146	8383065	100.4E6	4.727	5.312
12)	B 4,4'-DDE	5.598	6.303	17481446	194.0E6	9.681	10.255
13)	MA Dieldrin	5.731	6.451	17454442	196.3E6	9.318	10.261m
14)	MA Endrin	5.989	6.670	15388482	152.5E6	9.522	9.631
15)	B Endosulfa...	6.262	6.879	14518061	169.1E6	9.667	11.172
16)	A 4,4'-DDD	6.115	6.793	13928320	181.0E6	9.425	11.916 #
17)	MA 4,4'-DDT	6.356	7.092	12073980	133.6E6	7.953	8.693
18)	B Endrin al...	6.432	7.004	13420374	139.8E6	10.299	10.594
19)	B Endosulfa...	6.646	7.227	11812439	156.6E6	8.226	10.047
20)	A Methoxychlor	6.903	7.550	40077912	350.1E6	48.567	48.525
21)	B Endrin ke...	7.138	7.695	18256659	154.8E6	10.350	10.043m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061821\
Data File : PD063904.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 13:41
Operator : AR\AJ
Sample : PB137170BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 23:30:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

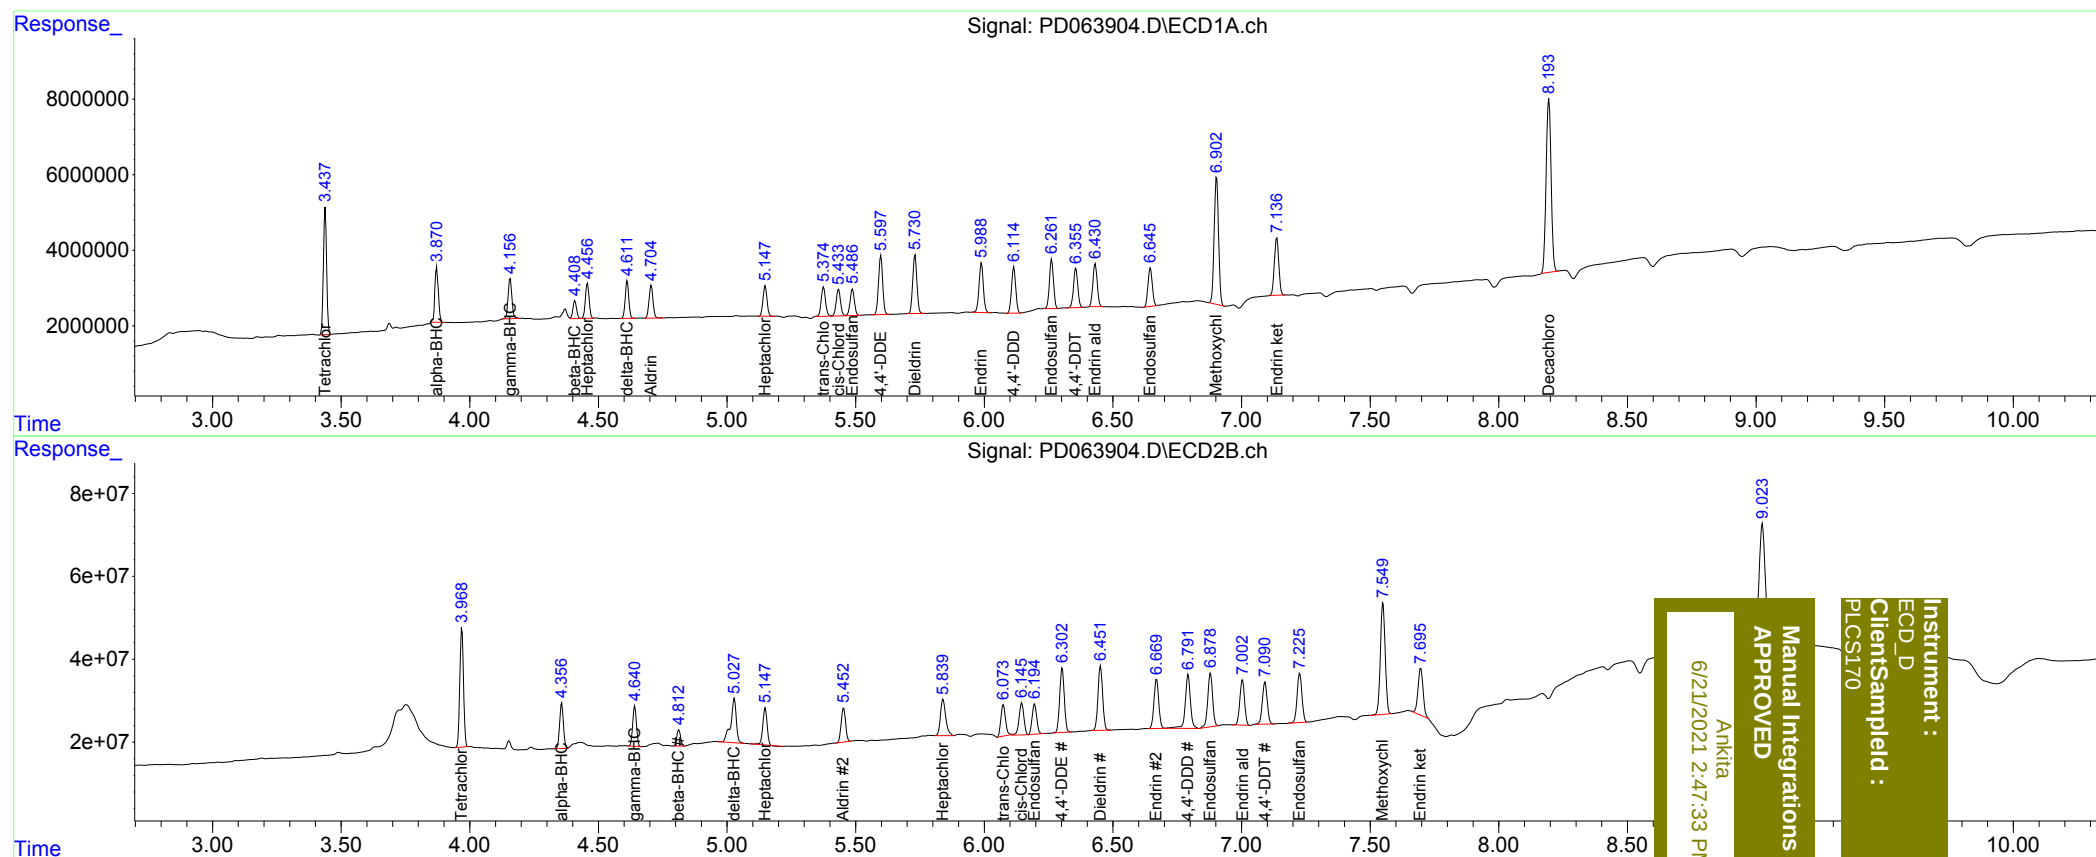

6/21/2021 2:47:33 PM

Ankita

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
PLCS170