

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061821\
 Data File : PD063914.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2021 16:08
 Operator : AR\AJ
 Sample : M2649-03MSD
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG5H8MSD

Manual Integrations
 APPROVED

Ankita
 6/28/2021 8:33:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 08:17:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 21 04:24:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	3.970	10535707	93385530	6.777m	5.896
27)	SA Decachlor...	8.190	9.025	56064206	1035.8E6	32.389	74.690m#
Target Compounds							
2)	A alpha-BHC	3.874	4.357	60439537	557.2E6	25.839	22.426m
3)	MA gamma-BHC...	4.162	4.622	474.7E6	2363.8E6	208.604	103.597m#
4)	MA Heptachlor	4.457	5.150	54424417	535.1E6	24.928	22.971
5)	MB Aldrin	4.705	5.454	55926160	534.2E6	27.593	24.248
6)	B beta-BHC	4.408	4.818	29979881	232.3E6	30.876	23.818m
7)	B delta-BHC	4.610	5.031	105.4E6	454.1E6	48.843	19.379 #
8)	B Heptachlo...	5.149	5.840	51214249	347.5E6	27.008	16.891m#
9)	A Endosulfan I	5.509	6.199	591.2E6	776.0E6	323.105m	39.174m#
10)	B trans-Chl...	5.374	6.061	64505982	1304.8E6	33.171m	62.032 #
11)	B cis-Chlor...	5.433	6.145	49611324	539.3E6	26.112	26.776
12)	B 4,4'-DDE	5.597	6.301	82550481	723.2E6	41.811	35.796
13)	MA Dieldrin	5.729	6.453	541.4E6	2516.9E6	258.697m	120.312m#
14)	MA Endrin	5.987	6.670	117.1E6	988.8E6	64.738	56.513m
15)	B Endosulfa...	6.263	6.880	148.0E6	1156.0E6	90.589	71.440m
16)	A 4,4'-DDD	6.114	6.790	71594147	1354.2E6	43.363m	80.448m#
17)	MA 4,4'-DDT	6.355	7.093	70514671	1212.1E6	41.898	73.626 #
18)	B Endrin al...	6.429	7.002	76349960	625.3E6	53.478m	44.447m
19)	B Endosulfa...	6.658	7.228	613.0E6	854.9E6	394.873	51.943m#
20)	A Methoxychlor	6.901	7.550	248.3E6	2515.1E6	269.331m	325.094
21)	B Endrin ke...	7.135	7.698	67690854	770.3E6	35.681	48.539 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061821\
Data File : PD063914.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2021 16:08
Operator : AR\AJ
Sample : M2649-03MSD
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 08:17:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 21 04:24:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

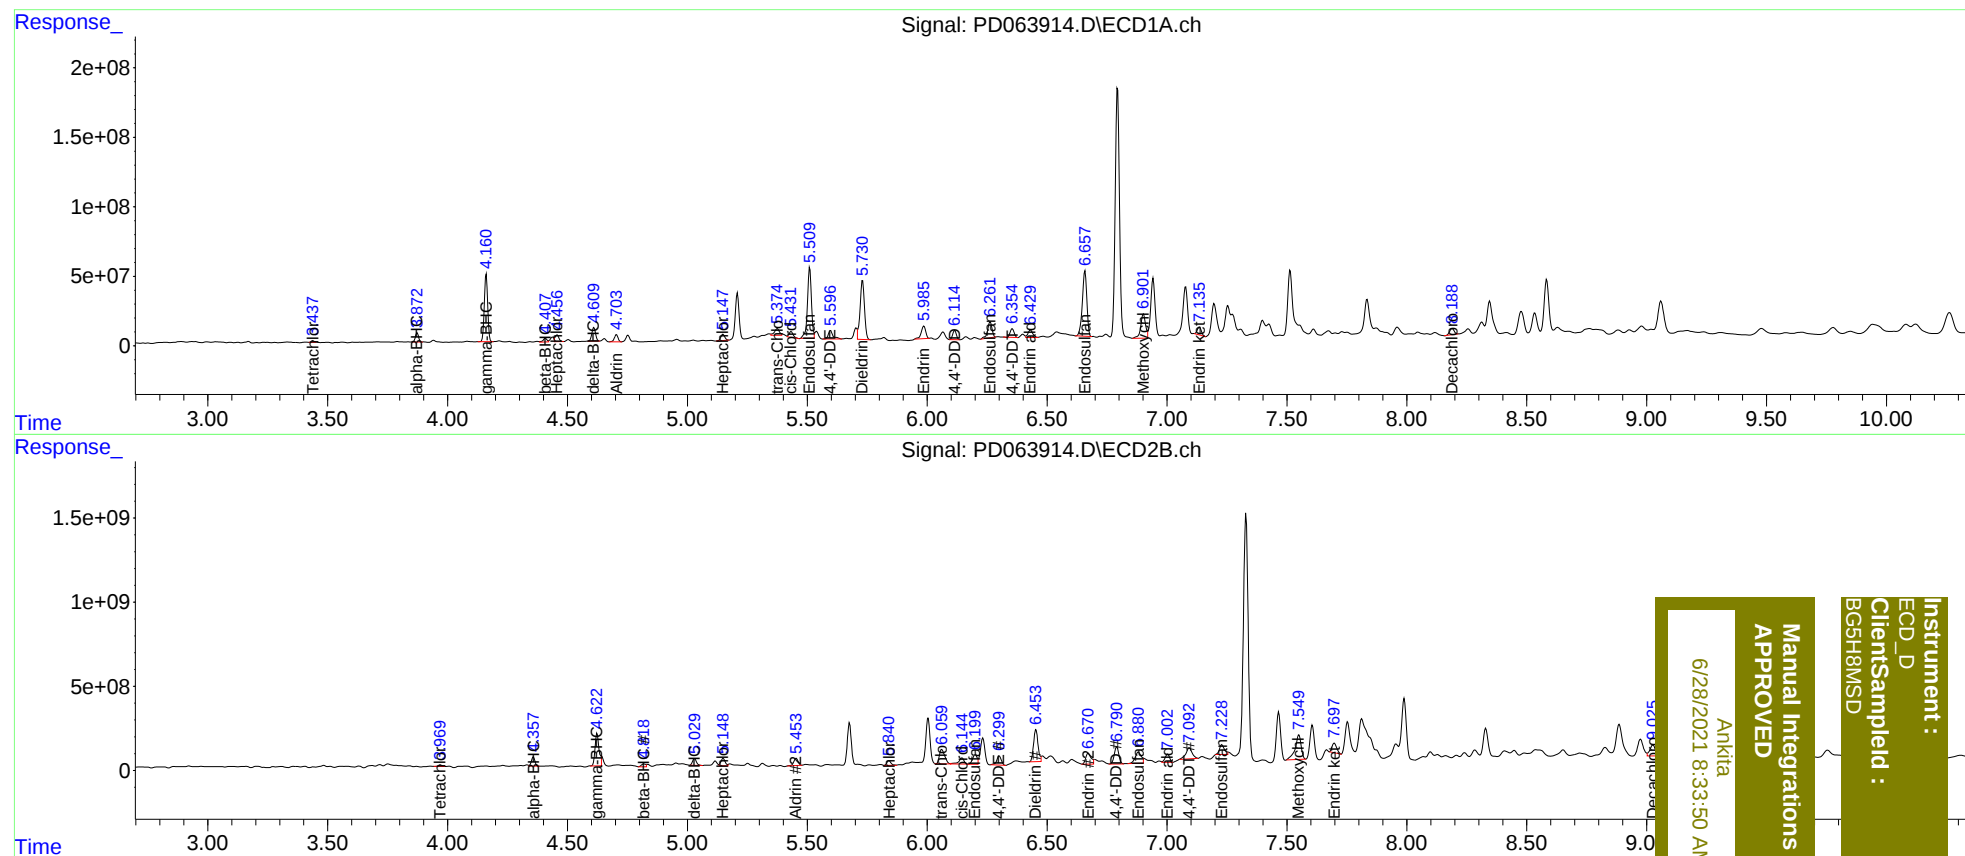

Manual Integrations
APPROVED

6/28/2021 8:33:50 AM

Ankita

Instrument :
ECD_D
Client Sampled :
BG5H8MSD