

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061824\
 Data File : PD083731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2024 21:33
 Operator : AR\AJ
 Sample : PIBLK193
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 23:07:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.772	21372169	99894061	16.373	18.326
2)	SA Decachlor...	9.112	7.896	47580209	129.0E6	24.469	21.240
Target Compounds							
7)	B delta-BHC	4.823	0.000	1967751	0	0.749	N.D. #
10)	B trans-Chl...	6.003	0.000	1630602	0	0.801	N.D. #
11)	B cis-Chlor...	6.003f	0.000	1630602	0	0.783	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061824\
Data File : PD083731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2024 21:33
Operator : AR\AJ
Sample : PIBLK193
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 23:07:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

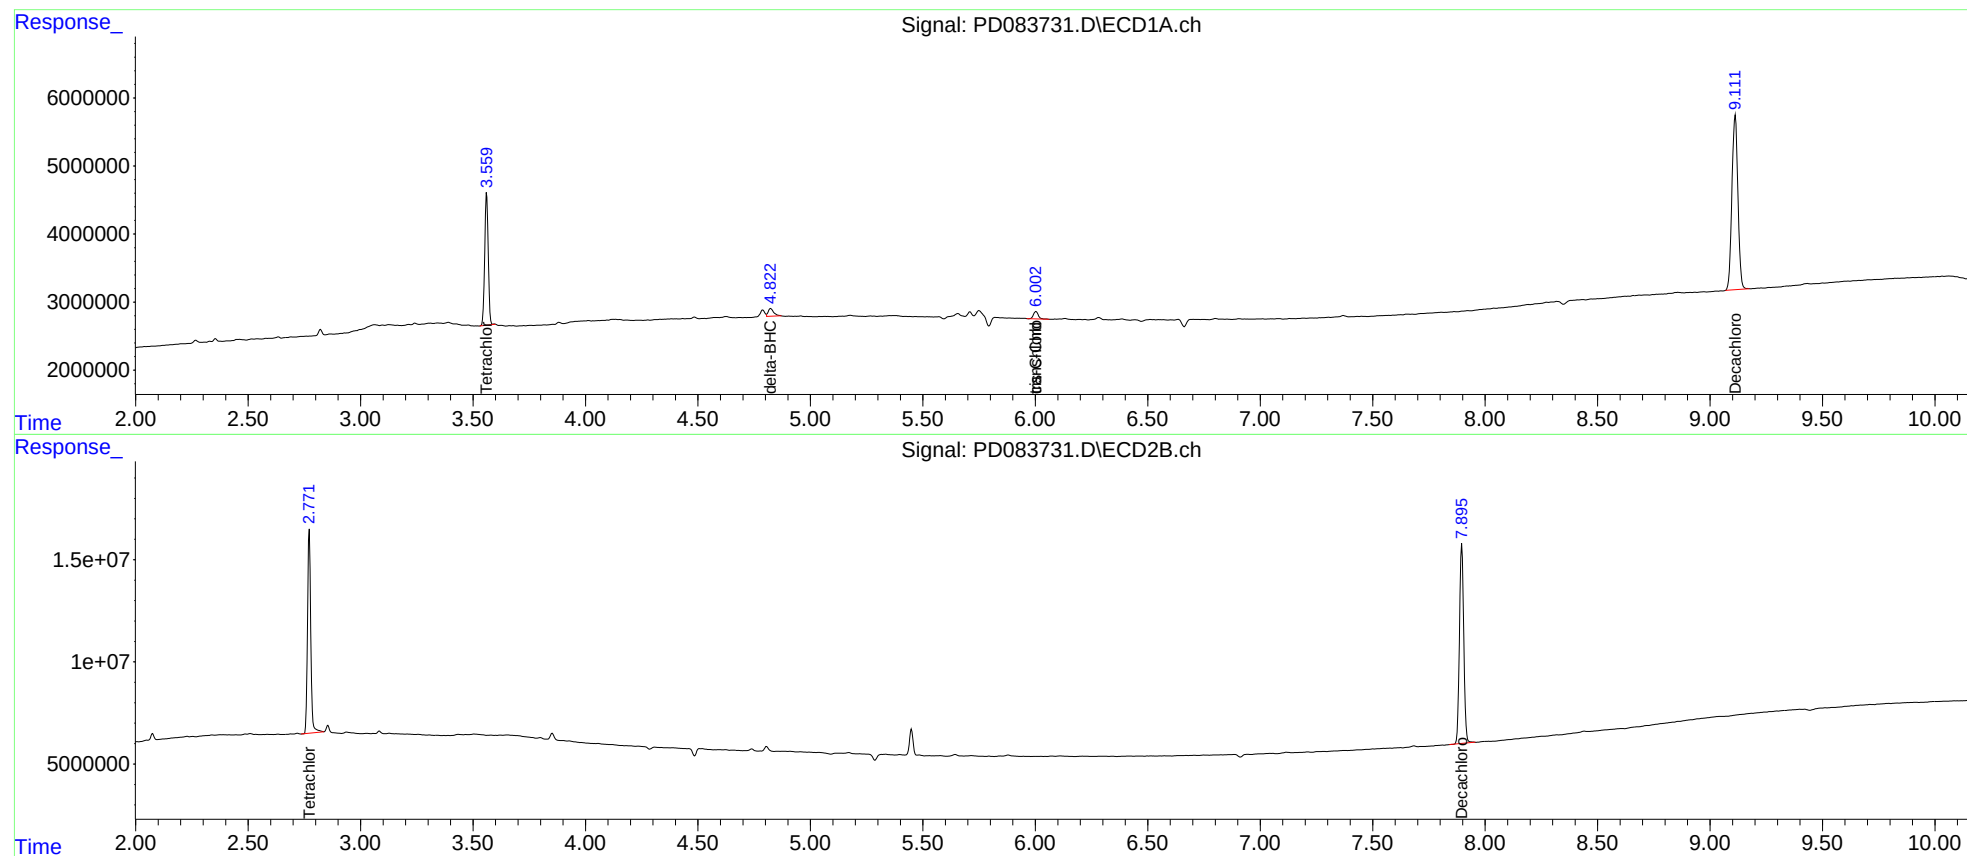

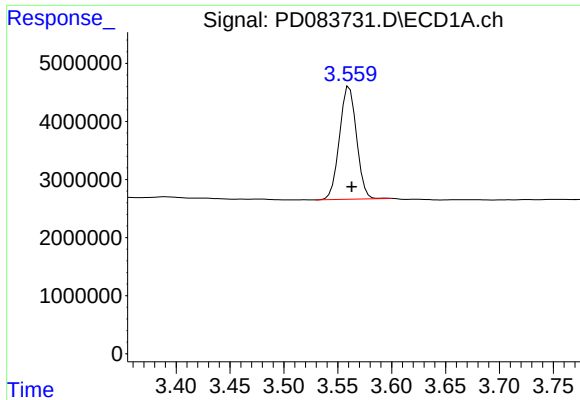


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: -0.002 min
Response: 21372169
Conc: 16.37 ng/ml

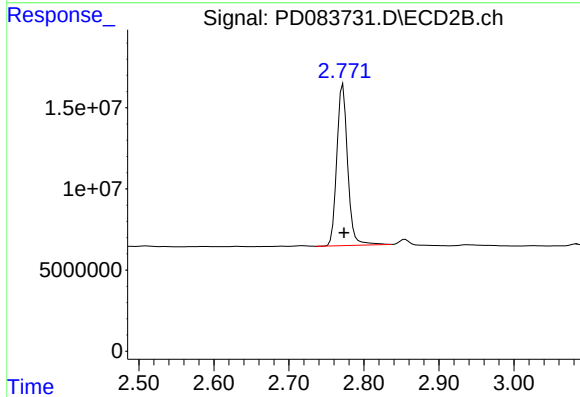


#1 Tetrachloro-m-xylene

R.T.: 2.772 min
Delta R.T.: -0.002 min
Response: 99894061
Conc: 18.33 ng/ml

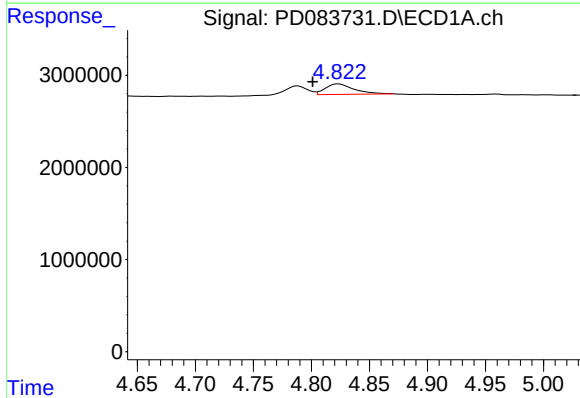


#7 delta-BHC

R.T.: 4.823 min
Delta R.T.: 0.022 min
Response: 1967751
Conc: 0.75 ng/ml

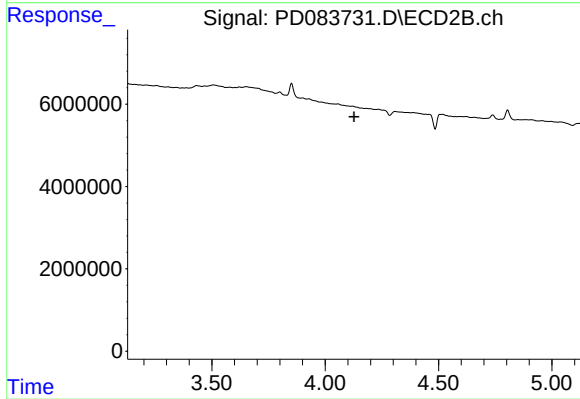


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.128 min
Response: 0
Conc: N.D.

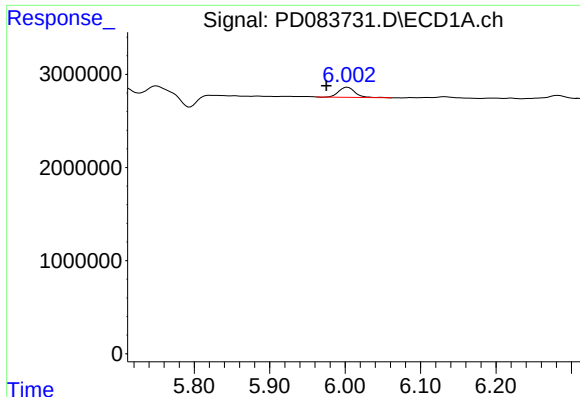


#10 trans-Chlordane

R.T.: 6.003 min
Delta R.T.: 0.028 min
Response: 1630602
Conc: 0.80 ng/ml

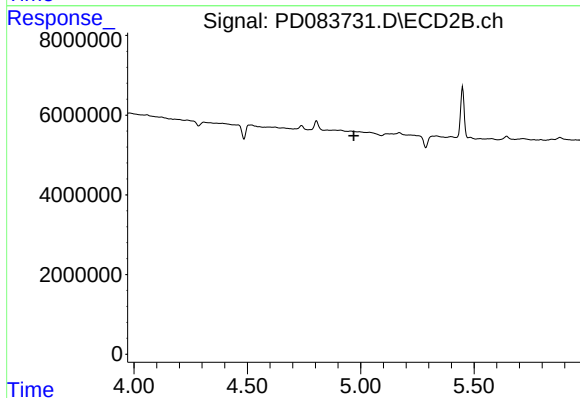


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 4.970 min
Response: 0
Conc: N.D.

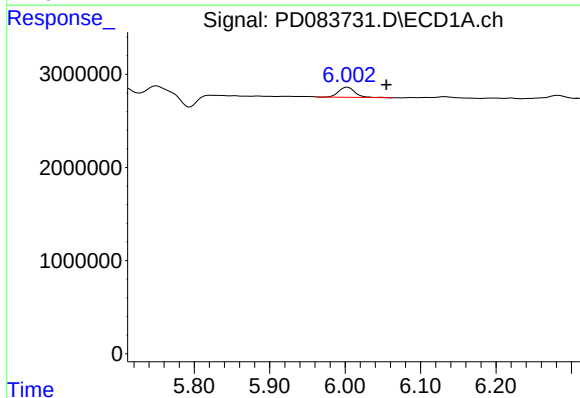


#11 cis-Chlordane

R.T.: 6.003 min
Delta R.T.: -0.052 min
Response: 1630602
Conc: 0.78 ng/ml

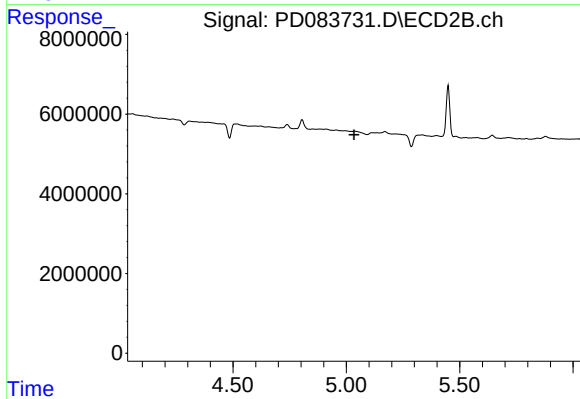


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.034 min
Response: 0
Conc: N.D.

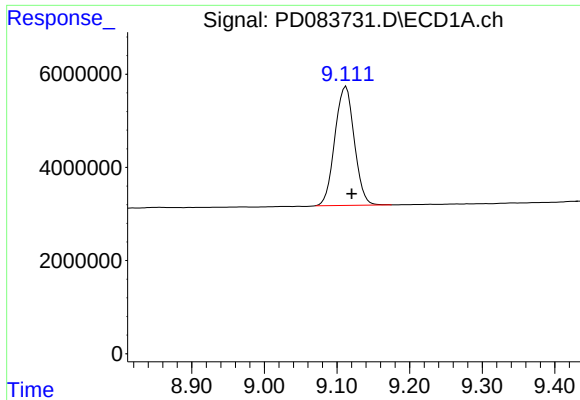

#27 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: -0.008 min
Response: 47580209
Conc: 24.47 ng/ml

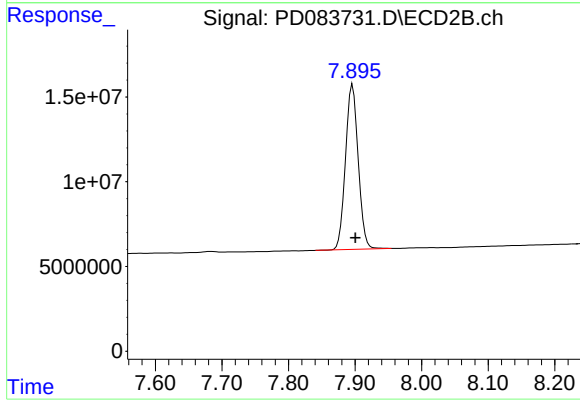

#27 Decachlorobiphenyl

R.T.: 7.896 min
Delta R.T.: -0.004 min
Response: 128969765
Conc: 21.24 ng/ml