

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061825\
 Data File : PD088999.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jun 2025 17:14
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 18 04:58:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061825.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 18 04:57:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.880	189.1E6	1461.7E6	74.427	72.845
28)	SA Decachlor...	9.072	8.072	254.7E6	1356.9E6	72.647	72.156
Target Compounds							
23)	Chlordane-1	4.715	3.905	155.4E6	649.4E6	752.189	723.585
24)	Chlordane-2	5.241	4.488	151.8E6	644.2E6	731.923	712.747
25)	Chlordane-3	5.946	5.126	652.5E6	2038.6E6	766.181	721.284
26)	Chlordane-4	6.032	5.191	778.3E6	1714.5E6	761.234	719.370
27)	Chlordane-5	6.870	6.090	133.3E6	787.6E6	752.966	720.870



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061825\
Data File : PD088999.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jun 2025 17:14
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 18 04:58:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061825.M
Quant Title : GC Extractables
QLast Update : Wed Jun 18 04:57:57 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

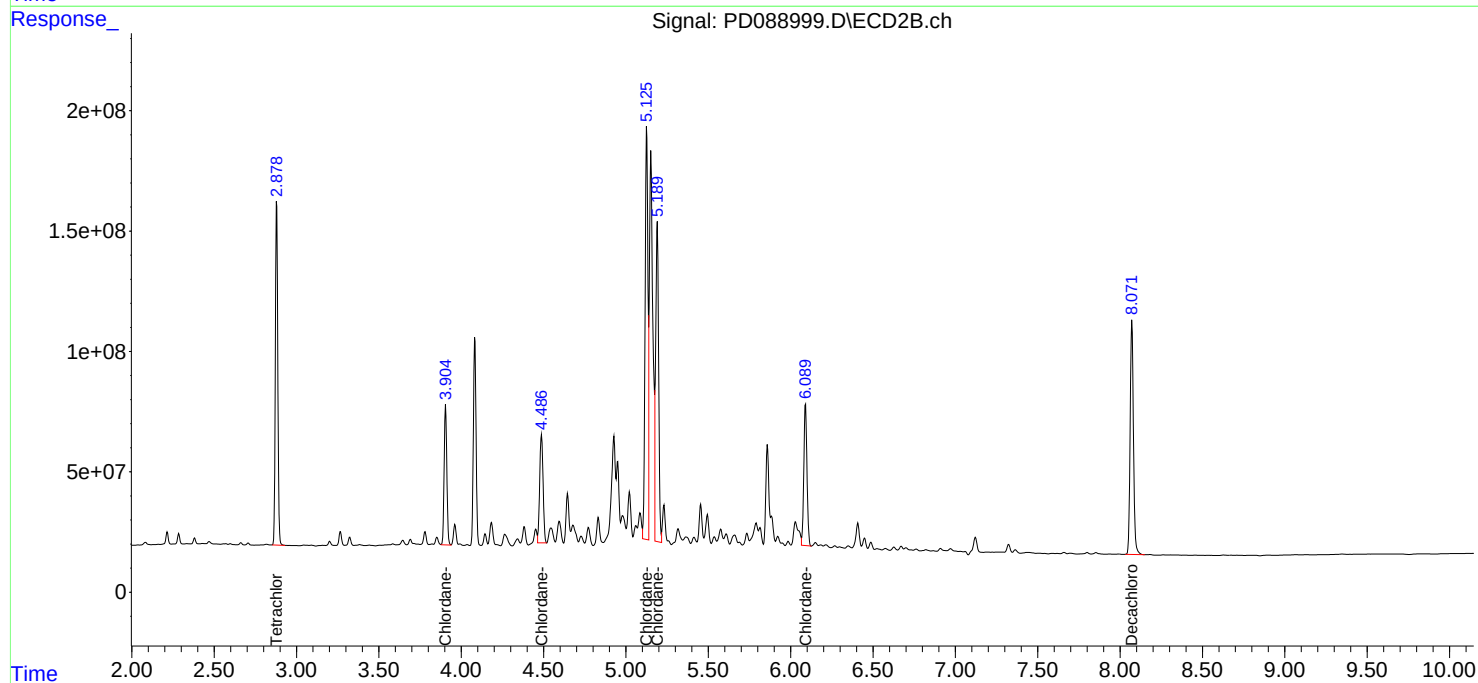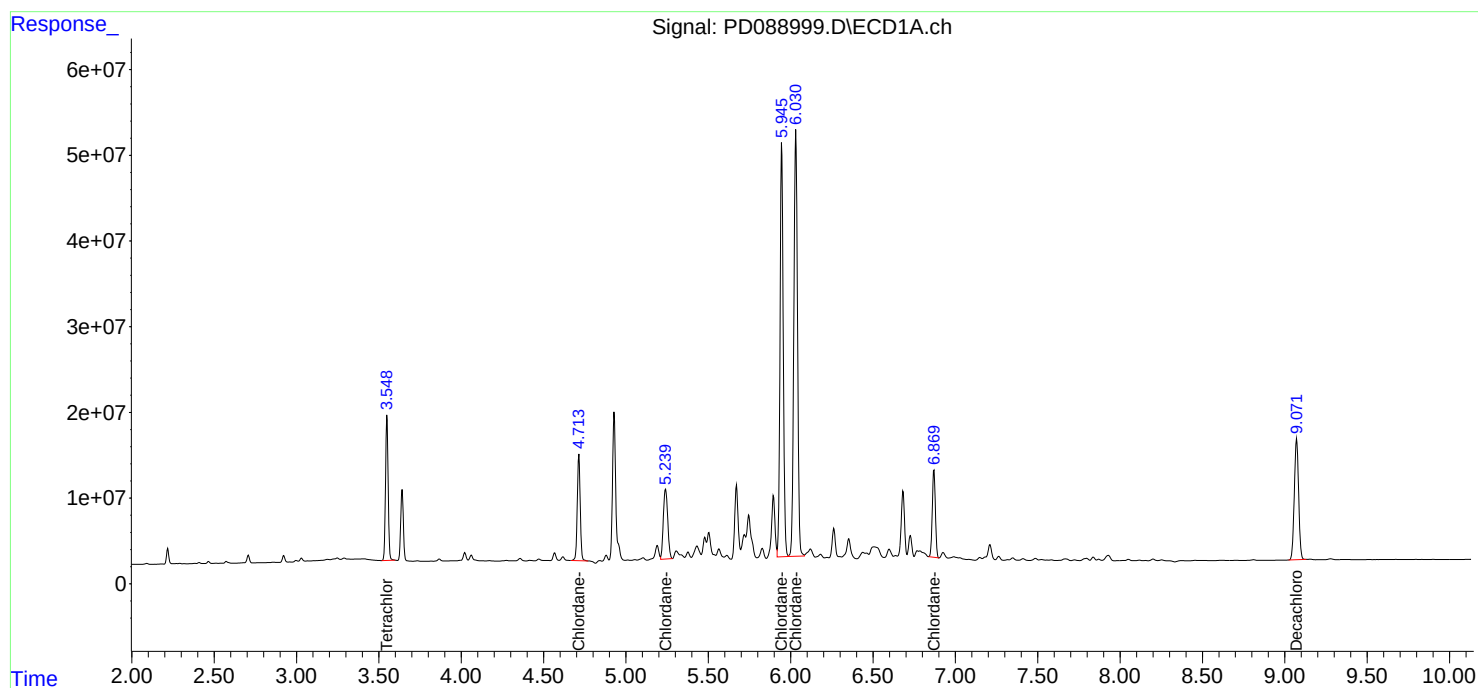


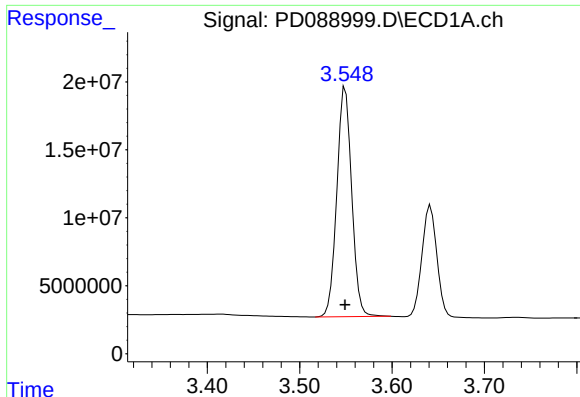

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: 0.000 min
Response: 189079191
Conc: 74.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

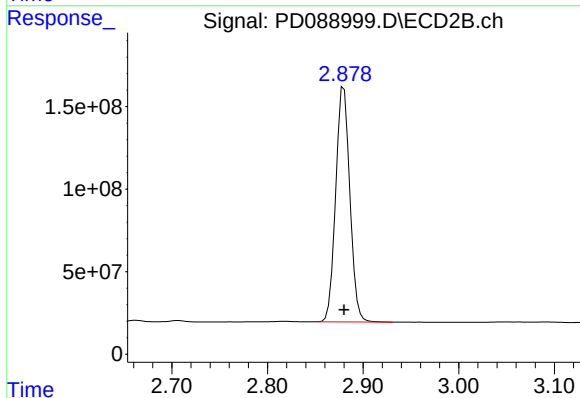


#1 Tetrachloro-m-xylene

R.T.: 2.880 min
Delta R.T.: 0.000 min
Response: 1461666514
Conc: 72.85 ng/ml

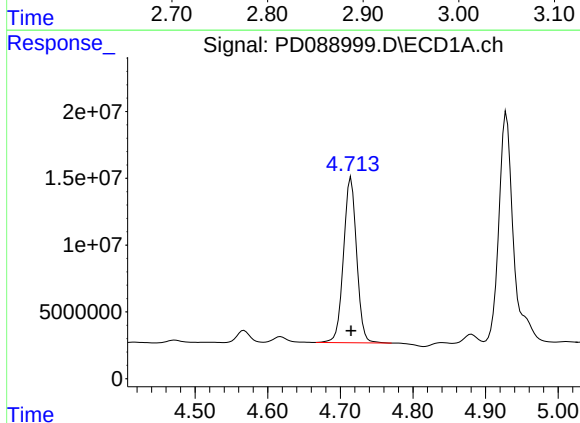


#23 Chlordane-1

R.T.: 4.715 min
Delta R.T.: 0.000 min
Response: 155422256
Conc: 752.19 ng/ml

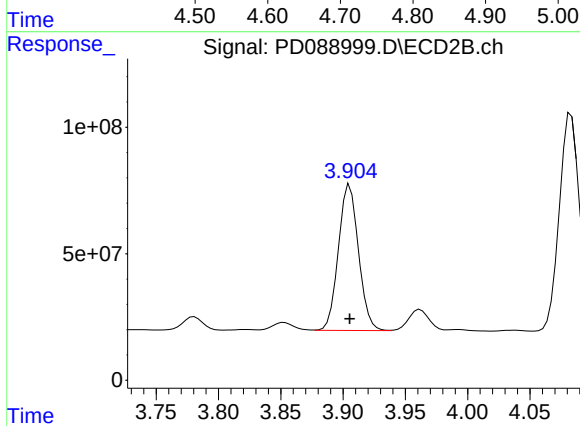

#23 Chlordane-1


R.T.: 3.905 min
Delta R.T.: 0.000 min
Response: 649350031
Conc: 723.58 ng/ml

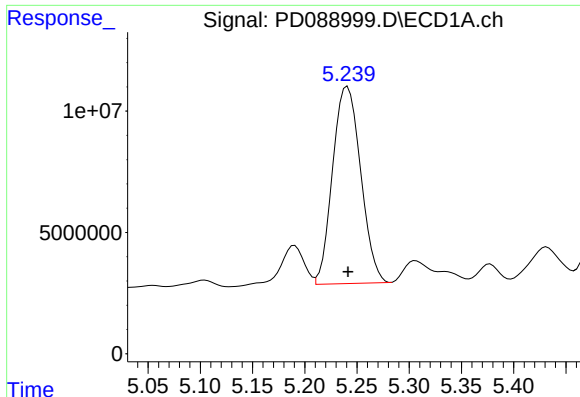

#24 Chlordane-2


R.T.: 5.241 min
Delta R.T.: 0.000 min
Response: 151816807
Conc: 731.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

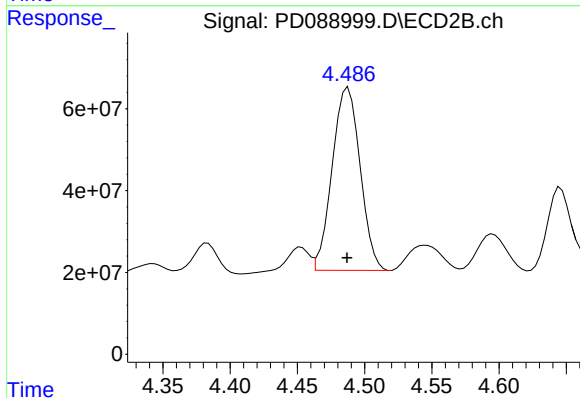


#24 Chlordane-2

R.T.: 4.488 min
Delta R.T.: 0.000 min
Response: 644244326
Conc: 712.75 ng/ml

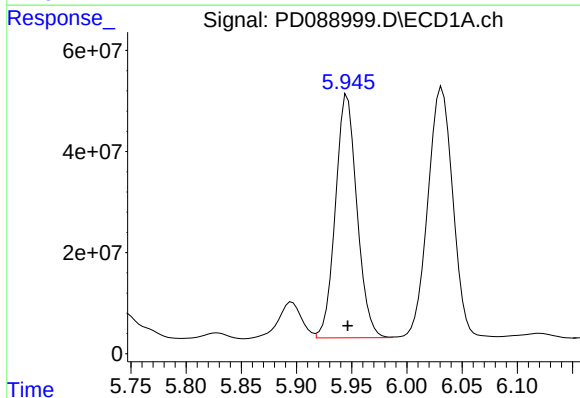


#25 Chlordane-3

R.T.: 5.946 min
Delta R.T.: 0.000 min
Response: 652535754
Conc: 766.18 ng/ml

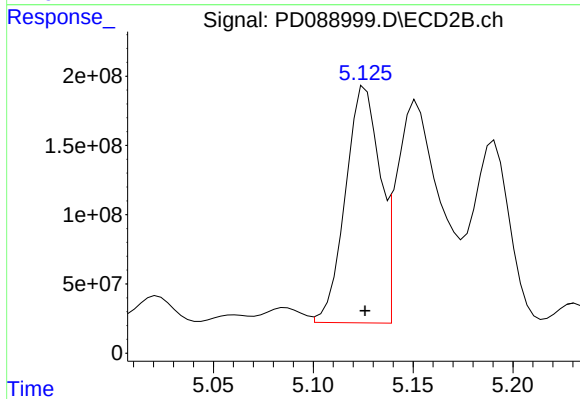

#25 Chlordane-3


R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 2038629200
Conc: 721.28 ng/ml

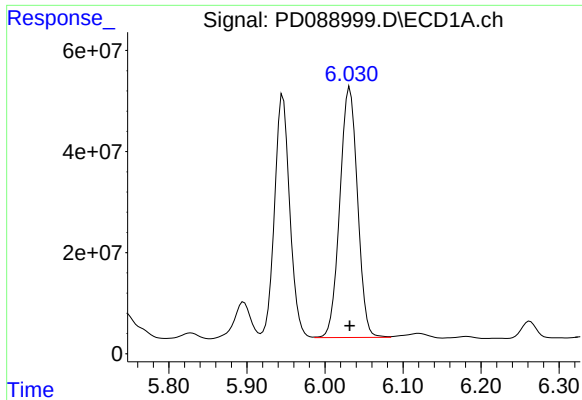

#26 Chlordane-4


R.T.: 6.032 min
Delta R.T.: 0.000 min
Response: 778297765
Conc: 761.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

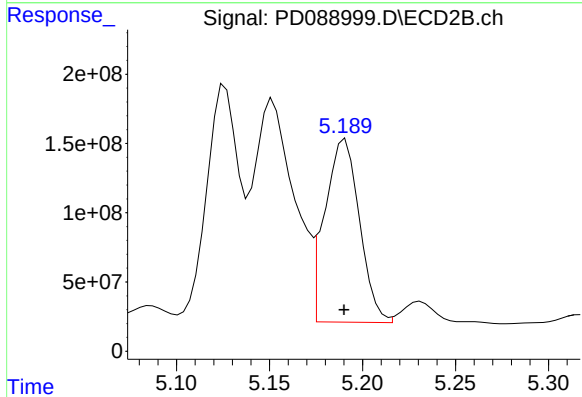


#26 Chlordane-4

R.T.: 5.191 min
Delta R.T.: 0.000 min
Response: 1714456950
Conc: 719.37 ng/ml

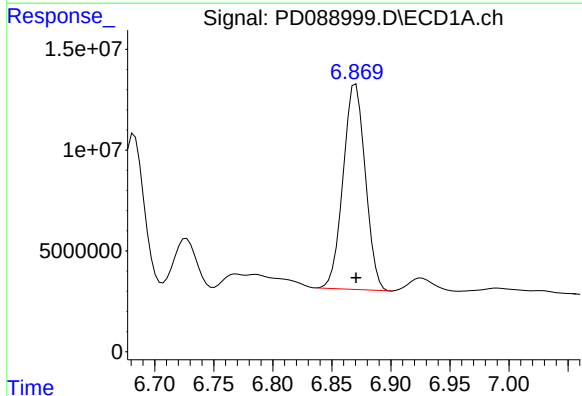


#27 Chlordane-5

R.T.: 6.870 min
Delta R.T.: 0.000 min
Response: 133348919
Conc: 752.97 ng/ml

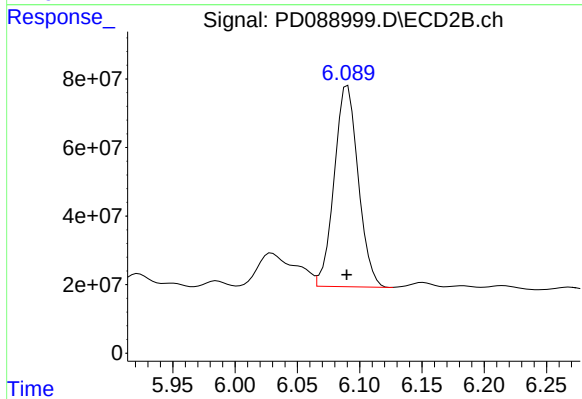

#27 Chlordane-5


R.T.: 6.090 min
Delta R.T.: 0.000 min
Response: 787567049
Conc: 720.87 ng/ml

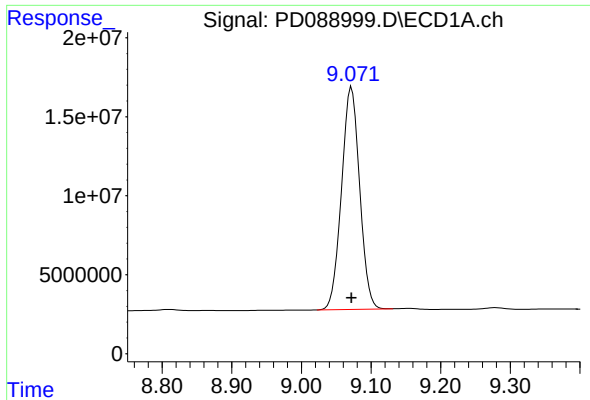

#28 Decachlorobiphenyl

R.T.: 9.072 min
Delta R.T.: 0.000 min
Response: 254695532
Conc: 72.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

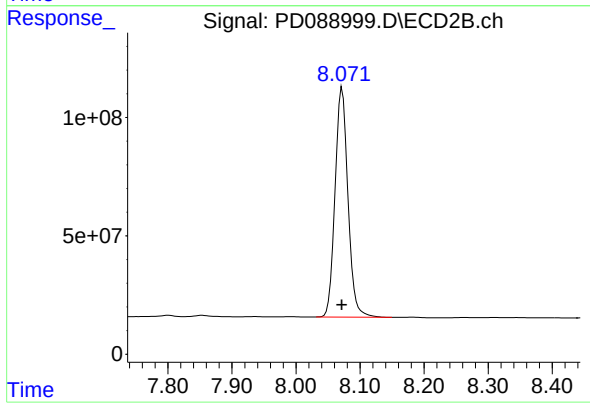

#28 Decachlorobiphenyl

R.T.: 8.072 min
Delta R.T.: 0.000 min
Response: 1356905092
Conc: 72.16 ng/ml