

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061923\
 Data File : PD075883.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2023 08:38
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 13:21:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds									
4)	MA	Heptachlor	4.946f	0.000	655505	0	0.183	N.D.	#
6)	B	beta-BHC	4.563f	0.000	115596	0	0.080	N.D.	#
8)	B	Heptachlo...	5.694	0.000	959884	0	0.298	N.D.	#
9)	A	Endosulfan I	6.093	0.000	140265	0	0.047	N.D.	#
10)	B	gamma-Chl...	5.967	0.000	186272	0	0.058	N.D.	#
11)	B	alpha-Chl...	6.055f	0.000	400390	0	0.124	N.D.	#
21)	B	Endrin ke...	7.693f	0.000	291408	0	0.105	N.D.	#
22)		Mirex	8.156f	0.000	59657	0	0.028	N.D.	#
25)		Chlordane-3	5.967	0.000	186272	0	0.359	N.D.	#
26)		Chlordane-4	6.055f	0.000	400390	0	0.635	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061923\
Data File : PD075883.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2023 08:38
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 13:21:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

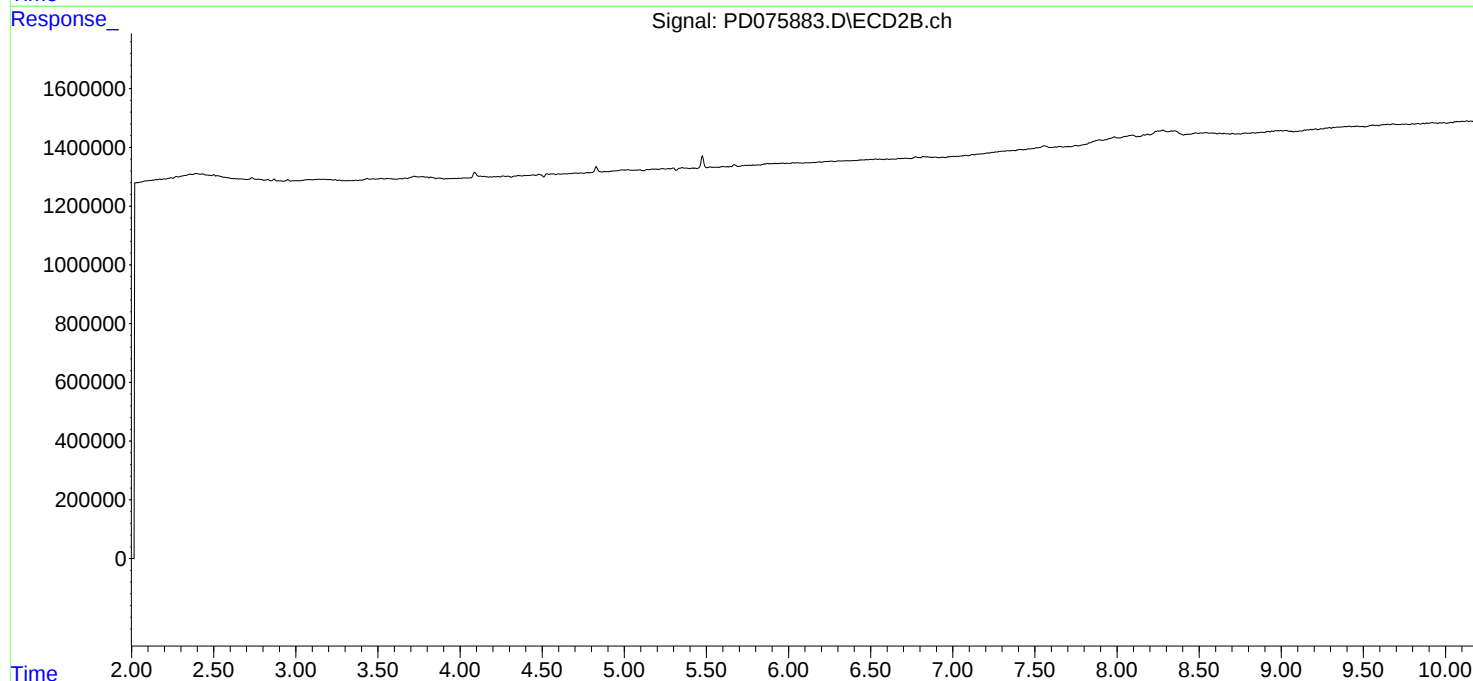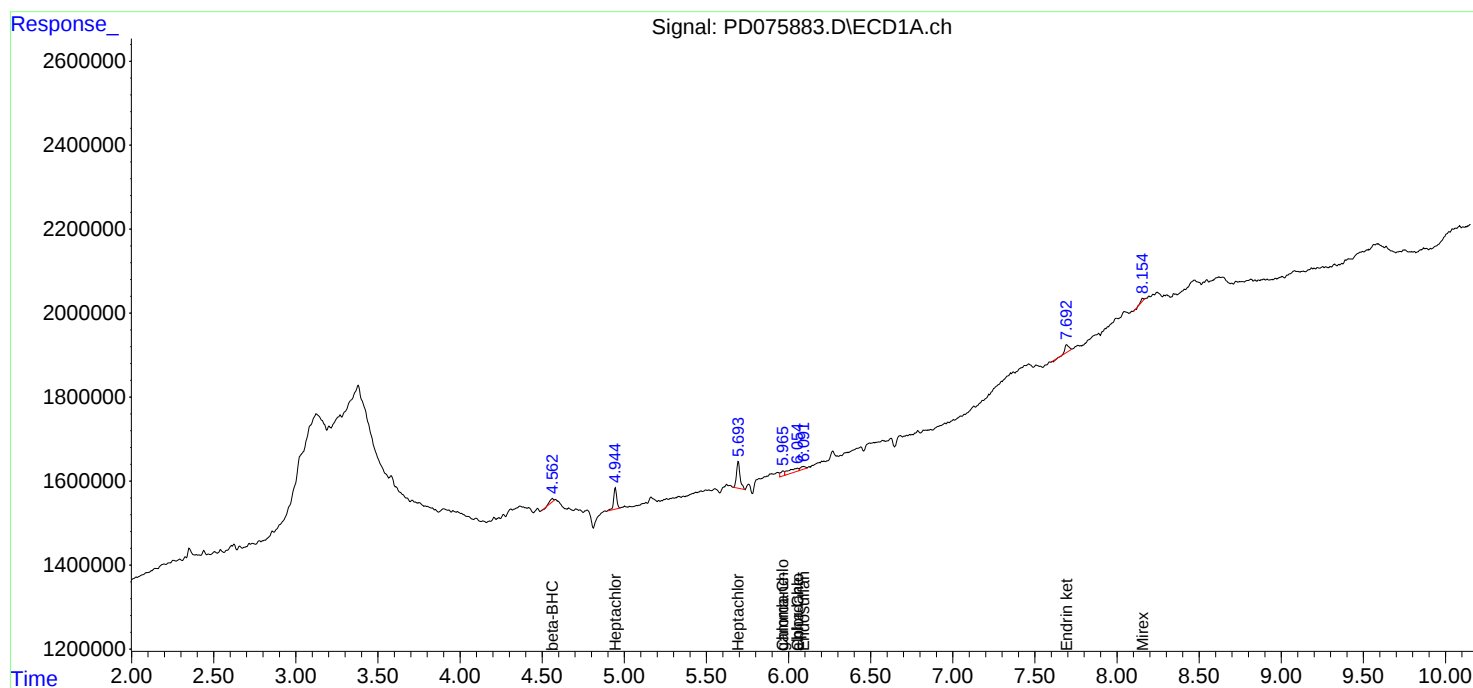


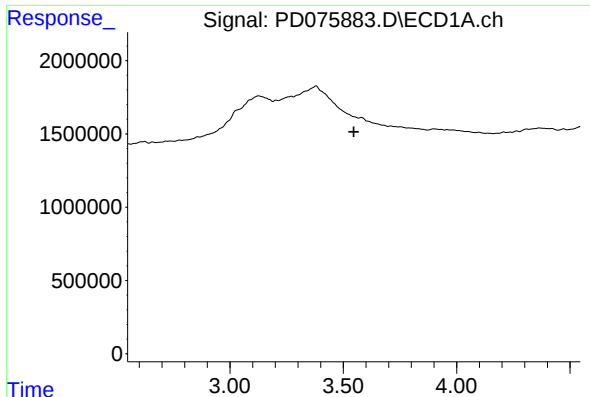

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.546 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
HEXANE

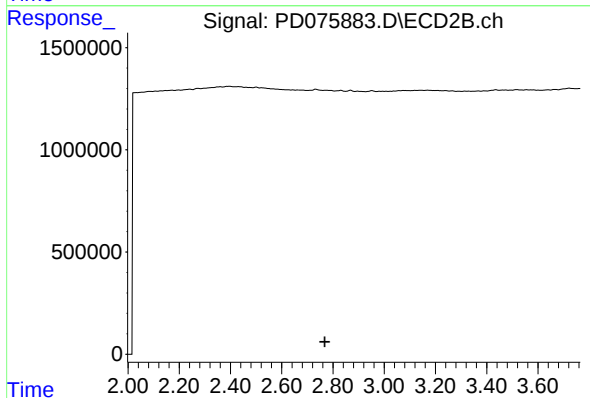


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.767 min
Response: 0
Conc: N.D.

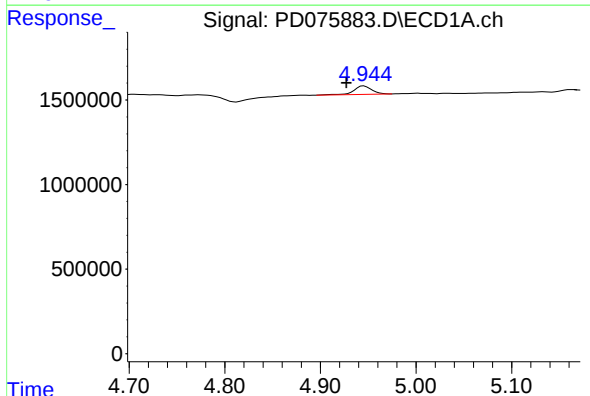


#4 Heptachlor

R.T.: 4.946 min
Delta R.T.: 0.019 min
Response: 655505
Conc: 0.18 ng/ml

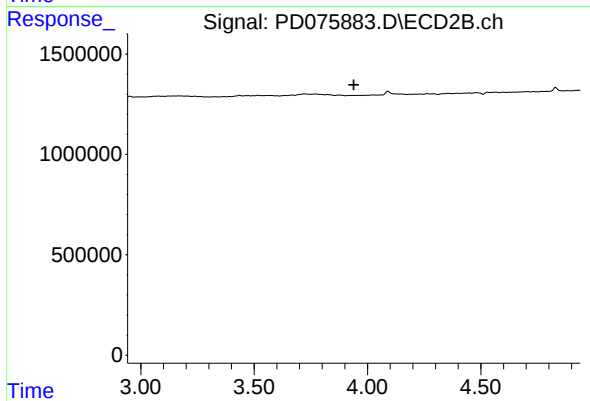

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 3.940 min
Response: 0
Conc: N.D.

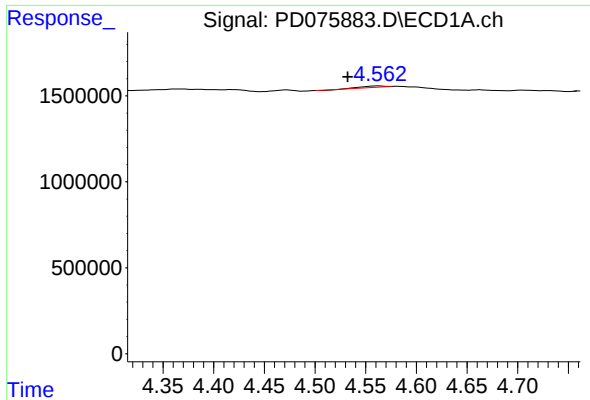

#6 beta-BHC


R.T.: 4.563 min
Delta R.T.: 0.031 min
Response: 115596
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

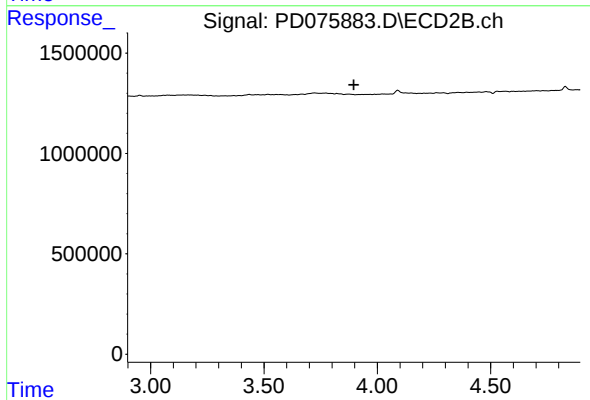


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 3.896 min
Response: 0
Conc: N.D.

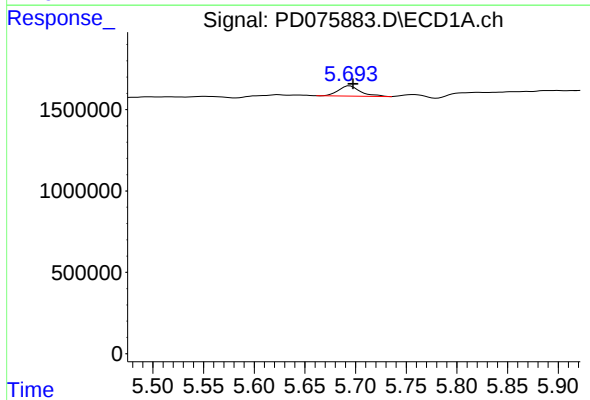


#8 Heptachlor epoxide

R.T.: 5.694 min
Delta R.T.: -0.003 min
Response: 959884
Conc: 0.30 ng/ml

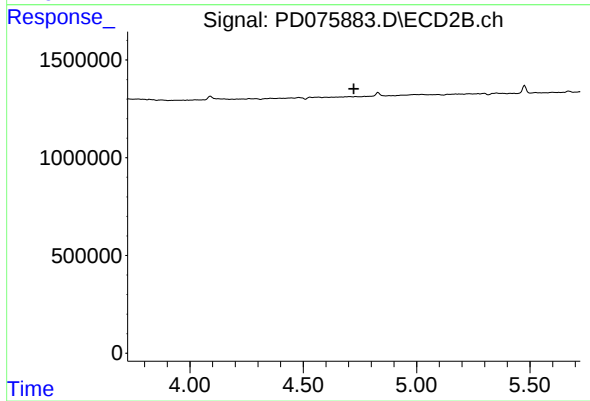

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

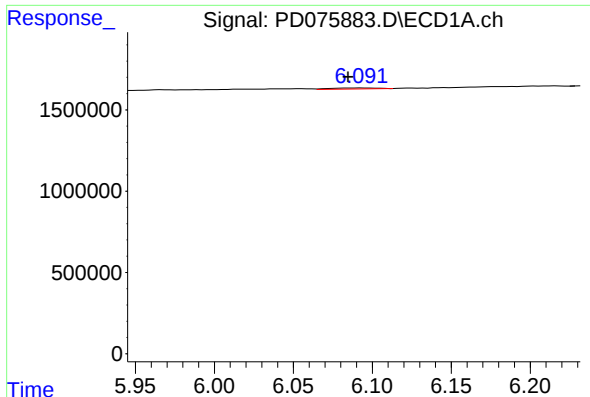

#9 Endosulfan I


R.T.: 6.093 min
Delta R.T.: 0.008 min
Response: 140265
Conc: 0.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

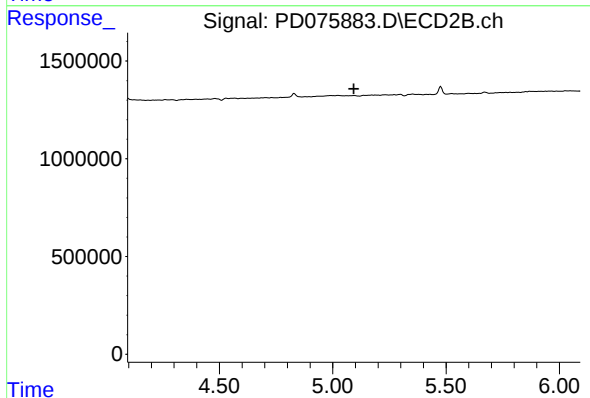


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

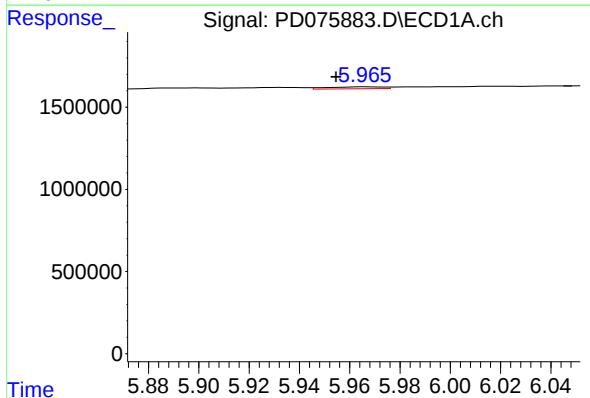


#10 gamma-Chlordane

R.T.: 5.967 min
Delta R.T.: 0.012 min
Response: 186272
Conc: 0.06 ng/ml

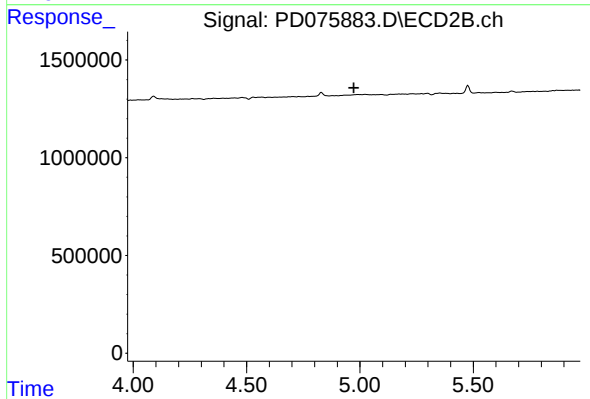

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

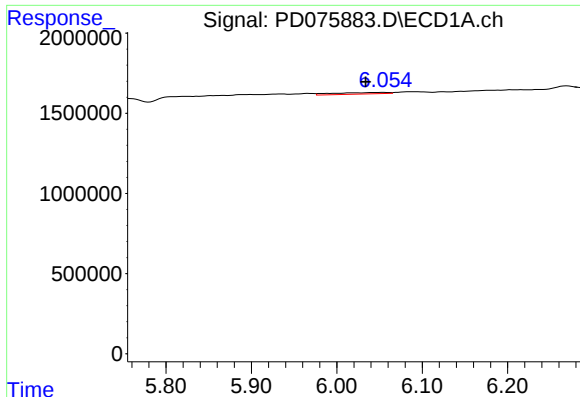

#11 alpha-Chlordane


R.T.: 6.055 min
Delta R.T.: 0.021 min
Response: 400390
Conc: 0.12 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

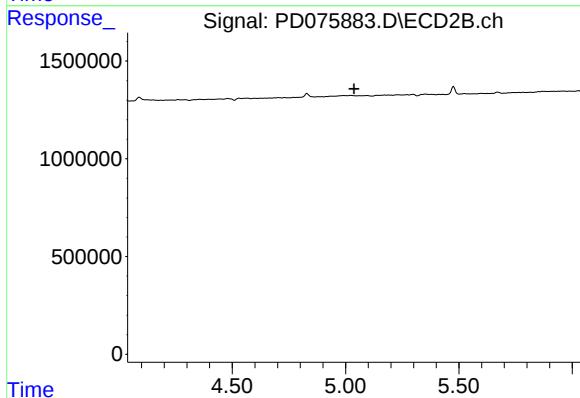


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

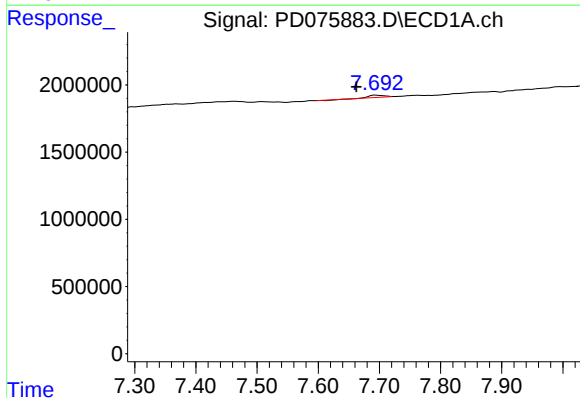


#21 Endrin ketone

R.T.: 7.693 min
Delta R.T.: 0.031 min
Response: 291408
Conc: 0.10 ng/ml

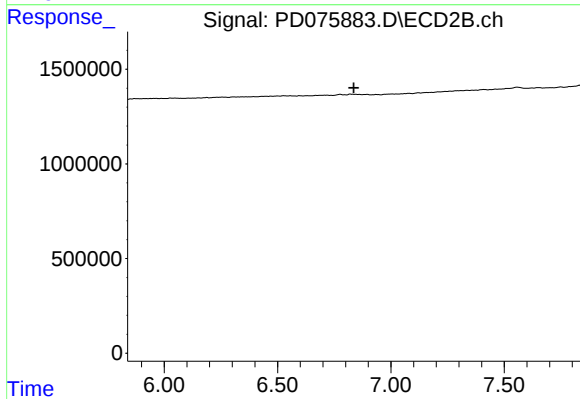

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

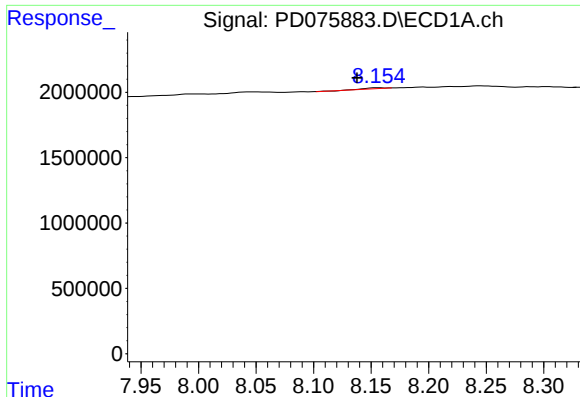

#22 Mirex


R.T.: 8.156 min
Delta R.T.: 0.018 min
Response: 59657
Conc: 0.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

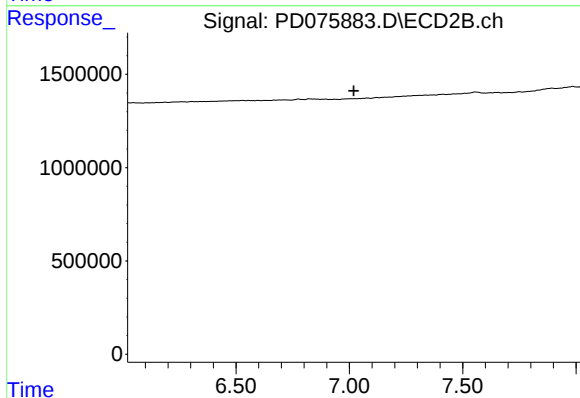


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.019 min
Response: 0
Conc: N.D.

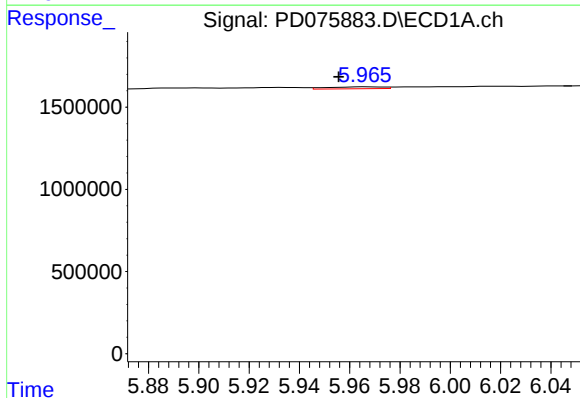


#25 Chlordane-3

R.T.: 5.967 min
Delta R.T.: 0.011 min
Response: 186272
Conc: 0.36 ng/ml

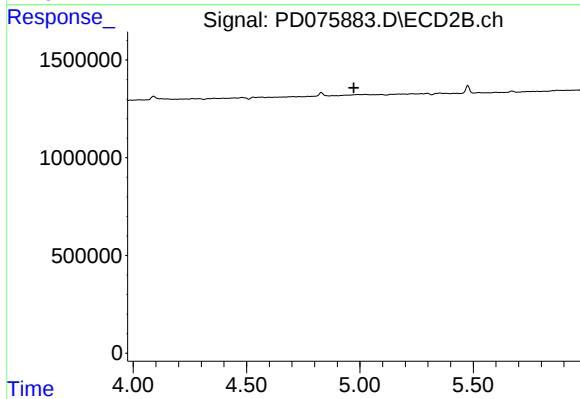

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

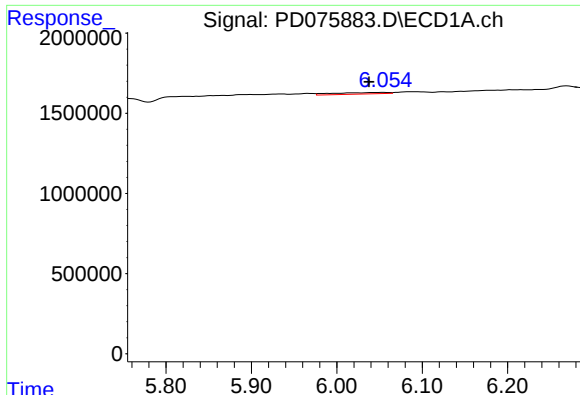

#26 Chlordane-4


R.T.: 6.055 min
Delta R.T.: 0.017 min
Response: 400390
Conc: 0.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
HEXANE

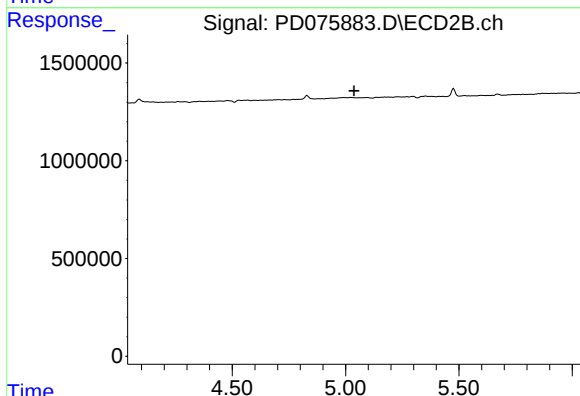


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

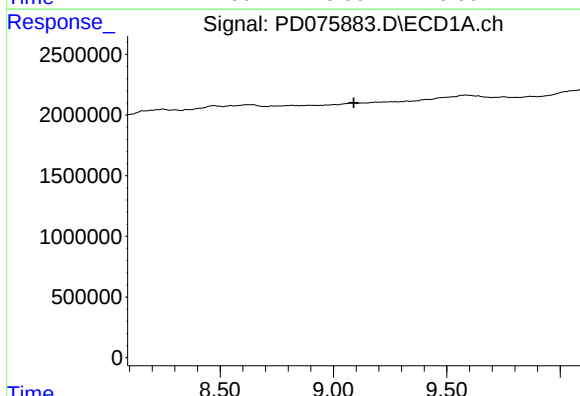

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.089 min
Response: 0
Conc: N.D.

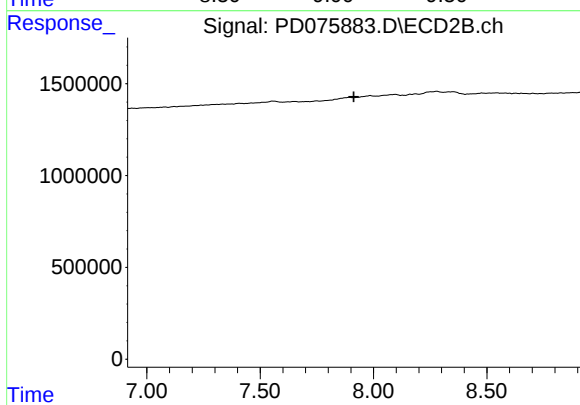

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.913 min
Response: 0
Conc: N.D.