

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061923\
 Data File : PD075888.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2023 10:27
 Operator : AR\AJ
 Sample : PB153534BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 13:23:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.553	2.768	49968385	25327349	23.458	23.345
28)	SA Decachlor...	9.097	7.915	57367830	24351699	22.645	24.905
Target Compounds							
2)	A alpha-BHC	4.027f	0.000	244091	0	0.066	N.D. #
4)	MA Heptachlor	4.951f	0.000	187065	0	0.052	N.D. #
7)	B delta-BHC	4.779	0.000	1800041	0	0.542	N.D. #
9)	A Endosulfan I	6.095	0.000	26953	0	0.009	N.D. #
10)	B gamma-Chl...	5.944	0.000	2343853	0	0.728	N.D. #
15)	B Endosulfa...	6.795f	0.000	114695	0	0.044	N.D. #
21)	B Endrin ke...	7.691f	0.000	703495	0	0.253	N.D. #
25)	Chlordane-3	5.944	0.000	2343853	0	4.513	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061923\
Data File : PD075888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2023 10:27
Operator : AR\AJ
Sample : PB153534BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 13:23:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

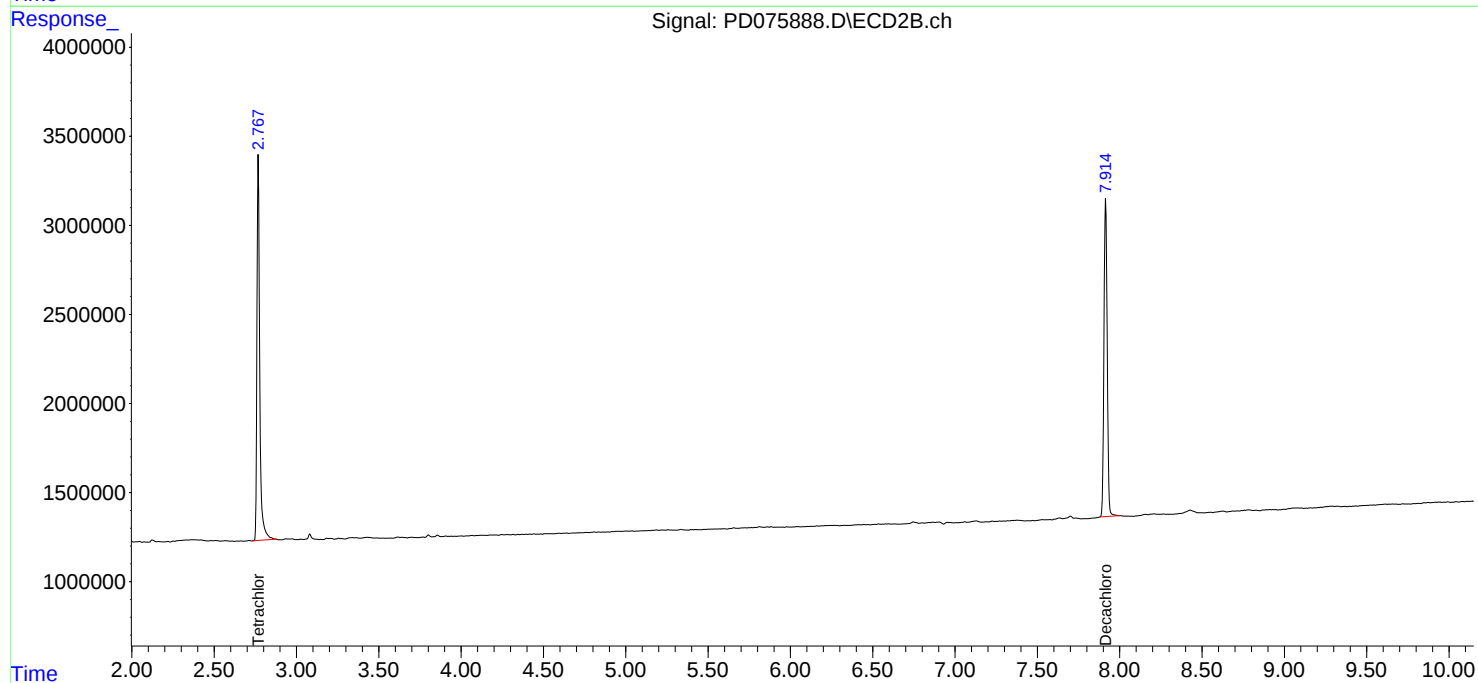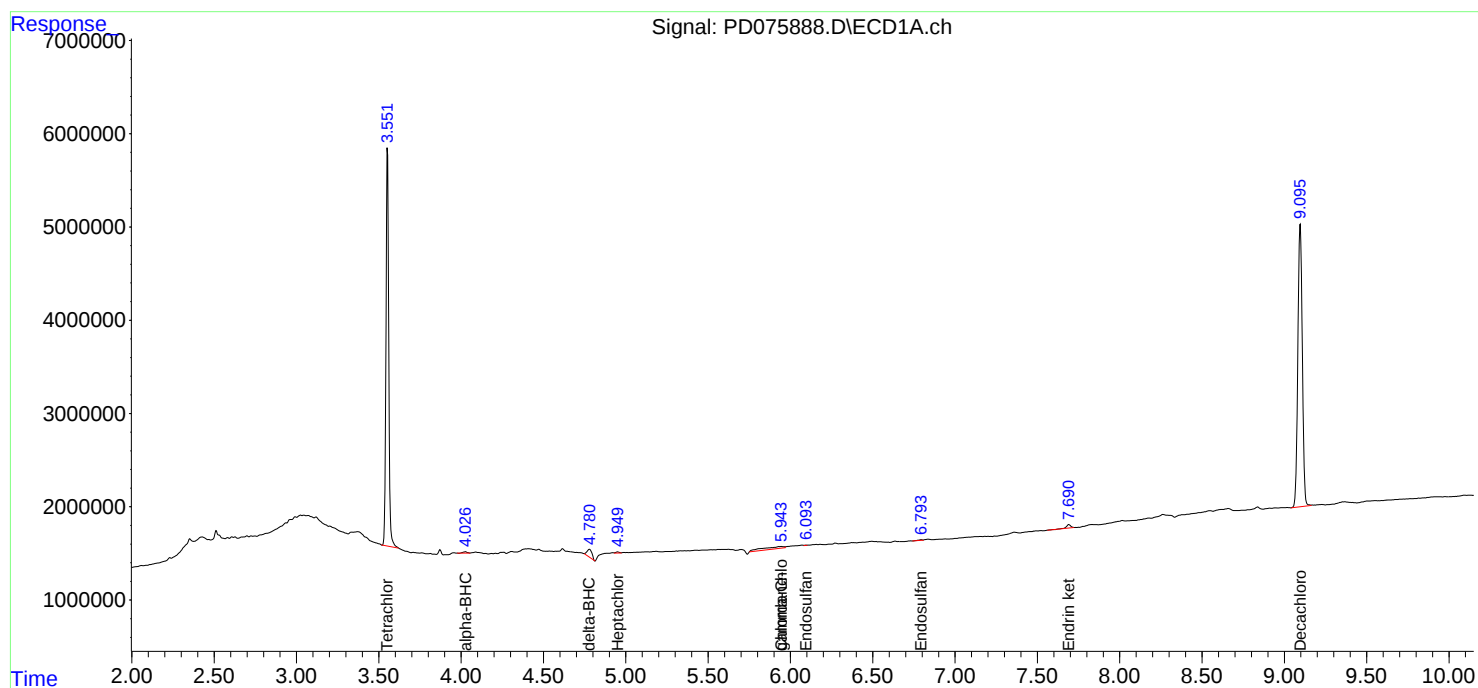


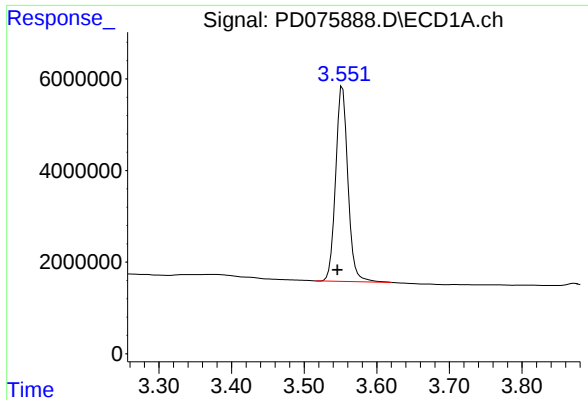

#1 Tetrachloro-m-xylene


R.T.: 3.553 min
Delta R.T.: 0.007 min
Response: 49968385
Conc: 23.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

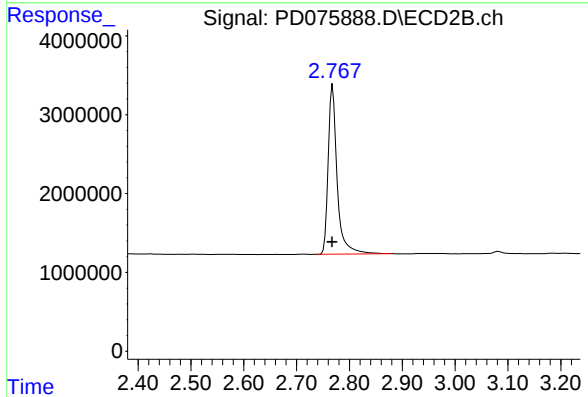


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: 0.001 min
Response: 25327349
Conc: 23.34 ng/ml

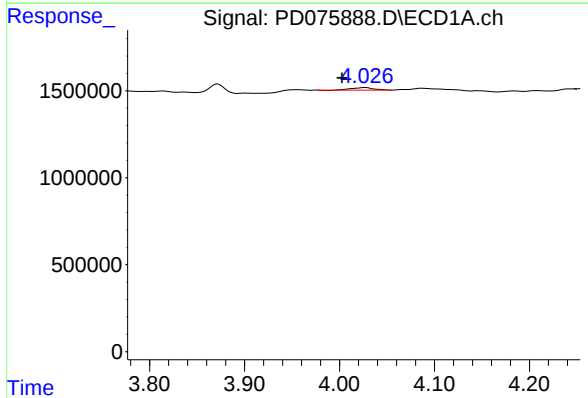


#2 alpha-BHC

R.T.: 4.027 min
Delta R.T.: 0.025 min
Response: 244091
Conc: 0.07 ng/ml

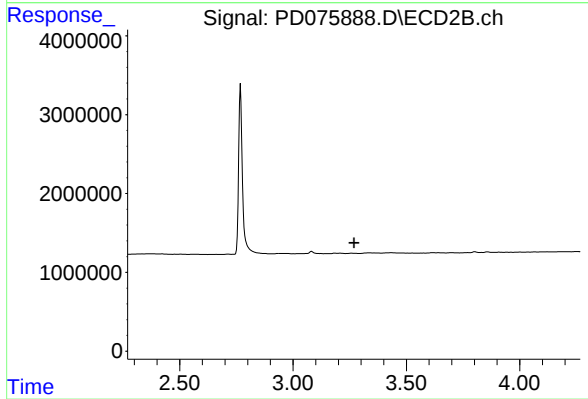

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 3.270 min
Response: 0
Conc: N.D.

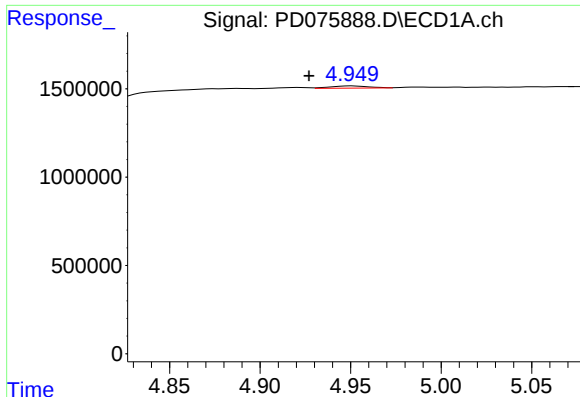

#4 Heptachlor


R.T.: 4.951 min
Delta R.T.: 0.024 min
Response: 187065
Conc: 0.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

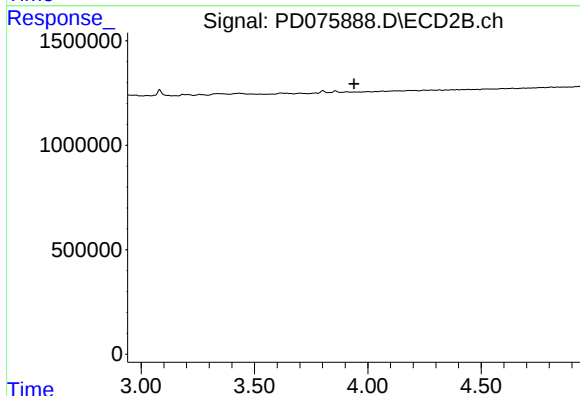


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 3.940 min
Response: 0
Conc: N.D.

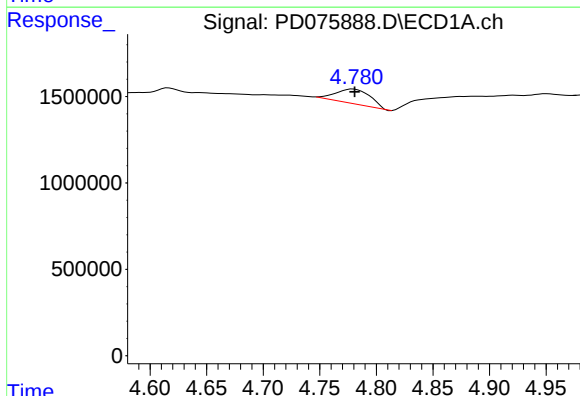


#7 delta-BHC

R.T.: 4.779 min
Delta R.T.: -0.002 min
Response: 1800041
Conc: 0.54 ng/ml

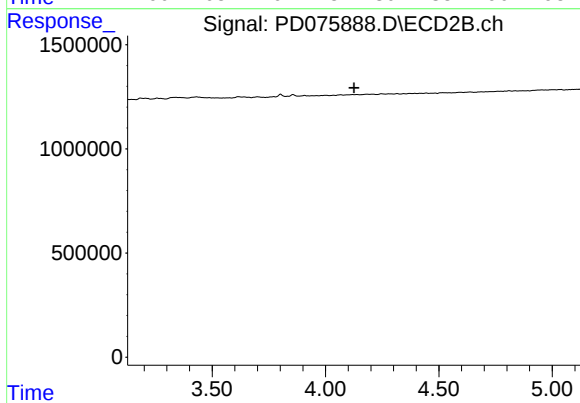

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.127 min
Response: 0
Conc: N.D.

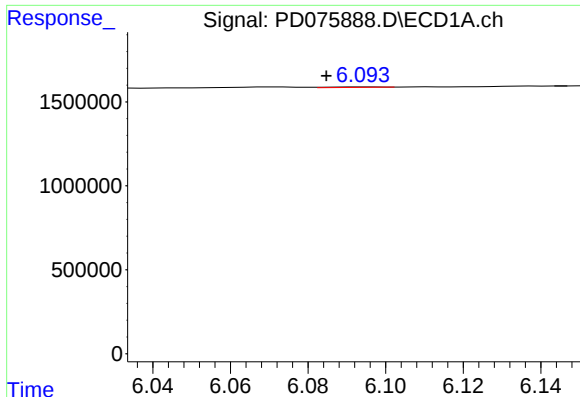

#9 Endosulfan I


R.T.: 6.095 min
Delta R.T.: 0.010 min
Response: 26953
Conc: 0.01 ng/ml

Instrument :
ECD_D
ClientSampleId :

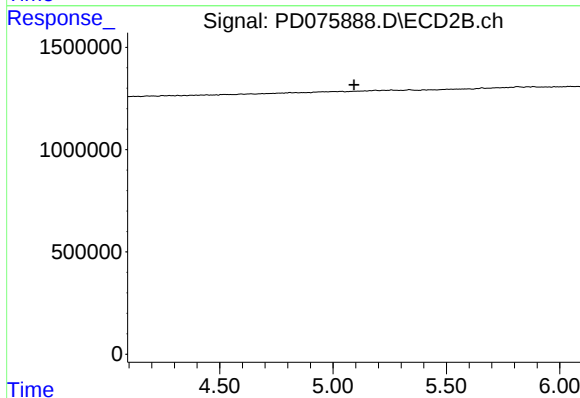


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

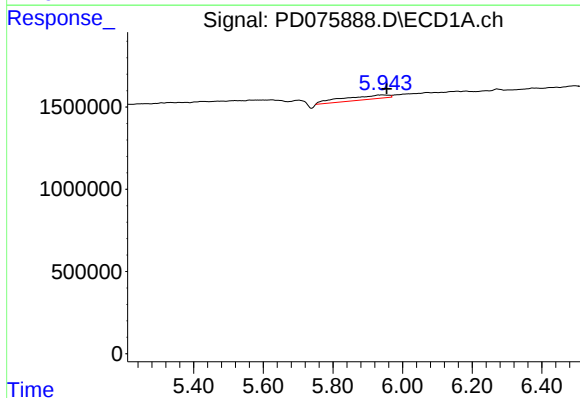


#10 gamma-Chlordane

R.T.: 5.944 min
Delta R.T.: -0.010 min
Response: 2343853
Conc: 0.73 ng/ml

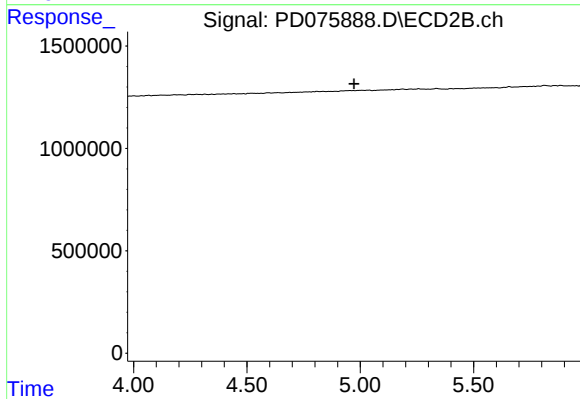

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

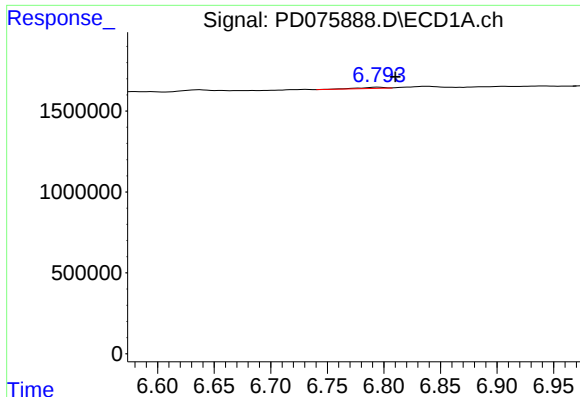

#15 Endosulfan II


R.T.: 6.795 min
Delta R.T.: -0.015 min
Response: 114695
Conc: 0.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

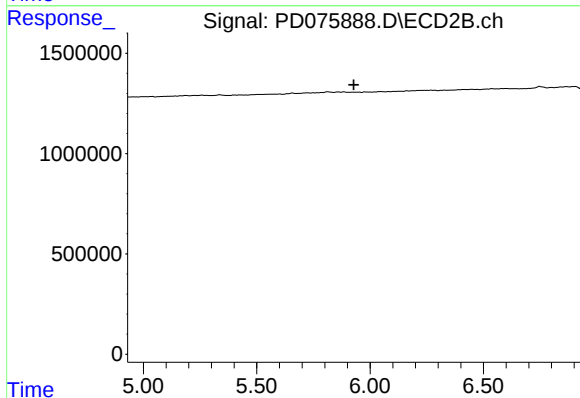


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

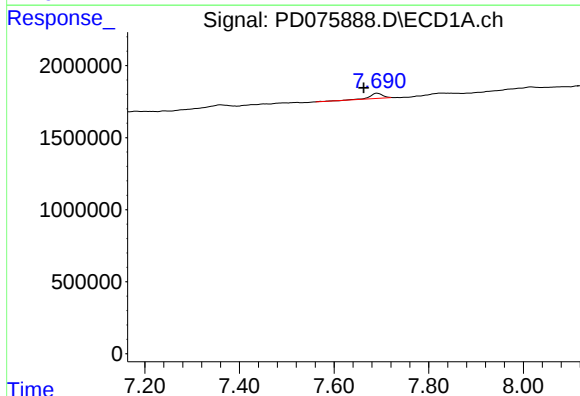


#21 Endrin ketone

R.T.: 7.691 min
Delta R.T.: 0.029 min
Response: 703495
Conc: 0.25 ng/ml

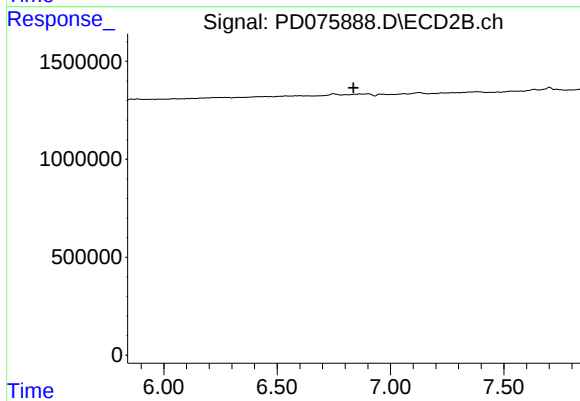

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

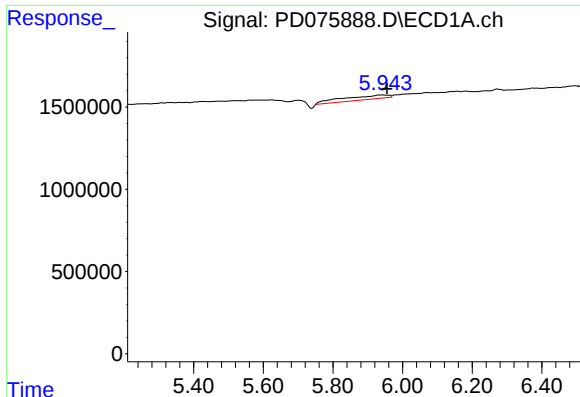

#25 Chlordane-3


R.T.: 5.944 min
Delta R.T.: -0.011 min
Response: 2343853
Conc: 4.51 ng/ml

Instrument :
ECD_D
ClientSampleId :

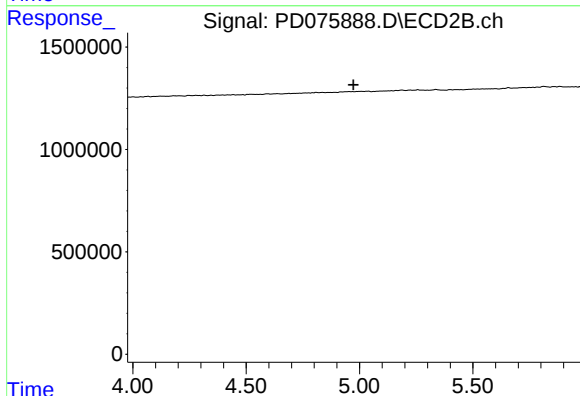


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

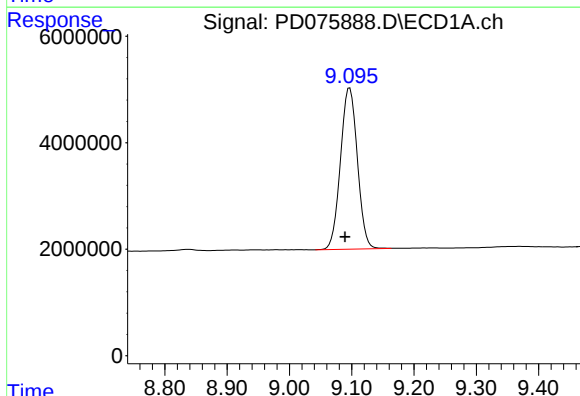

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.008 min
Response: 57367830
Conc: 22.64 ng/ml

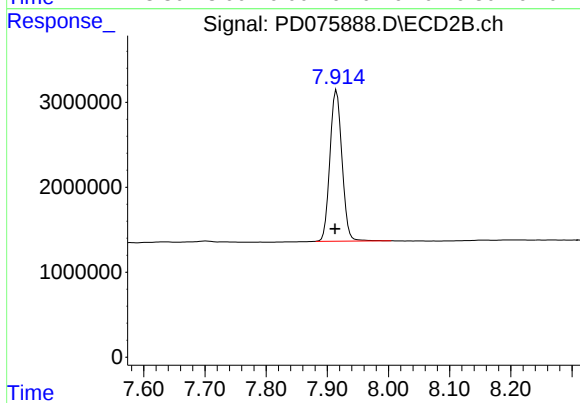

#28 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: 0.002 min
Response: 24351699
Conc: 24.90 ng/ml