

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061923\
 Data File : PD075897.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2023 13:40
 Operator : AR\AJ
 Sample : PB153525BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB153525BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 22:19:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.768	49734503	24382586	23.348	22.474
28)	SA Decachlor...	9.089	7.914	56696565	22472420	22.380	22.983
Target Compounds							
6)	B beta-BHC	4.553f	0.000	413494	0	0.288	N.D. #
7)	B delta-BHC	4.774	0.000	2783872	0	0.838	N.D. #
8)	B Heptachlo...	5.694	0.000	1252400	0	0.389	N.D. #
9)	A Endosulfan I	6.061f	0.000	151611	0	0.051	N.D. #
11)	B alpha-Chl...	6.026	0.000	127831	0	0.040	N.D. #
15)	B Endosulfa...	6.839f	0.000	94536	0	0.037	N.D. #
21)	B Endrin ke...	7.693f	0.000	274095	0	0.098	N.D. #
26)	Chlordane-4	6.026	0.000	127831	0	0.203	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061923\
Data File : PD075897.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2023 13:40
Operator : AR\AJ
Sample : PB153525BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB153525BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 22:19:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

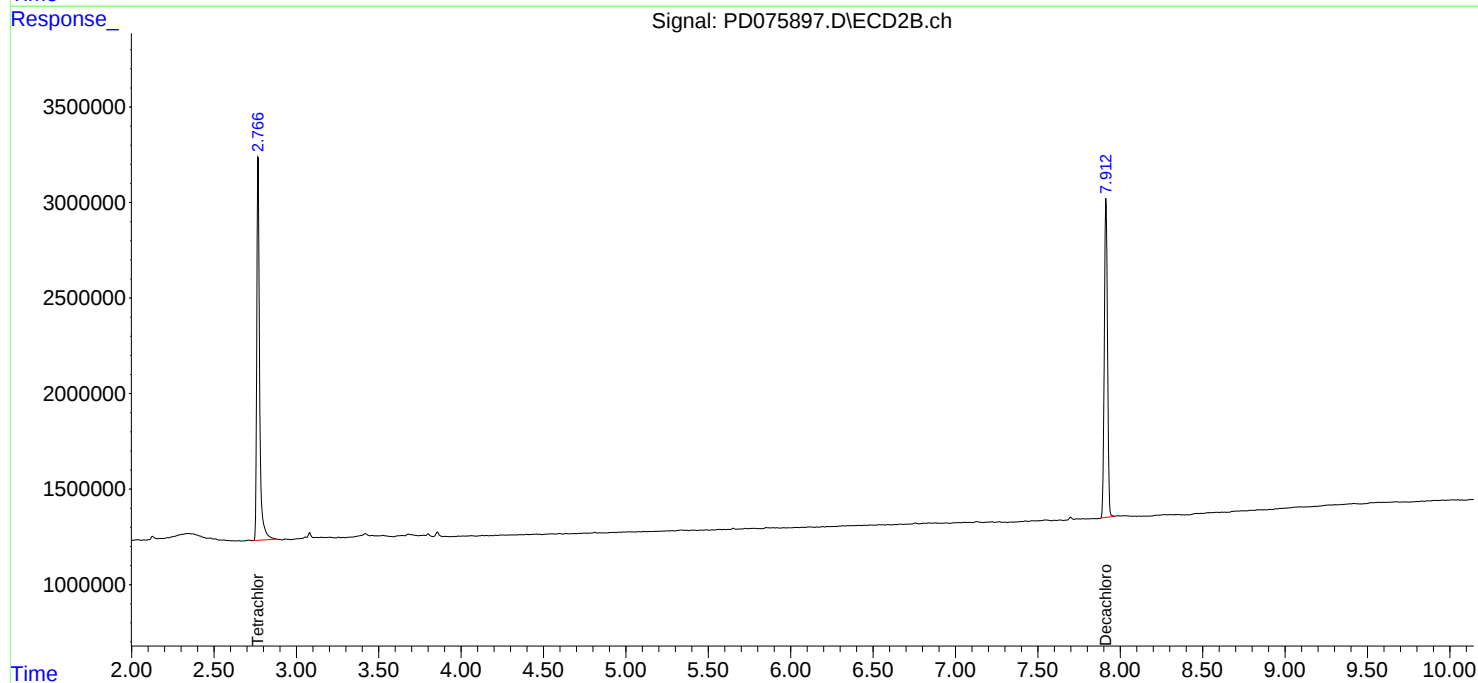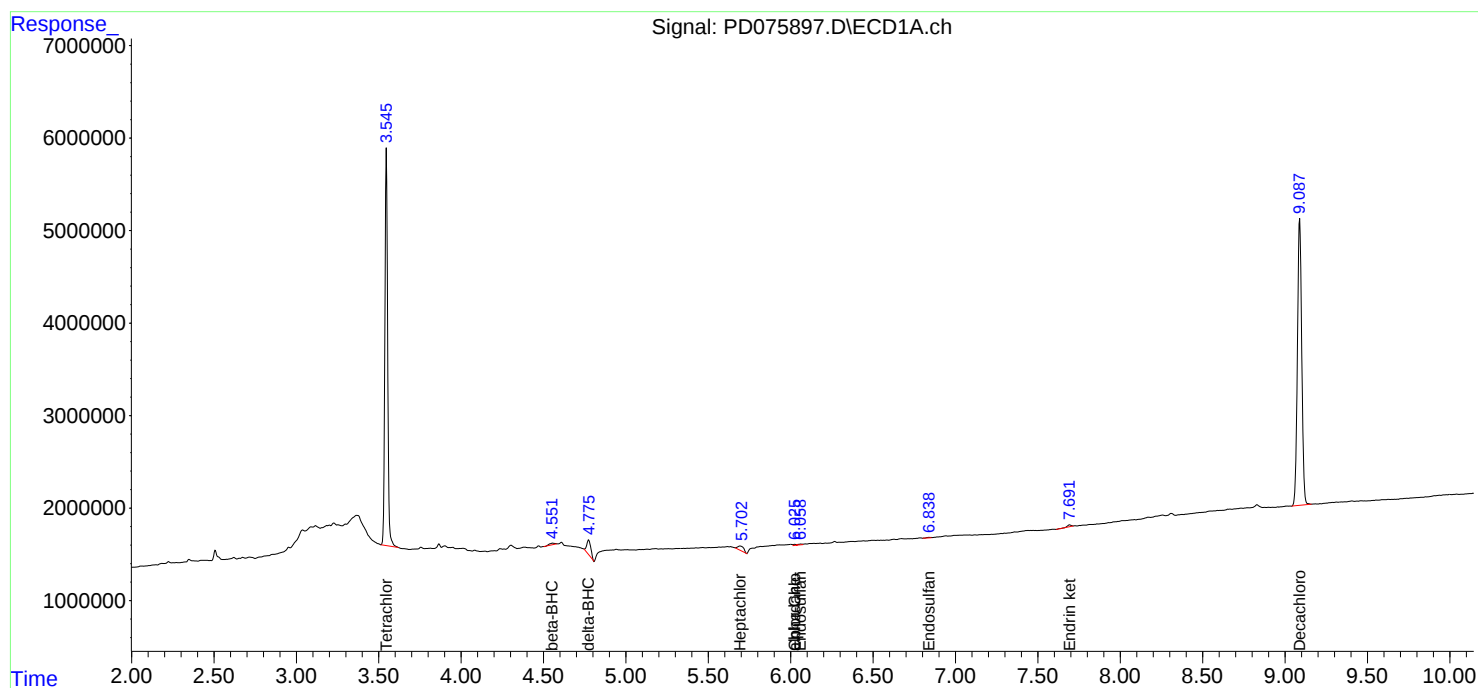


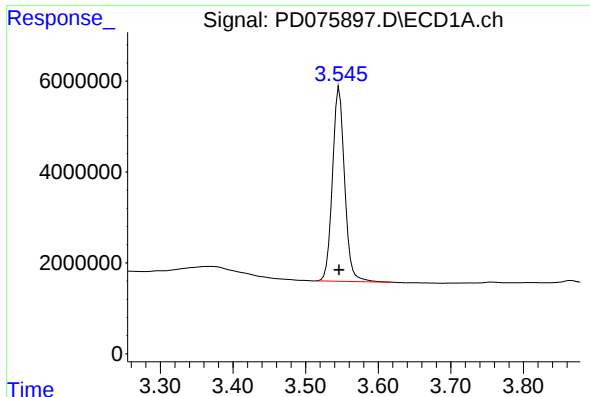

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 49734503
Conc: 23.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153525BL

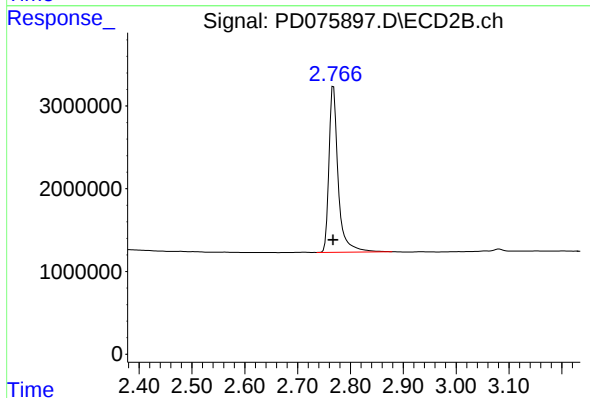


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: 0.000 min
Response: 24382586
Conc: 22.47 ng/ml

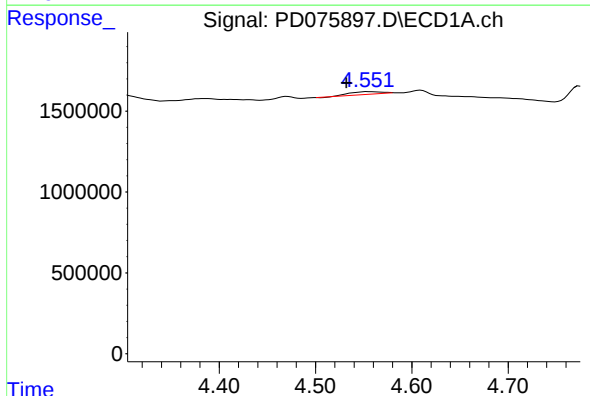


#6 beta-BHC

R.T.: 4.553 min
Delta R.T.: 0.021 min
Response: 413494
Conc: 0.29 ng/ml

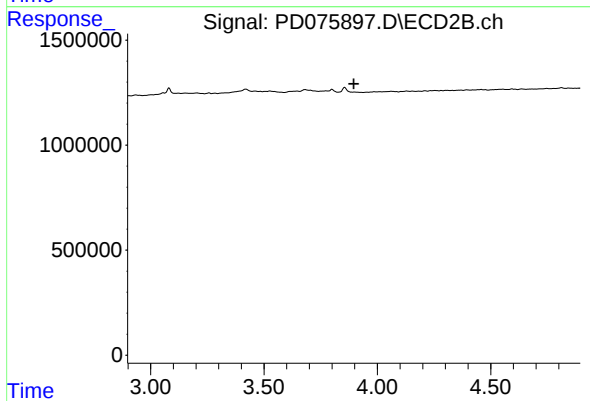

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 3.896 min
Response: 0
Conc: N.D.

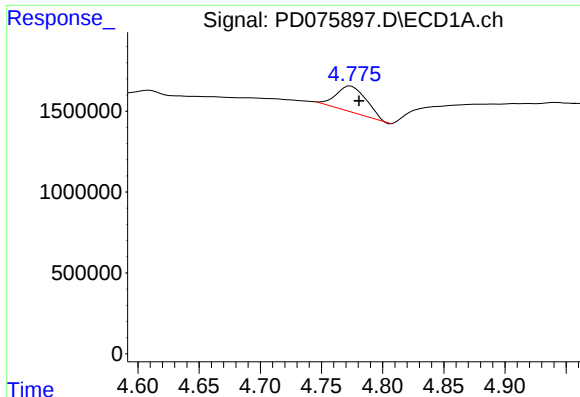

#7 delta-BHC


R.T.: 4.774 min
Delta R.T.: -0.007 min
Response: 2783872
Conc: 0.84 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153525BL

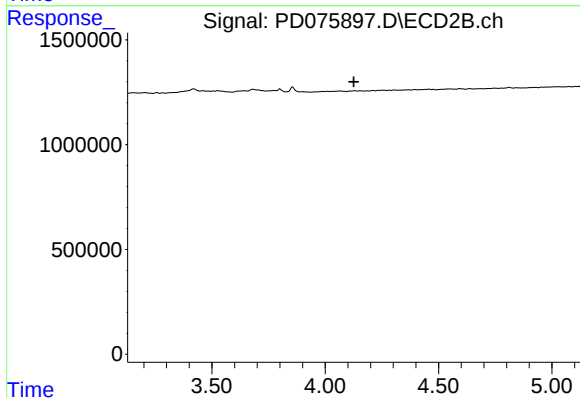


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.127 min
Response: 0
Conc: N.D.

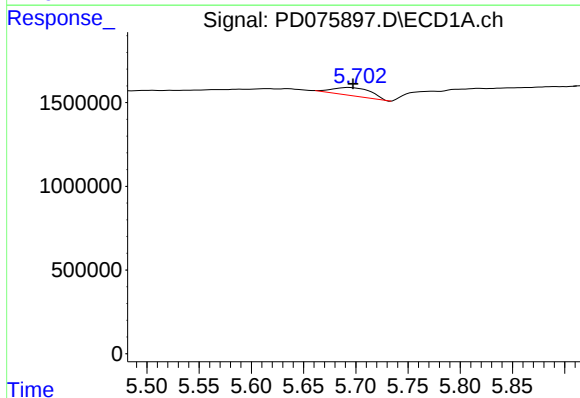


#8 Heptachlor epoxide

R.T.: 5.694 min
Delta R.T.: -0.004 min
Response: 1252400
Conc: 0.39 ng/ml

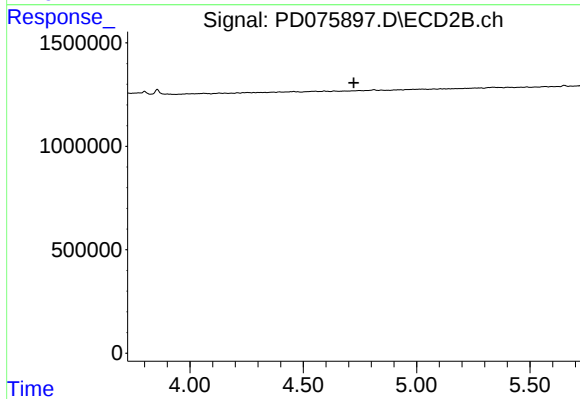

#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

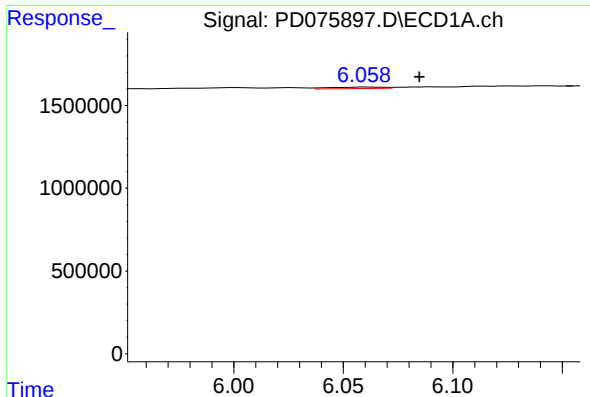

#9 Endosulfan I

R.T.: 6.061 min
Delta R.T.: -0.024 min
Response: 151611
Conc: 0.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153525BL

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

#11 alpha-Chlordane

R.T.: 6.026 min
Delta R.T.: -0.008 min
Response: 127831
Conc: 0.04 ng/ml

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

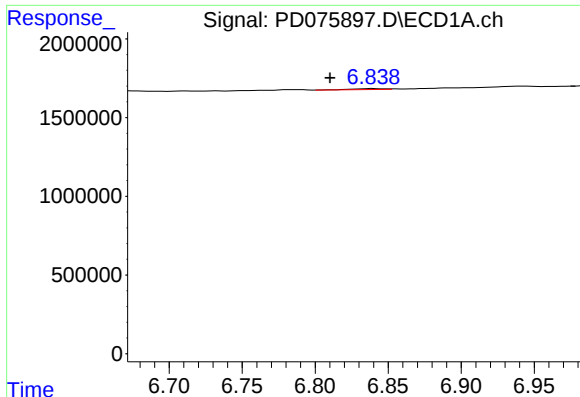

#15 Endosulfan II


R.T.: 6.839 min
Delta R.T.: 0.029 min
Response: 94536
Conc: 0.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153525BL

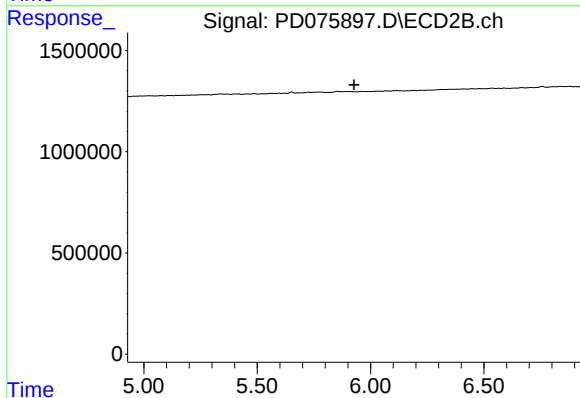


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

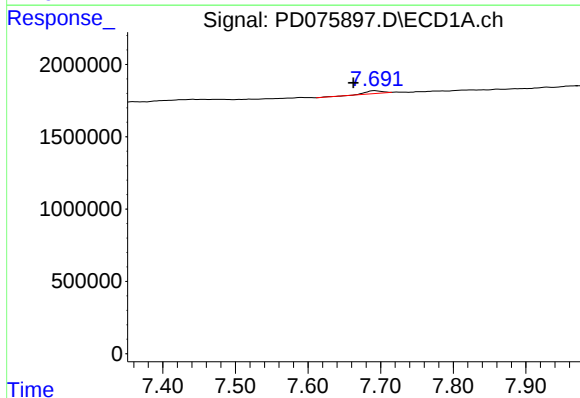


#21 Endrin ketone

R.T.: 7.693 min
Delta R.T.: 0.030 min
Response: 274095
Conc: 0.10 ng/ml

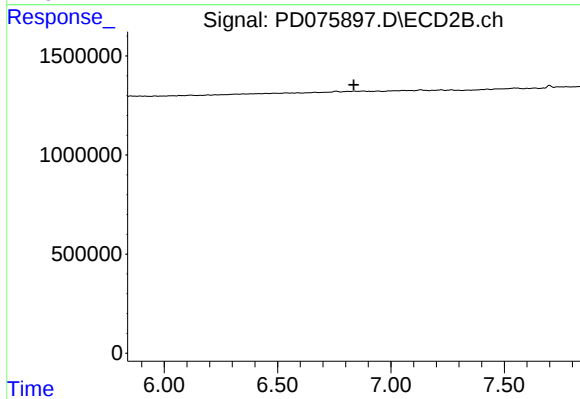

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

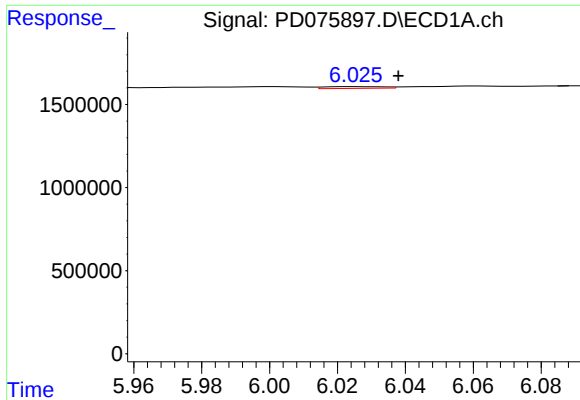

#26 Chlordane-4


R.T.: 6.026 min
Delta R.T.: -0.012 min
Response: 127831
Conc: 0.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153525BL

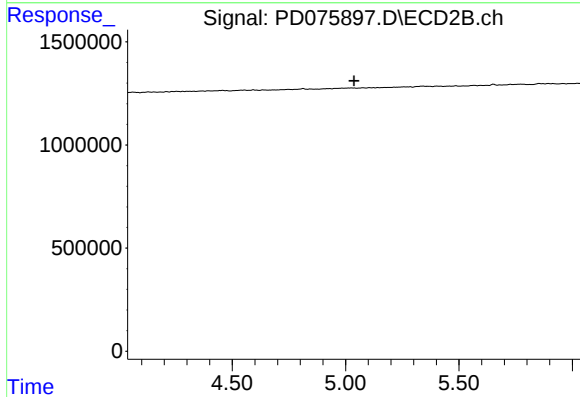


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

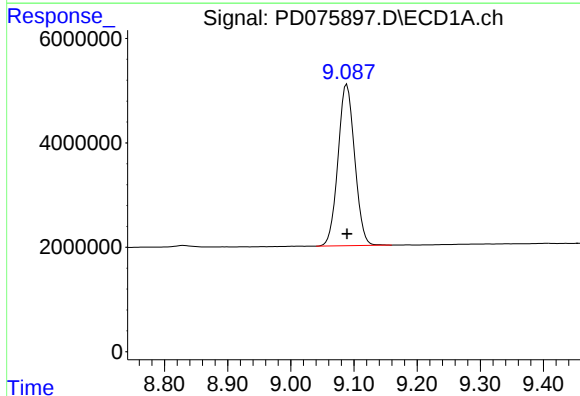

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.000 min
Response: 56696565
Conc: 22.38 ng/ml

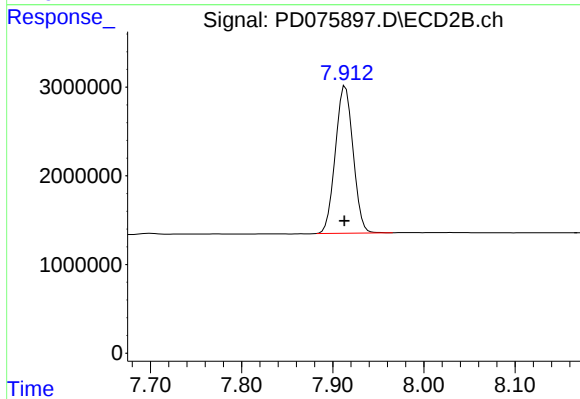

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.001 min
Response: 22472420
Conc: 22.98 ng/ml