

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061923\
 Data File : PD075926.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2023 22:23
 Operator : AR\AJ
 Sample : 03289-20
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-07-4.0-6.0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 01:26:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.768	29352481	14498910	13.780	13.364
28)	SA Decachlor...	9.084	7.910	32284564	13000717	12.744	13.296
Target Compounds							
5)	MB Aldrin	5.295f	0.000	155338	0	0.044	N.D. #
7)	B delta-BHC	4.770	0.000	1599234	0	0.481	N.D. #
8)	B Heptachlo...	5.689	0.000	894657	0	0.278	N.D. #
9)	A Endosulfan I	6.094	0.000	40758	0	0.014	N.D. #
10)	B gamma-Chl...	5.950	0.000	424191	0	0.132	N.D. #
11)	B alpha-Chl...	6.035	0.000	551418	0	0.171	N.D. #
12)	B 4,4'-DDE	6.203	5.224	859525	344738	0.301	0.309
16)	A 4,4'-DDD	6.727	0.000	100443	0	0.044	N.D. #
17)	MA 4,4'-DDT	7.036	6.028	663178	221967	0.292	0.273
21)	B Endrin ke...	7.690f	0.000	312380	0	0.112	N.D. #
25)	Chlordane-3	5.950	0.000	424191	0	0.817	N.D. #
26)	Chlordane-4	6.035	0.000	551418	0	0.875	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061923\
Data File : PD075926.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2023 22:23
Operator : AR\AJ
Sample : 03289-20
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SB-07-4.0-6.0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 01:26:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

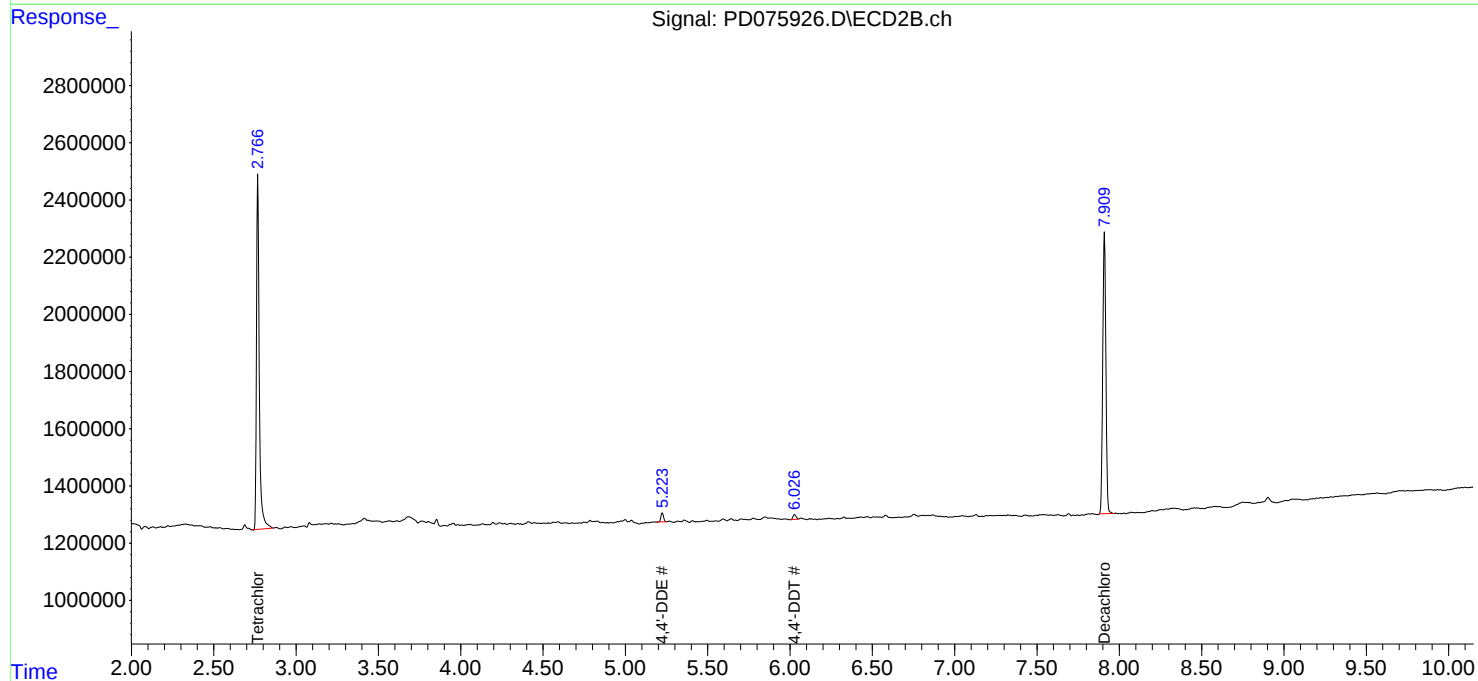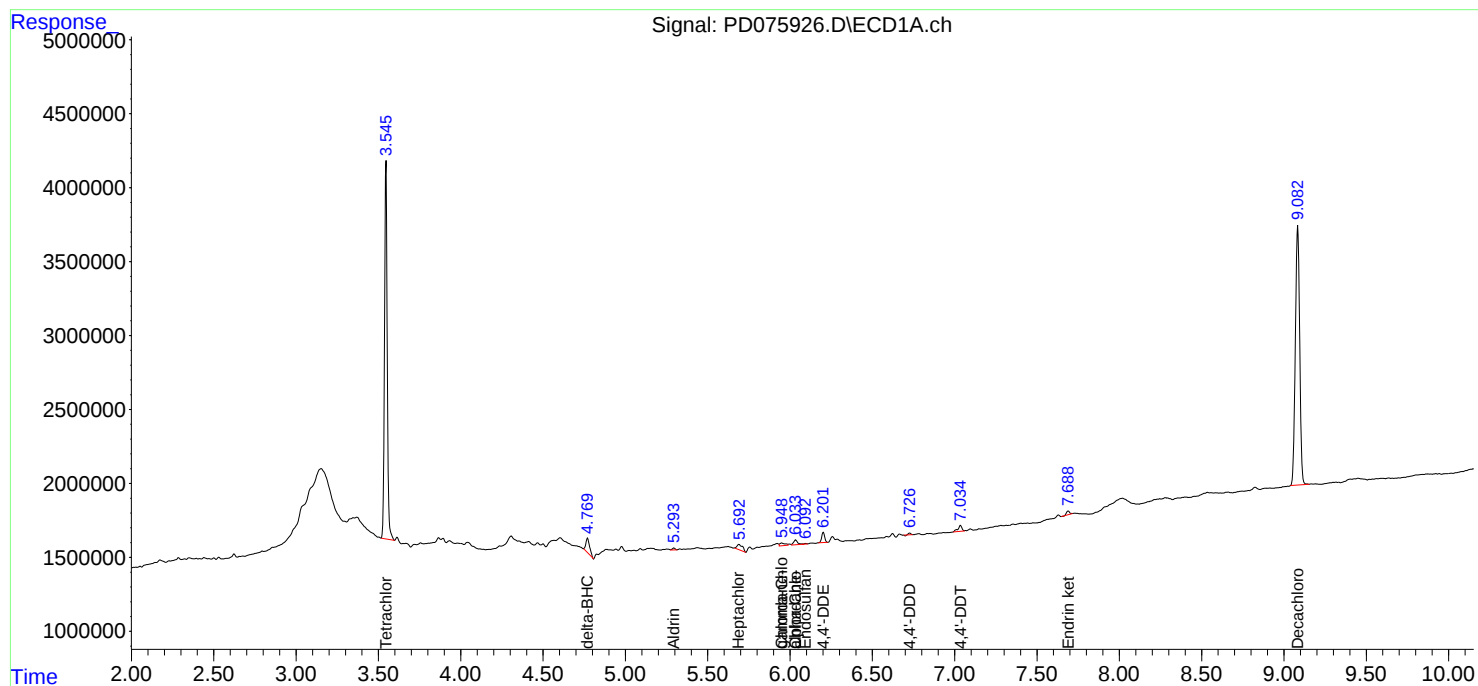


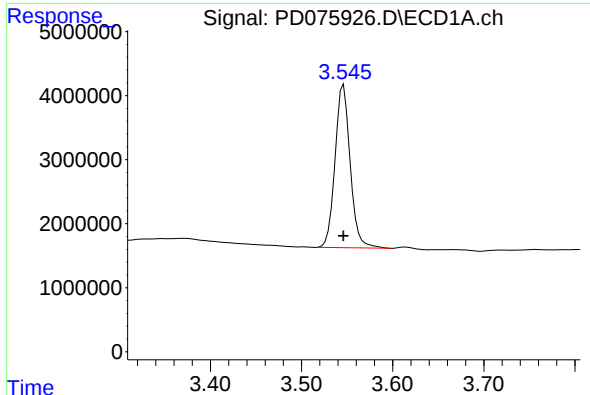

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 29352481
Conc: 13.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-07-4.0-6.0

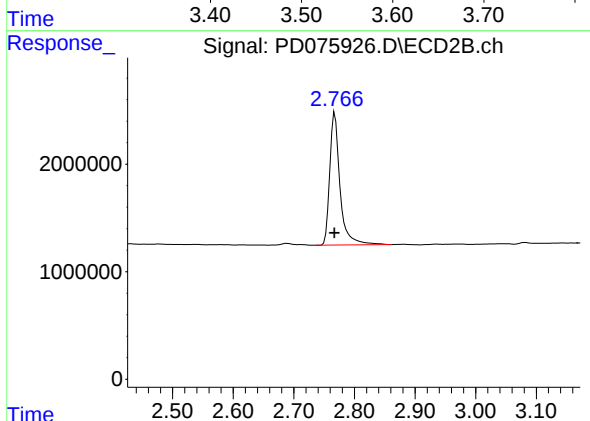


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: 0.000 min
Response: 14498910
Conc: 13.36 ng/ml

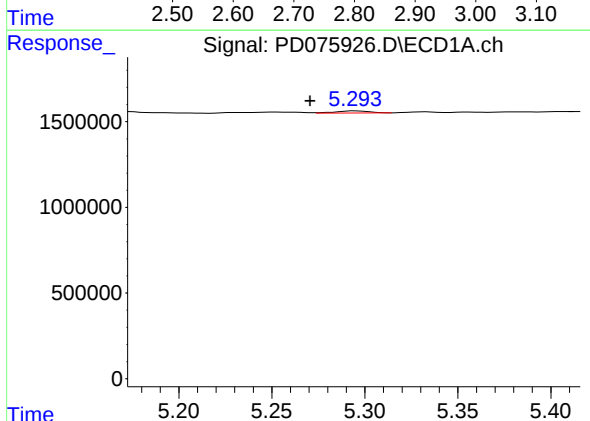


#5 Aldrin

R.T.: 5.295 min
Delta R.T.: 0.024 min
Response: 155338
Conc: 0.04 ng/ml

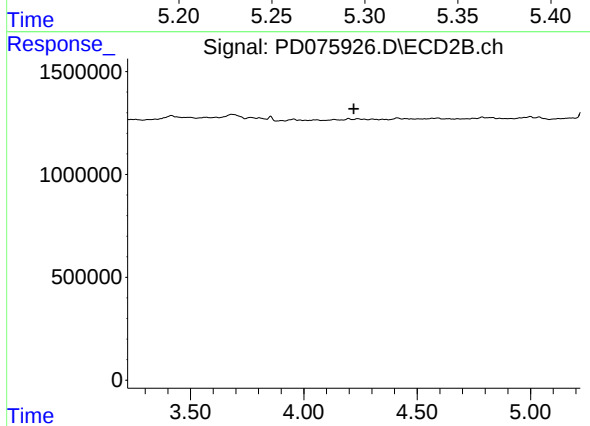

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.220 min
Response: 0
Conc: N.D.

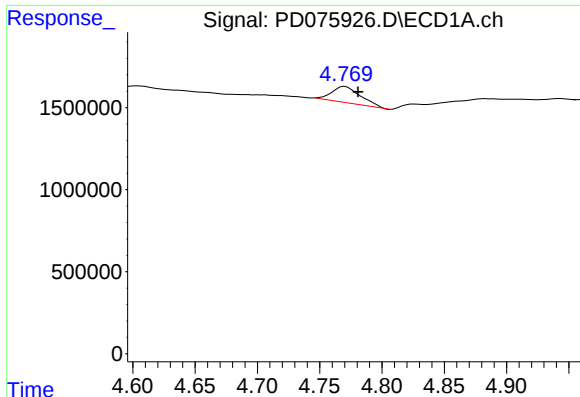

#7 delta-BHC


R.T.: 4.770 min
Delta R.T.: -0.010 min
Response: 1599234
Conc: 0.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-07-4.0-6.0

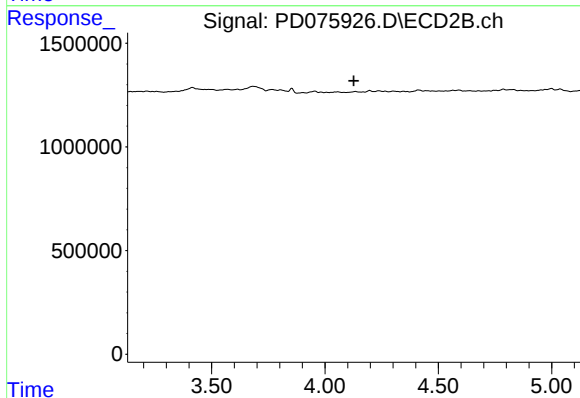


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.127 min
Response: 0
Conc: N.D.

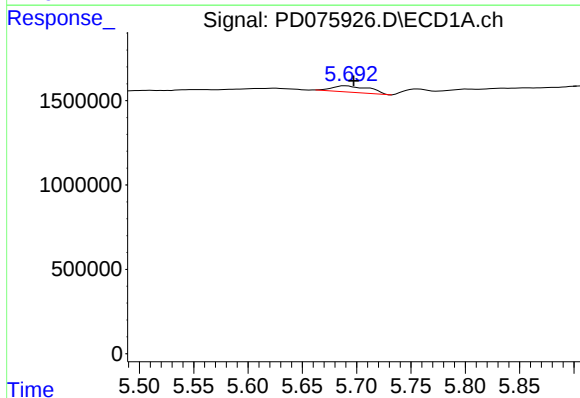


#8 Heptachlor epoxide

R.T.: 5.689 min
Delta R.T.: -0.008 min
Response: 894657
Conc: 0.28 ng/ml

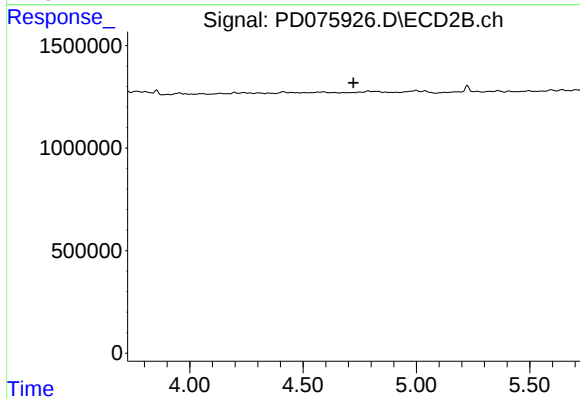

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

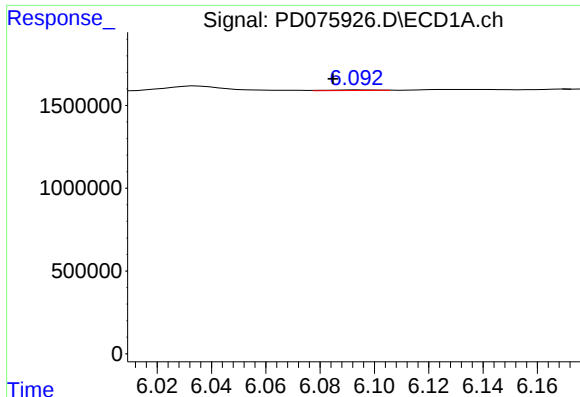

#9 Endosulfan I


R.T.: 6.094 min
Delta R.T.: 0.010 min
Response: 40758
Conc: 0.01 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-07-4.0-6.0

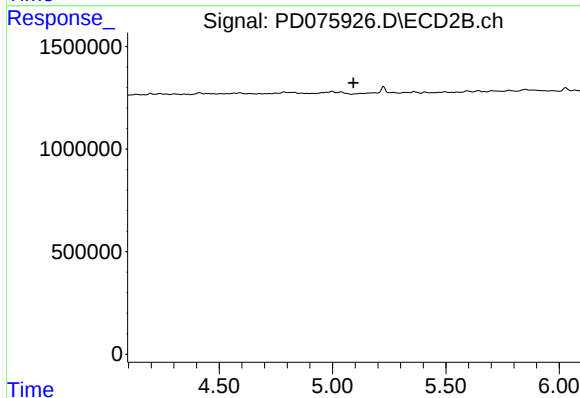


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

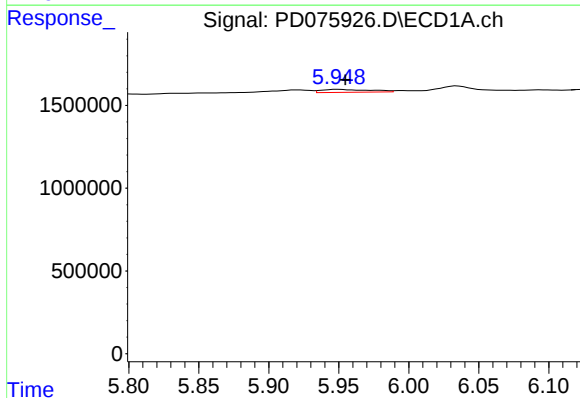


#10 gamma-Chlordane

R.T.: 5.950 min
Delta R.T.: -0.005 min
Response: 424191
Conc: 0.13 ng/ml

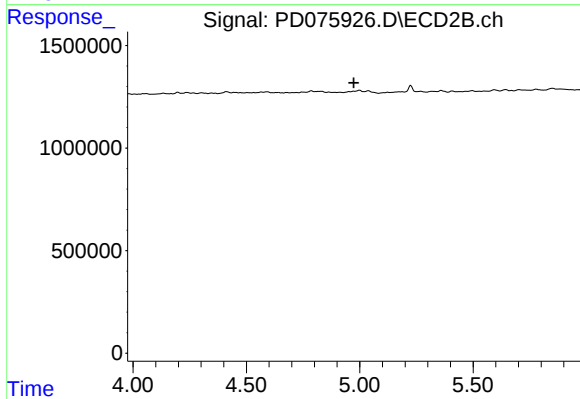

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

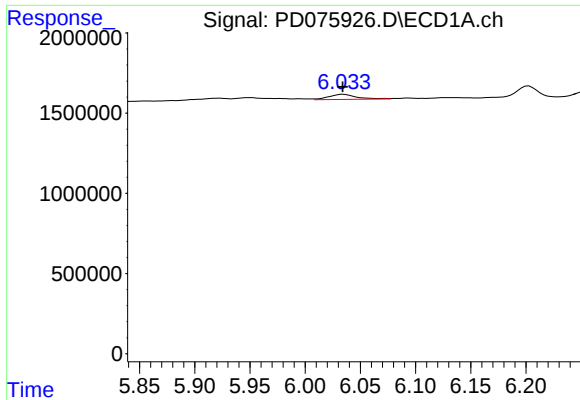

#11 alpha-Chlordane


R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 551418
Conc: 0.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-07-4.0-6.0

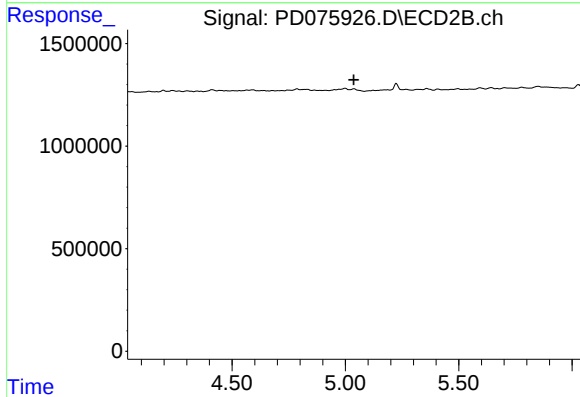


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

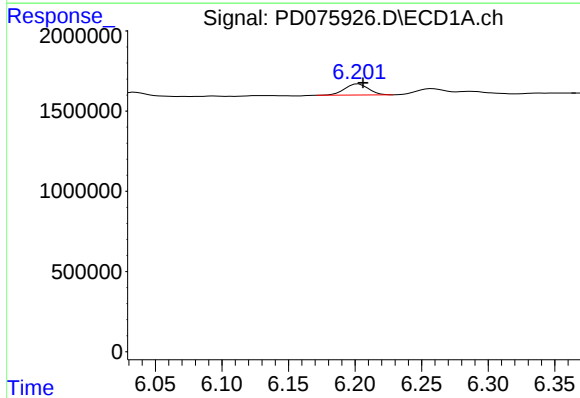


#12 4,4'-DDE

R.T.: 6.203 min
Delta R.T.: -0.003 min
Response: 859525
Conc: 0.30 ng/ml

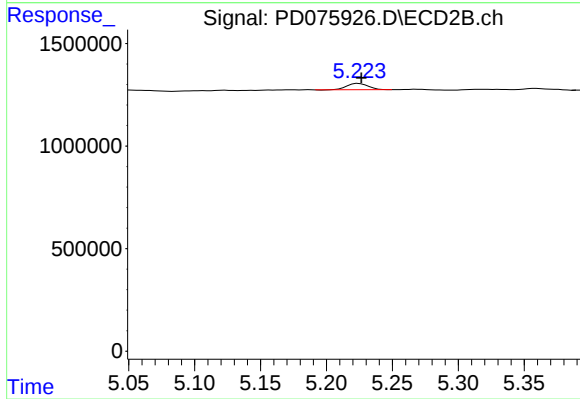

#12 4,4'-DDE


R.T.: 5.224 min
Delta R.T.: -0.002 min
Response: 344738
Conc: 0.31 ng/ml

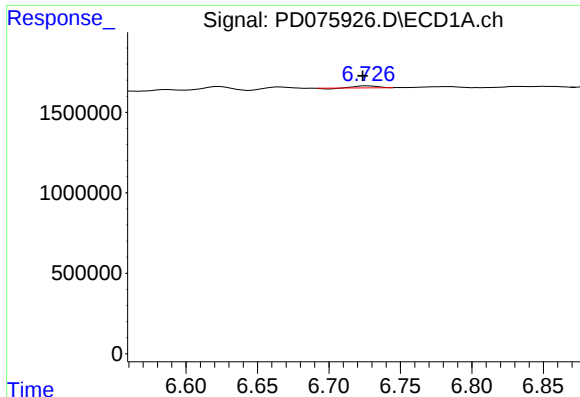

#16 4,4'-DDD


R.T.: 6.727 min
Delta R.T.: 0.004 min
Response: 100443
Conc: 0.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-07-4.0-6.0

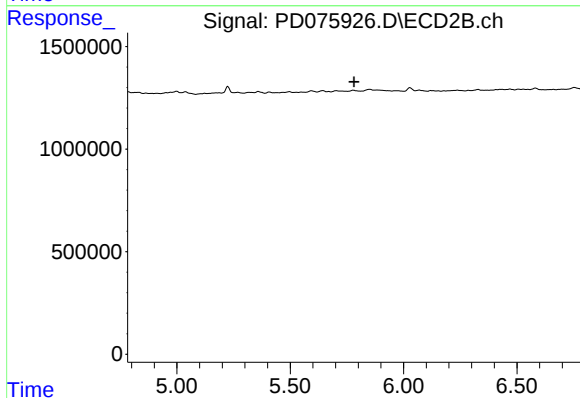


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.781 min
Response: 0
Conc: N.D.

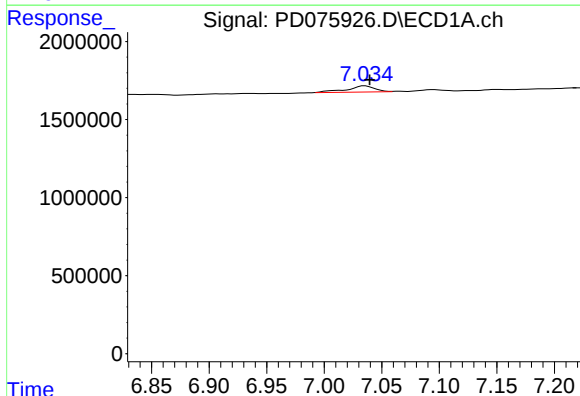


#17 4,4'-DDT

R.T.: 7.036 min
Delta R.T.: -0.004 min
Response: 663178
Conc: 0.29 ng/ml

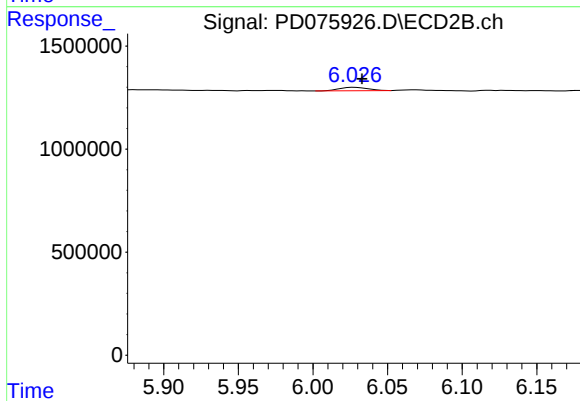

#17 4,4'-DDT


R.T.: 6.028 min
Delta R.T.: -0.005 min
Response: 221967
Conc: 0.27 ng/ml

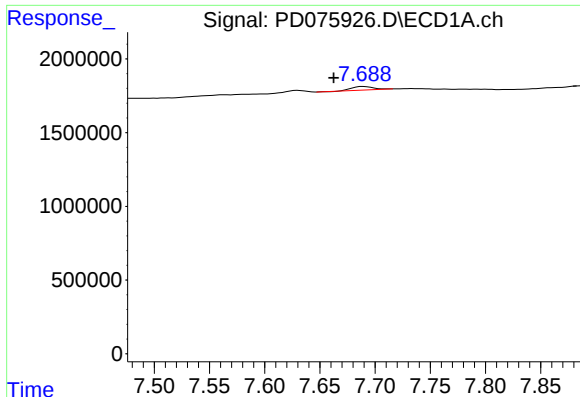

#21 Endrin ketone


R.T.: 7.690 min
Delta R.T.: 0.027 min
Response: 312380
Conc: 0.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-07-4.0-6.0

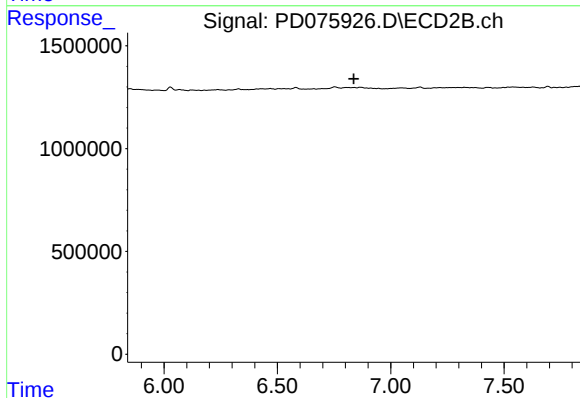


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

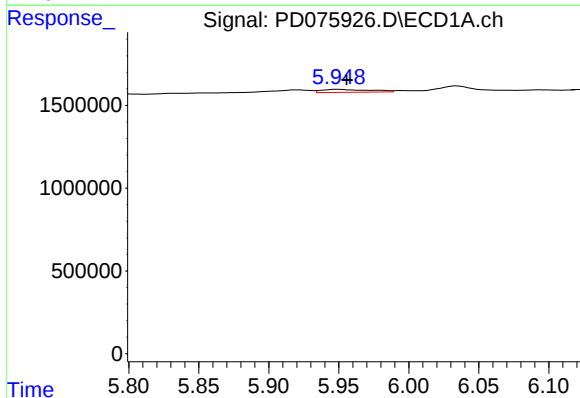


#25 Chlordane-3

R.T.: 5.950 min
Delta R.T.: -0.006 min
Response: 424191
Conc: 0.82 ng/ml

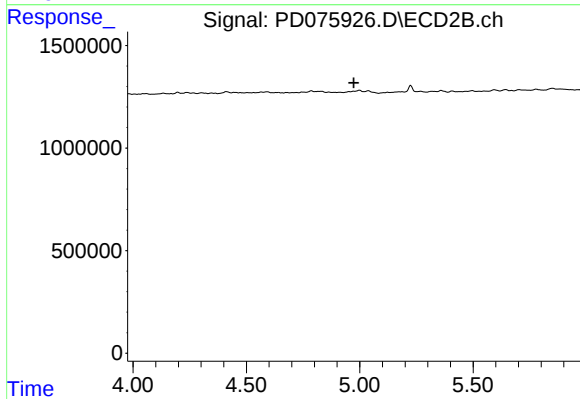

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

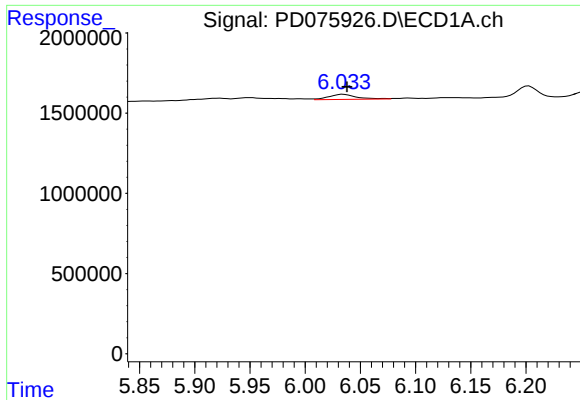

#26 Chlordane-4


R.T.: 6.035 min
Delta R.T.: -0.003 min
Response: 551418
Conc: 0.87 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-07-4.0-6.0

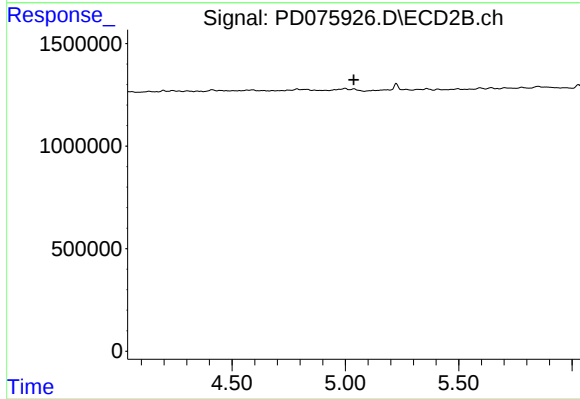


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

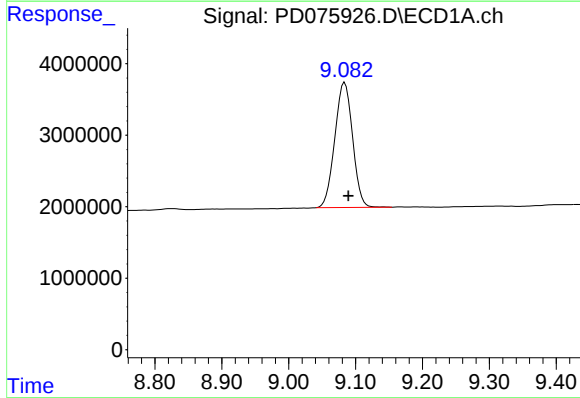

#28 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.005 min
Response: 32284564
Conc: 12.74 ng/ml

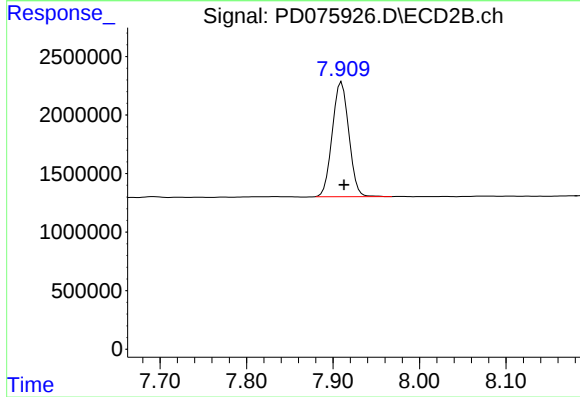

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: -0.003 min
Response: 13000717
Conc: 13.30 ng/ml