

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061924\
 Data File : PD083757.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2024 18:04
 Operator : AR\AJ
 Sample : P2899-16MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AB6MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/20/2024
 Supervised By : Ankita Jodhani 06/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 22:40:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	10301571	42706895	7.892	7.835m
27)	SA Decachlor...	9.110	7.894	12334669	43313263	6.343m	7.133m
Target Compounds							
2)	A alpha-BHC	4.016	3.271	81943763	303.9E6	36.922m	35.649
3)	MA gamma-BHC...	4.350	3.598	80383679	274.7E6	36.948m	35.177m
4)	MA Heptachlor	4.942	3.937	82692626	297.2E6	34.039m	37.965
5)	MB Aldrin	5.287	4.214	78863408	256.2E6	33.195	33.154m
6)	B beta-BHC	4.547	3.895	33093738	125.2E6	32.838m	35.084m
7)	B delta-BHC	4.797	4.125	87741101	283.3E6	33.401	33.222
8)	B Heptachlo...	5.713	4.717	72919397	248.4E6	35.306m	33.950
9)	A Endosulfan I	6.101	5.086	71042724	232.9E6	36.328	35.230
10)	B trans-Chl...	5.970	4.966	73572211	261.2E6	36.133m	35.962
11)	B cis-Chlor...	6.050	5.030	75401929	259.3E6	36.209	35.214
12)	B 4,4'-DDE	6.223	5.218	151.9E6	462.2E6	73.215	65.037
13)	MA Dieldrin	6.377	5.350	160.3E6	514.2E6	77.508	70.585
14)	MA Endrin	6.607	5.625	138.1E6	470.2E6	81.755	72.702
15)	B Endosulfa...	6.827	5.919	117.2E6	416.2E6	65.170	65.583
16)	A 4,4'-DDD	6.737	5.772	178.7E6	314.9E6	121.979m	55.851 #
17)	MA 4,4'-DDT	7.057	6.022	128.4E6	390.8E6	85.244	69.034
18)	B Endrin al...	6.958	6.098	104.2E6	294.1E6	78.094	61.388
19)	B Endosulfa...	7.193	6.320	128.9E6	384.3E6	75.371	62.208
20)	A Methoxychlor	7.532	6.595	328.8E6	882.0E6	379.991	303.480m
21)	B Endrin ke...	7.681	6.824	144.2E6	426.1E6	77.360	63.384m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061924\
Data File : PD083757.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2024 18:04
Operator : AR\AJ
Sample : P2899-16MSD
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 22:40:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

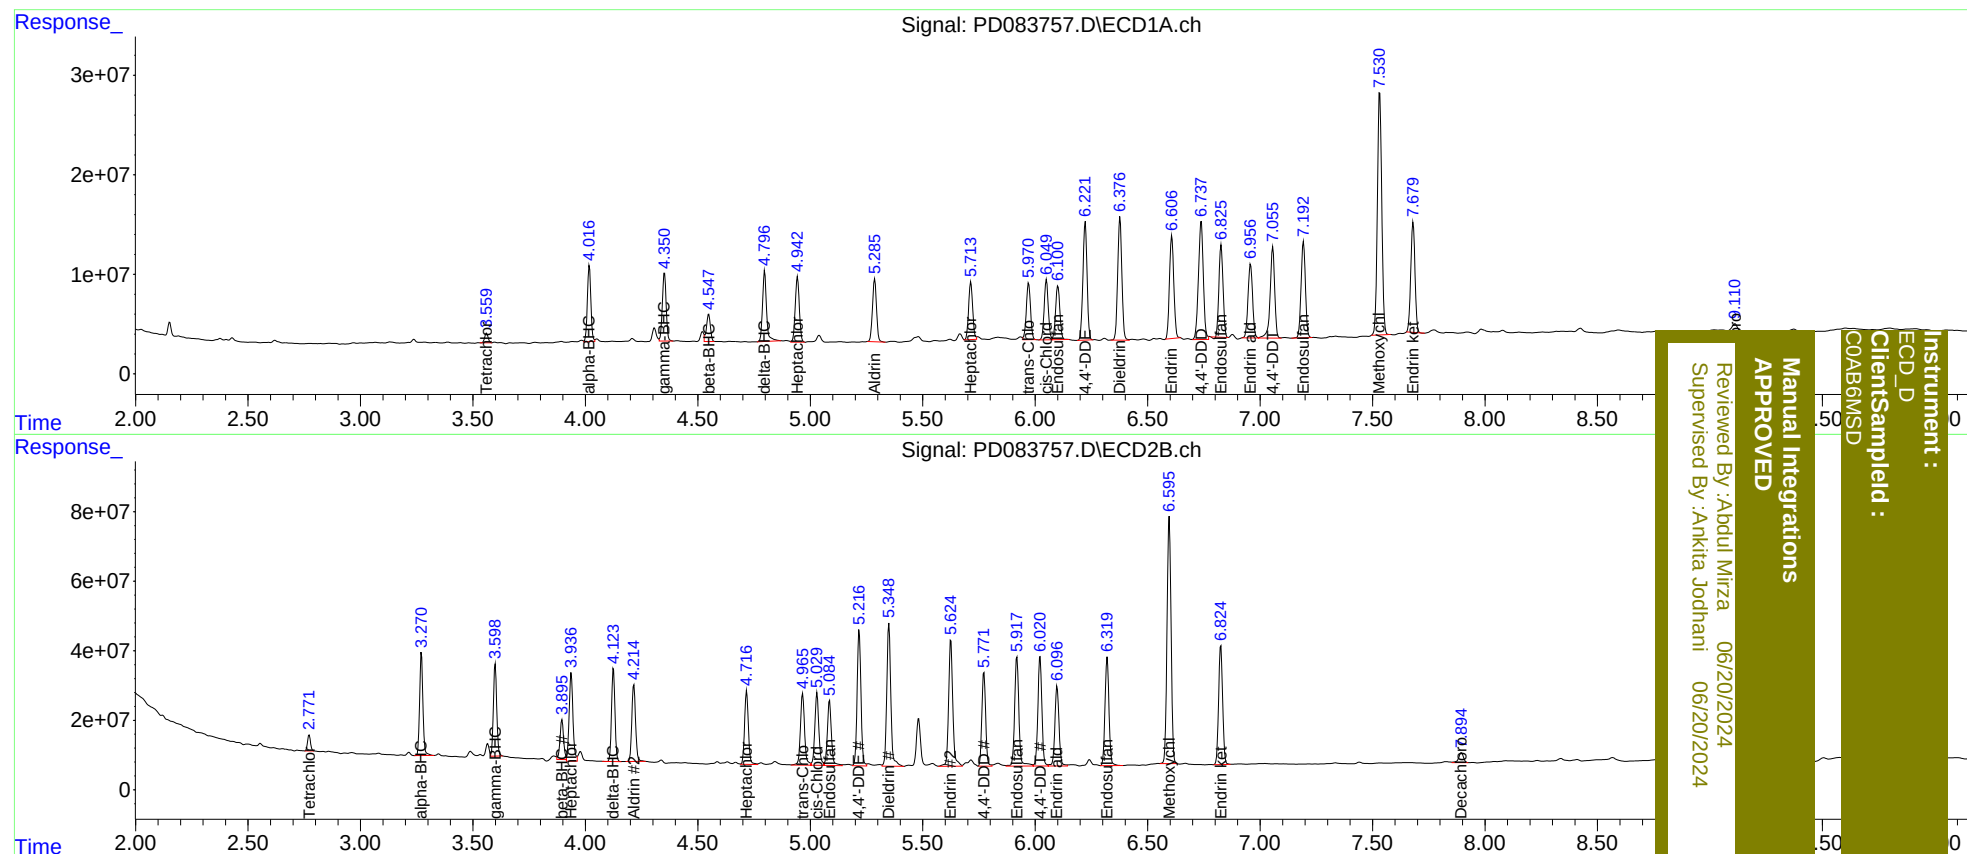

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/20/2024
Supervised By: Ankita Jodhani 06/20/2024

Instrument :
ECD_D
Client Sampled :
COAB6MSD