

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061924\
 Data File : PD083741.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2024 14:17
 Operator : AR\AJ
 Sample : P2899-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA5

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/20/2024
 Supervised By :Ankita Jodhani 06/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 22:30:52 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.771	13109956	42441720	10.044m	7.786m
2)	SA Decachlor...	9.111	7.894	22507965	54289765	11.575m	8.941m
Target Compounds							
9)	A Endosulfan I	6.087	5.103	3641743	9474985	1.862m	1.433m
12)	B 4,4'-DDE	6.222	5.217	6998933	10817298	3.374m	1.522m#
17)	MA 4,4'-DDT	7.057	6.016	4434429	24276464	2.944m	4.289m#
19)	B Endosulfa...	7.197	6.347	1683500	7304534	0.984m	1.182m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061924\
Data File : PD083741.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2024 14:17
Operator : AR\AJ
Sample : P2899-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 22:30:52 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

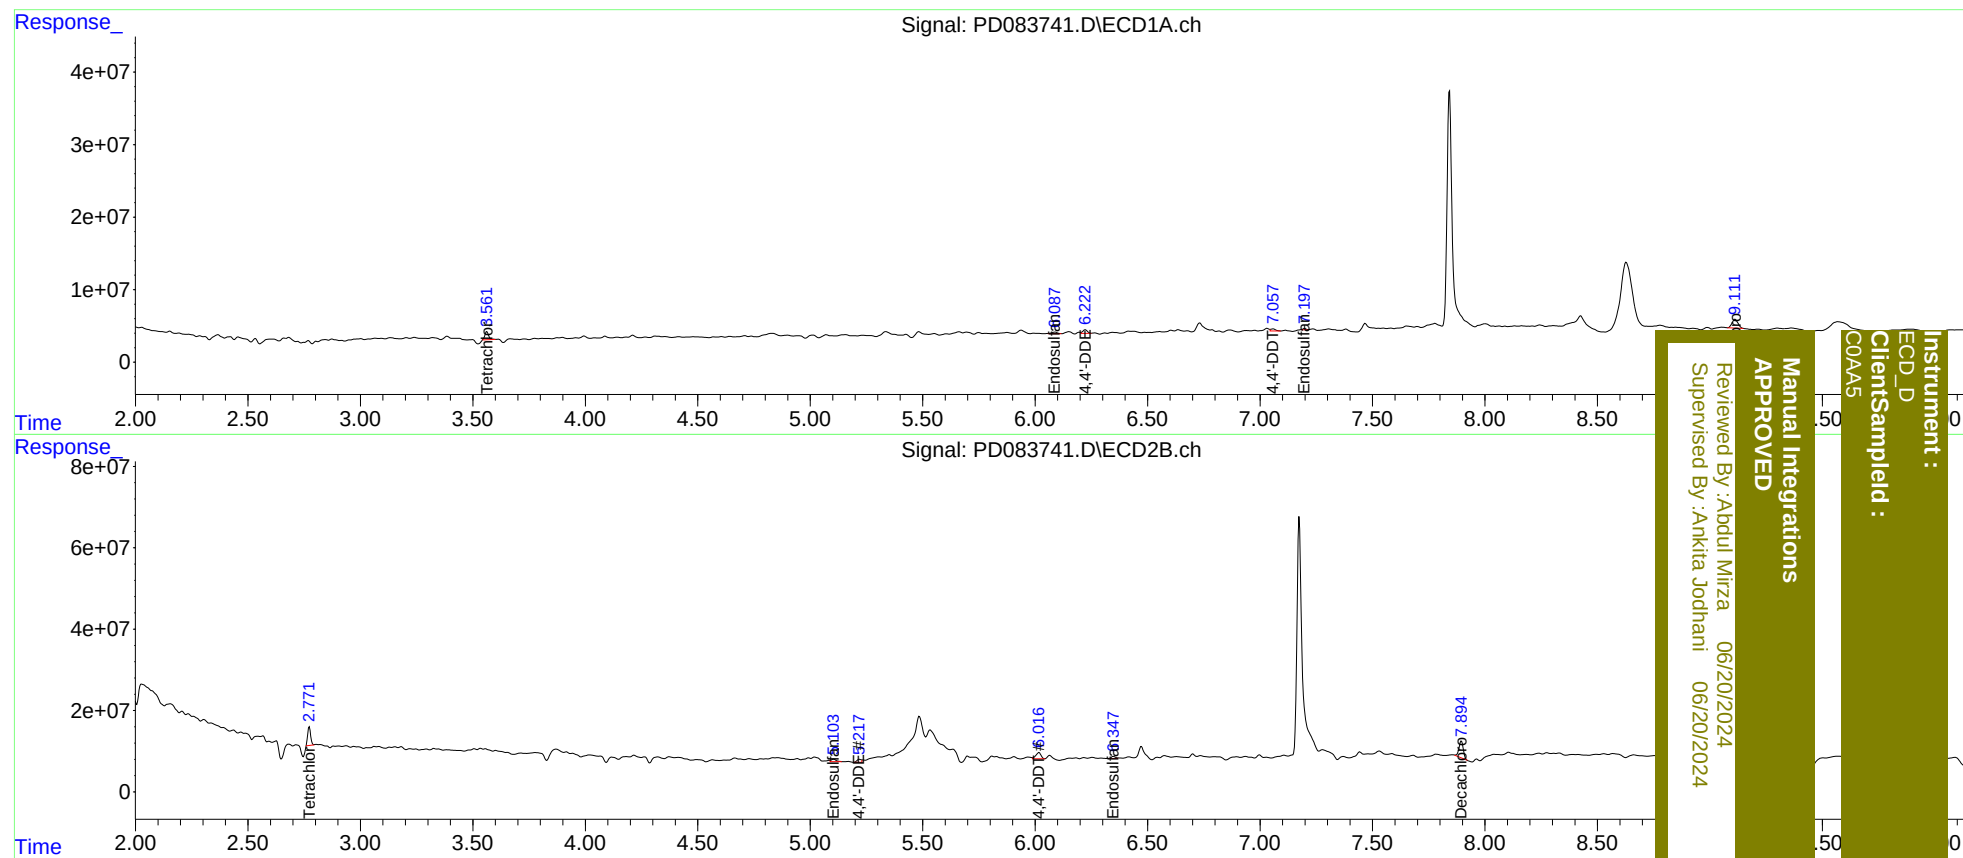

Instrument :
ECD_D
ClientSampled :
COAAS

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/20/2024
Supervised By :Ankita Jodhani 06/20/2024