

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061924\
 Data File : PD083745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Jun 2024 15:10
 Operator : AR\AJ
 Sample : P2899-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA9

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/20/2024
 Supervised By : Ankita Jodhani 06/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 22:33:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.560	2.771	6362330	27379684	4.874m	5.023m
2) SA Decachlor...	9.109	7.896	11843251	35553032	6.091	5.855
Target Compounds						
14) MA Endrin	6.603	5.631	2781581	4752143	1.647m	0.735m#
17) MA 4,4'-DDT	7.029	6.016	8650261	25881494	5.742m	4.572m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061924\
Data File : PD083745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Jun 2024 15:10
Operator : AR\AJ
Sample : P2899-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 22:33:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

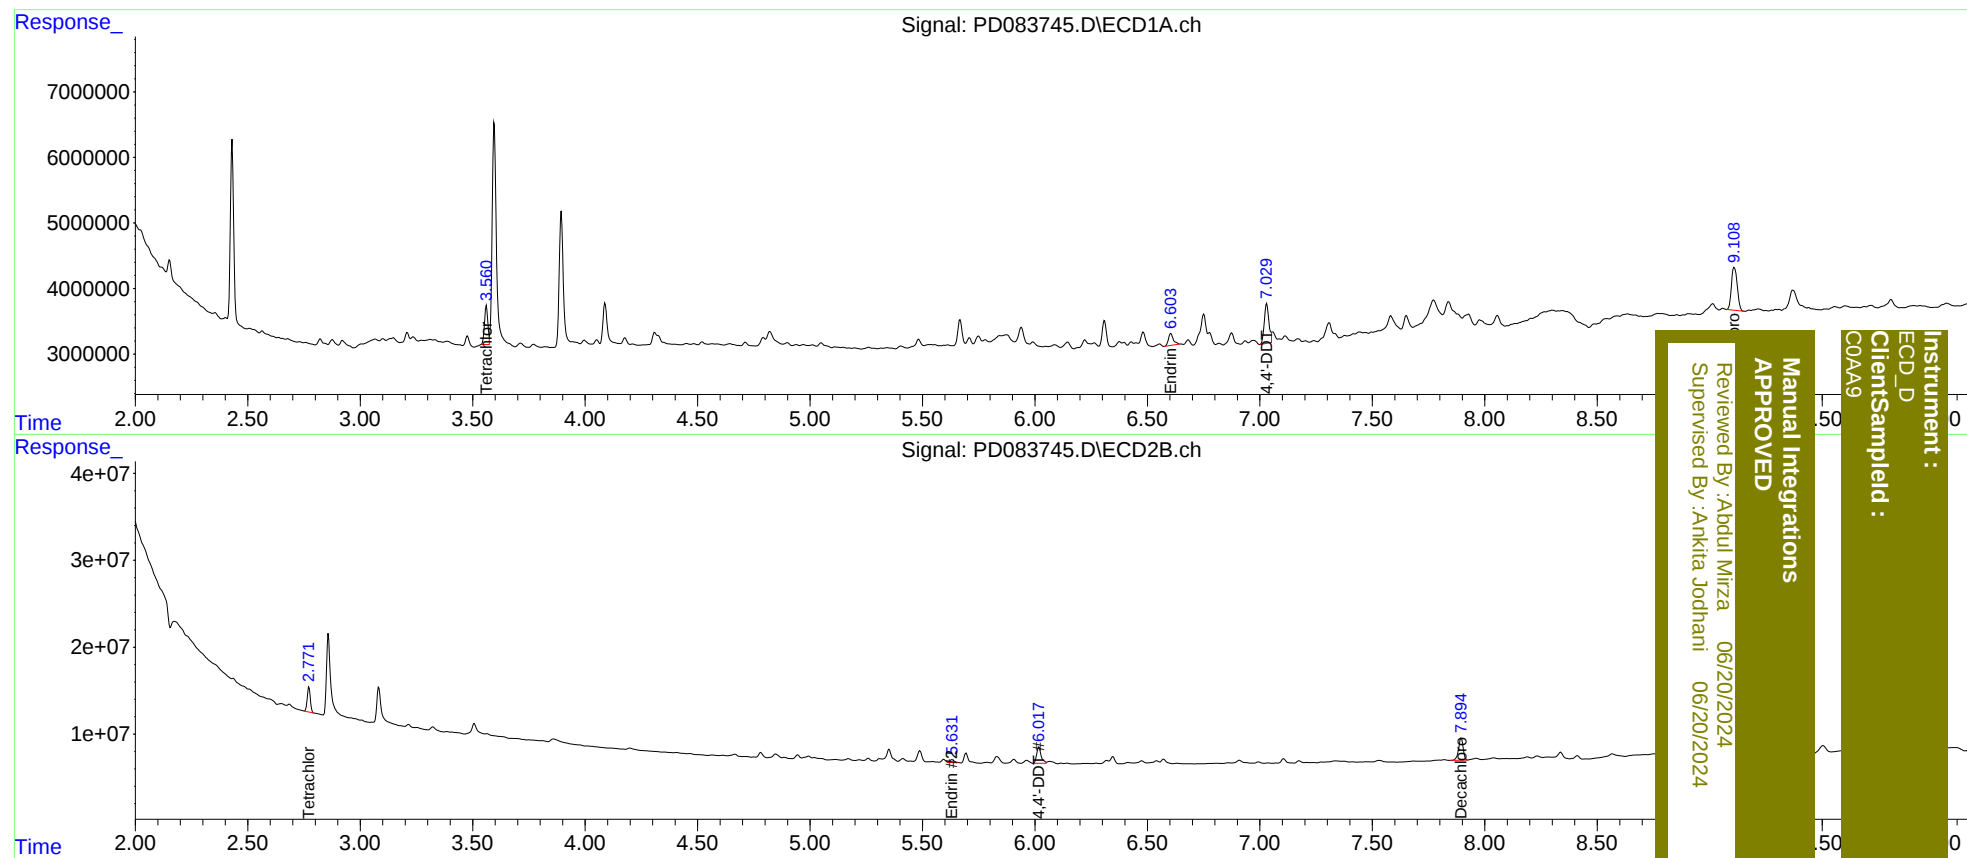

Reviewed By: Abdul Mirza 06/20/2024
Supervised By: Ankita Jodhani 06/20/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
COAA9