

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061925\
 Data File : PD089022.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jun 2025 16:52
 Operator : AR\AJ
 Sample : INDA335
 Misc :
 ALS Vial : 99 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 19 12:08:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060525CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 06 11:09:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.881	53471426	337.0E6	20.890	22.005
27)	SA Decachlor...	9.074	8.072	150.1E6	797.3E6	38.755	40.634
Target Compounds							
2)	A alpha-BHC	3.999	3.393	104.6E6	538.1E6	20.674	22.003
3)	MA gamma-BHC...	4.330	3.729	102.6E6	495.0E6	21.085	21.915
4)	MA Heptachlor	4.929	4.082	101.6E6	507.9E6	20.801	21.958
5)	MB Aldrin	5.271	4.369	3300968	18896589	0.697	0.840
8)	B Heptachlo...	5.683	0.000	2369414	0	0.540	N.D. #
9)	A Endosulfan I	6.075	5.247	84166470	422.4E6	20.907	21.732
10)	B trans-Chl...	5.890f	0.000	1728993	0	0.406	N.D. #
11)	B cis-Chlor...	6.075f	5.247f	84166470	422.4E6	19.339	20.120
13)	MA Dieldrin	6.347	5.513	181.6E6	907.4E6	41.451	43.455
14)	MA Endrin	6.574	5.789	154.0E6	807.4E6	41.585	42.676
15)	B Endosulfa...	6.771	0.000	1472308	0	0.388	N.D. #
16)	A 4,4'-DDD	6.705	5.929	127.9E6	736.1E6	40.920	42.855
17)	MA 4,4'-DDT	7.021	6.183	134.5E6	770.8E6	40.898	43.204
18)	B Endrin al...	6.917	6.258	874156	8495161	0.303	0.593 #
20)	A Methoxychlor	7.494	6.754	360.5E6	1734.1E6	201.814	213.544
21)	B Endrin ke...	7.631	6.990	2596766	20013467	0.674	1.009 #
23)	Toxaphene-2	0.000	6.183f	0	770.8E6	N.D.	6129.301
24)	Toxaphene-3	7.021	6.754	134.5E6	1734.1E6	1242.848	4266.875 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061925\
Data File : PD089022.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jun 2025 16:52
Operator : AR\AJ
Sample : INDA335
Misc :
ALS Vial : 99 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 19 12:08:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060525CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 06 11:09:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

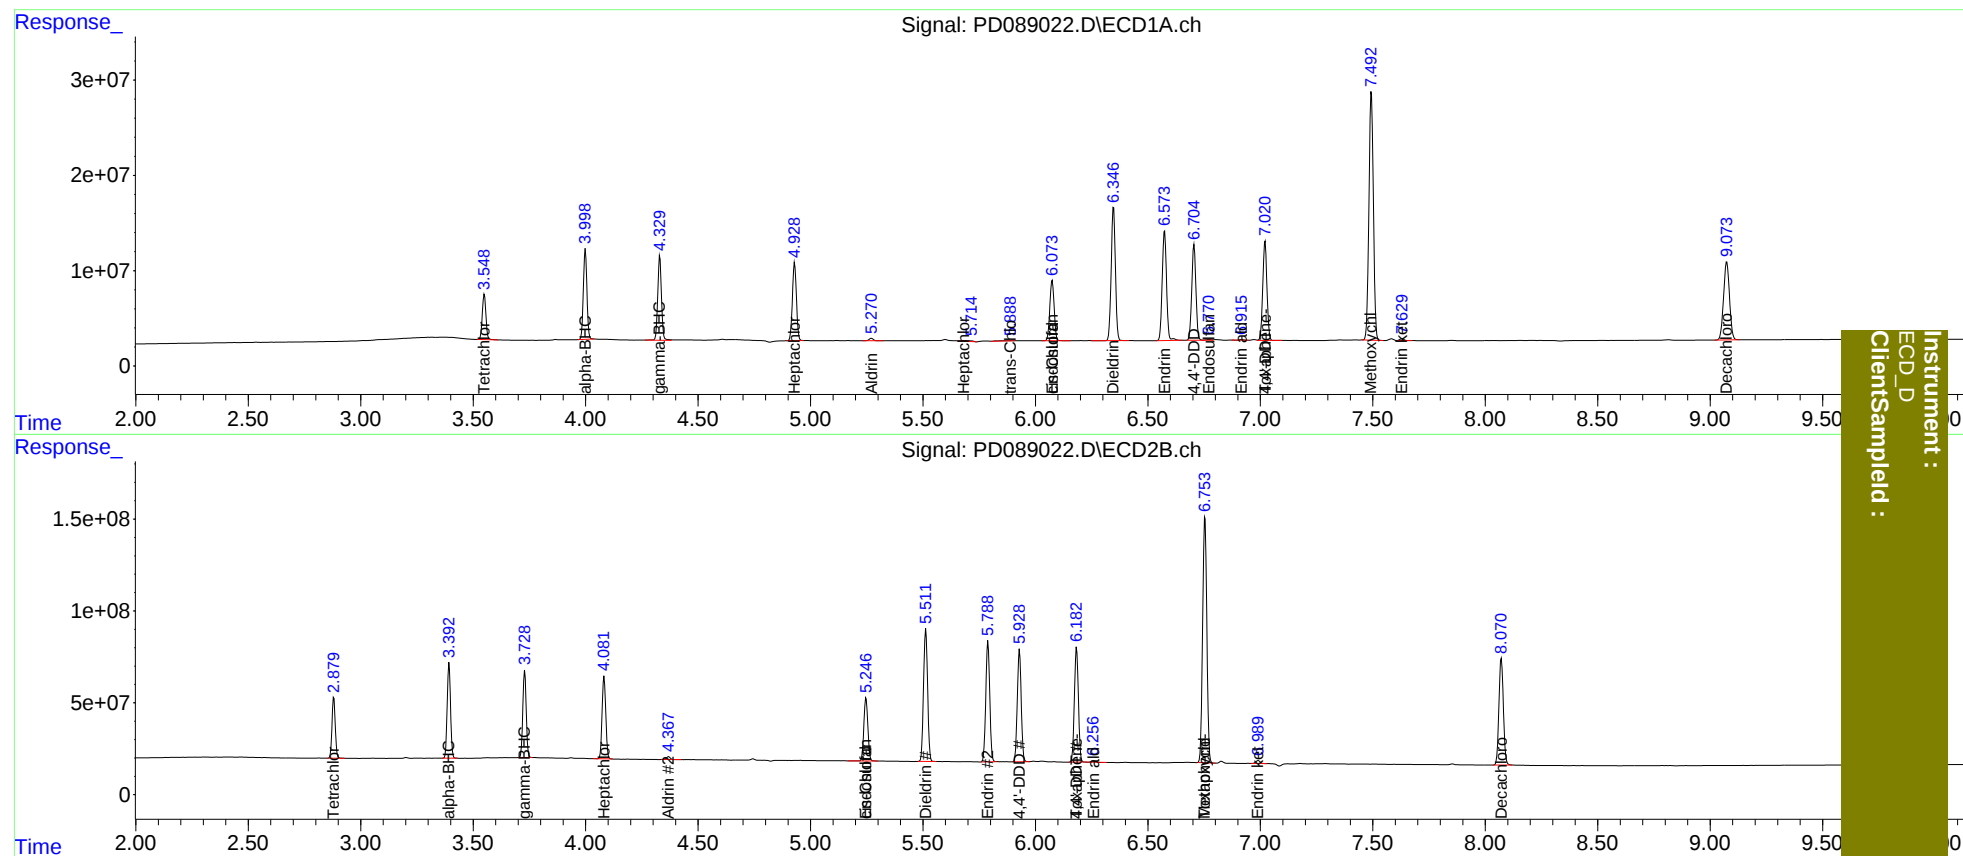

Instrument :
ECD_D
ClientSampled :
0