

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062018\
 Data File : PD048190.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2018 16:49
 Operator : UA/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 02:14:26 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 01:43:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.040	25775649	350.8E6	21.154	18.116
28)	SA Decachlor...	8.138	9.112	25628147	395.0E6	19.803	21.265
Target Compounds							
3)	MA gamma-BHC...	0.000	4.729	0	4336620	N.D.	0.157 #
5)	MB Aldrin	0.000	5.596f	0	5943138	N.D.	0.231 #
6)	B beta-BHC	4.348f	0.000	1848249	0	2.553	N.D. #
7)	B delta-BHC	0.000	5.073	0	37060809	N.D.	2.180 #
8)	B Heptachlo...	0.000	5.878f	0	1103386	N.D.	0.062 #
18)	B Endrin al...	0.000	7.067	0	2468736	N.D.	0.146 #
23)	Chlordane-1	4.348	5.073	1848249	37060809	34.055	36.223
27)	Chlordane-5	0.000	7.016	0	3408645	N.D.	3.931 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062018\
Data File : PD048190.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 16:49
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 02:14:26 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 01:43:00 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

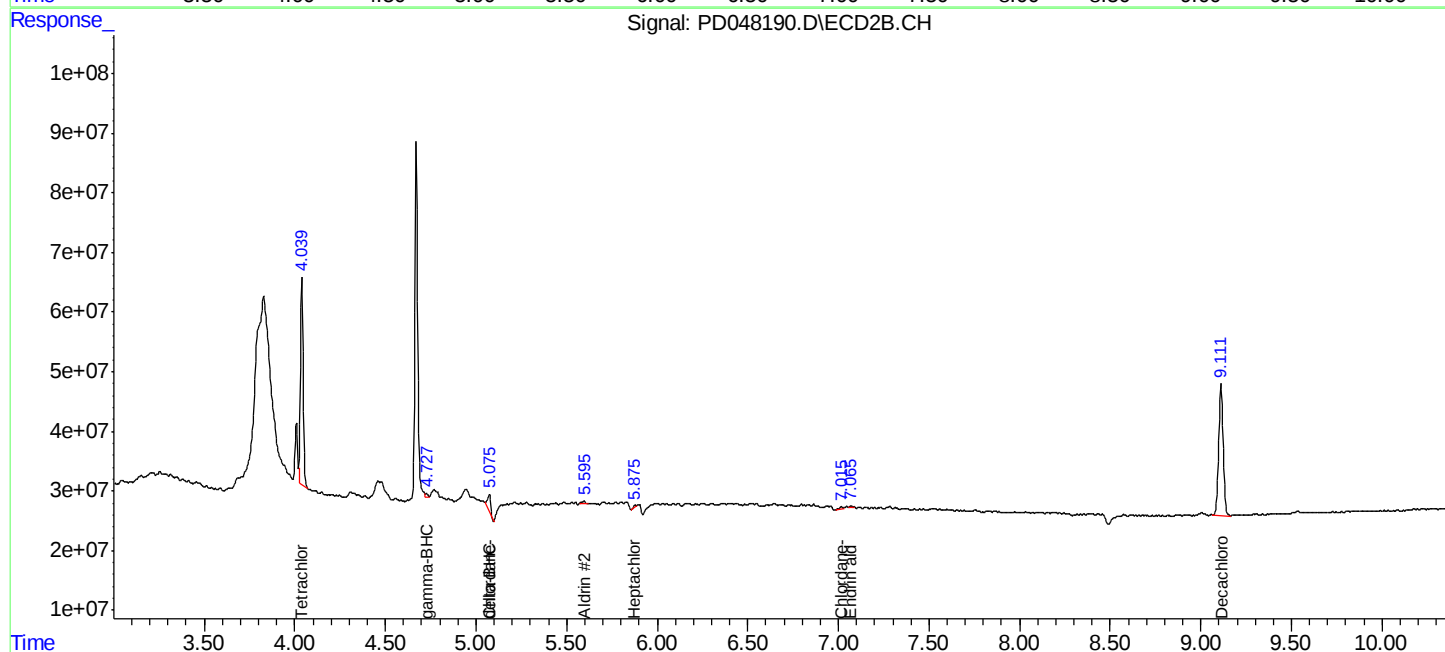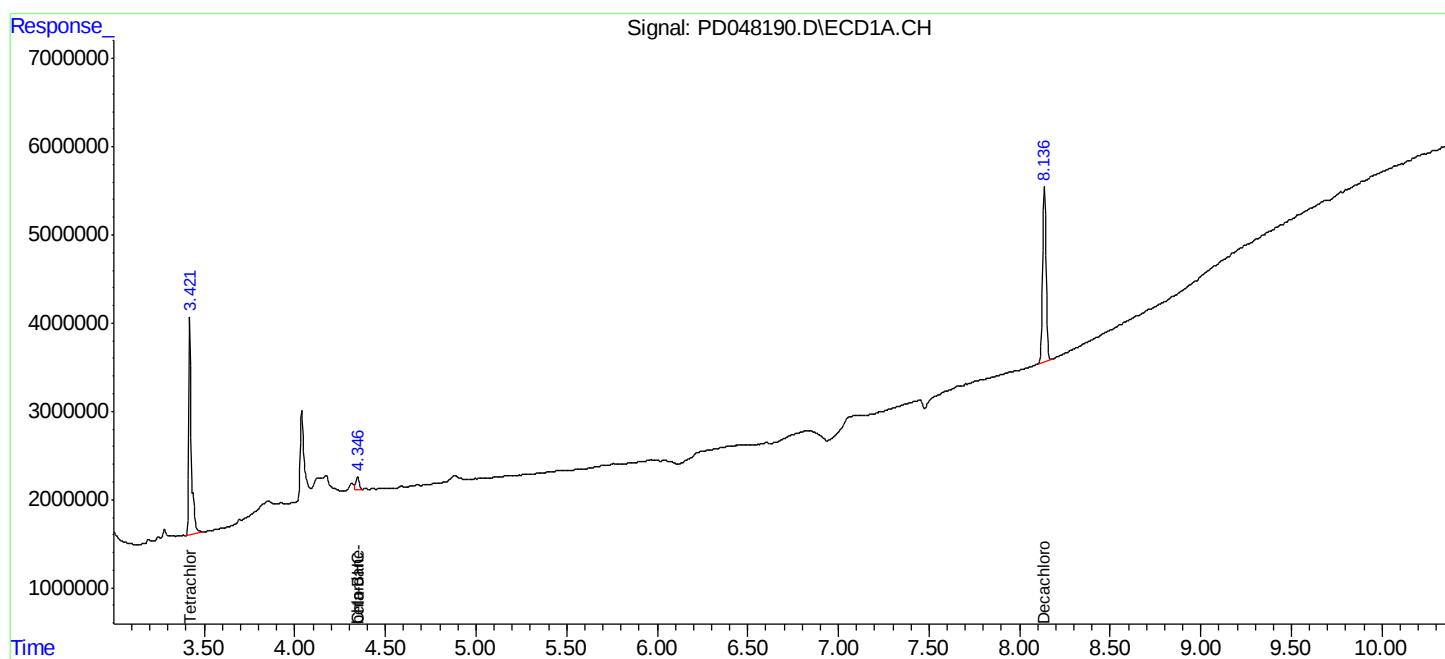


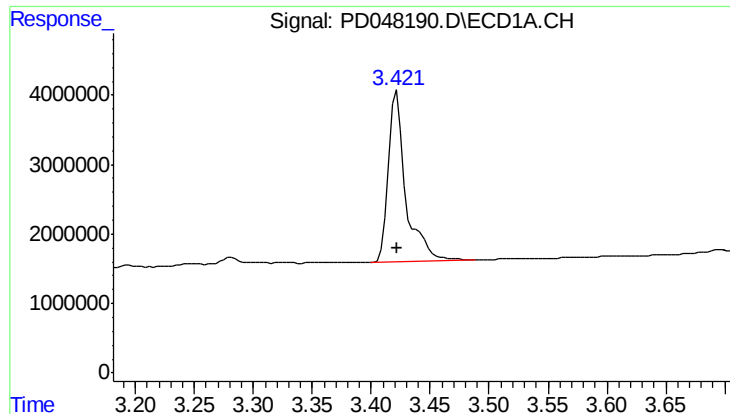

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 25775649
Conc: 21.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

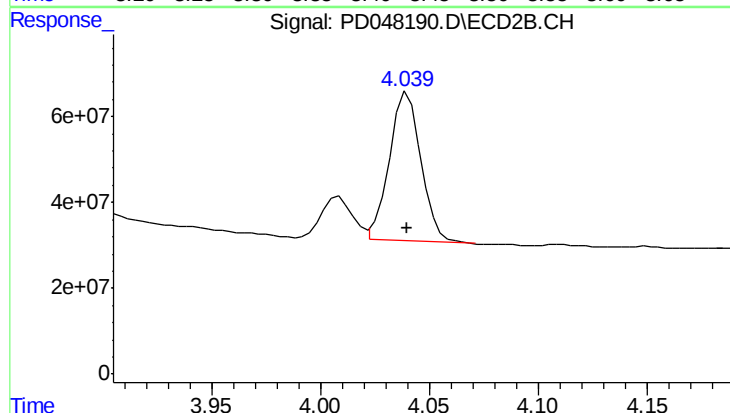


#1 Tetrachloro-m-xylene

R.T.: 4.040 min
Delta R.T.: 0.000 min
Response: 350778449
Conc: 18.12 ng/ml

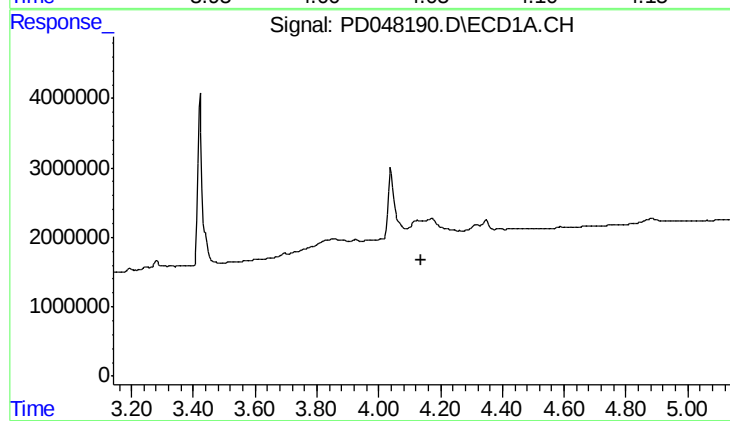


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 4.139 min
Response: 0
Conc: N.D.

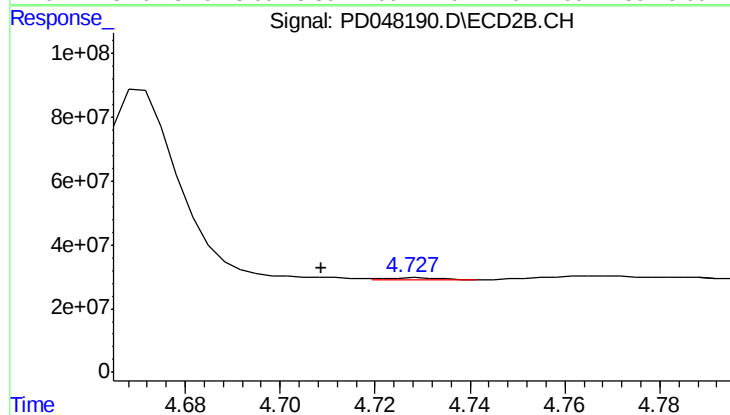

#3 gamma-BHC (Lindane)


R.T.: 4.729 min
Delta R.T.: 0.020 min
Response: 4336620
Conc: 0.16 ng/ml

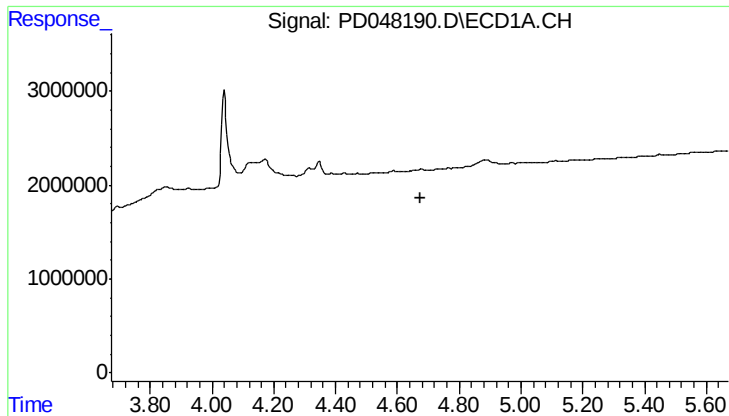

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

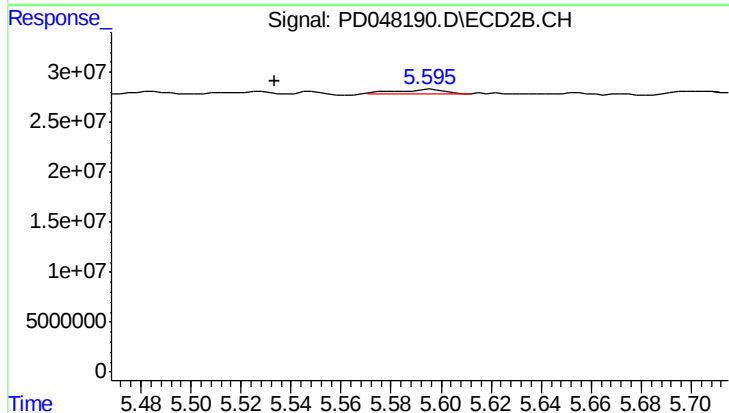


#5 Aldrin

R.T.: 5.596 min
Delta R.T.: 0.062 min
Response: 5943138
Conc: 0.23 ng/ml

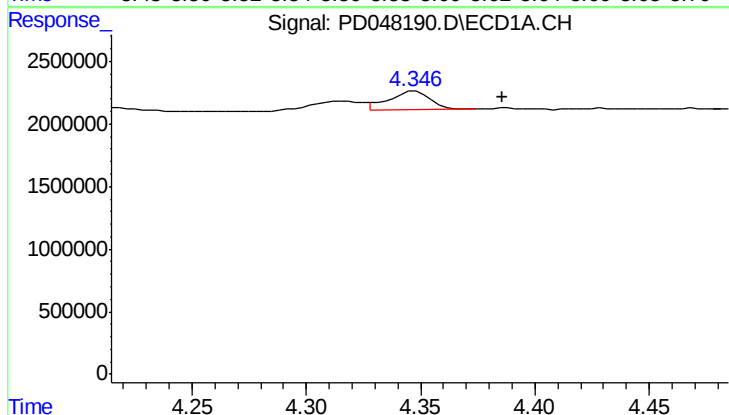


#6 beta-BHC

R.T.: 4.348 min
Delta R.T.: -0.038 min
Response: 1848249
Conc: 2.55 ng/ml

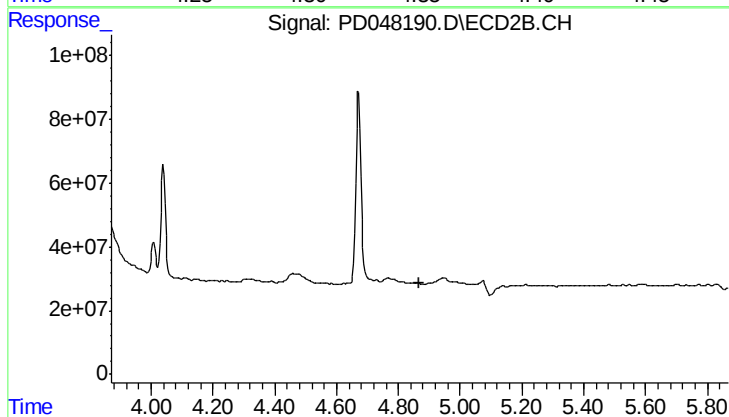

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.868 min
Response: 0
Conc: N.D.

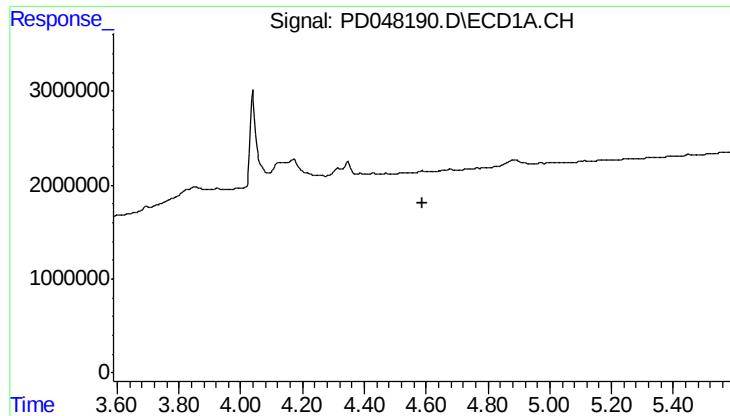

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.587 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

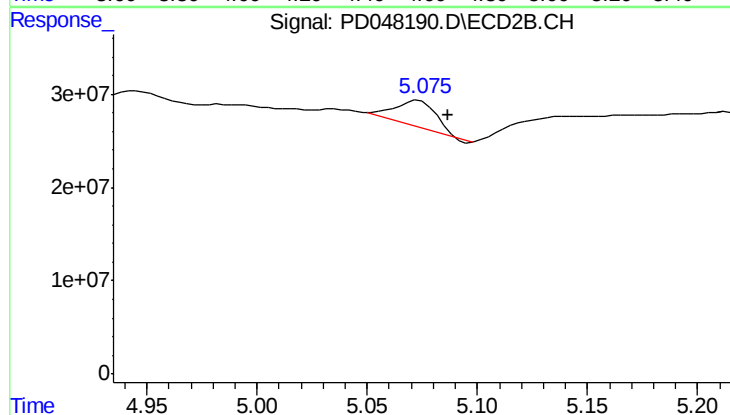


#7 delta-BHC

R.T.: 5.073 min
Delta R.T.: -0.014 min
Response: 37060809
Conc: 2.18 ng/ml

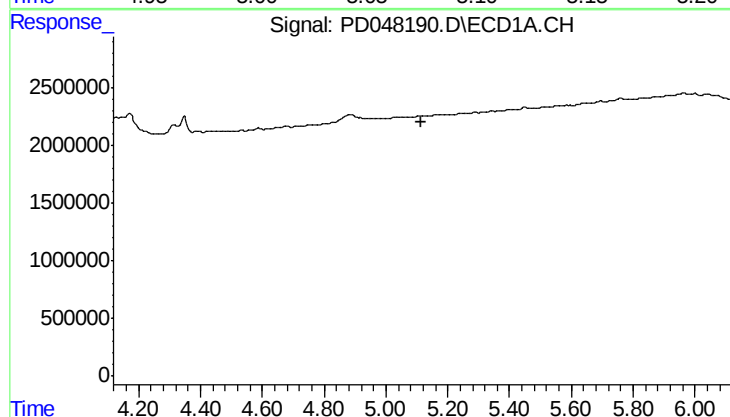


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.115 min
Response: 0
Conc: N.D.

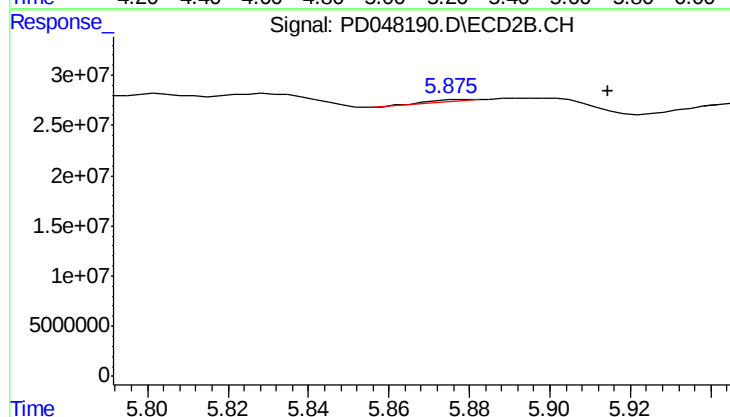

#8 Heptachlor epoxide


R.T.: 5.878 min
Delta R.T.: -0.037 min
Response: 1103386
Conc: 0.06 ng/ml

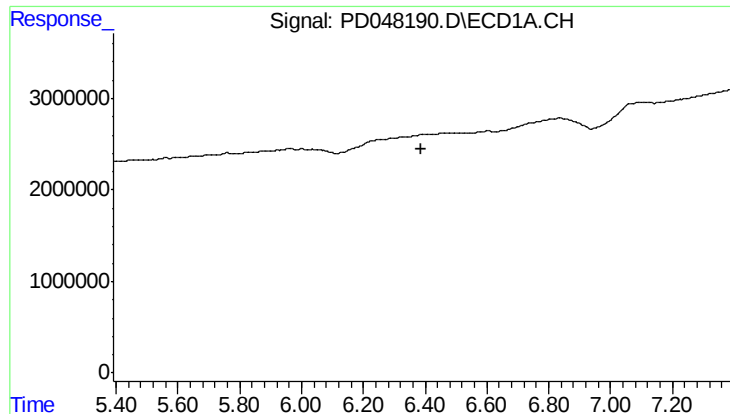

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.390 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

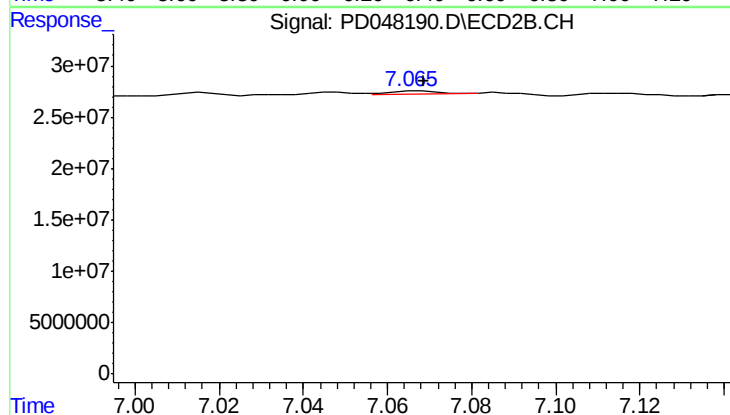


#18 Endrin aldehyde

R.T.: 7.067 min
Delta R.T.: -0.001 min
Response: 2468736
Conc: 0.15 ng/ml

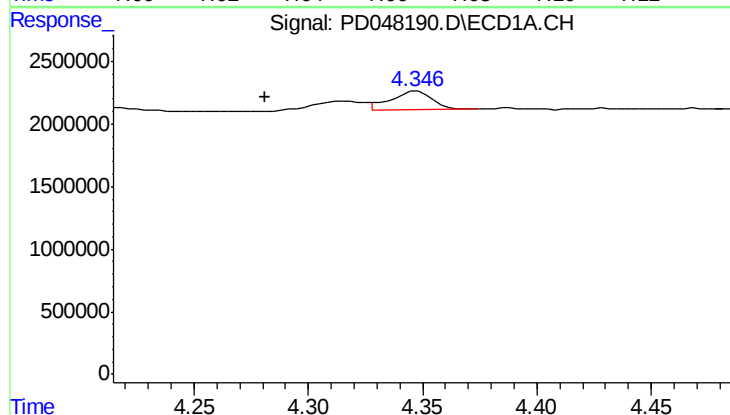


#23 Chlordane-1

R.T.: 4.348 min
Delta R.T.: 0.066 min
Response: 1848249
Conc: 34.05 ng/ml

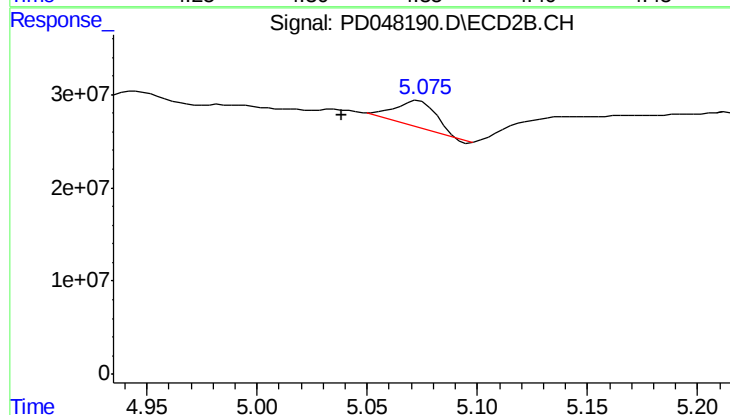

#23 Chlordane-1


R.T.: 5.073 min
Delta R.T.: 0.035 min
Response: 37060809
Conc: 36.22 ng/ml

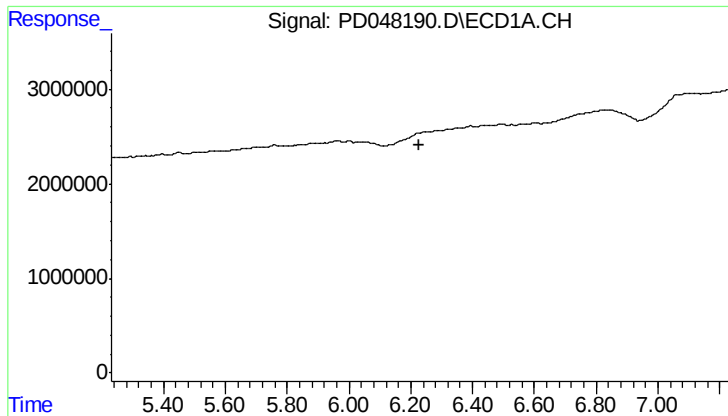

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.229 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

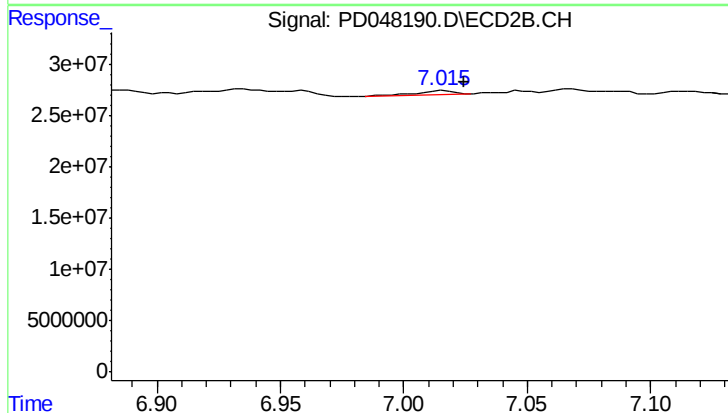


#27 Chlordane-5

R.T.: 7.016 min
Delta R.T.: -0.008 min
Response: 3408645
Conc: 3.93 ng/ml

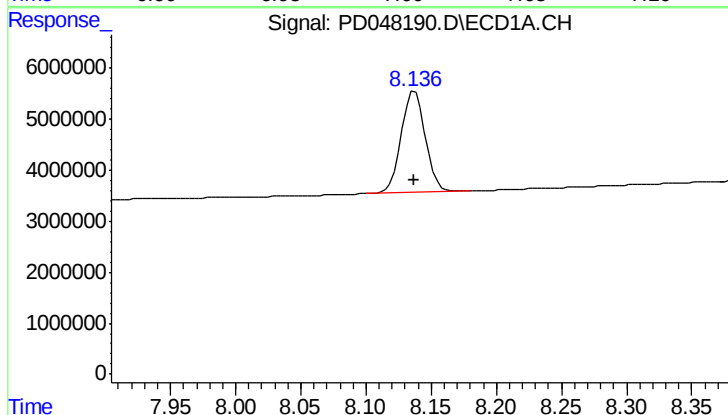

#28 Decachlorobiphenyl

R.T.: 8.138 min
Delta R.T.: 0.000 min
Response: 25628147
Conc: 19.80 ng/ml

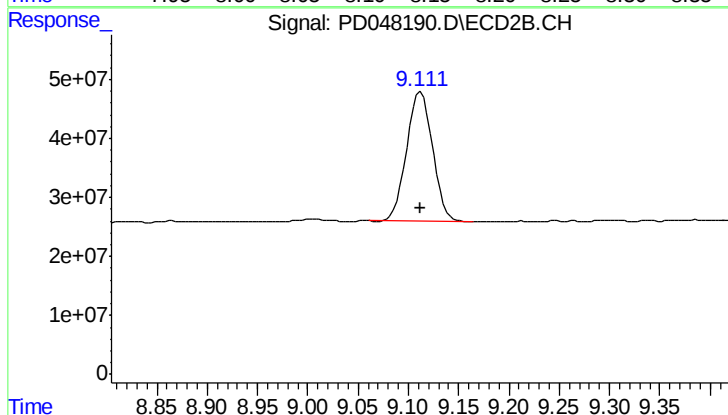

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 394972965
Conc: 21.27 ng/ml