

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062018\
 Data File : PD048195.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2018 17:56
 Operator : UA/AJ
 Sample : PB110427TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB110427TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 02:15:53 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 01:43:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.422	4.040	23274790	375.6E6	19.101	19.400
28) SA Decachlor...	8.138	9.112	22799526	350.0E6	17.617	18.842
Target Compounds						
3) MA gamma-BHC...	0.000	4.724	0	3857507	N.D.	0.140 #
6) B beta-BHC	0.000	4.845	0	10196317	N.D.	0.837 #
14) MA Endrin	0.000	6.766	0	5039659	N.D.	0.248 #
15) B Endosulfa...	0.000	6.939	0	4299262	N.D.	0.209 #
18) B Endrin al...	0.000	7.075	0	9048550	N.D.	0.535 #
20) A Methoxychlor	6.801f	0.000	2055847	0	2.766	N.D. #
23) Chlordane-1	0.000	4.979	0	12247653	N.D.	11.971 #
27) Chlordane-5	0.000	7.036	0	4614754	N.D.	5.322 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062018\
Data File : PD048195.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 17:56
Operator : UA/AJ
Sample : PB110427TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB110427TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 02:15:53 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 01:43:00 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

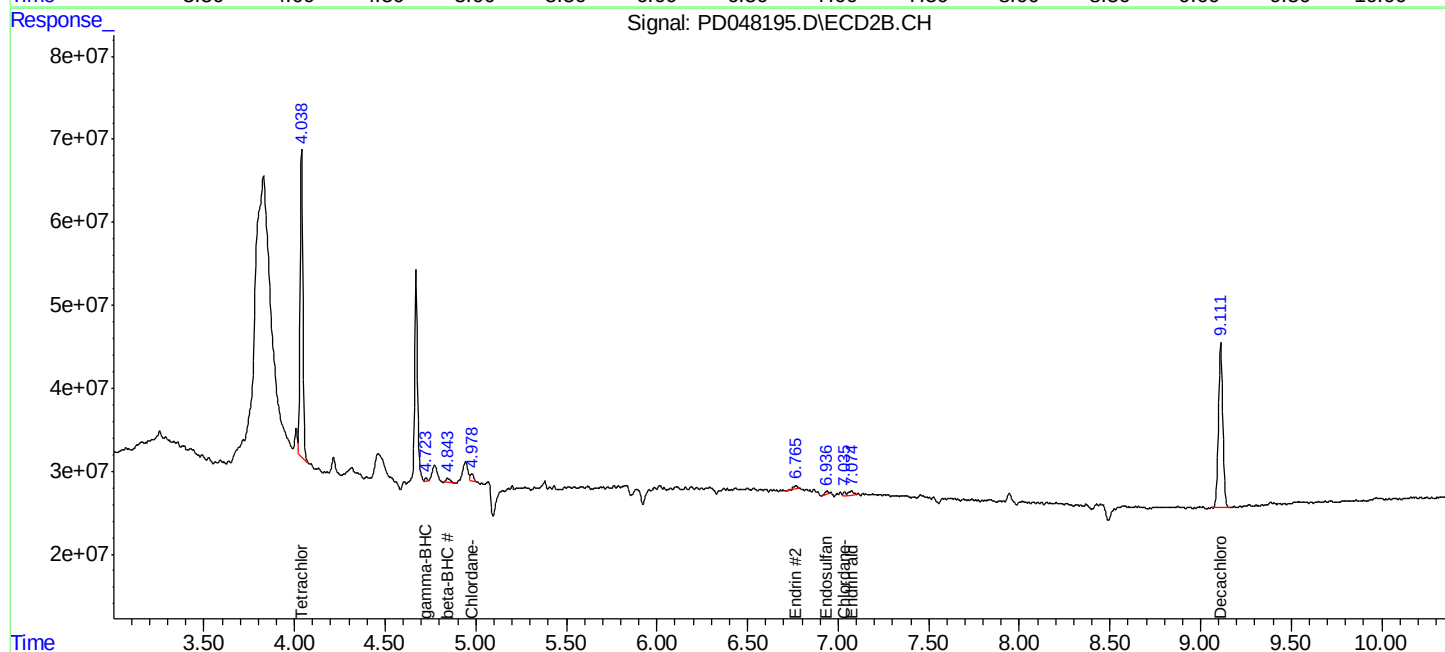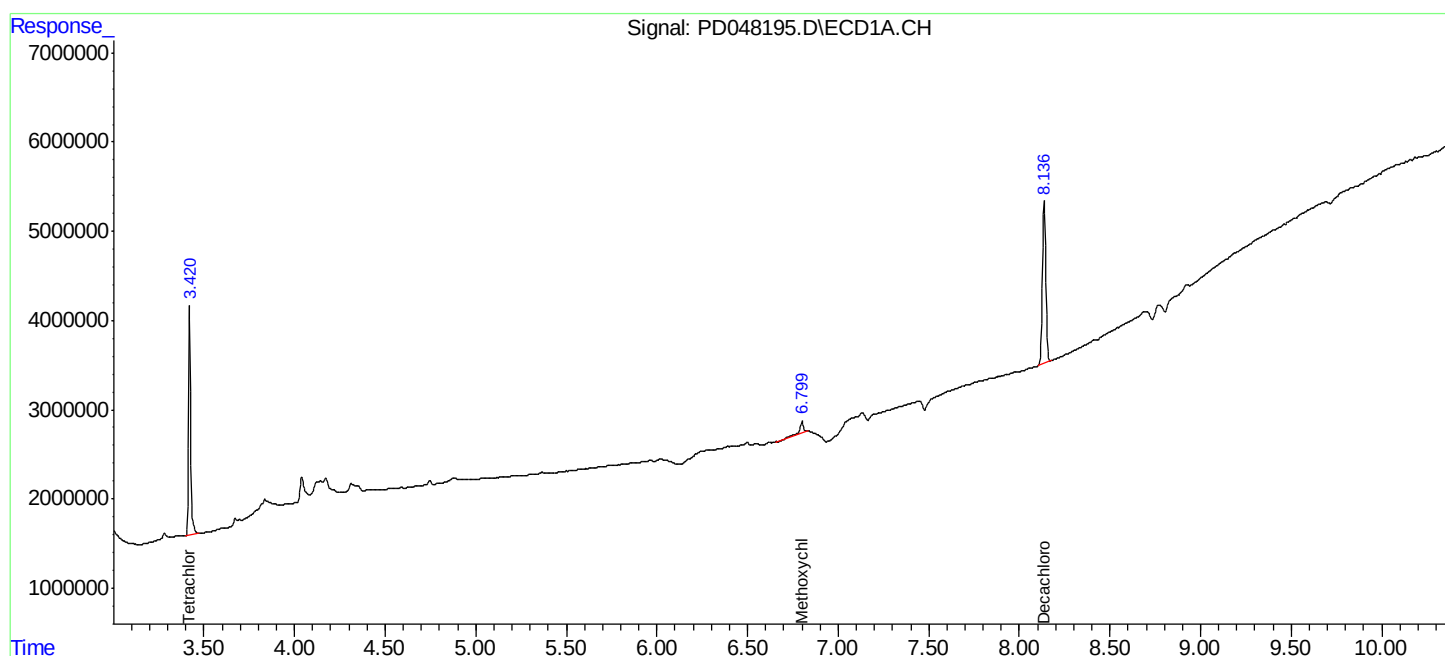


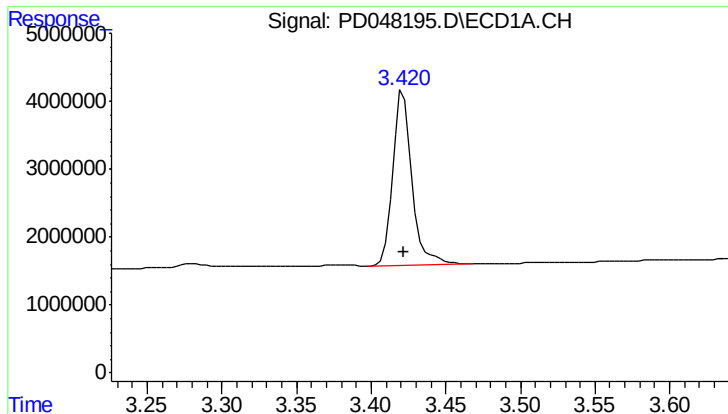

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 23274790
Conc: 19.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB110427TB

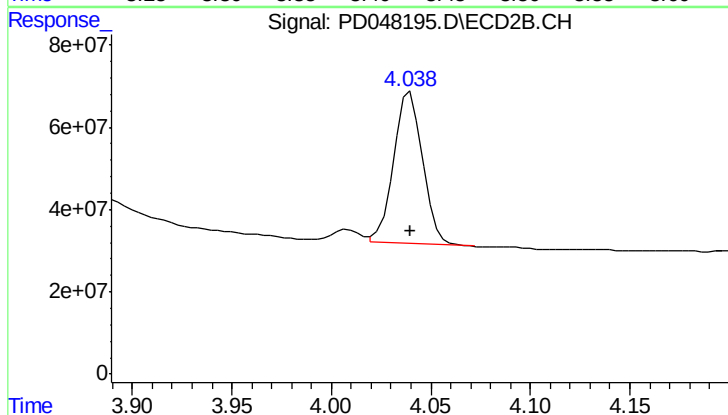


#1 Tetrachloro-m-xylene

R.T.: 4.040 min
Delta R.T.: 0.000 min
Response: 375641021
Conc: 19.40 ng/ml

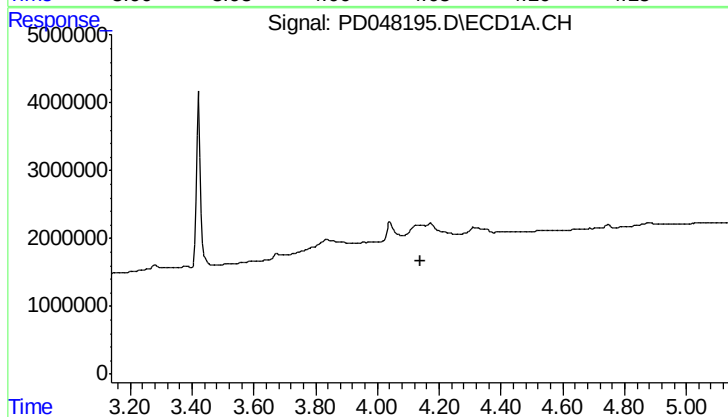


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 4.139 min
Response: 0
Conc: N.D.

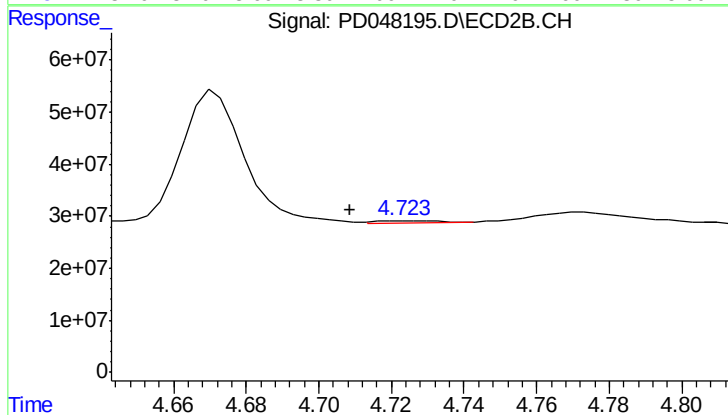

#3 gamma-BHC (Lindane)


R.T.: 4.724 min
Delta R.T.: 0.016 min
Response: 3857507
Conc: 0.14 ng/ml

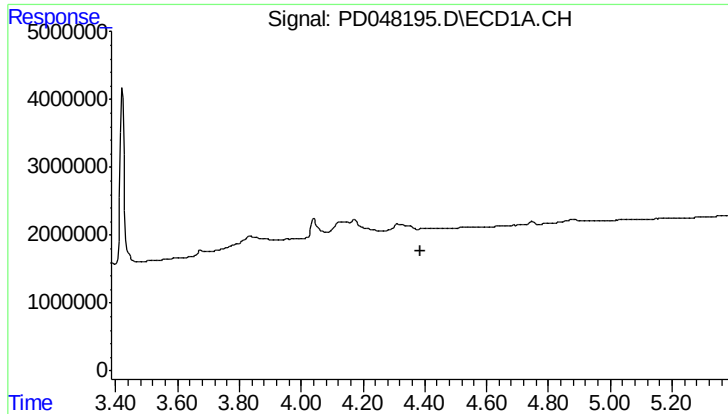

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.386 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB110427TB

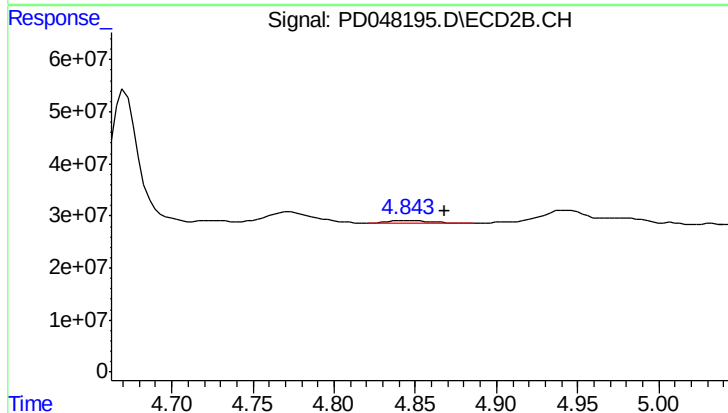


#6 beta-BHC

R.T.: 4.845 min
Delta R.T.: -0.023 min
Response: 10196317
Conc: 0.84 ng/ml

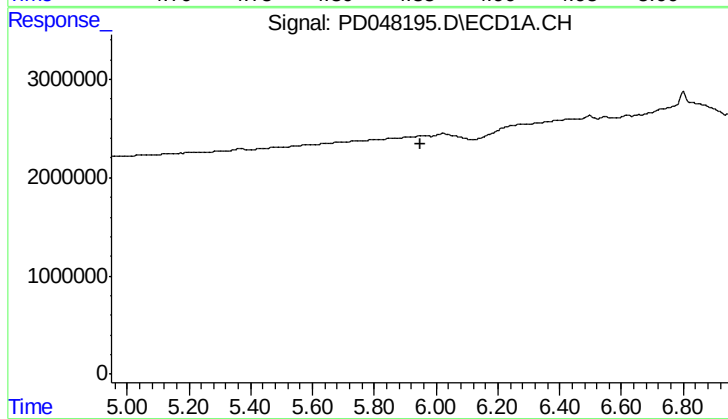


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.948 min
Response: 0
Conc: N.D.

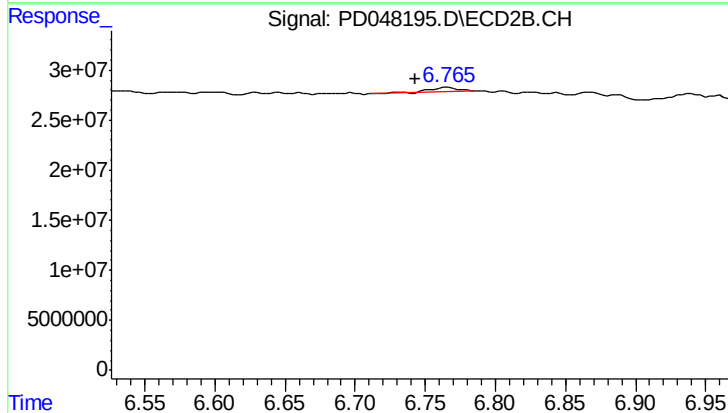

#14 Endrin


R.T.: 6.766 min
Delta R.T.: 0.023 min
Response: 5039659
Conc: 0.25 ng/ml

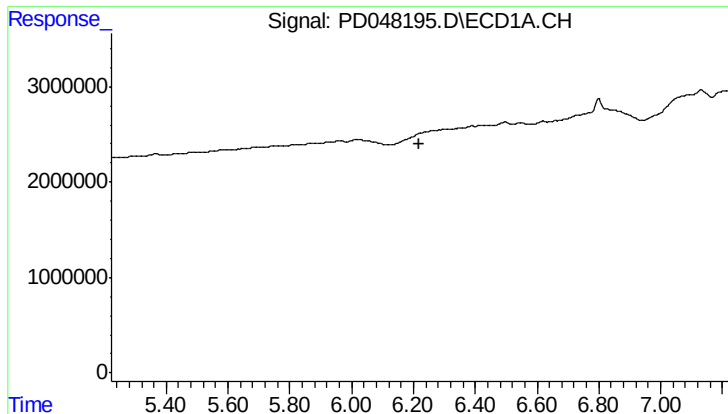

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB110427TB

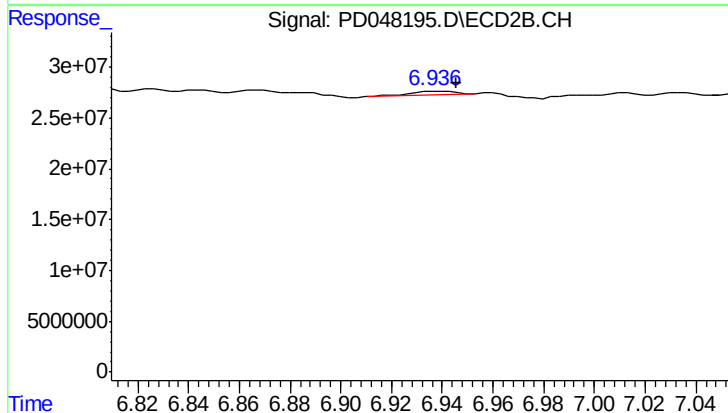


#15 Endosulfan II

R.T.: 6.939 min
Delta R.T.: -0.007 min
Response: 4299262
Conc: 0.21 ng/ml

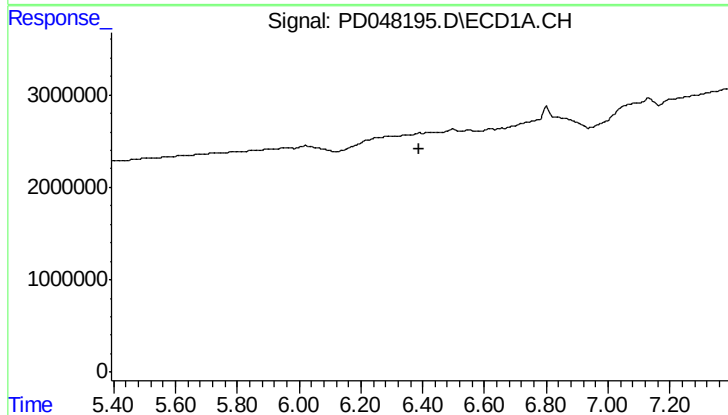


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.390 min
Response: 0
Conc: N.D.

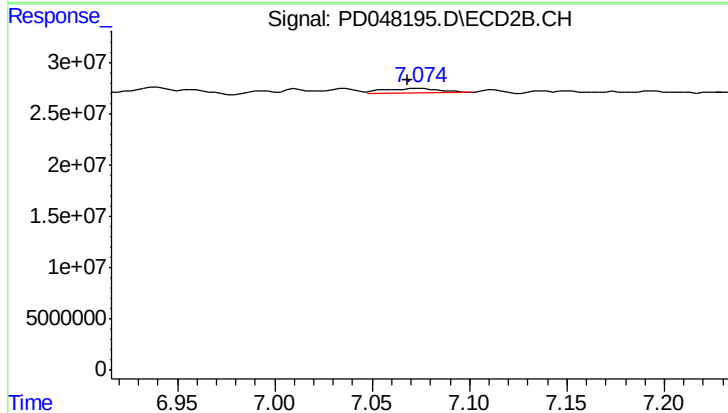

#18 Endrin aldehyde


R.T.: 7.075 min
Delta R.T.: 0.006 min
Response: 9048550
Conc: 0.54 ng/ml

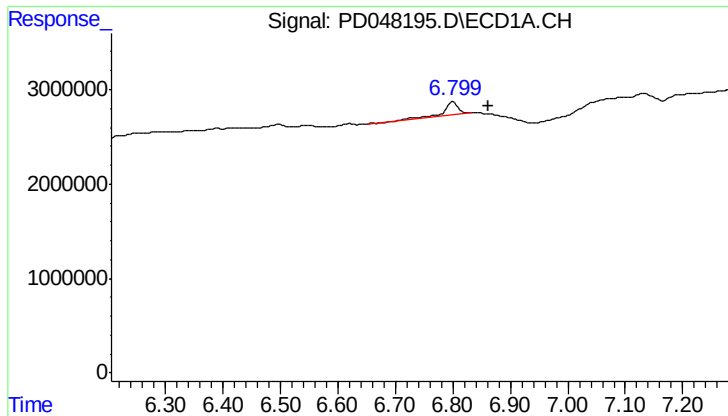

#20 Methoxychlor


R.T.: 6.801 min
Delta R.T.: -0.062 min
Response: 2055847
Conc: 2.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB110427TB

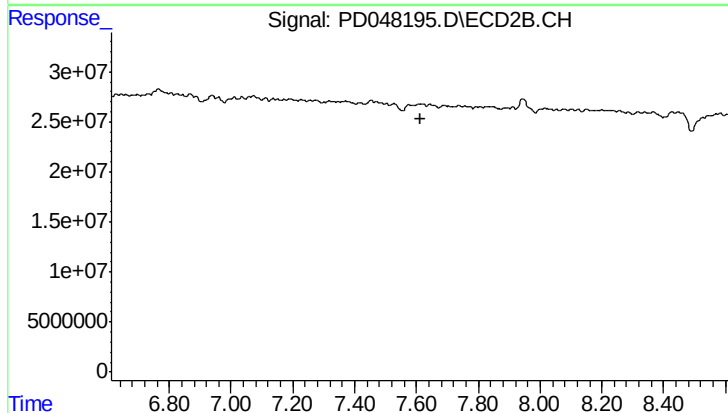


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.612 min
Response: 0
Conc: N.D.

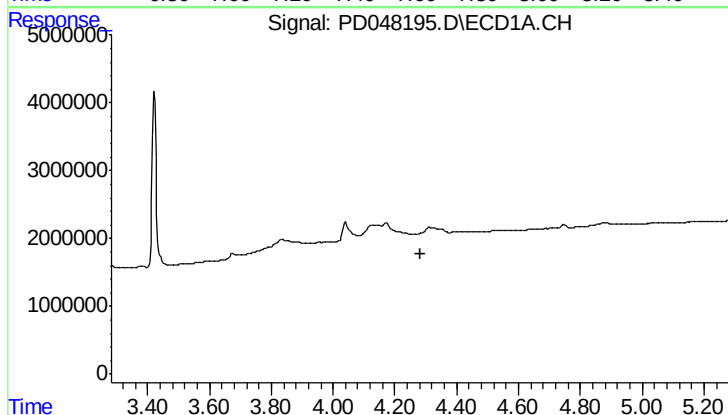


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.281 min
Response: 0
Conc: N.D.

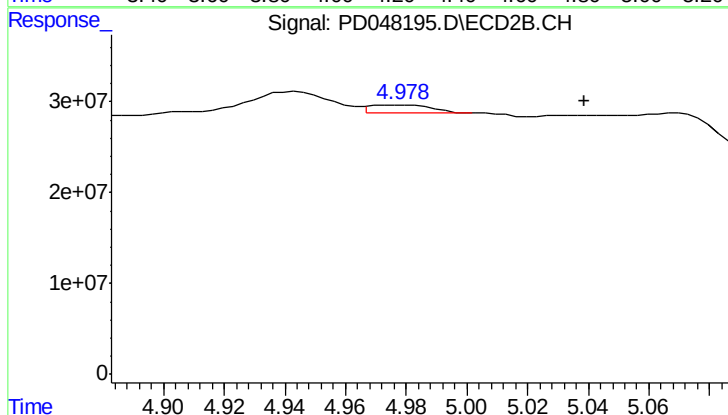

#23 Chlordane-1


R.T.: 4.979 min
Delta R.T.: -0.060 min
Response: 12247653
Conc: 11.97 ng/ml

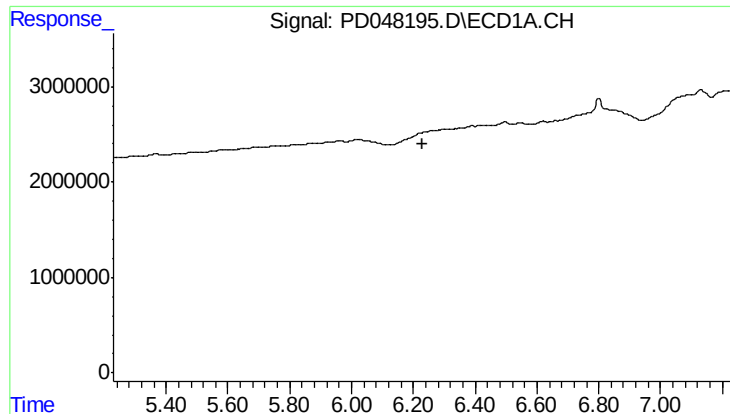

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.229 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PB110427TB

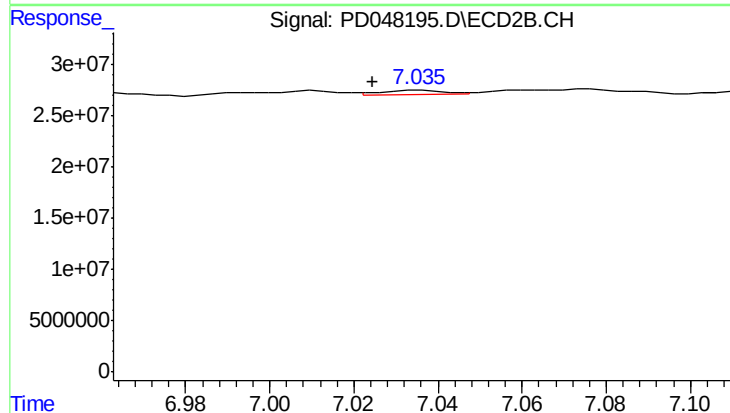


#27 Chlordane-5

R.T.: 7.036 min
Delta R.T.: 0.011 min
Response: 4614754
Conc: 5.32 ng/ml

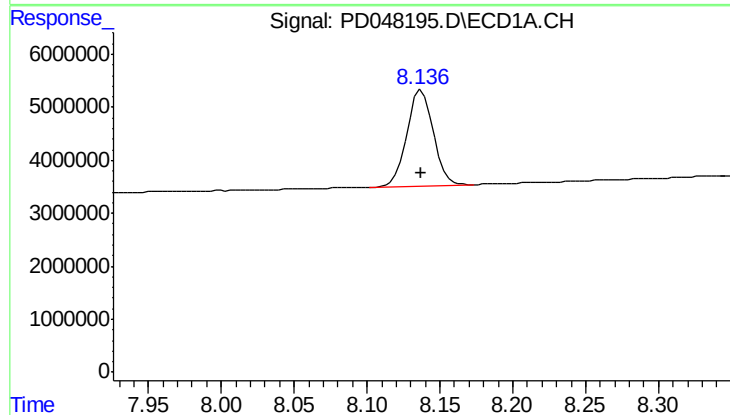

#28 Decachlorobiphenyl

R.T.: 8.138 min
Delta R.T.: 0.000 min
Response: 22799526
Conc: 17.62 ng/ml

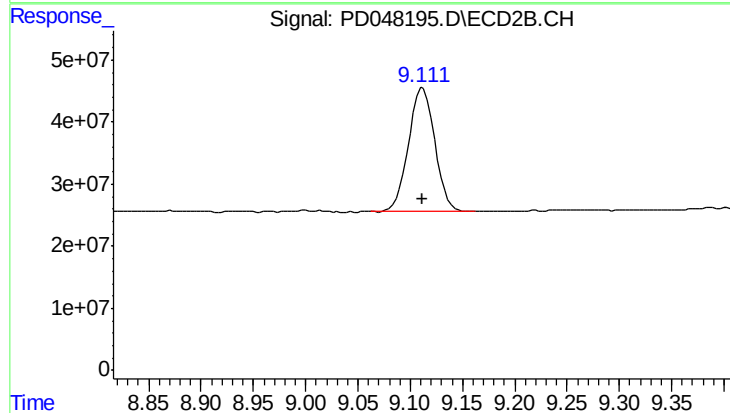

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 349965765
Conc: 18.84 ng/ml