

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062018\
 Data File : PD048200.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2018 19:04
 Operator : UA/AJ
 Sample : J3247-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OR-01-061918

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 02:17:00 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 01:43:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.040	25072464	404.2E6	20.576	20.877
28)	SA Decachlor...	8.137	9.111	23982688	355.9E6	18.532	19.161
Target Compounds							
3)	MA gamma-BHC...	0.000	4.733	0	3466153	N.D.	0.126 #
6)	B beta-BHC	4.348f	0.000	3153993	0	4.356	N.D. #
7)	B delta-BHC	0.000	5.072	0	44683141	N.D.	2.628 #
8)	B Heptachlo...	0.000	5.875f	0	788069	N.D.	0.045 #
15)	B Endosulfa...	0.000	6.925	0	2119214	N.D.	0.103 #
16)	A 4,4'-DDD	0.000	6.925f	0	2119214	N.D.	0.113 #
20)	A Methoxychlor	6.802f	0.000	1535680	0	2.066	N.D. #
23)	Chlordane-1	4.348	5.072	3153993	44683141	58.113	43.673



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062018\
Data File : PD048200.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 19:04
Operator : UA/AJ
Sample : J3247-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
OR-01-061918

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 02:17:00 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 01:43:00 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

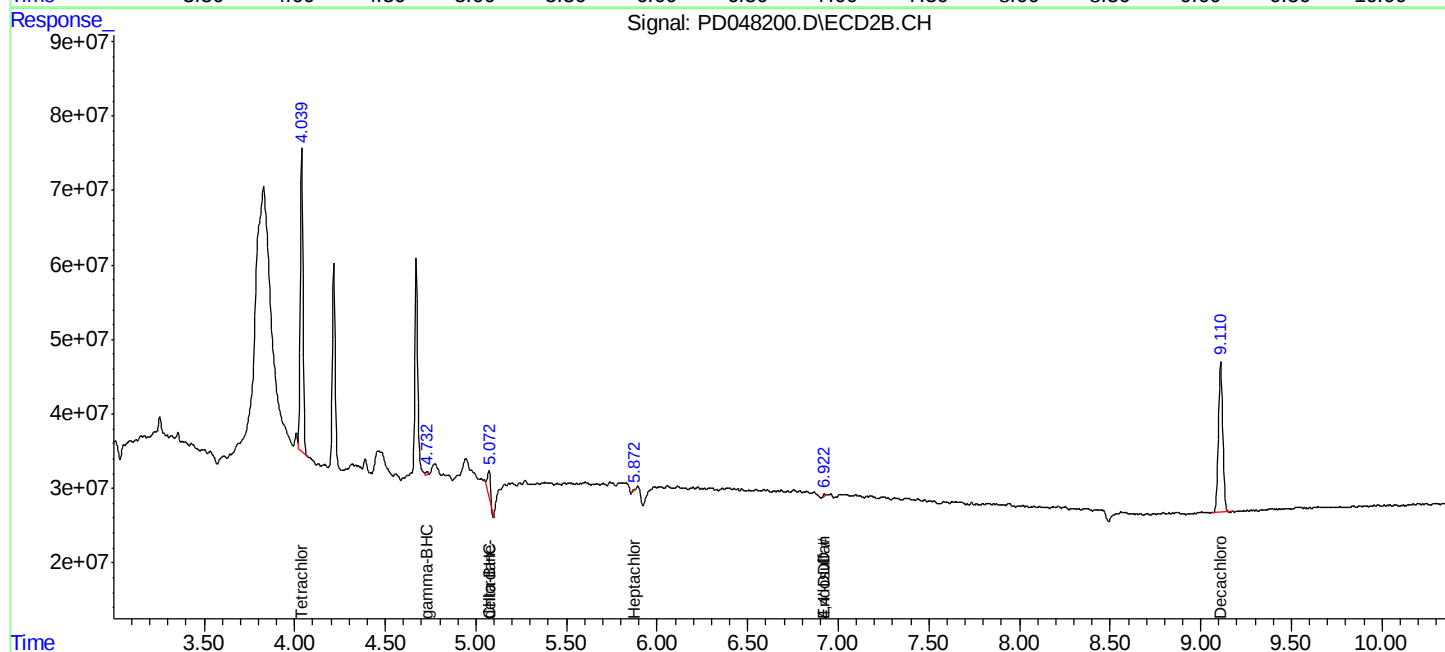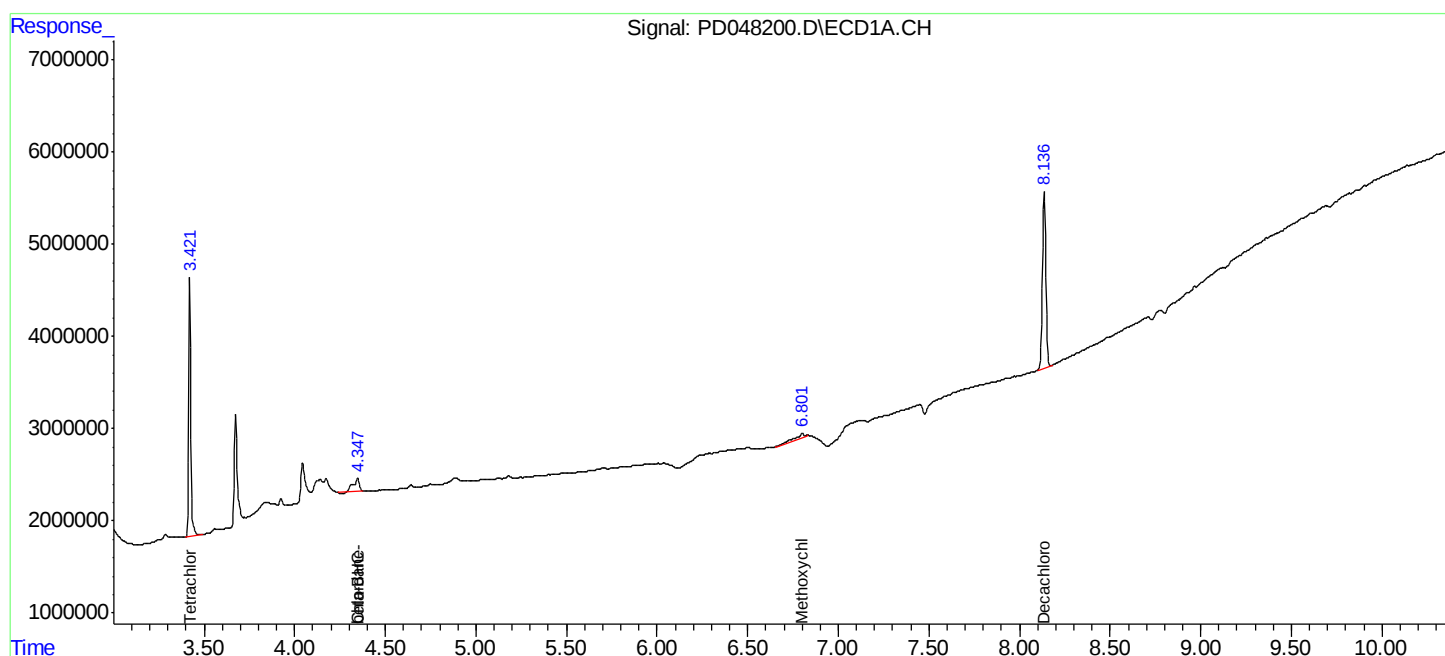


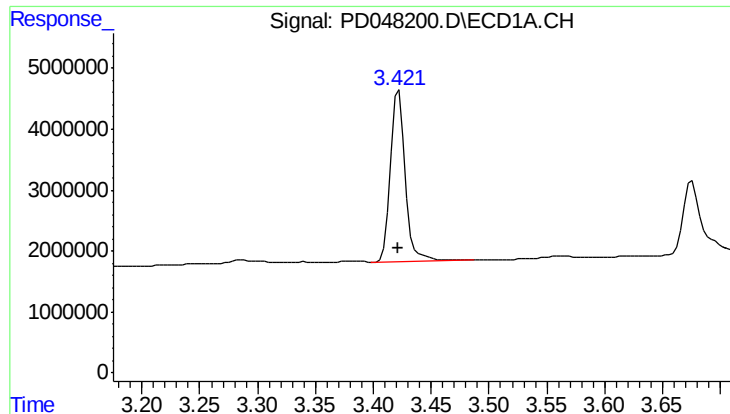

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 25072464
Conc: 20.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
OR-01-061918

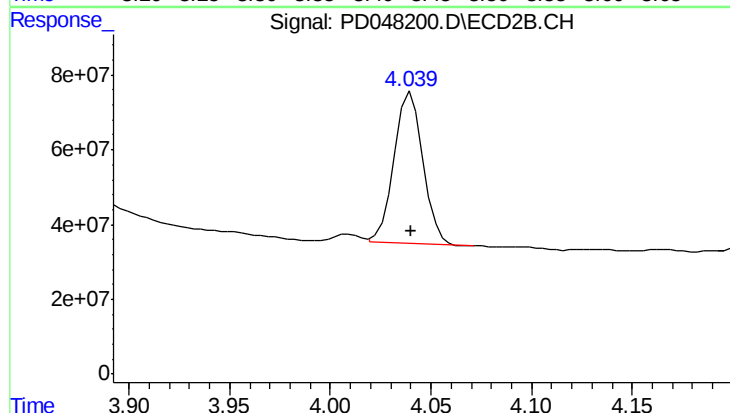


#1 Tetrachloro-m-xylene

R.T.: 4.040 min
Delta R.T.: 0.000 min
Response: 404237334
Conc: 20.88 ng/ml

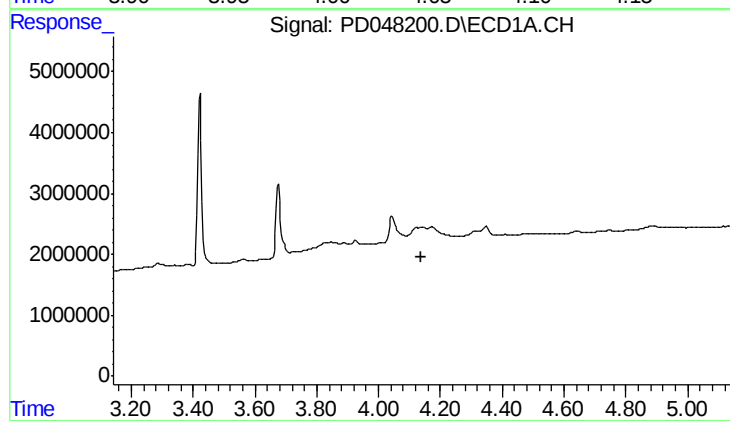


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T.: 4.139 min
Response: 0
Conc: N.D.

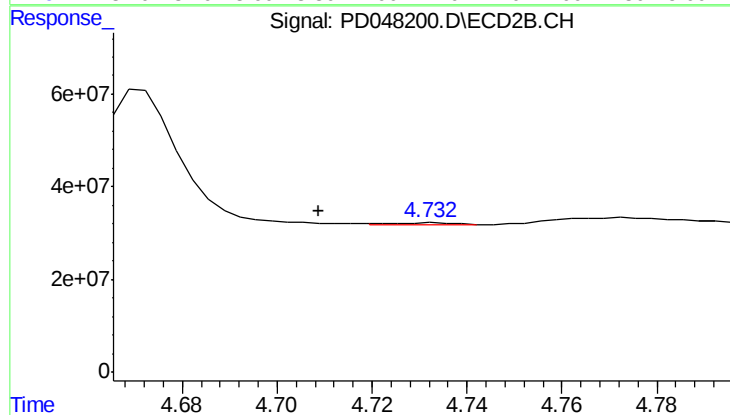

#3 gamma-BHC (Lindane)


R.T.: 4.733 min
Delta R.T.: 0.024 min
Response: 3466153
Conc: 0.13 ng/ml

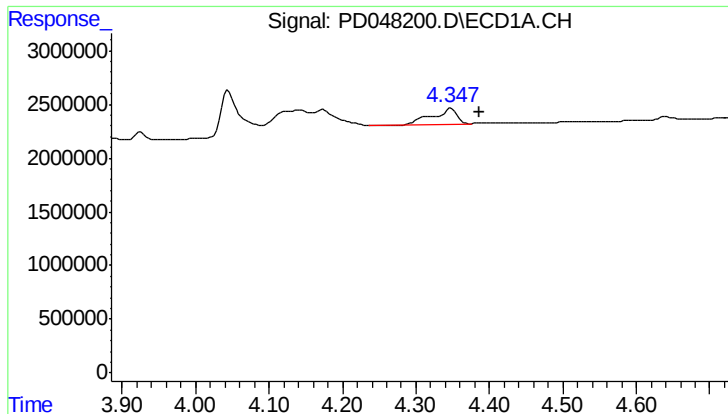

#6 beta-BHC


R.T.: 4.348 min
Delta R.T.: -0.038 min
Response: 3153993
Conc: 4.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
OR-01-061918

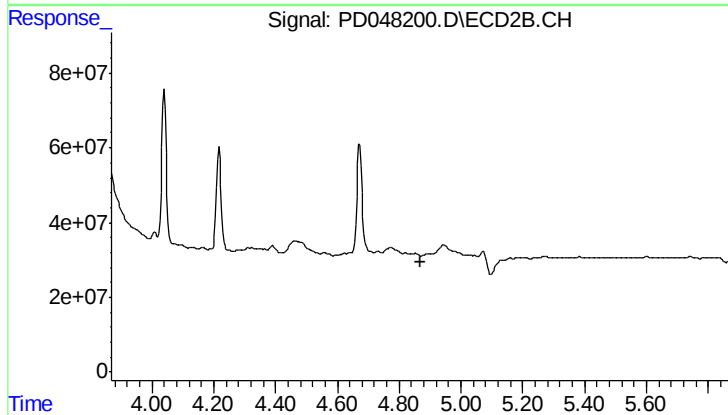


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.868 min
Response: 0
Conc: N.D.

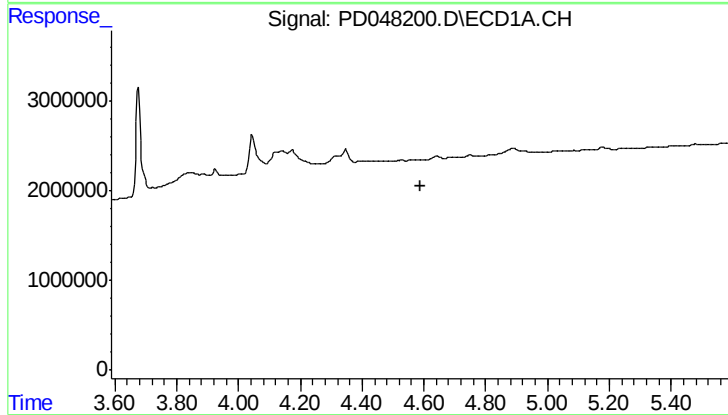


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.587 min
Response: 0
Conc: N.D.

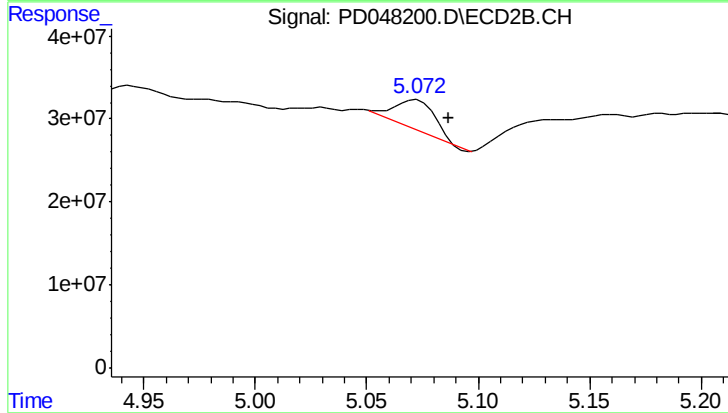

#7 delta-BHC


R.T.: 5.072 min
Delta R.T.: -0.015 min
Response: 44683141
Conc: 2.63 ng/ml

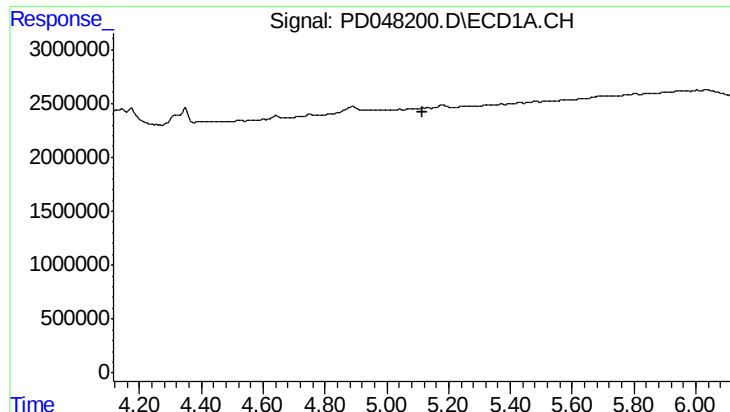

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.115 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
OR-01-061918

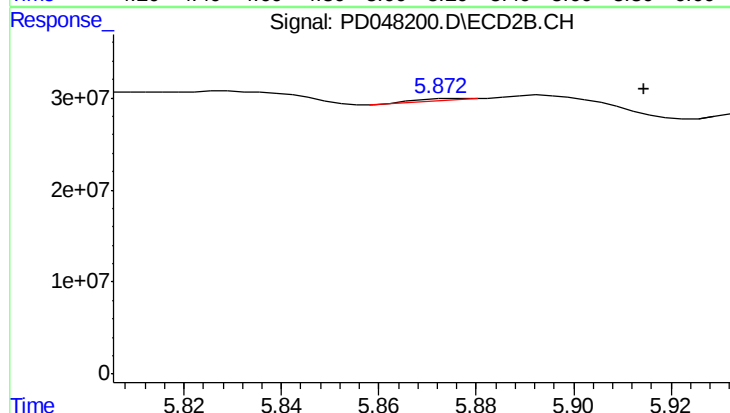


#8 Heptachlor epoxide

R.T.: 5.875 min
Delta R.T.: -0.039 min
Response: 788069
Conc: 0.04 ng/ml

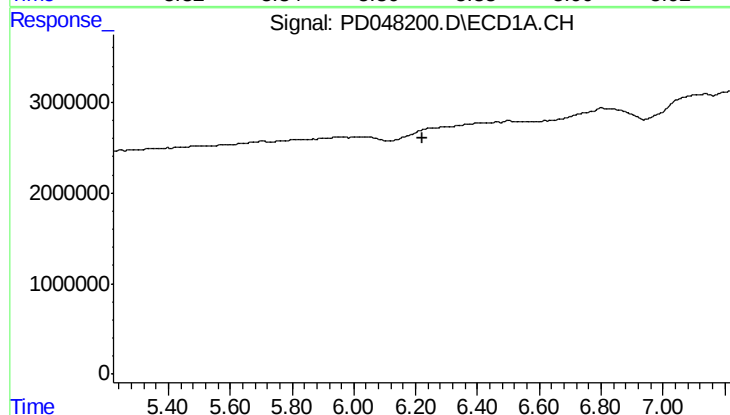


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.220 min
Response: 0
Conc: N.D.

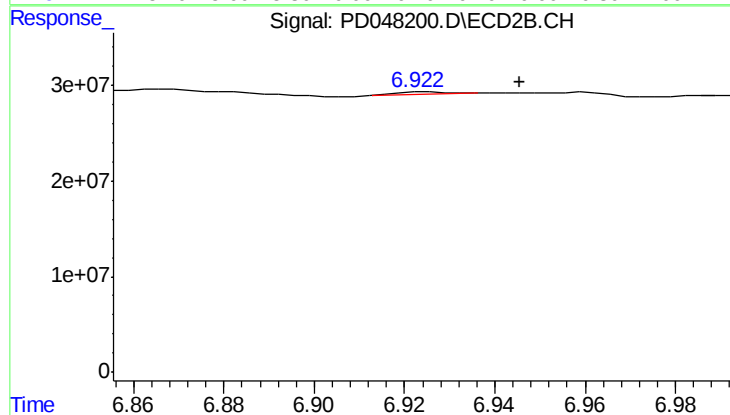

#15 Endosulfan II


R.T.: 6.925 min
Delta R.T.: -0.021 min
Response: 2119214
Conc: 0.10 ng/ml

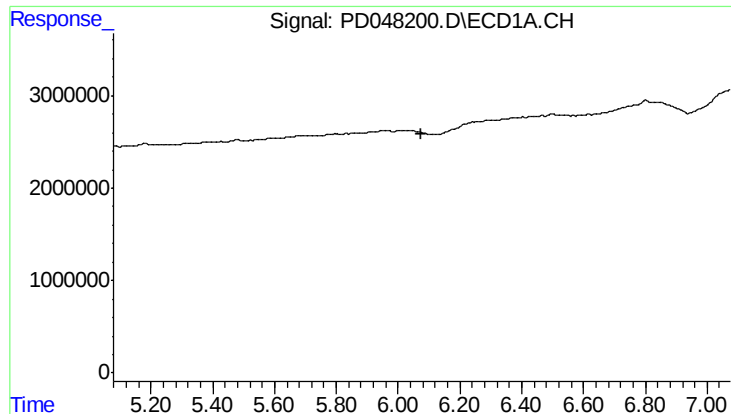

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
OR-01-061918

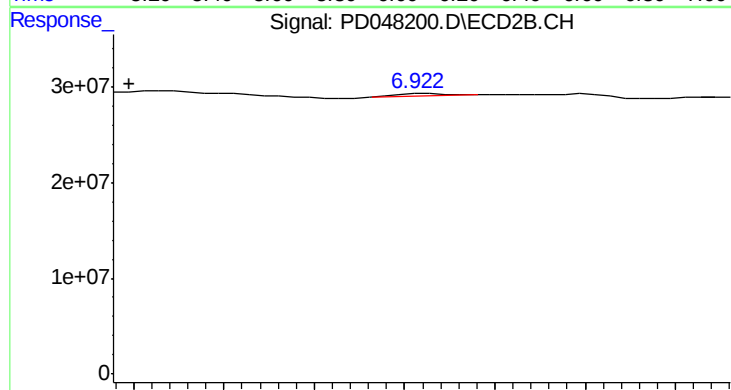


#16 4,4'-DDD

R.T.: 6.925 min
Delta R.T.: 0.066 min
Response: 2119214
Conc: 0.11 ng/ml

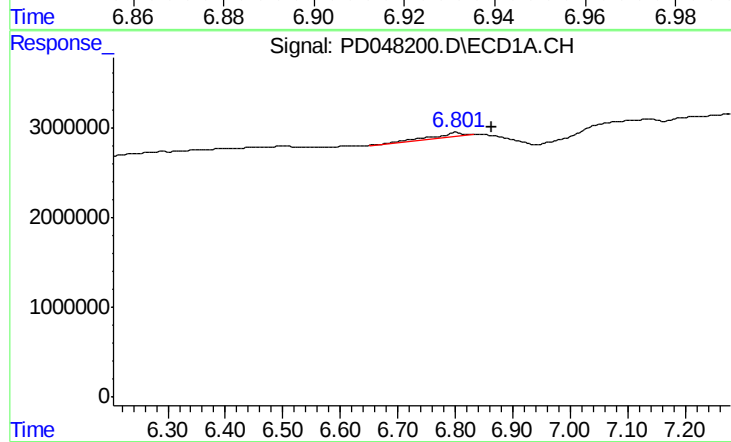


#20 Methoxychlor

R.T.: 6.802 min
Delta R.T.: -0.061 min
Response: 1535680
Conc: 2.07 ng/ml

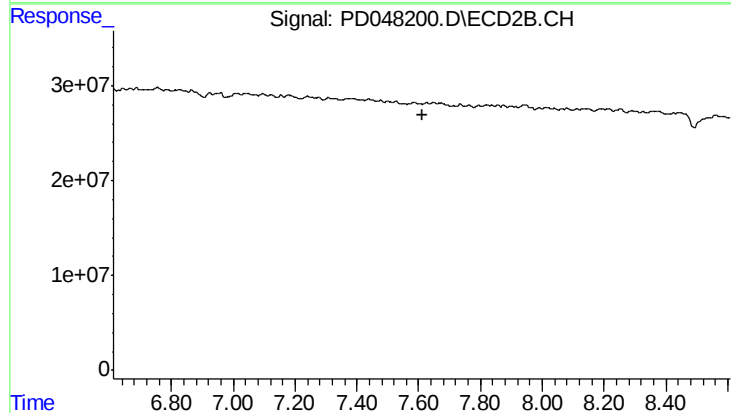

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.612 min
Response: 0
Conc: N.D.

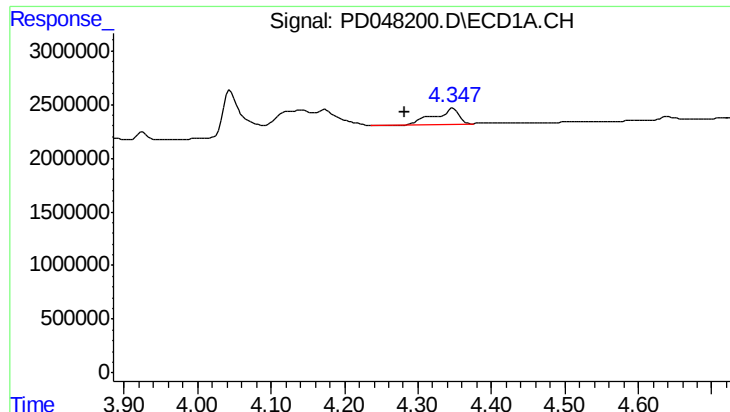

#23 Chlordane-1


R.T.: 4.348 min
Delta R.T.: 0.067 min
Response: 3153993
Conc: 58.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
OR-01-061918

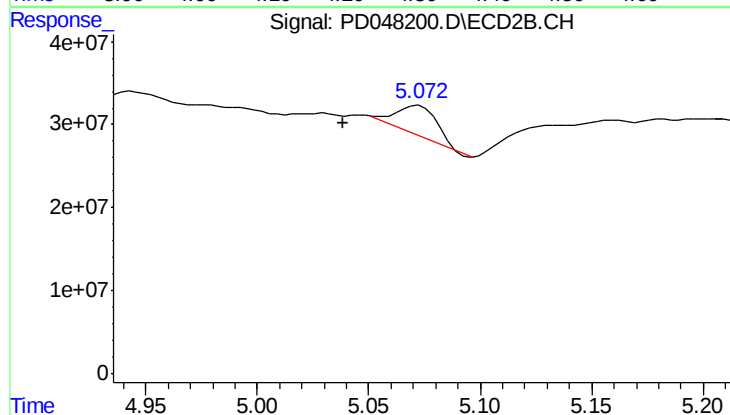


#23 Chlordane-1

R.T.: 5.072 min
Delta R.T.: 0.034 min
Response: 44683141
Conc: 43.67 ng/ml

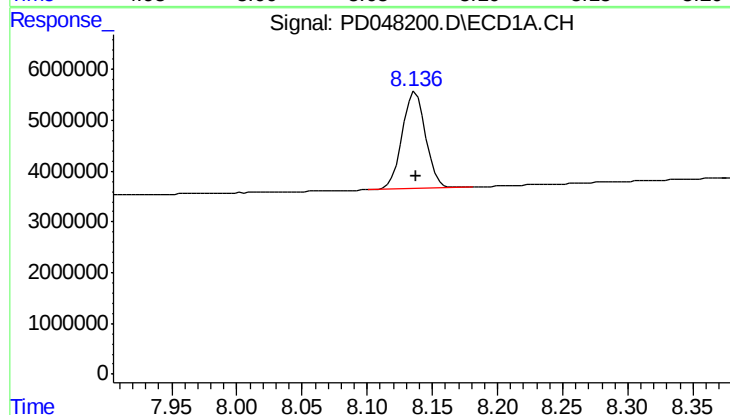

#28 Decachlorobiphenyl

R.T.: 8.137 min
Delta R.T.: 0.000 min
Response: 23982688
Conc: 18.53 ng/ml

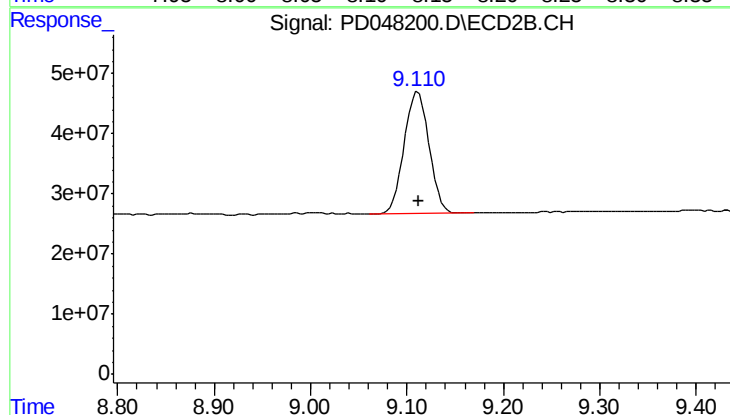

#28 Decachlorobiphenyl

R.T.: 9.111 min
Delta R.T.: 0.000 min
Response: 355887564
Conc: 19.16 ng/ml