

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062018\
 Data File : PD048181.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2018 14:46
 Operator : UA/AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 20 15:35:21 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD062018.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 20 15:33:51 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.040	133.0E6	1818.8E6	99.813	94.722
28)	SA Decachlor...	8.137	9.113	125.1E6	1662.0E6	96.855	90.246
Target Compounds							
23)	Chlordane-1	4.281	5.039	53811526	938.9E6	972.003	927.784
24)	Chlordane-2	4.777	5.505	54315201	898.7E6	952.915	901.787
25)	Chlordane-3	5.338	6.149	183.3E6	2998.7E6	1058.046	928.650
26)	Chlordane-4	5.396	6.226	157.0E6	3435.7E6	986.142	922.196
27)	Chlordane-5	6.228	7.025	53679510	786.4E6	969.336	912.619



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062018\
Data File : PD048181.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 14:46
Operator : UA/AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 20 15:35:21 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD062018.M
Quant Title : GC Extractables
QLast Update : Wed Jun 20 15:33:51 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

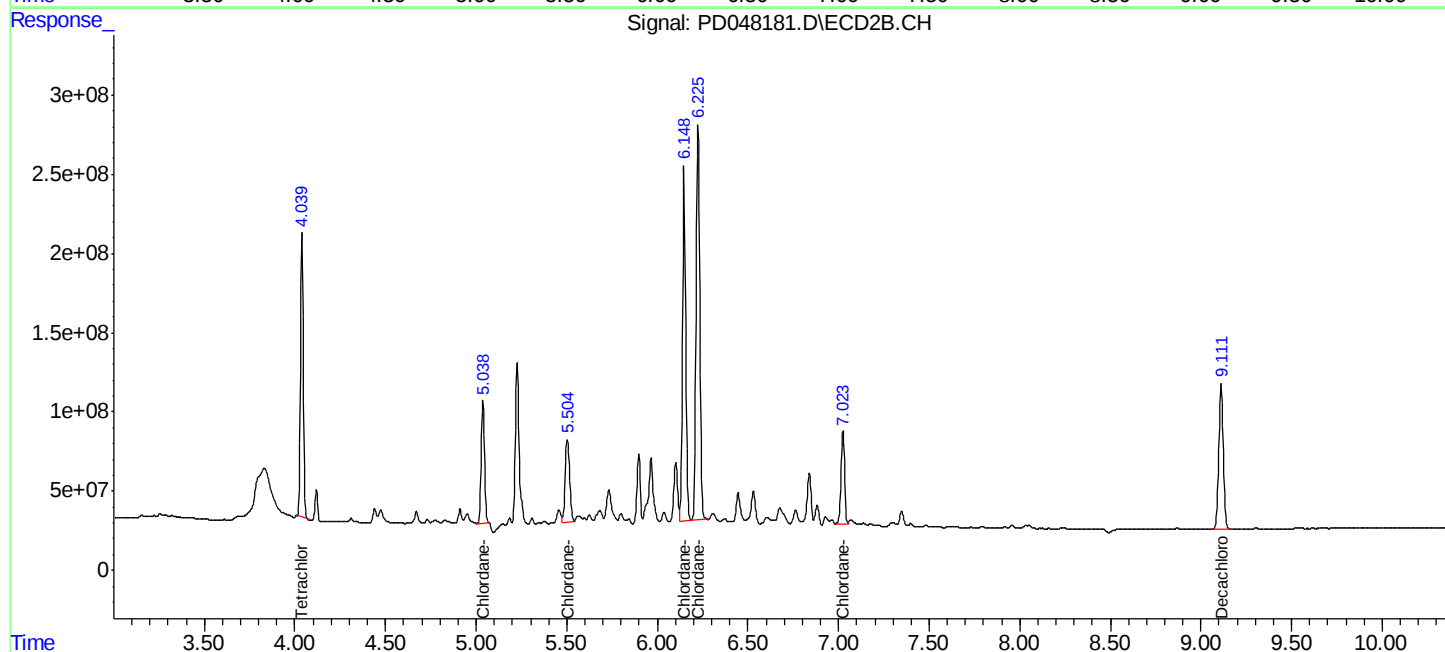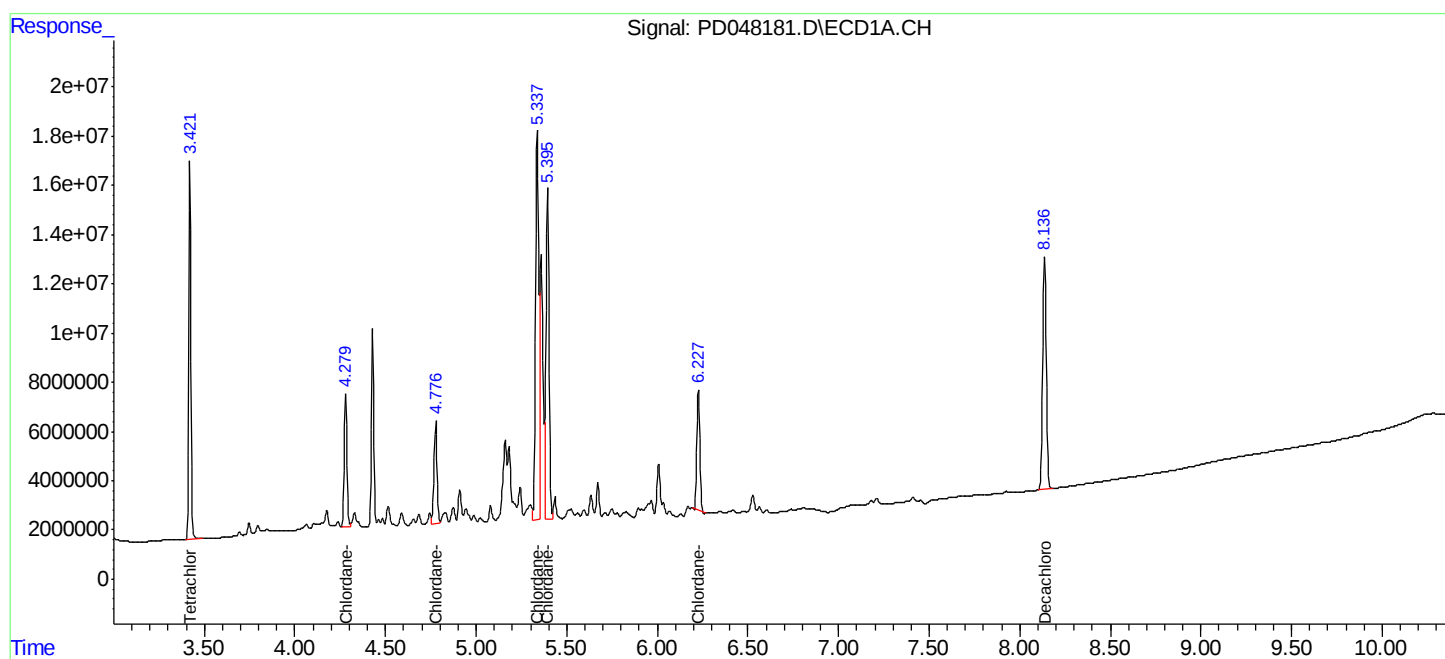


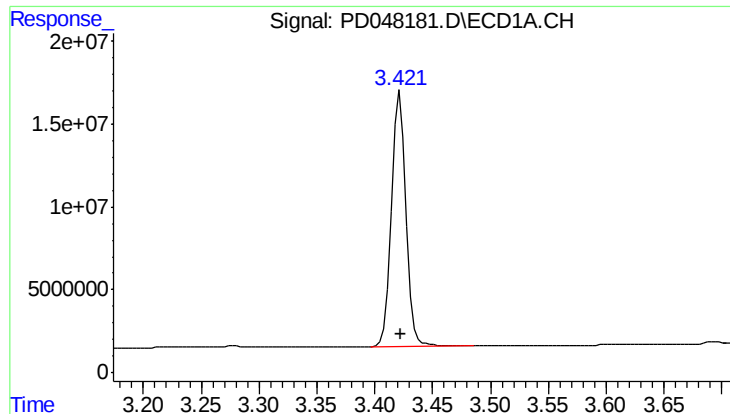

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 133049725
Conc: 99.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

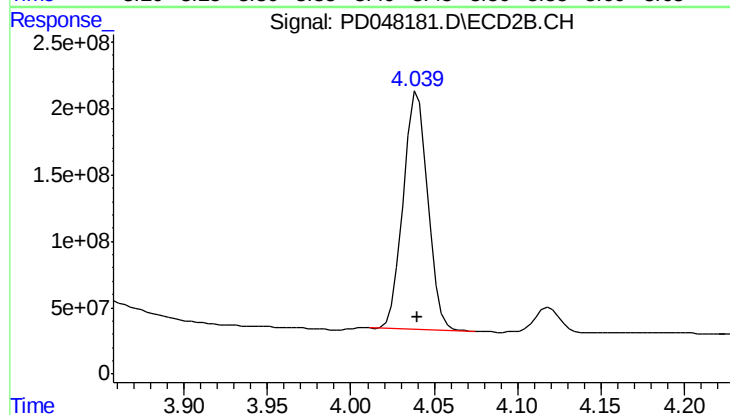


#1 Tetrachloro-m-xylene

R.T.: 4.040 min
Delta R.T.: 0.000 min
Response: 1818843246
Conc: 94.72 ng/ml

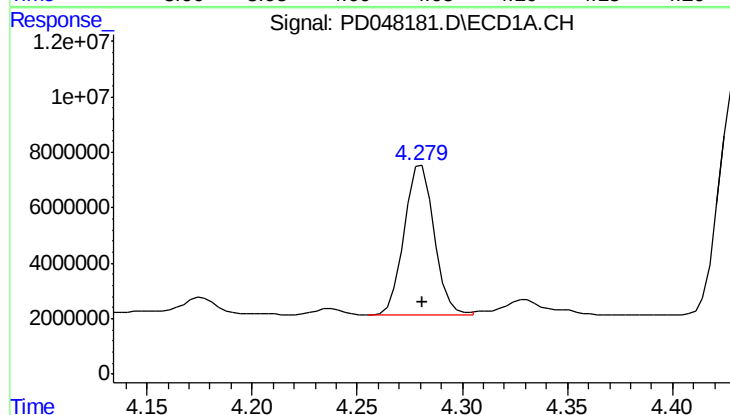


#23 Chlordane-1

R.T.: 4.281 min
Delta R.T.: 0.000 min
Response: 53811526
Conc: 972.00 ng/ml

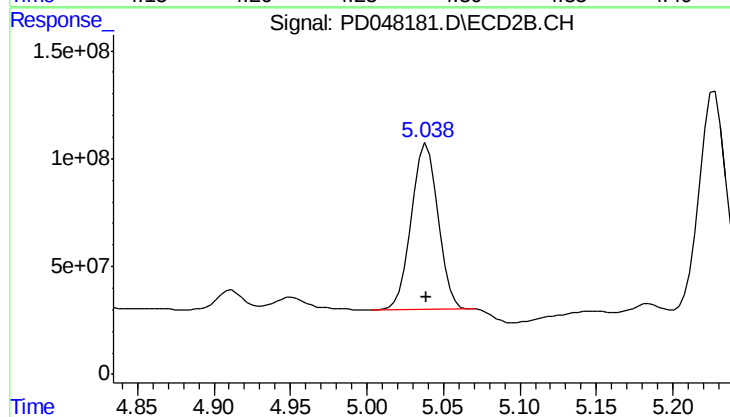

#23 Chlordane-1


R.T.: 5.039 min
Delta R.T.: 0.000 min
Response: 938921913
Conc: 927.78 ng/ml

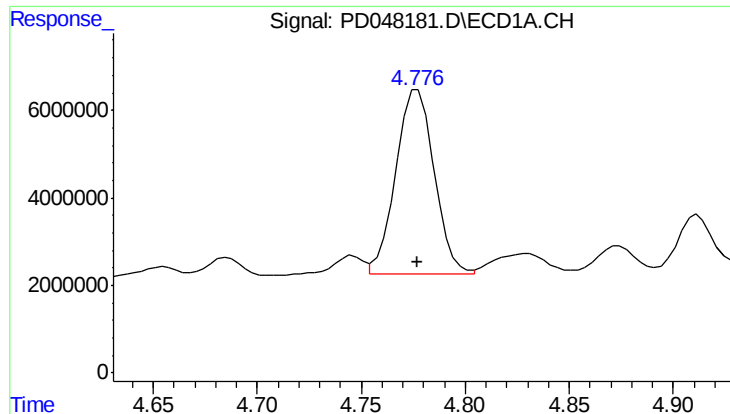

#24 Chlordane-2


R.T.: 4.777 min
Delta R.T.: 0.000 min
Response: 54315201
Conc: 952.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

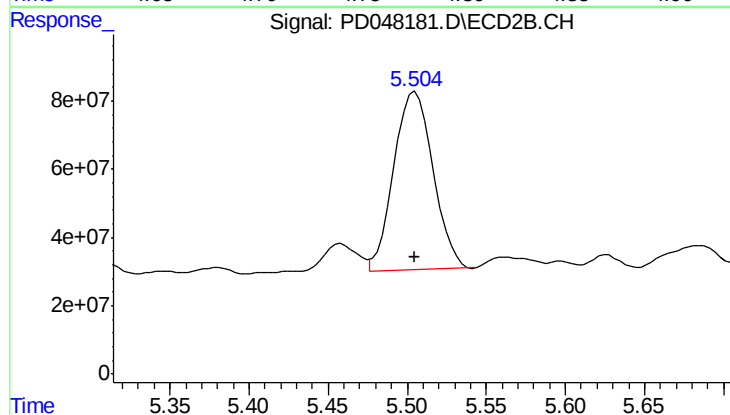


#24 Chlordane-2

R.T.: 5.505 min
Delta R.T.: 0.000 min
Response: 898664921
Conc: 901.79 ng/ml

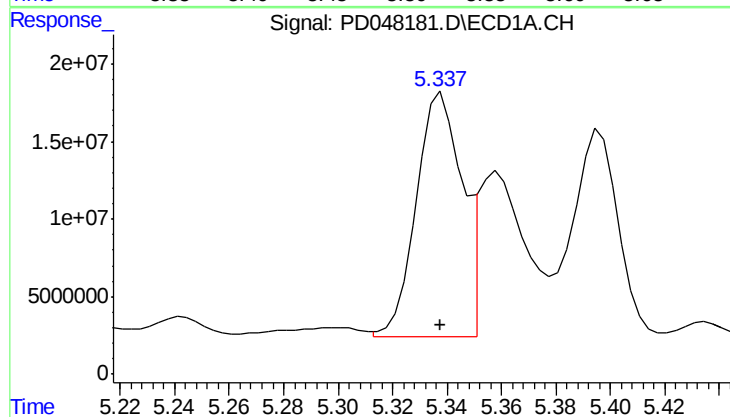


#25 Chlordane-3

R.T.: 5.338 min
Delta R.T.: 0.000 min
Response: 183267426
Conc: 1058.05 ng/ml

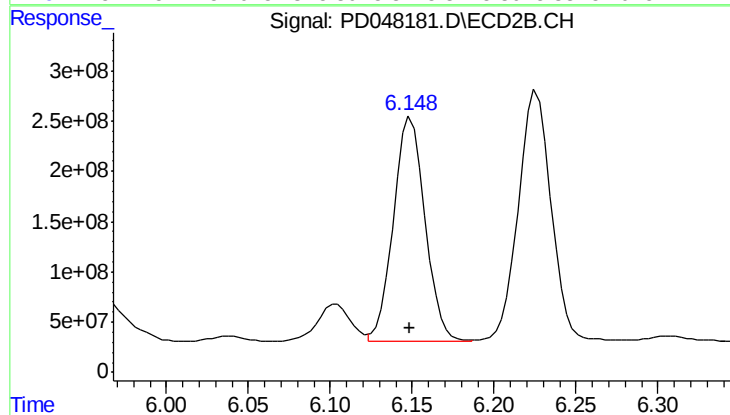

#25 Chlordane-3


R.T.: 6.149 min
Delta R.T.: 0.000 min
Response: 2998730916
Conc: 928.65 ng/ml

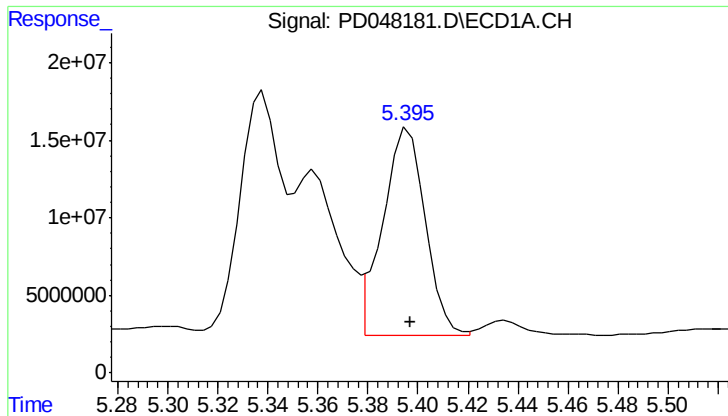

#26 Chlordane-4


R.T.: 5.396 min
Delta R.T.: 0.000 min
Response: 157038108
Conc: 986.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

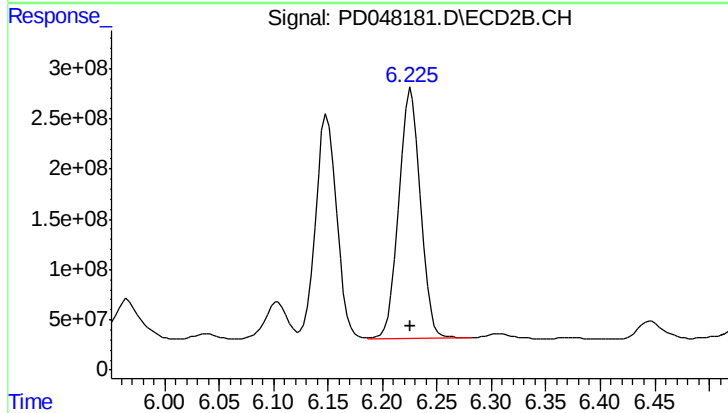


#26 Chlordane-4

R.T.: 6.226 min
Delta R.T.: 0.000 min
Response: 3435748873
Conc: 922.20 ng/ml

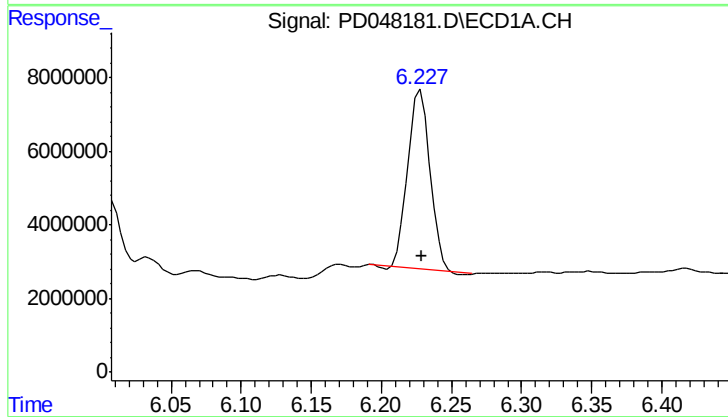


#27 Chlordane-5

R.T.: 6.228 min
Delta R.T.: 0.000 min
Response: 53679510
Conc: 969.34 ng/ml

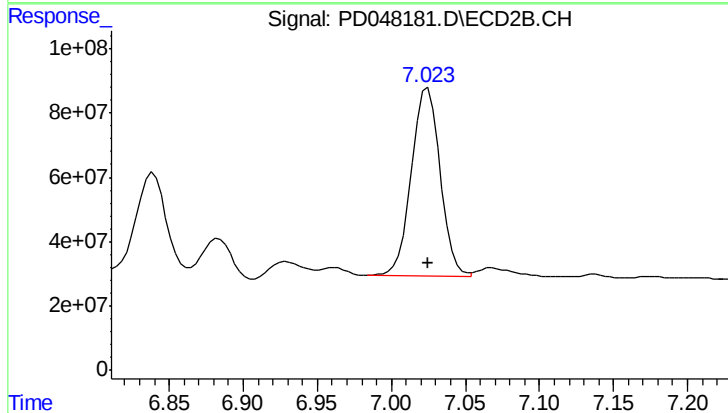

#27 Chlordane-5


R.T.: 7.025 min
Delta R.T.: 0.000 min
Response: 786439757
Conc: 912.62 ng/ml

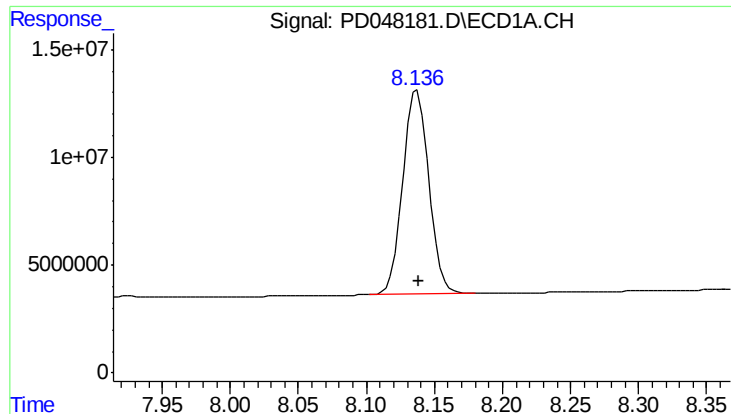

#28 Decachlorobiphenyl

R.T.: 8.137 min
Delta R.T.: 0.000 min
Response: 125131059
Conc: 96.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

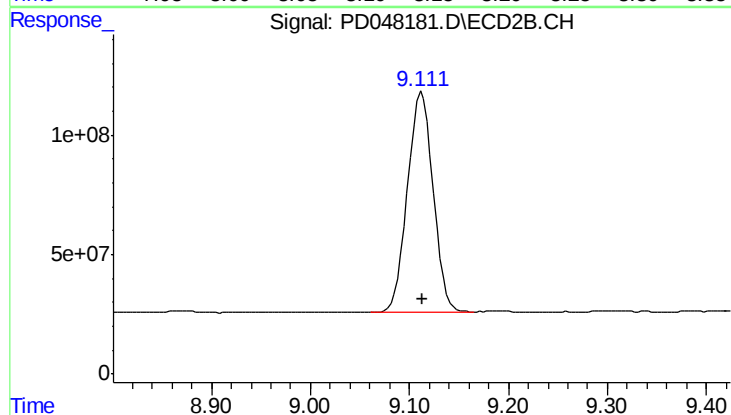

#28 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 1662035273
Conc: 90.25 ng/ml