

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062018\
Data File : PD048190.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 16:49
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

UGO
6/21/2018 4:43:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:10:26 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 01:43:00 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	4.040	23883333	350.8E6	19.601m	18.116
28)	SA Decachlor...	8.138	9.112	25628147	395.0E6	19.803	21.265

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062018\
Data File : PD048190.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 16:49
Operator : UA/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

UGO
6/21/2018 4:43:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:10:26 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 01:43:00 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

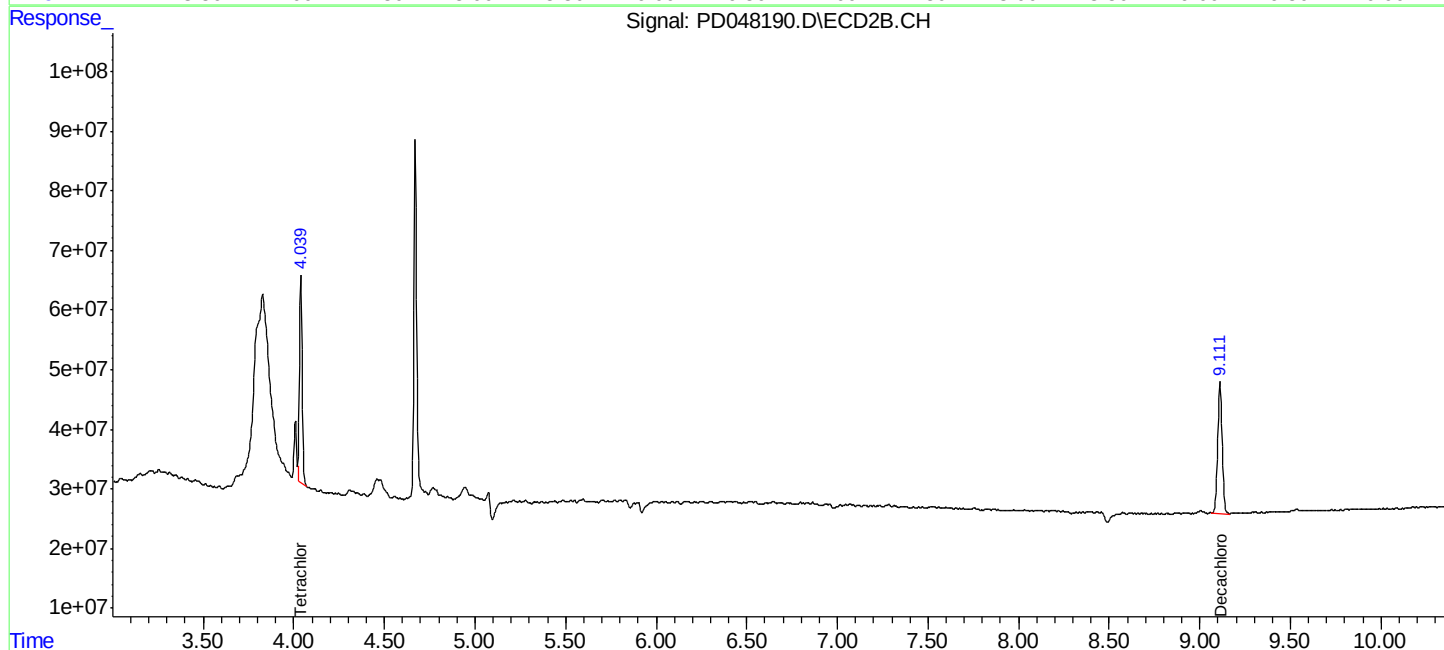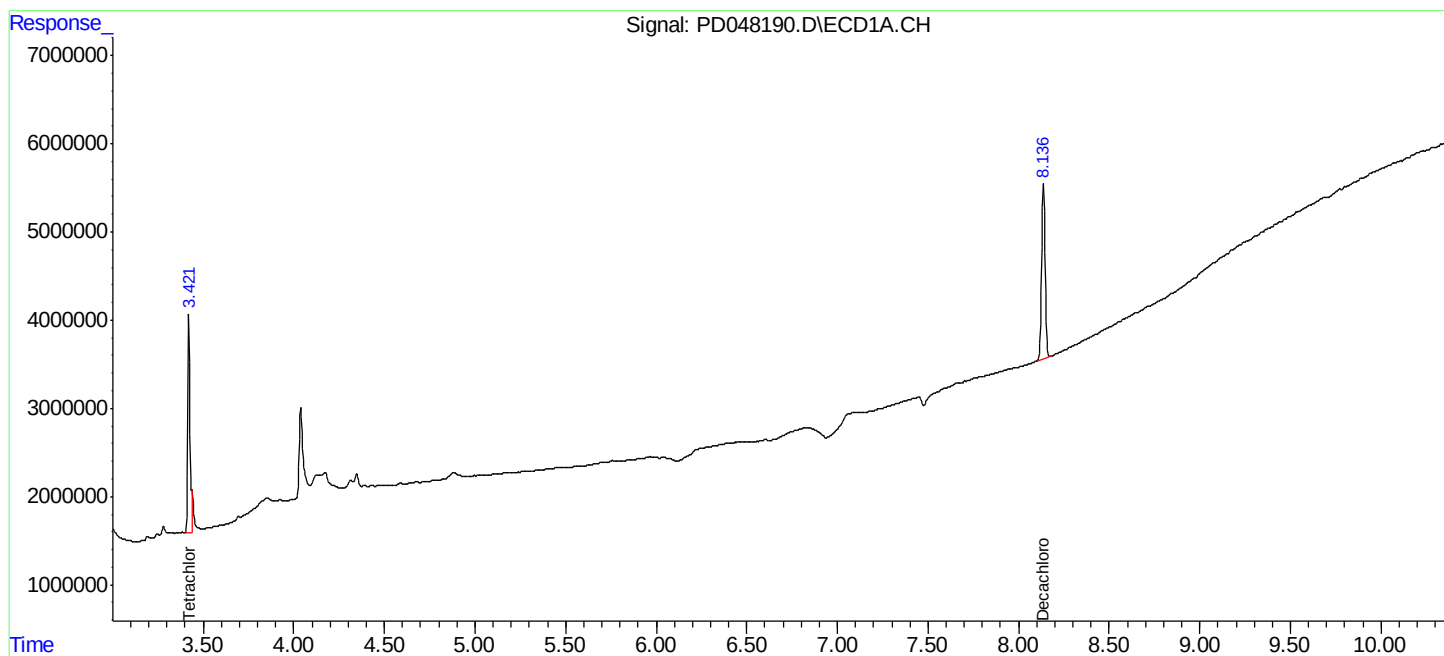

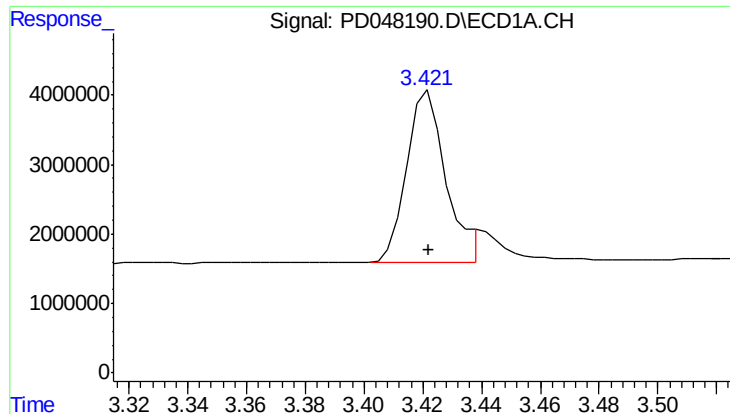


#1 Tetrachloro-m-xylene

R.T.: 3.421 min
Delta R.T.: -0.001 min
Response: 23883333
Conc: 19.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

UGO
6/21/2018 4:43:54 PM

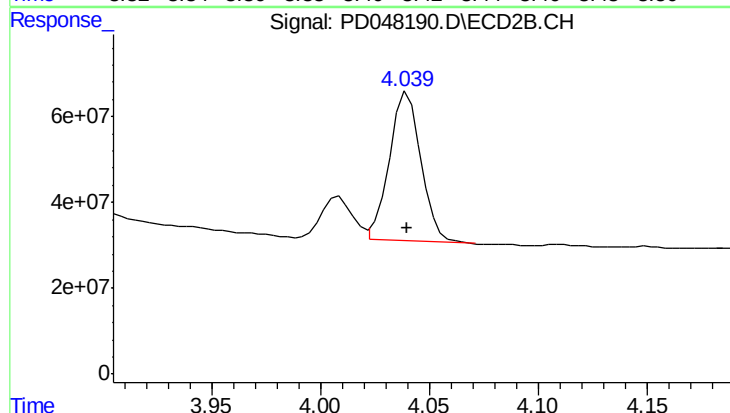


#1 Tetrachloro-m-xylene

R.T.: 4.040 min
Delta R.T.: 0.000 min
Response: 350778449
Conc: 18.12 ng/ml

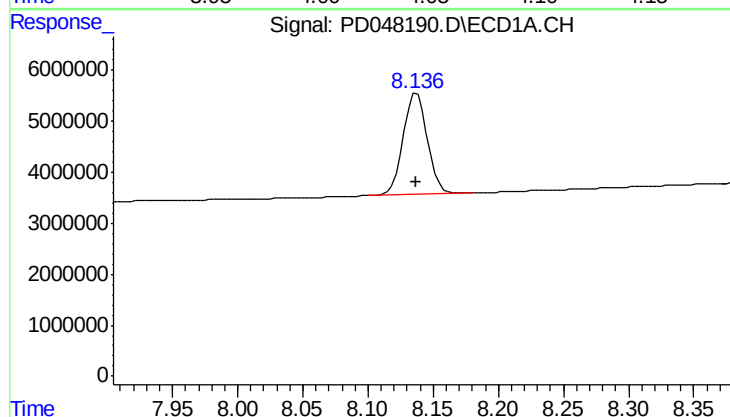

#28 Decachlorobiphenyl

R.T.: 8.138 min
Delta R.T.: 0.000 min
Response: 25628147
Conc: 19.80 ng/ml

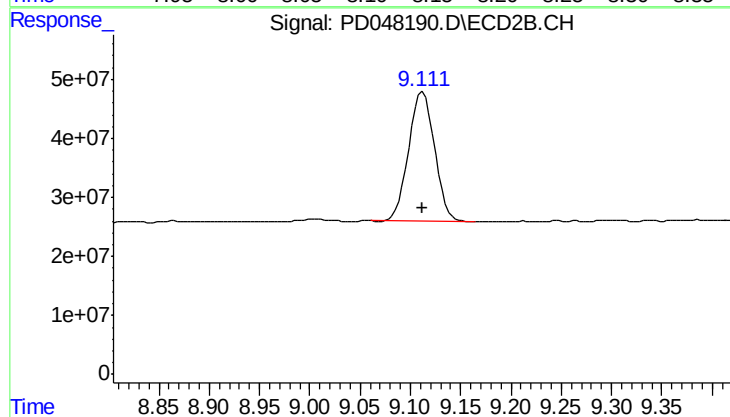

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 394972965
Conc: 21.27 ng/ml