

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062018\
 Data File : PD048217.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jun 2018 22:55
 Operator : UA/AJ
 Sample : J3573-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-54-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 03:52:59 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 01:43:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.040	20071910	332.4E6	16.473	17.165
28)	SA Decachlor...	8.137	9.112	18056296	273.1E6	13.952	14.704

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062018\
Data File : PD048217.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jun 2018 22:55
Operator : UA/AJ
Sample : J3573-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SB-54-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:52:59 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 01:43:00 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

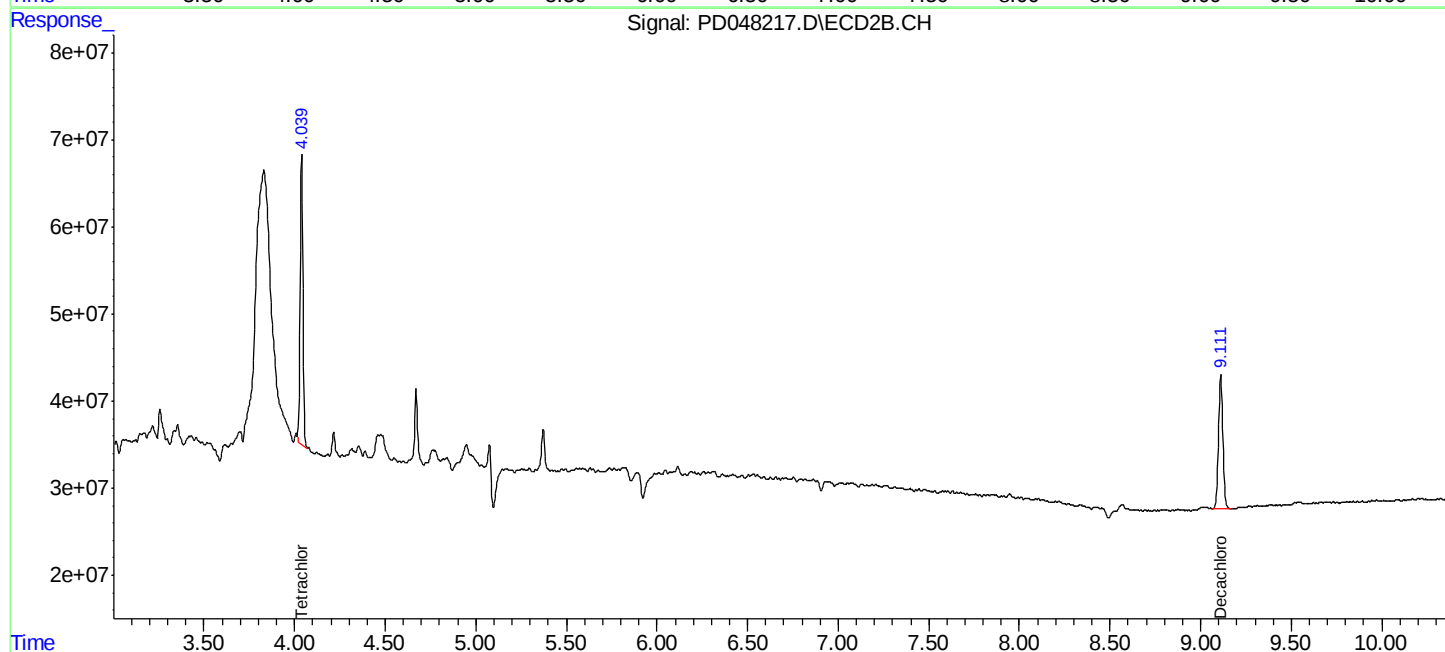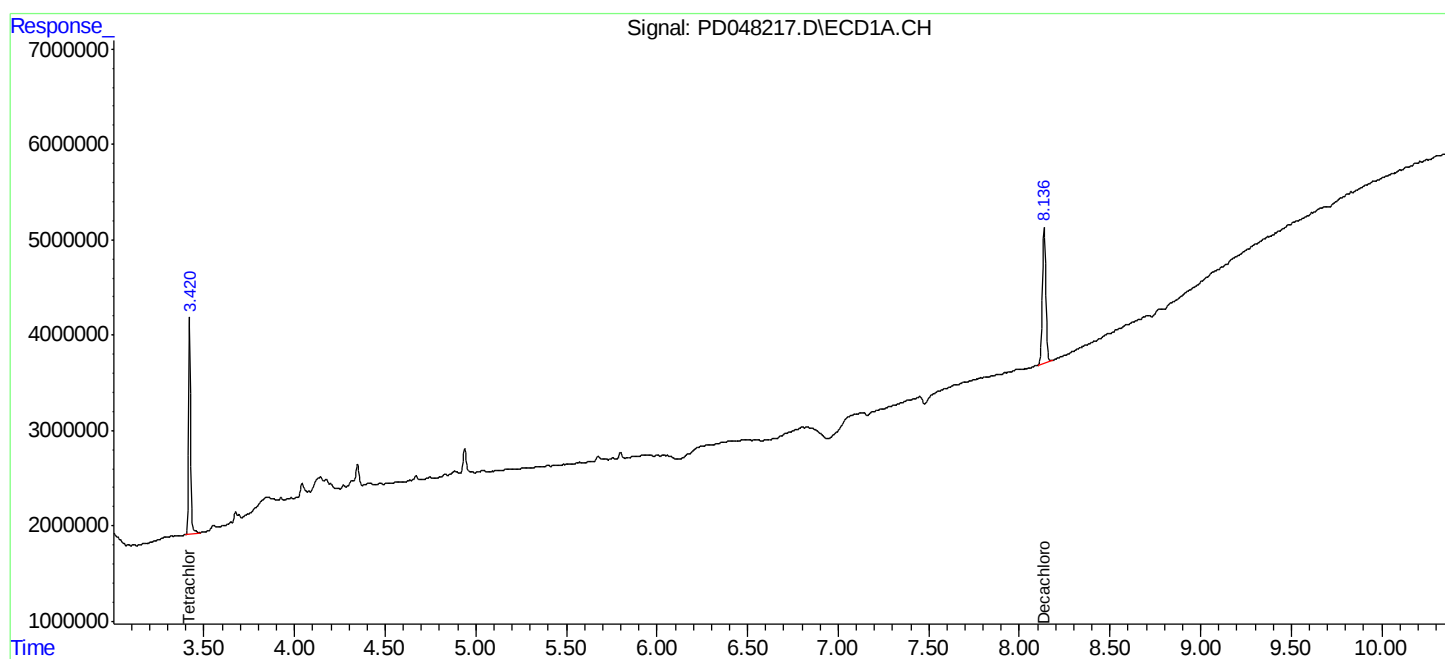


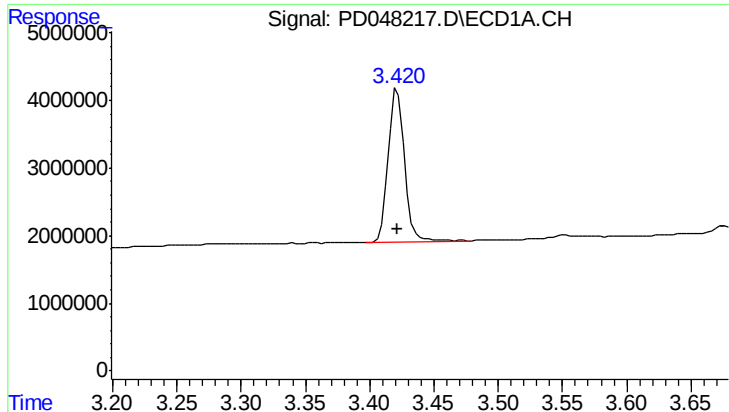

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 20071910
Conc: 16.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-54-COMP

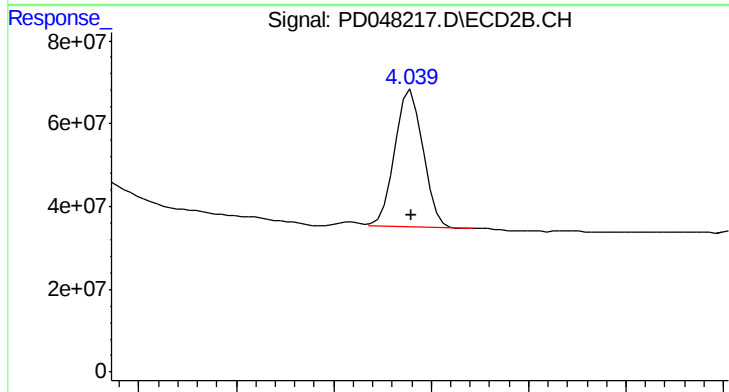


#1 Tetrachloro-m-xylene

R.T.: 4.040 min
Delta R.T.: 0.000 min
Response: 332363535
Conc: 17.17 ng/ml

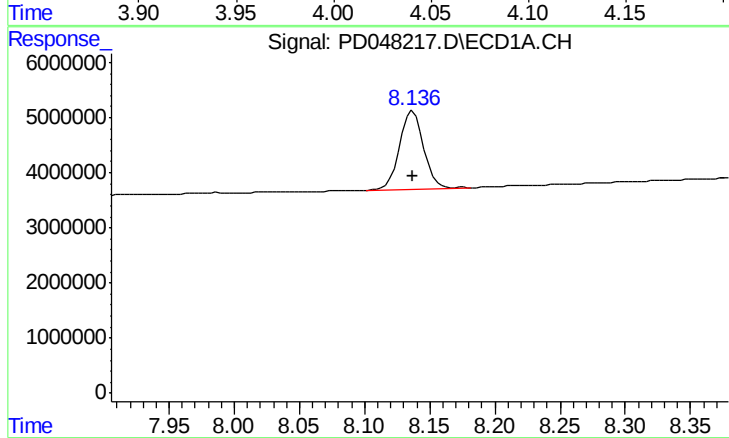

#28 Decachlorobiphenyl

R.T.: 8.137 min
Delta R.T.: 0.000 min
Response: 18056296
Conc: 13.95 ng/ml

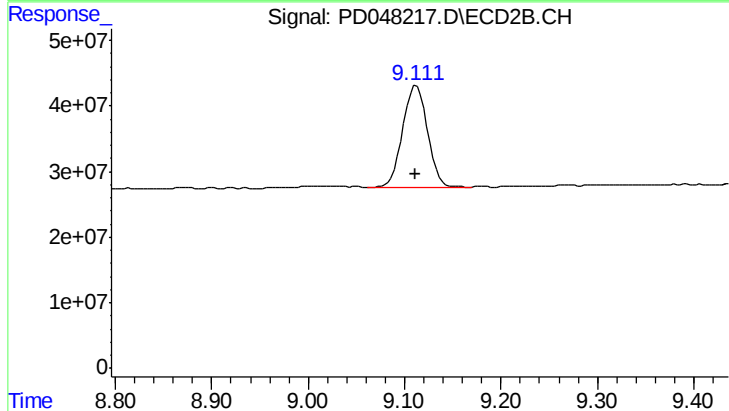

#28 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.000 min
Response: 273115974
Conc: 14.70 ng/ml