

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062019\
 Data File : PD053672.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2019 8:02
 Operator : SM\AJ
 Sample : PIBLK50
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK50

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 09:05:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062019CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 21 08:58:58 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.984	13765717	21633007	18.979	19.182
27)	SA Decachlor...	8.014	9.029	24166010	37698187	38.399	38.578


Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062019\
Data File : PD053672.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2019 8:02
Operator : SM\AJ
Sample : PIBLK50
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 09:05:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062019CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 21 08:58:58 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

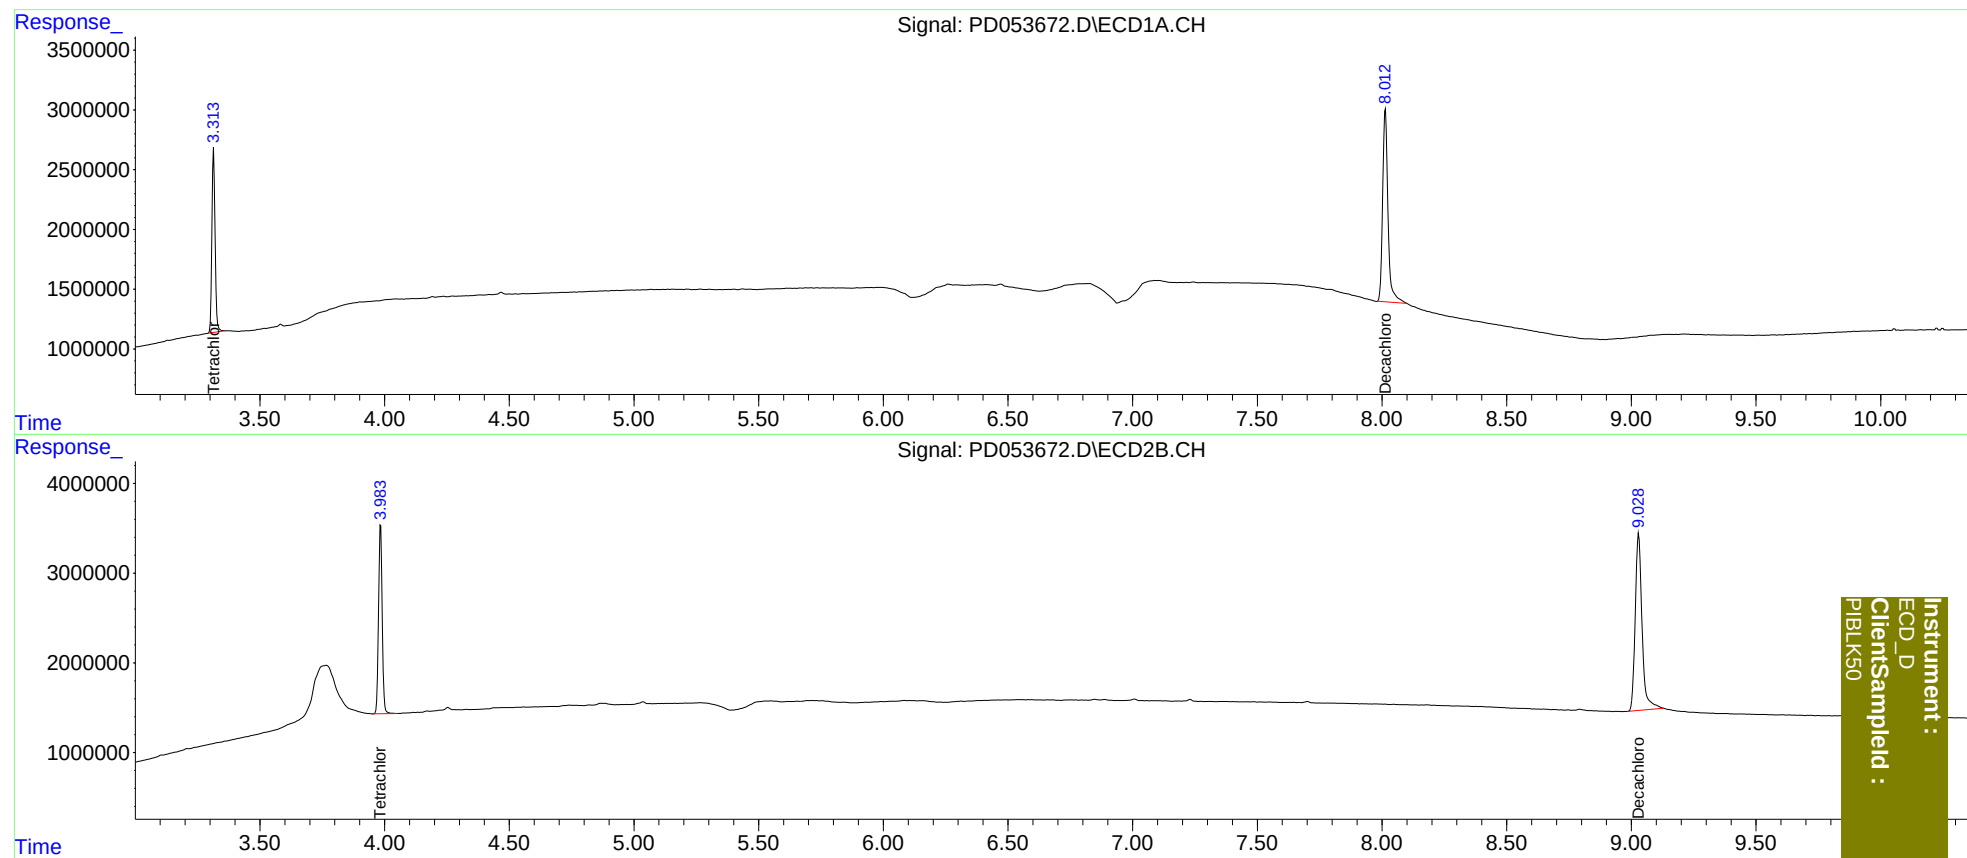


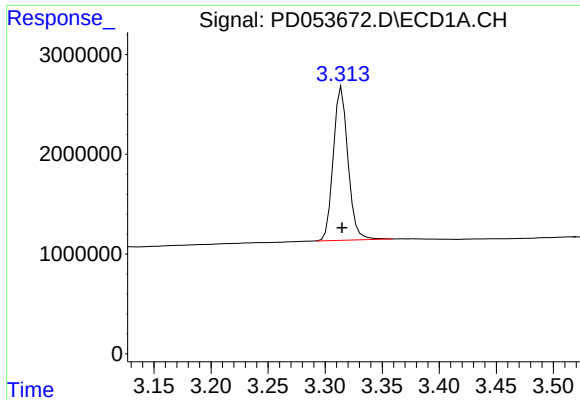

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: 0.000 min
Response: 13765717
Conc: 18.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK50

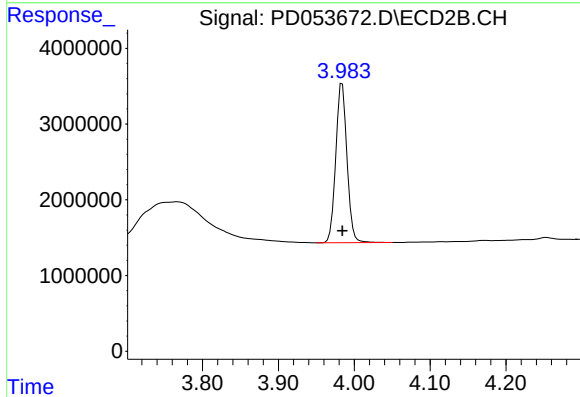


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: 0.000 min
Response: 21633007
Conc: 19.18 ng/ml

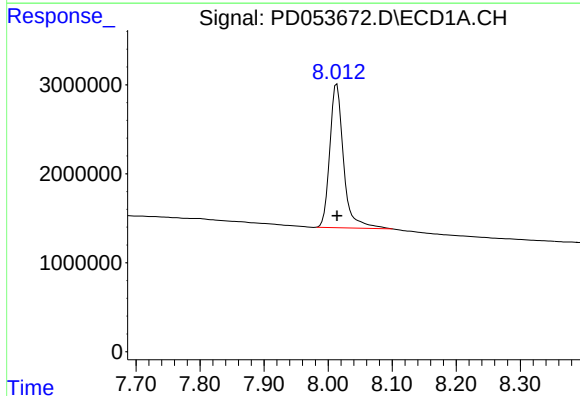

#27 Decachlorobiphenyl

R.T.: 8.014 min
Delta R.T.: 0.000 min
Response: 24166010
Conc: 38.40 ng/ml

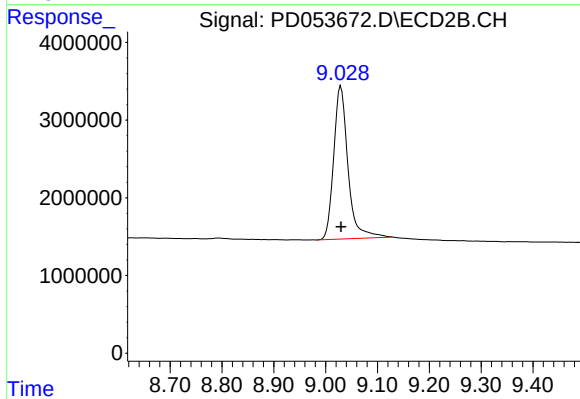

#27 Decachlorobiphenyl

R.T.: 9.029 min
Delta R.T.: 0.000 min
Response: 37698187
Conc: 38.58 ng/ml