

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062022\
 Data File : PD070386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2022 10:31
 Operator : AR\AJ
 Sample : N3374-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4S6MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/21/2022
 Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 03:05:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 16:58:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.399	4.120	26111460	171.0E6	18.004m	12.659m#
27)	SA Decachlor...	8.127	9.277	38883701	144.5E6	24.277	20.020m
Target Compounds							
2)	A alpha-BHC	3.834	4.512	96333987	604.8E6	45.586m	30.895m#
3)	MA gamma-BHC...	4.116	4.801	96128210	581.0E6	47.871	31.864m#
4)	MA Heptachlor	4.409	5.326	89233969	490.3E6	45.341	27.366 #
5)	MB Aldrin	4.652	5.636	125.4E6	541.0E6	65.715	32.552 #
6)	B beta-BHC	4.364	4.966	46149679	211.6E6	51.560m	26.751 #
7)	B delta-BHC	4.566	5.190	105.1E6	515.9E6	52.054	39.986
8)	B Heptachlo...	5.096	6.023	87371519	478.2E6	49.878	40.978
9)	A Endosulfan I	5.432	6.384	79329338	471.4E6	47.163	34.957 #
10)	B trans-Chl...	5.320	6.259	83728050	492.4E6	46.550	34.072 #
11)	B cis-Chlor...	5.378	6.333	88812325	476.4E6	50.212	33.927 #
12)	B 4,4'-DDE	5.544	6.484	164.9E6	881.3E6	97.690	67.780 #
13)	MA Dieldrin	5.673	6.642	189.2E6	930.6E6	99.737	67.948 #
14)	MA Endrin	5.930	6.861	163.0E6	809.0E6	95.780	70.313 #
15)	B Endosulfa...	6.204	7.066	146.8E6	776.4E6	90.494	70.587
16)	A 4,4'-DDD	6.059	6.975	142.1E6	807.7E6	93.839	73.151
17)	MA 4,4'-DDT	6.298	7.277	141.9E6	803.2E6	97.500	78.115
18)	B Endrin al...	6.373	7.191	96339299	512.4E6	77.444	60.917
19)	B Endosulfa...	6.585	7.415	147.8E6	718.8E6	93.281	72.717
20)	A Methoxychlor	6.847	7.731	424.3E6	1793.1E6	501.295	379.812
21)	B Endrin ke...	7.076	7.888	183.1E6	831.0E6	102.662	81.569

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062022\
Data File : PD070386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2022 10:31
Operator : AR\AJ
Sample : N3374-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:05:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 16:58:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

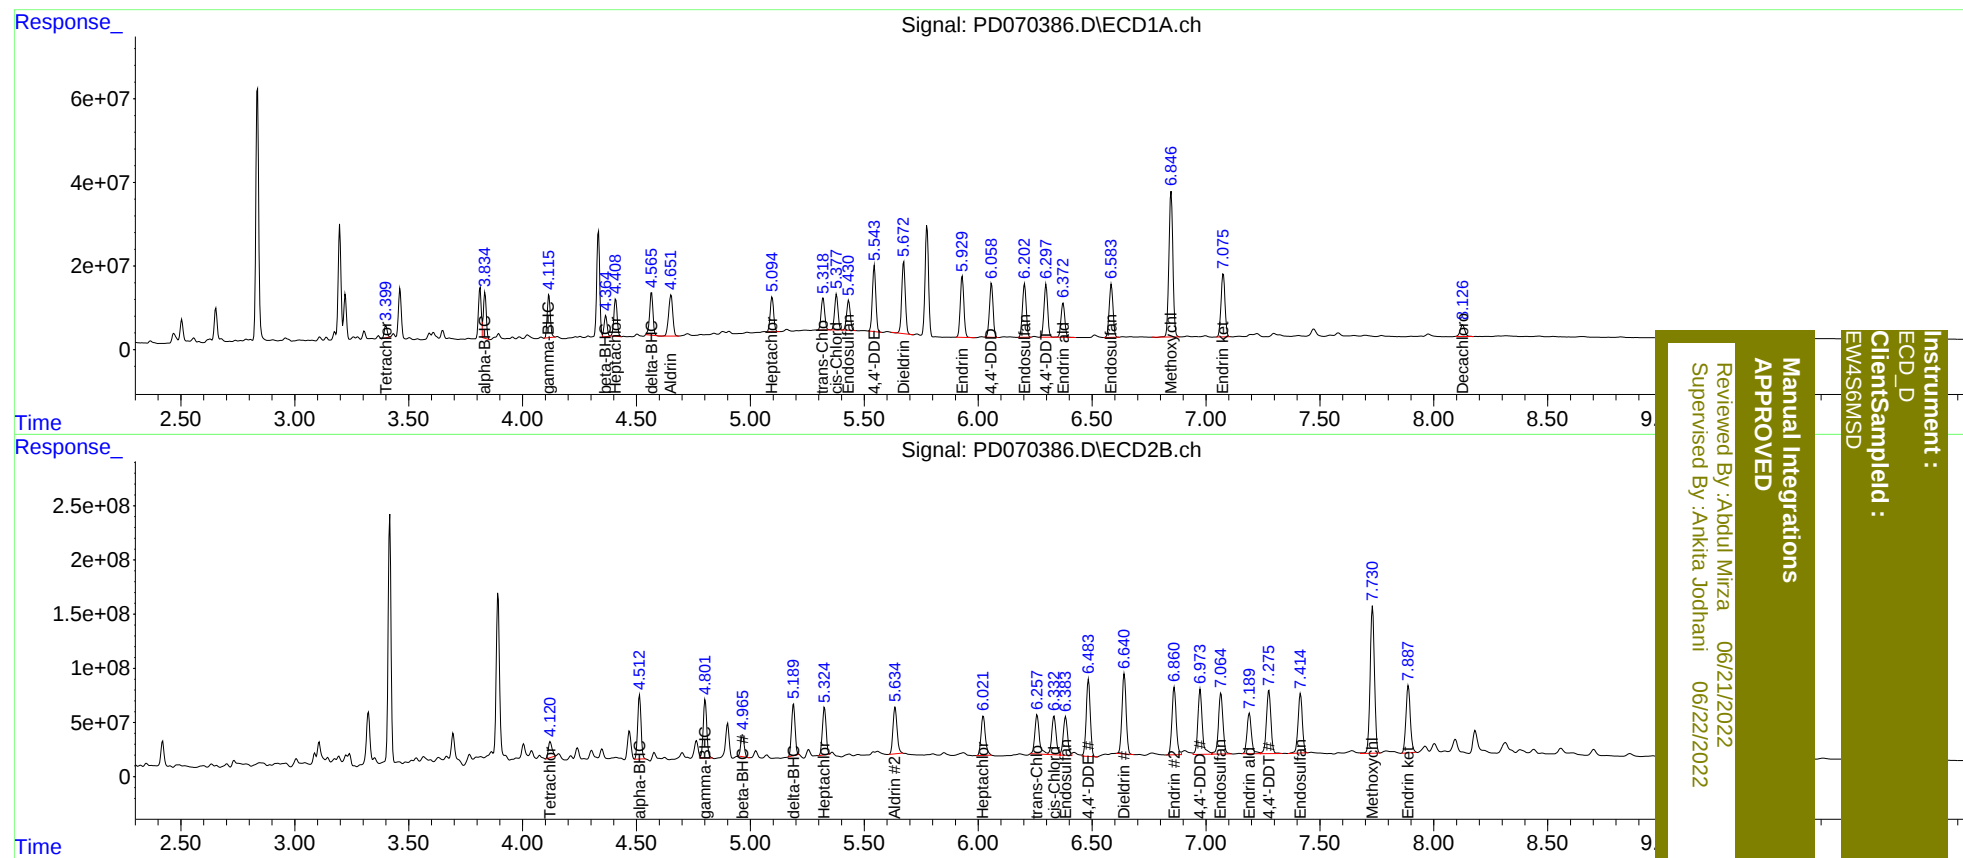

Reviewed By: Abdul Mirza 06/21/2022
Supervised By: Ankita Jodhani 06/22/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EW/MS6MSD