

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062022\
 Data File : PD070400.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2022 13:49
 Operator : AR\AJ
 Sample : N3395-06MS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0154MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/21/2022
 Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 03:08:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 16:58:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.399	4.120	26828499	233.4E6	18.498	17.277
27)	SA Decachlor...	8.125	9.277	55589551	236.3E6	34.707	32.748
Target Compounds							
2)	A alpha-BHC	3.835	4.513	140.0E6	1039.0E6	66.226	53.076
3)	MA gamma-BHC...	4.115	4.801	130.8E6	955.7E6	65.120	52.412
4)	MA Heptachlor	4.409	5.325	112.2E6	814.8E6	57.005	45.477
5)	MB Aldrin	4.654	5.636	120.2E6	822.9E6	63.029	49.511
6)	B beta-BHC	4.365	4.964	52465790	413.2E6	58.617	52.232m
7)	B delta-BHC	4.566	5.188	136.4E6	879.3E6	67.593	68.155m
8)	B Heptachlo...	5.095	6.023	113.7E6	711.5E6	64.932	60.978
9)	A Endosulfan I	5.430	6.383	104.6E6	669.8E6	62.179	49.666
10)	B trans-Chl...	5.319	6.258	115.4E6	730.5E6	64.162	50.541
11)	B cis-Chlor...	5.377	6.333	110.9E6	708.0E6	62.712	50.423
12)	B 4,4'-DDE	5.543	6.484	224.6E6	1314.8E6	133.020	101.118
13)	MA Dieldrin	5.673	6.641	249.6E6	1401.3E6	131.600	102.316
14)	MA Endrin	5.930	6.861	208.9E6	1128.0E6	122.767	98.037
15)	B Endosulfa...	6.203	7.066	206.2E6	1103.5E6	127.086	100.327
16)	A 4,4'-DDD	6.058	6.974	194.8E6	1081.7E6	128.634	97.972
17)	MA 4,4'-DDT	6.297	7.276	187.9E6	1023.6E6	129.116	99.557
18)	B Endrin al...	6.372	7.190	151.8E6	823.7E6	122.049	97.931
19)	B Endosulfa...	6.584	7.415	196.4E6	991.5E6	124.012	100.312
20)	A Methoxychlor	6.846	7.730	483.6E6	2191.7E6	571.412	464.245
21)	B Endrin ke...	7.075	7.888	240.8E6	1076.2E6	135.017	105.640

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062022\
Data File : PD070400.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2022 13:49
Operator : AR\AJ
Sample : N3395-06MS
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:08:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 16:58:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

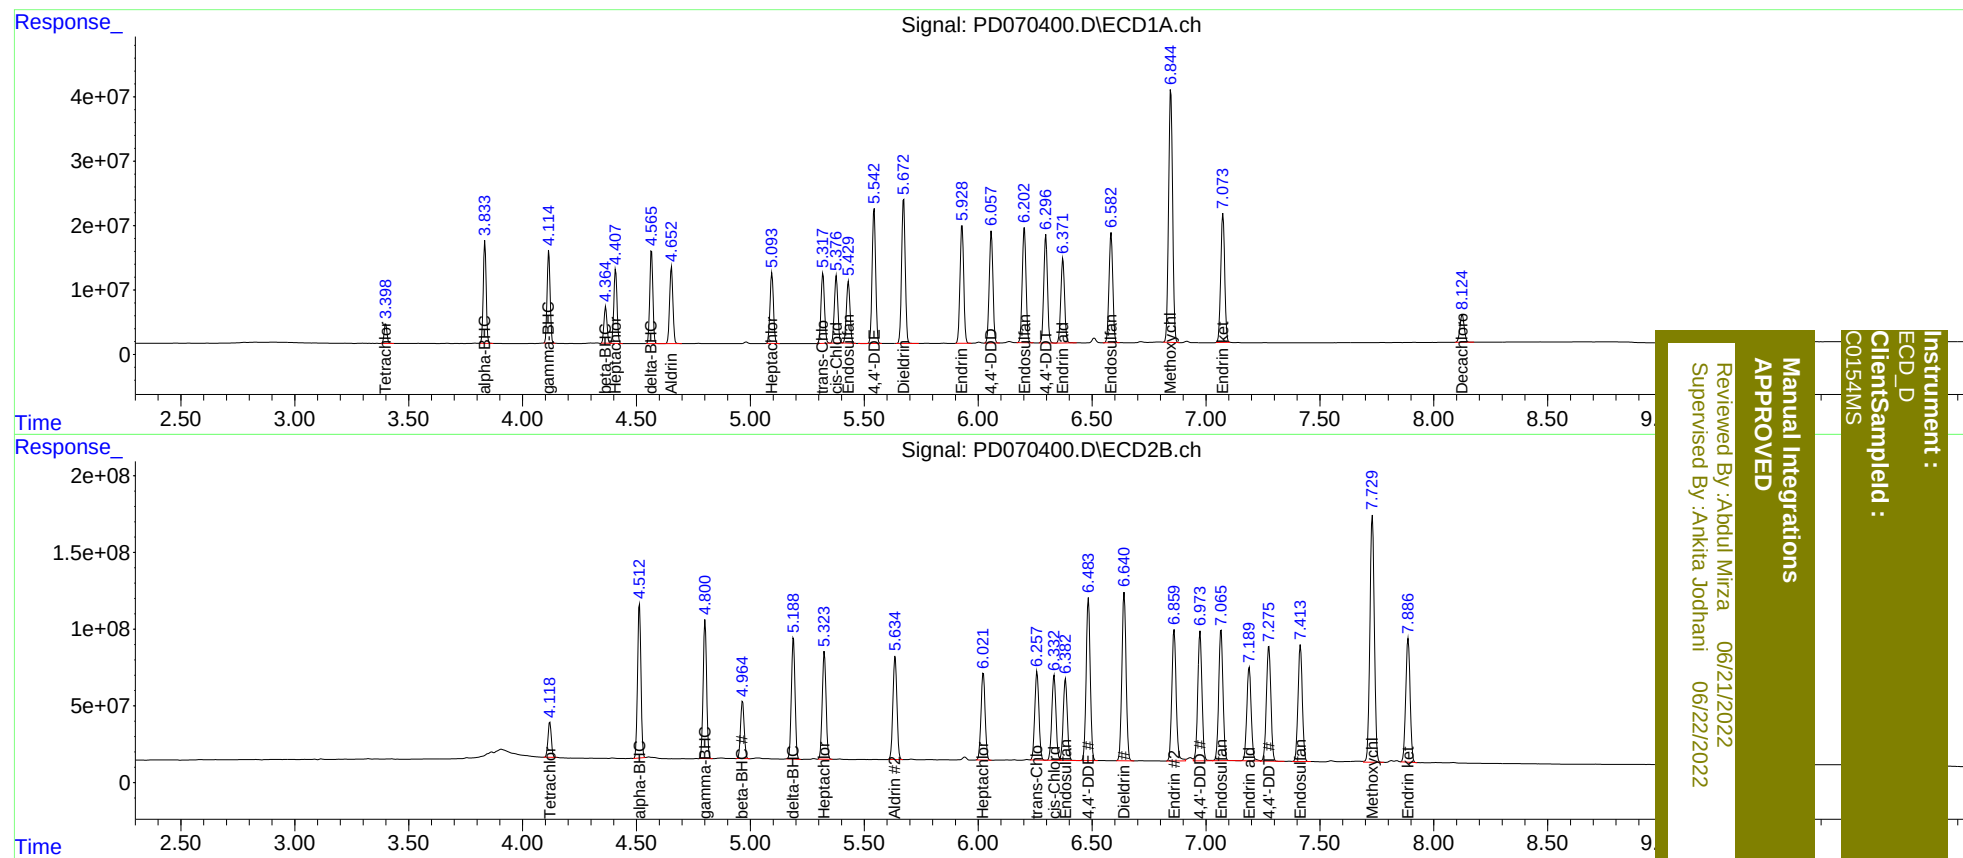

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/21/2022
Supervised By: Ankita Jodhani 06/22/2022

Instrument :
ECD_D
Client Sampled :
C0154MS