

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062022\
 Data File : PD070401.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2022 14:03
 Operator : AR\AJ
 Sample : N3395-07MSD
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0154MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/21/2022
 Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 03:09:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 16:58:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.400	4.120	27486919	238.0E6	18.952	17.619
27)	SA Decachlor...	8.126	9.277	56239642	242.5E6	35.113	33.597
Target Compounds							
2)	A alpha-BHC	3.835	4.513	139.7E6	1038.3E6	66.089	53.038
3)	MA gamma-BHC...	4.115	4.801	131.0E6	952.7E6	65.258	52.244
4)	MA Heptachlor	4.409	5.324	111.7E6	738.0E6	56.741	41.192 #
5)	MB Aldrin	4.654	5.635	119.6E6	790.5E6	62.697	47.562
6)	B beta-BHC	4.365	4.964	52019381	405.5E6	58.118	51.263m
7)	B delta-BHC	4.566	5.188	135.8E6	844.8E6	67.312	65.478m
8)	B Heptachlo...	5.095	6.022	114.1E6	614.9E6	65.156	52.699
9)	A Endosulfan I	5.430	6.383	104.4E6	642.4E6	62.084	47.636
10)	B trans-Chl...	5.319	6.258	115.1E6	688.7E6	64.001	47.654 #
11)	B cis-Chlor...	5.377	6.333	110.4E6	680.9E6	62.431	48.490
12)	B 4,4'-DDE	5.544	6.484	223.9E6	1266.7E6	132.646	97.416 #
13)	MA Dieldrin	5.673	6.641	248.8E6	1357.4E6	131.137	99.112
14)	MA Endrin	5.930	6.860	208.2E6	1091.4E6	122.325	94.858
15)	B Endosulfa...	6.203	7.066	206.3E6	1101.3E6	127.116	100.134
16)	A 4,4'-DDD	6.058	6.974	194.4E6	1063.7E6	128.412	96.338
17)	MA 4,4'-DDT	6.297	7.276	187.1E6	1025.0E6	128.605	99.692
18)	B Endrin al...	6.372	7.190	151.4E6	821.9E6	121.710	97.719
19)	B Endosulfa...	6.584	7.415	196.4E6	992.6E6	124.018	100.423
20)	A Methoxychlor	6.846	7.731	482.3E6	2195.5E6	569.861	465.038
21)	B Endrin ke...	7.075	7.888	240.6E6	1079.5E6	134.916	105.966

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062022\
Data File : PD070401.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2022 14:03
Operator : AR\AJ
Sample : N3395-07MSD
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:09:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 16:58:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

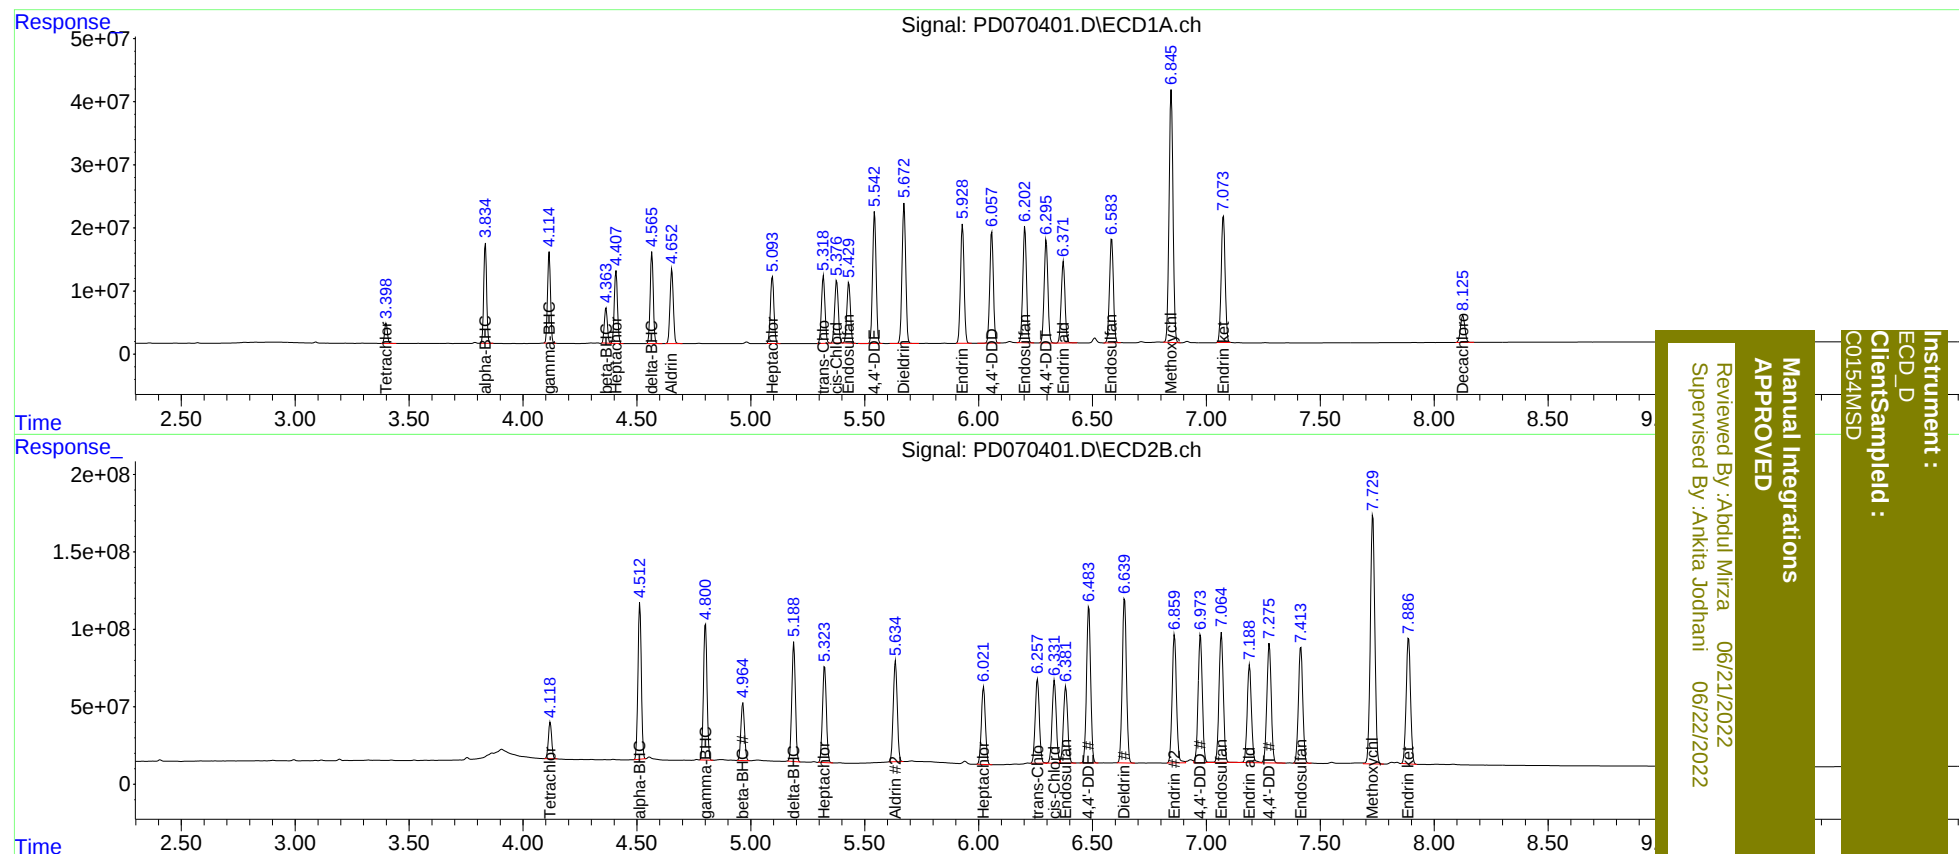

Reviewed By: Abdul Mirza 06/21/2022
Supervised By: Ankita Jodhani 06/22/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
C0154M/MSD