

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062022\
 Data File : PD070385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2022 10:17
 Operator : AR\AJ
 Sample : N3374-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4S6MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/21/2022
 Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 03:04:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 16:58:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.399	4.119	25047493	165.2E6	17.270m	12.227m#
27)	SA Decachlor...	8.128	9.277	36809406	138.1E6	22.982	19.133
Target Compounds							
2)	A alpha-BHC	3.834	4.512	91358809	608.8E6	43.232m	31.099m#
3)	MA gamma-BHC...	4.116	4.800	93926192	582.1E6	46.775	31.922m#
4)	MA Heptachlor	4.410	5.325	87543795	498.6E6	44.482	27.831 #
5)	MB Aldrin	4.653	5.636	123.4E6	550.5E6	64.694	33.124 #
6)	B beta-BHC	4.365	4.966	42820605	214.5E6	47.841m	27.119 #
7)	B delta-BHC	4.567	5.189	103.6E6	522.5E6	51.346	40.500
8)	B Heptachlo...	5.096	6.023	84520373	484.6E6	48.250	41.528
9)	A Endosulfan I	5.432	6.383	77231704	482.6E6	45.915	35.788
10)	B trans-Chl...	5.320	6.258	81530689	499.5E6	45.329	34.561
11)	B cis-Chlor...	5.379	6.333	86274447	488.7E6	48.778	34.807 #
12)	B 4,4'-DDE	5.545	6.484	160.5E6	888.5E6	95.099	68.335 #
13)	MA Dieldrin	5.674	6.641	183.7E6	936.6E6	96.835	68.388 #
14)	MA Endrin	5.931	6.861	159.0E6	803.1E6	93.417	69.802 #
15)	B Endosulfa...	6.204	7.065	143.0E6	769.9E6	88.121	70.002
16)	A 4,4'-DDD	6.059	6.974	138.0E6	796.7E6	91.151	72.155
17)	MA 4,4'-DDT	6.298	7.276	136.9E6	782.6E6	94.050	76.116
18)	B Endrin al...	6.373	7.190	95145341	512.7E6	76.484	60.956
19)	B Endosulfa...	6.585	7.415	143.1E6	711.0E6	90.357	71.931
20)	A Methoxychlor	6.848	7.731	409.7E6	1750.3E6	484.081	370.743
21)	B Endrin ke...	7.076	7.888	178.5E6	824.6E6	100.103	80.940

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062022\
Data File : PD070385.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2022 10:17
Operator : AR\AJ
Sample : N3374-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:04:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 16:58:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

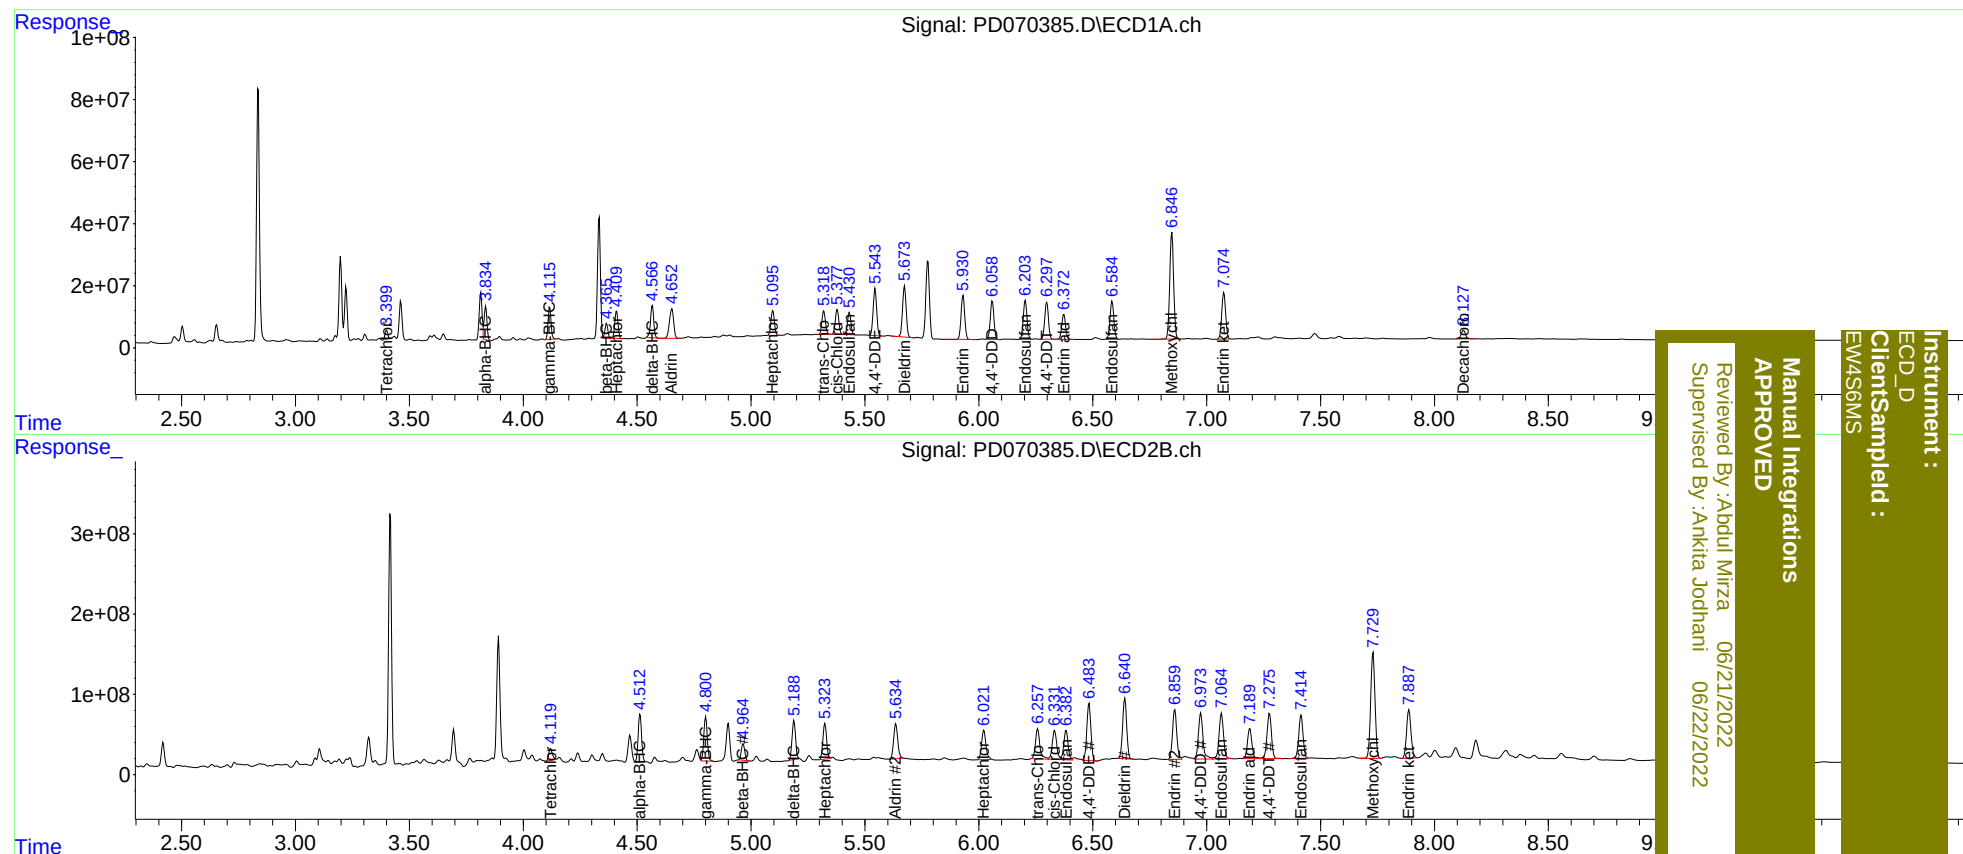

Reviewed By: Abdul Mirza 06/21/2022
Supervised By: Ankita Jodhani 06/22/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EW/MS6MS