

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062022\
 Data File : PD070423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2022 20:11
 Operator : AR\AJ
 Sample : PB145667BS
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS667

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/21/2022
 Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 03:14:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 16:58:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.399	4.120	30952695	264.2E6	21.342	19.556
27)	SA Decachlor...	8.127	9.278	68178925	305.3E6	42.567	42.308
Target Compounds							
2)	A alpha-BHC	3.834	4.513	10130761	94836311	4.794	4.844
3)	MA gamma-BHC...	4.115	4.802	10258067	94360842	5.108	5.175
4)	MA Heptachlor	4.409	5.325	10116275	93988130	5.140	5.246
5)	MB Aldrin	4.653	5.636	12462596	92117809	6.534	5.542
6)	B beta-BHC	4.365	4.966	4937148	43746814	5.516	5.530
7)	B delta-BHC	4.564	5.188	7959032	47341310	3.944m	3.669m
8)	B Heptachlo...	5.095	6.020	10146145	70783127	5.792	6.066m
9)	A Endosulfan I	5.430	6.384	9430663	76397245	5.607	5.665
10)	B trans-Chl...	5.318	6.259	10280739	80991143	5.716	5.604
11)	B cis-Chlor...	5.377	6.333	10512927	80062234	5.944	5.702
12)	B 4,4'-DDE	5.543	6.484	19146289	147.8E6	11.342	11.369
13)	MA Dieldrin	5.672	6.642	20682200	154.2E6	10.903	11.262
14)	MA Endrin	5.930	6.861	17646998	114.8E6	10.370	9.981
15)	B Endosulfa...	6.203	7.067	17519751	131.7E6	10.796	11.976
16)	A 4,4'-DDD	6.057	6.973	16772734	126.2E6	11.078	11.429m
17)	MA 4,4'-DDT	6.297	7.277	12872787	98958776	8.846	9.625
18)	B Endrin al...	6.372	7.190	15796939	110.5E6	12.699	13.134
19)	B Endosulfa...	6.584	7.416	15943324	104.6E6	10.066	10.582
20)	A Methoxychlor	6.846	7.732	42412748	247.4E6	50.111	52.412
21)	B Endrin ke...	7.073	7.888	20357989	124.6E6	11.416m	12.233

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062022\
Data File : PD070423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2022 20:11
Operator : AR\AJ
Sample : PB145667BS
Misc :
ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:14:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 16:58:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

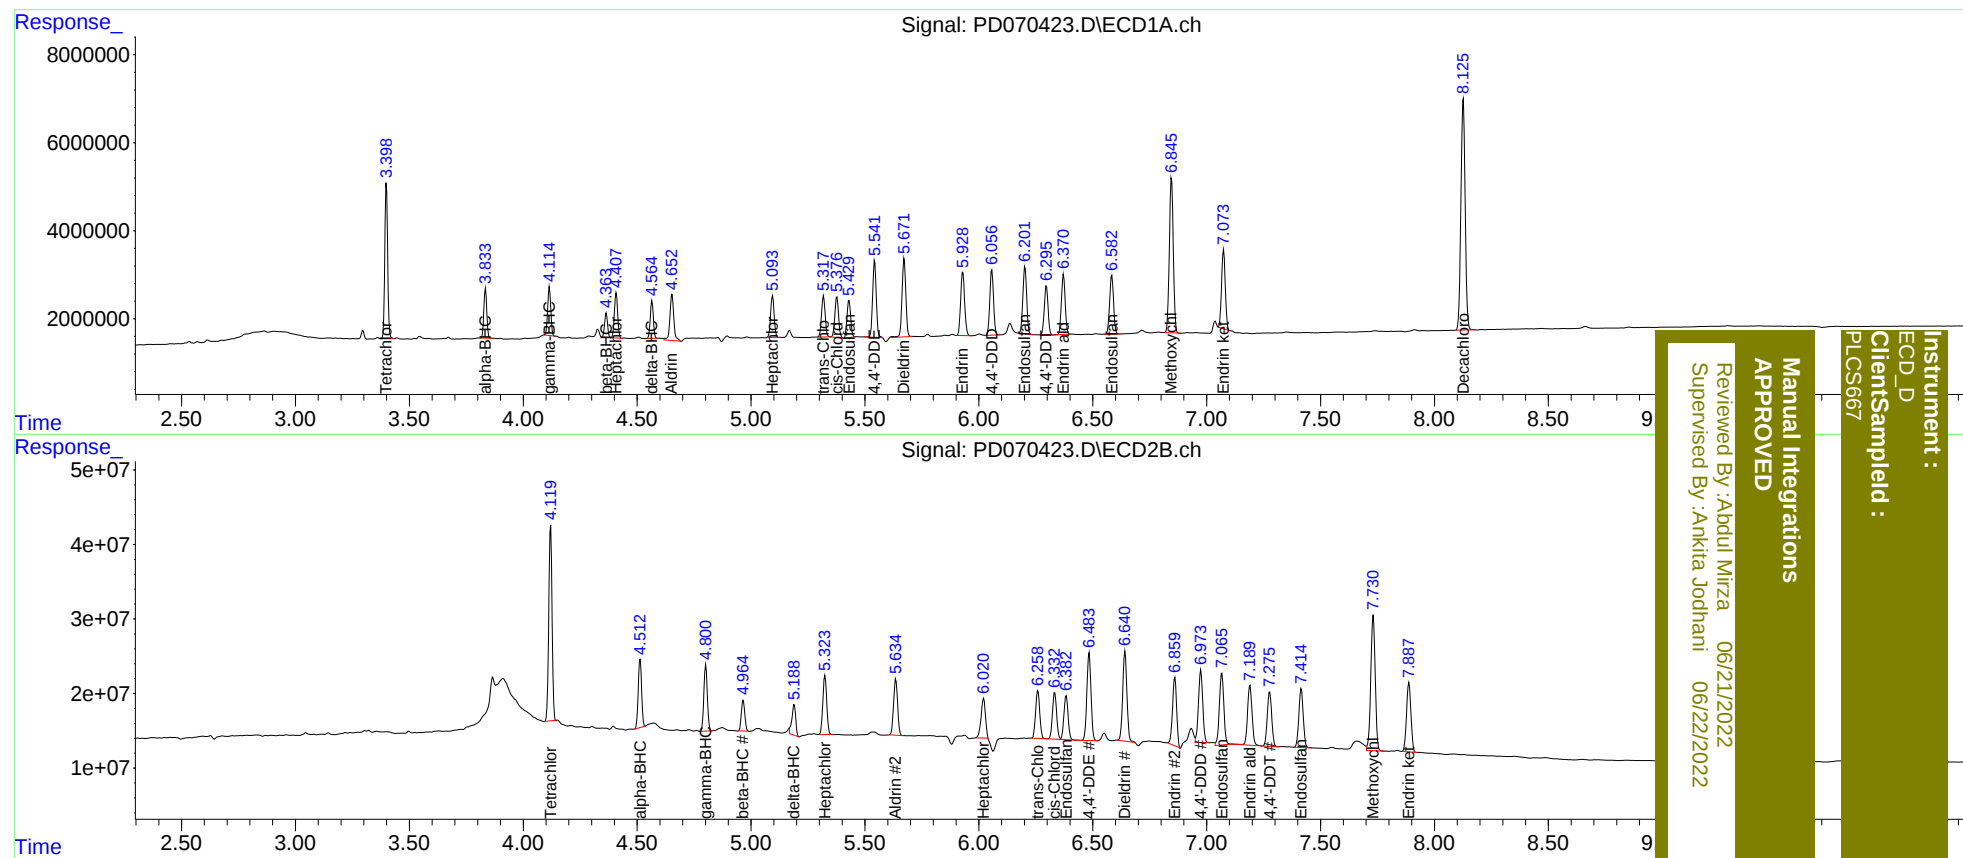

Instrument :
ECD_D
ClientSampled :
PLCS667

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 06/21/2022
Supervised By: Ankita Jodhani 06/22/2022