

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062022\
 Data File : PD070429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2022 21:36
 Operator : AR\AJ
 Sample : N3355-12MS
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EY0C9MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/21/2022
 Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 03:15:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 16:58:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.399	4.120	30336755	259.5E6	20.917	19.206
27)	SA Decachlor...	8.126	9.276	44291358	201.8E6	27.653	27.958
Target Compounds							
2)	A alpha-BHC	3.835	4.513	79505325	633.0E6	37.622	32.337
3)	MA gamma-BHC...	4.115	4.802	75804357	589.5E6	37.750	32.330
4)	MA Heptachlor	4.409	5.325	65537281	500.7E6	33.300	27.950
5)	MB Aldrin	4.654	5.635	73162783	518.2E6	38.356	31.180
6)	B beta-BHC	4.364	4.965	30903101	254.0E6	34.526	32.108m
7)	B delta-BHC	4.566	5.188	78525116	549.3E6	38.910	42.576m
8)	B Heptachlo...	5.095	6.022	66056442	434.6E6	37.710	37.248
9)	A Endosulfan I	5.431	6.384	60695105	426.4E6	36.084	31.617
10)	B trans-Chl...	5.319	6.259	66553722	458.9E6	37.002	31.751
11)	B cis-Chlor...	5.378	6.333	64795063	448.9E6	36.634	31.967
12)	B 4,4'-DDE	5.543	6.484	129.5E6	826.5E6	76.694	63.560
13)	MA Dieldrin	5.673	6.641	144.0E6	883.5E6	75.911	64.506
14)	MA Endrin	5.929	6.861	118.2E6	695.6E6	69.447	60.456
15)	B Endosulfa...	6.203	7.066	122.0E6	715.9E6	75.209	65.093
16)	A 4,4'-DDD	6.058	6.974	114.1E6	698.2E6	75.387	63.236
17)	MA 4,4'-DDT	6.296	7.276	106.4E6	642.5E6	73.102	62.490
18)	B Endrin al...	6.372	7.190	93028942	547.3E6	74.782	65.067
19)	B Endosulfa...	6.584	7.415	118.0E6	650.6E6	74.491	65.819
20)	A Methoxychlor	6.846	7.731	293.5E6	1427.1E6	346.782	302.280
21)	B Endrin ke...	7.074	7.888	147.5E6	714.3E6	82.723	70.119

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062022\
Data File : PD070429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2022 21:36
Operator : AR\AJ
Sample : N3355-12MS
Misc :
ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:15:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 16:58:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

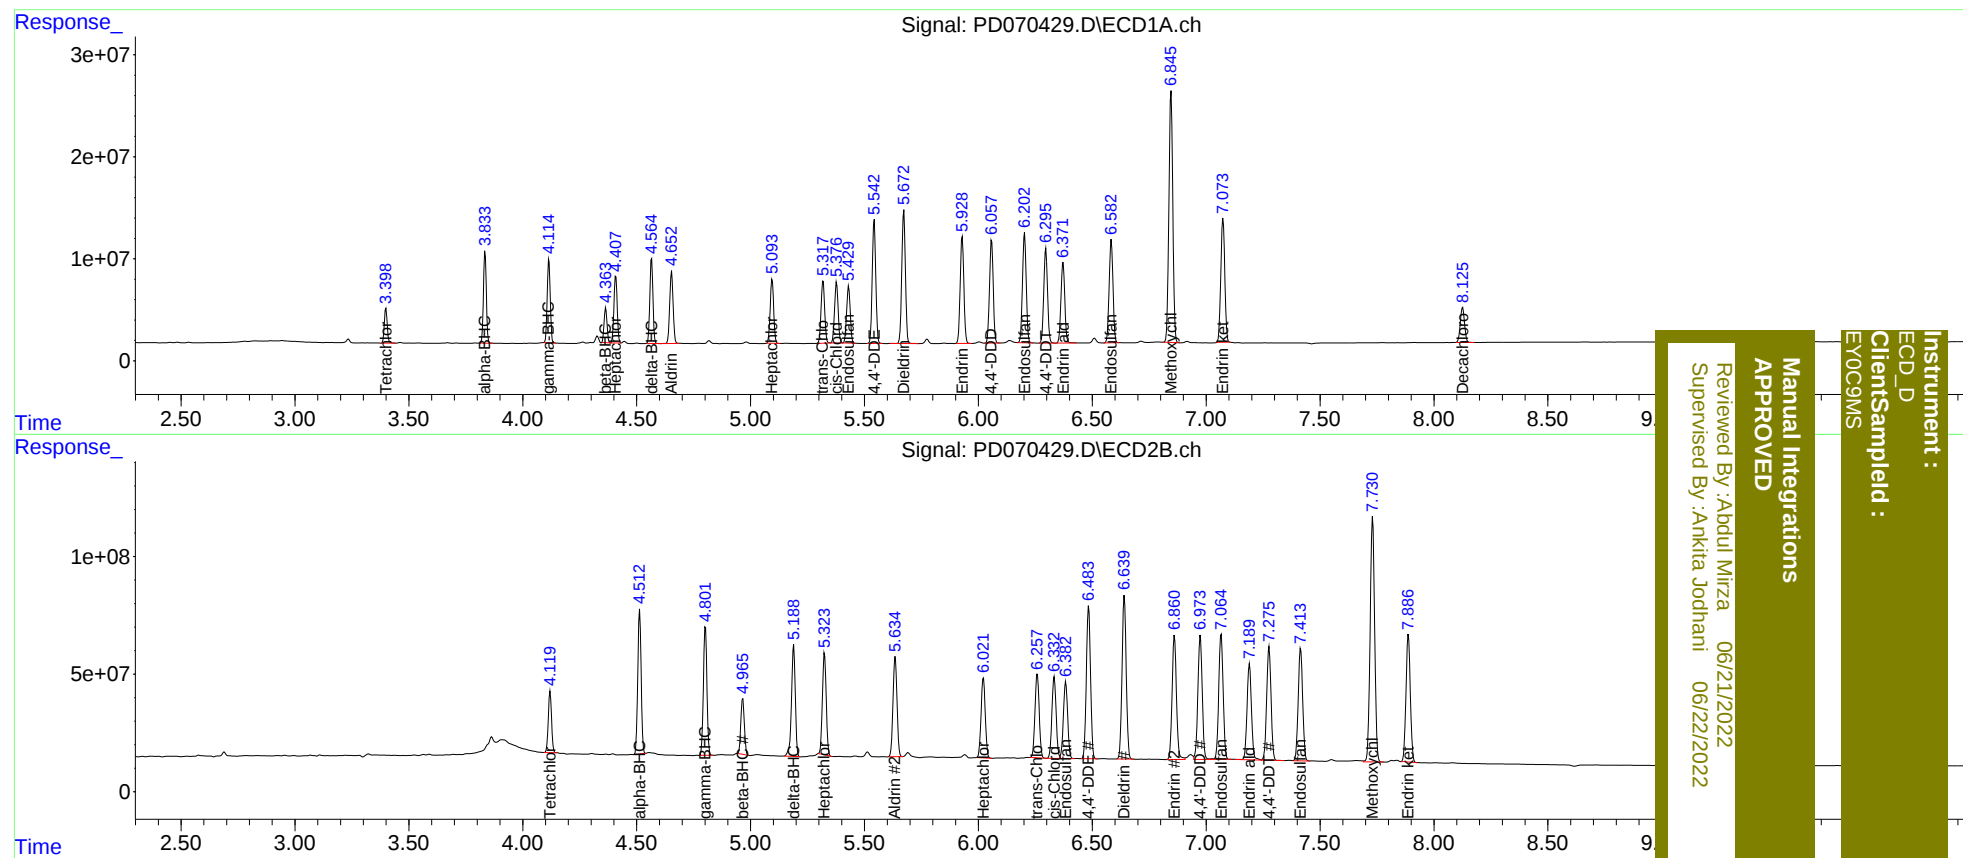

Instrument :
ECD_D
ClientSampled :
EYOC9MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 06/21/2022
Supervised By: Ankita Jodhani 06/22/2022