

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062022\
 Data File : PD070430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2022 21:50
 Operator : AR\AJ
 Sample : N3355-13MSD
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EY0C9MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/21/2022
 Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 03:16:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 16:58:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.400	4.121	30166396	257.3E6	20.800	19.046
27)	SA Decachlor...	8.126	9.276	43991580	199.8E6	27.466	27.679
Target Compounds							
2)	A alpha-BHC	3.835	4.514	85649932	671.9E6	40.530	34.323
3)	MA gamma-BHC...	4.115	4.802	81252889	624.8E6	40.464	34.264
4)	MA Heptachlor	4.409	5.325	70345666	533.0E6	35.743	29.749
5)	MB Aldrin	4.653	5.636	78211329	550.5E6	41.003	33.124
6)	B beta-BHC	4.365	4.965	33466294	267.0E6	37.390	33.752m
7)	B delta-BHC	4.566	5.188	84714782	583.5E6	41.977	45.226m
8)	B Heptachlo...	5.095	6.023	70658015	467.3E6	40.337	40.051
9)	A Endosulfan I	5.430	6.384	65058870	451.4E6	38.679	33.470
10)	B trans-Chl...	5.319	6.259	71720103	487.1E6	39.874	33.703
11)	B cis-Chlor...	5.378	6.334	69726207	475.4E6	39.422	33.854
12)	B 4,4'-DDE	5.543	6.485	139.5E6	877.8E6	82.661	67.509
13)	MA Dieldrin	5.673	6.642	155.2E6	939.0E6	81.809	68.560
14)	MA Endrin	5.929	6.861	126.9E6	718.5E6	74.568	62.449
15)	B Endosulfa...	6.203	7.067	131.4E6	754.6E6	81.005	68.604
16)	A 4,4'-DDD	6.057	6.975	122.8E6	739.5E6	81.120	66.980
17)	MA 4,4'-DDT	6.297	7.277	114.5E6	681.7E6	78.704	66.297
18)	B Endrin al...	6.372	7.191	99722892	579.6E6	80.163	68.913
19)	B Endosulfa...	6.584	7.415	126.4E6	689.0E6	79.830	69.707
20)	A Methoxychlor	6.846	7.731	313.2E6	1505.2E6	370.090	318.835
21)	B Endrin ke...	7.074	7.888	158.7E6	758.0E6	88.972	74.406

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062022\
Data File : PD070430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2022 21:50
Operator : AR\AJ
Sample : N3355-13MSD
Misc :
ALS Vial : 48 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 03:16:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 16:58:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

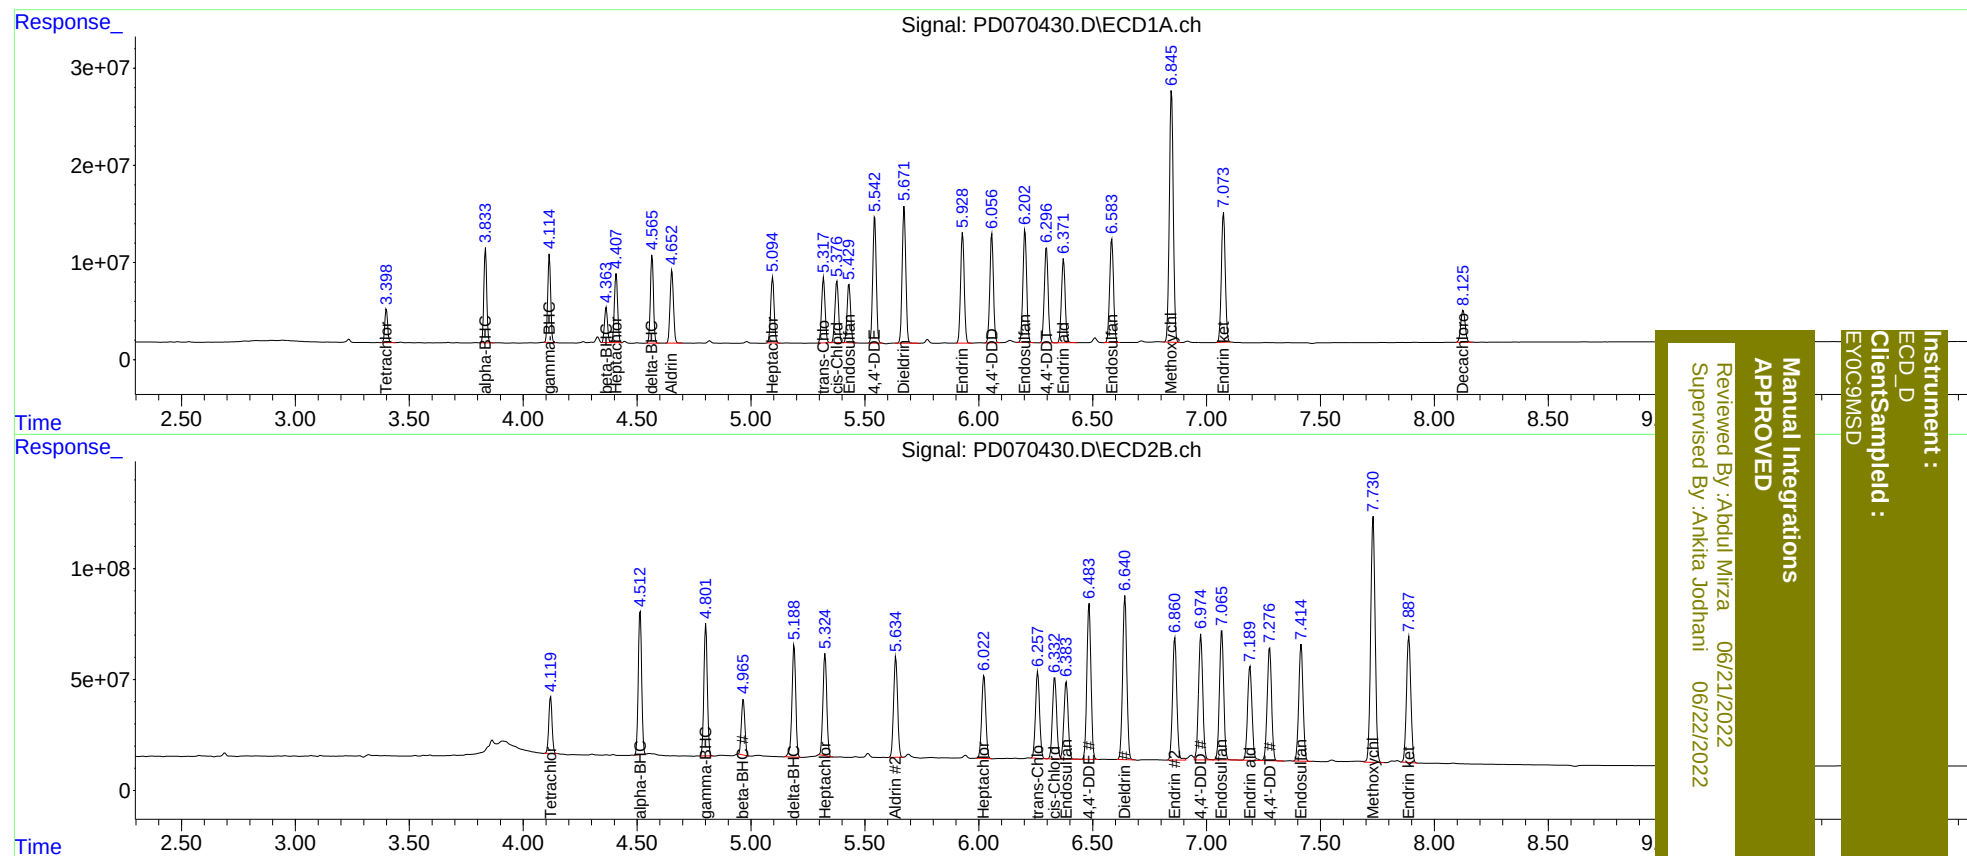

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/21/2022
Supervised By: Ankita Jodhani 06/22/2022

Instrument :
ECD_D
Client Sampled :
EY0C9MSD