

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062024\
 Data File : PD083772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jun 2024 13:03
 Operator : AR\AJ
 Sample : P2899-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA4

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/21/2024
 Supervised By : Ankita Jodhani 06/21/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 04:51:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.561	2.771	13102233	60678826	10.038m	11.132m
2) SA Decachlor...	9.115	7.896	27383263	71521858	14.082m	11.779m
Target Compounds						
3) MA gamma-BHC...	4.351	3.598	5910175	11457092	2.717m	1.467m#
15) B Endosulfa...	6.822	5.906	5974392	12220483	3.321m	1.926m#
17) MA 4,4'-DDT	7.031	6.017	12403719	25426563	8.234m	4.492m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062024\
Data File : PD083772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jun 2024 13:03
Operator : AR\AJ
Sample : P2899-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 04:51:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

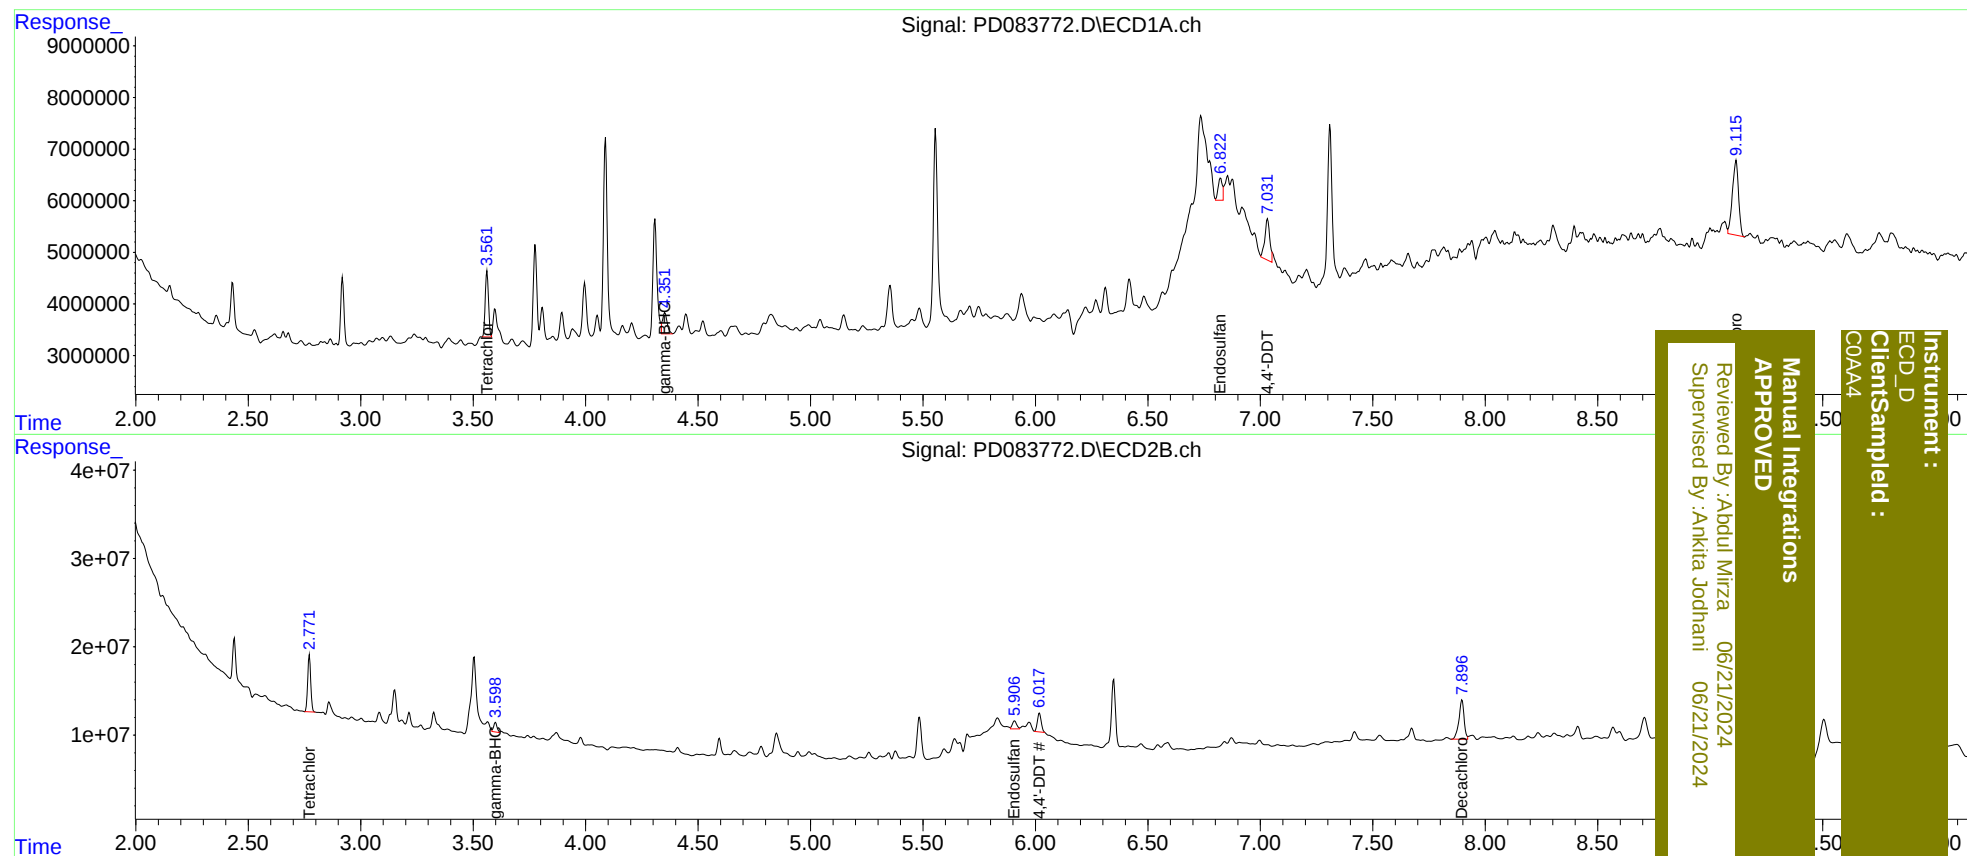

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/21/2024
Supervised By: Ankita Jodhani 06/21/2024

Instrument :
ECD_D
ClientSampled :
COAA4