

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062119\
 Data File : PD053677.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2019 9:11
 Operator : SM\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 00:35:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 22 00:19:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.984	8769217	13379006	12.407	12.225
28)	SA Decachlor...	8.013	9.029	9232778	14440097	14.202	14.278
Target Compounds							
8)	B Heptachlo...	0.000	5.845	0	9643643	N.D.	6.588 #
9)	A Endosulfan I	5.322	6.205	4902622	8301346	6.018	6.038
10)	B gamma-Chl...	5.212	6.083	5411714	9103716	6.041	5.781
12)	B 4,4'-DDE	5.439	6.310	8871596	15733888	11.736	11.757
13)	MA Dieldrin	5.562	6.461	10856718	18069272	12.187	12.001
19)	B Endosulfa...	6.471	7.231	9340195	14888380	12.464	12.173
20)	A Methoxychlor	6.738	7.552	18646819	35293321	68.649	68.736
21)	B Endrin ke...	6.957	7.700	8701656	15235235	10.484	11.124
25)	Chlordane-3	5.212	6.083	5411714	9103716	59.565	45.817


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062119\
Data File : PD053677.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2019 9:11
Operator : SM\AJ
Sample : RESCHK
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampled :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 00:35:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
Quant Title : GC Extractables
QLast Update : Sat Jun 22 00:19:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

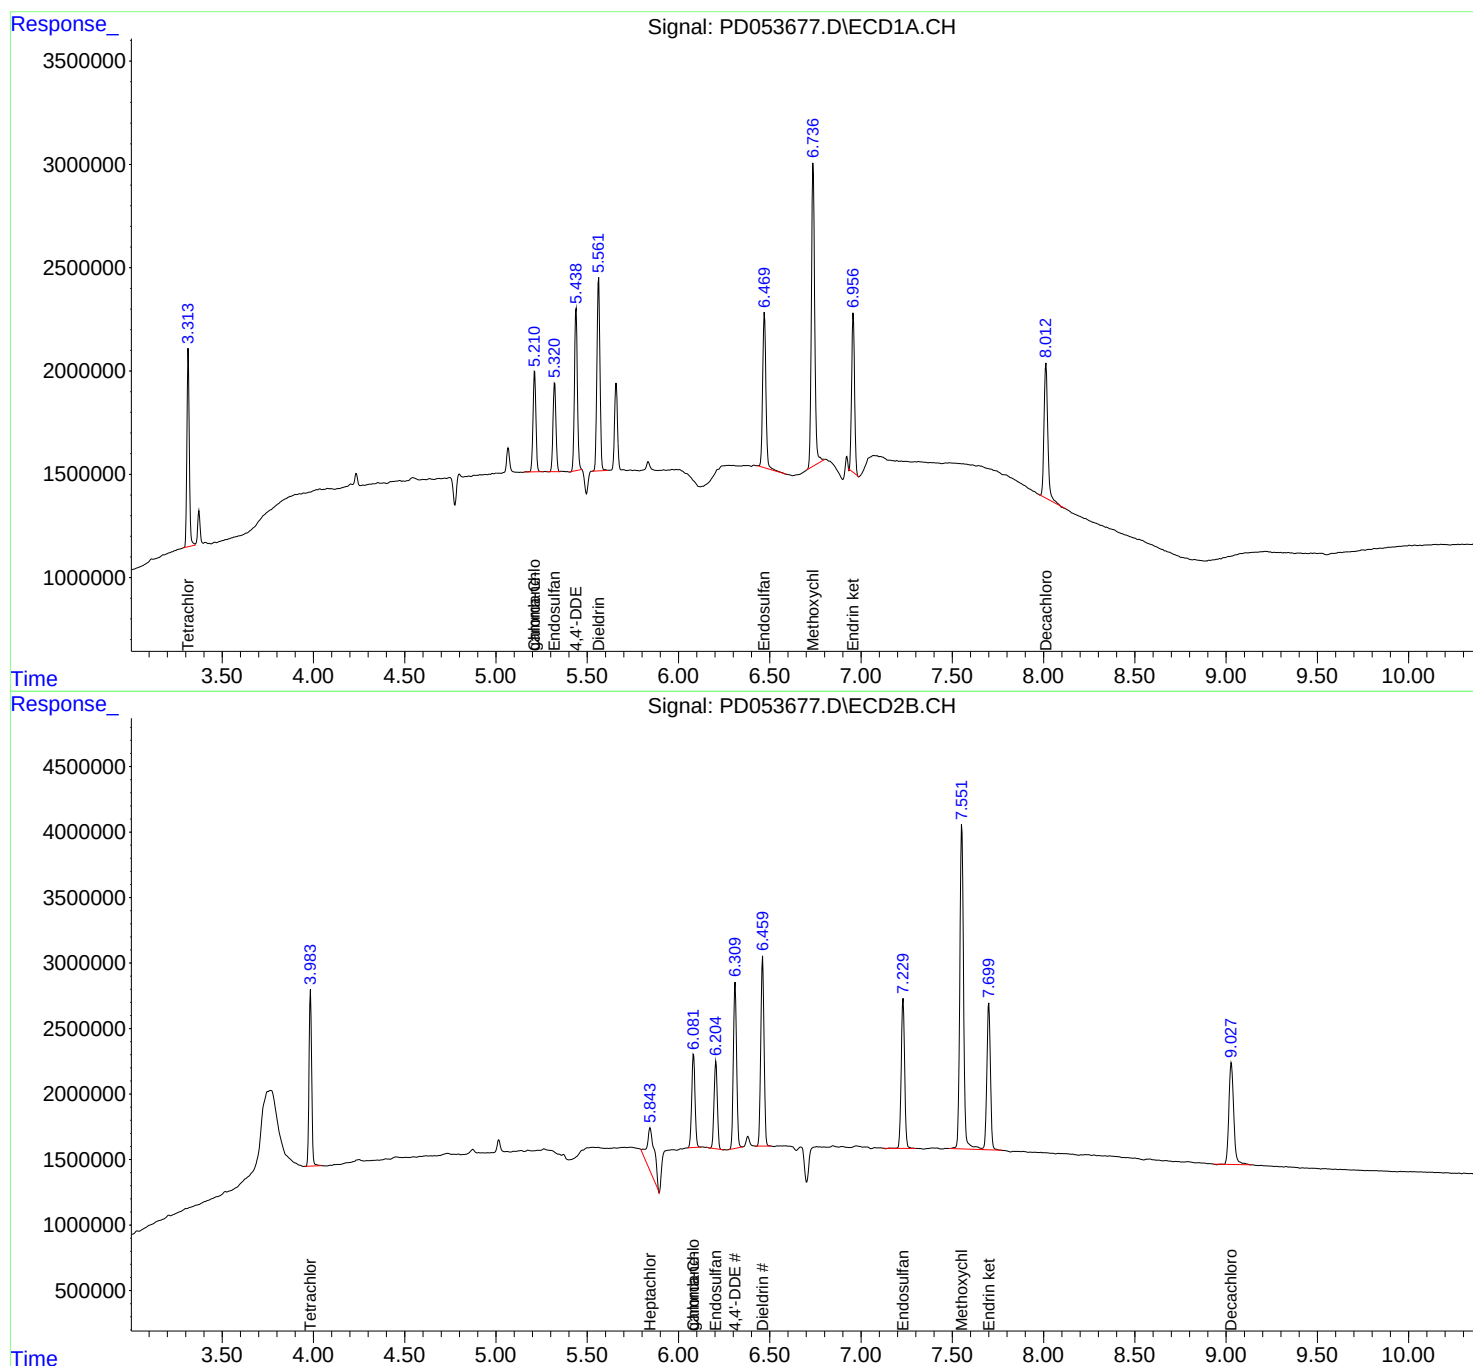


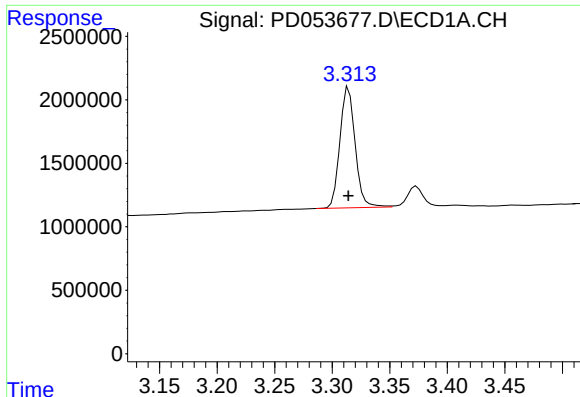

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: 0.000 min
Response: 8769217
Conc: 12.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

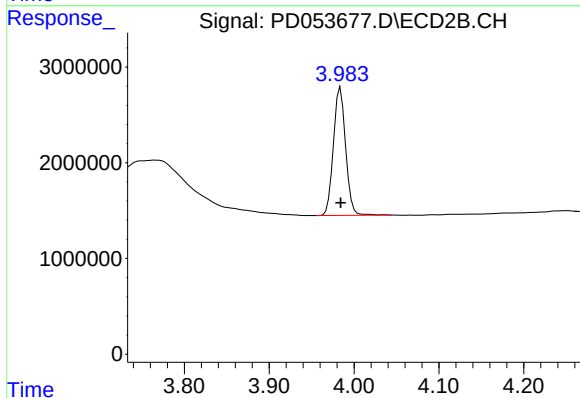


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: 0.000 min
Response: 13379006
Conc: 12.22 ng/ml

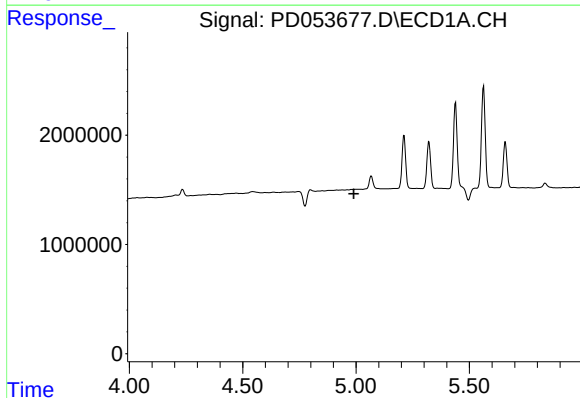


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.990 min
Response: 0
Conc: N.D.

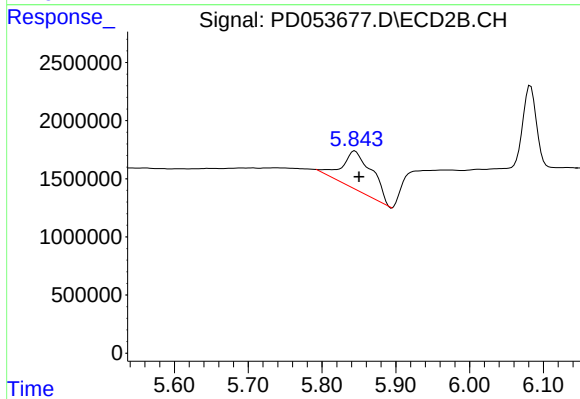

#8 Heptachlor epoxide


R.T.: 5.845 min
Delta R.T.: -0.005 min
Response: 9643643
Conc: 6.59 ng/ml

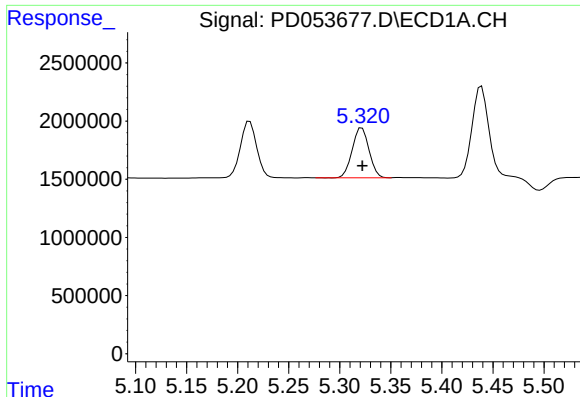

#9 Endosulfan I


R.T.: 5.322 min
Delta R.T.: 0.000 min
Response: 4902622
Conc: 6.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

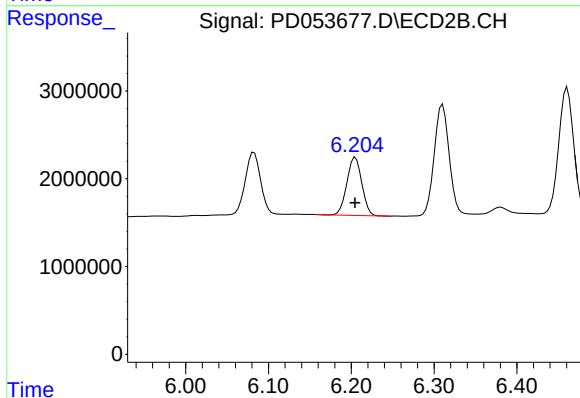


#9 Endosulfan I

R.T.: 6.205 min
Delta R.T.: 0.000 min
Response: 8301346
Conc: 6.04 ng/ml

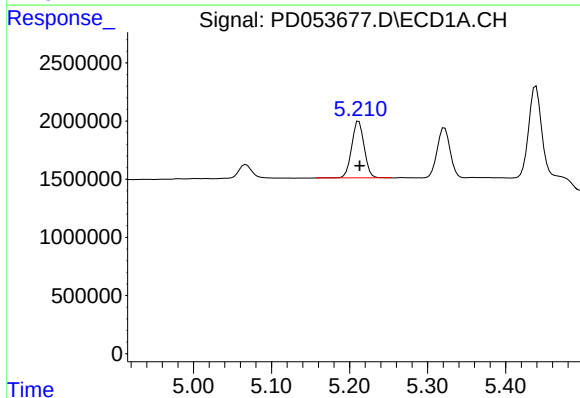


#10 gamma-Chlordane

R.T.: 5.212 min
Delta R.T.: -0.001 min
Response: 5411714
Conc: 6.04 ng/ml

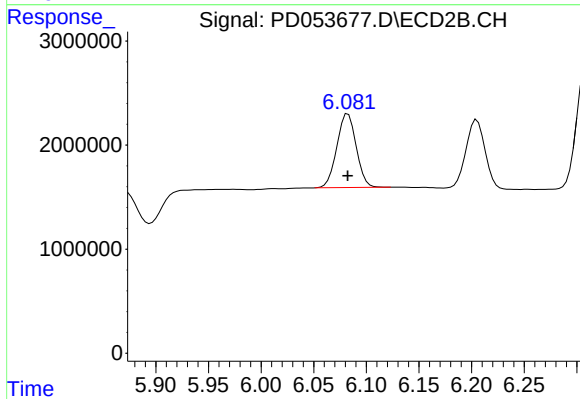

#10 gamma-Chlordane


R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 9103716
Conc: 5.78 ng/ml

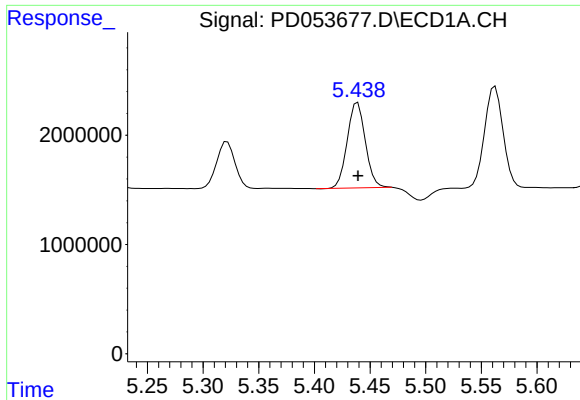

#12 4,4'-DDE


R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 8871596
Conc: 11.74 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

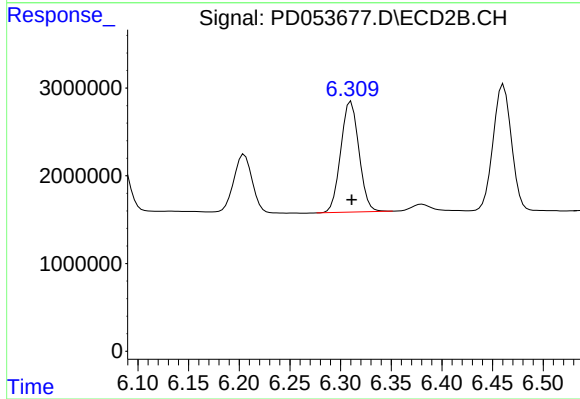


#12 4,4'-DDE

R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 15733888
Conc: 11.76 ng/ml

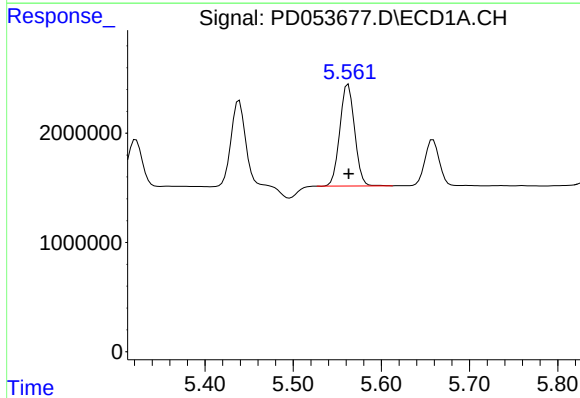


#13 Dieldrin

R.T.: 5.562 min
Delta R.T.: 0.000 min
Response: 10856718
Conc: 12.19 ng/ml

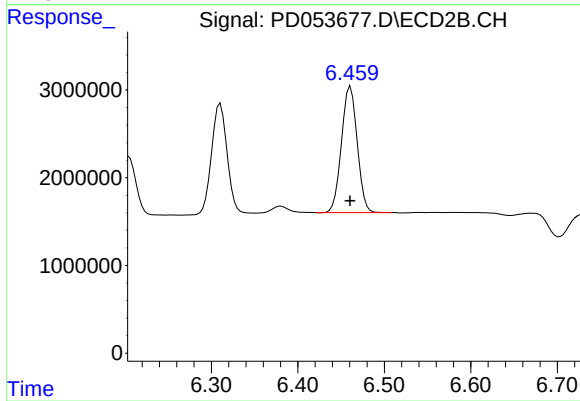

#13 Dieldrin


R.T.: 6.461 min
Delta R.T.: 0.000 min
Response: 18069272
Conc: 12.00 ng/ml

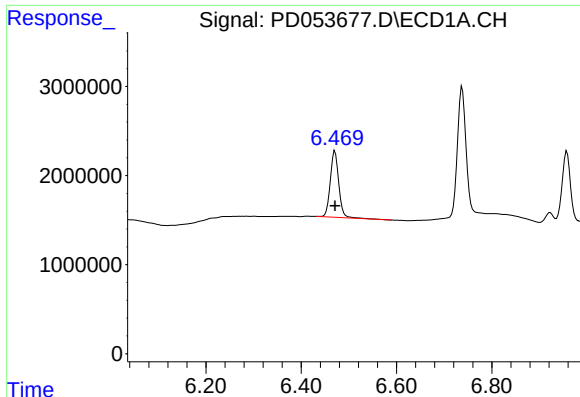

#19 Endosulfan Sulfate


R.T.: 6.471 min
Delta R.T.: 0.000 min
Response: 9340195
Conc: 12.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

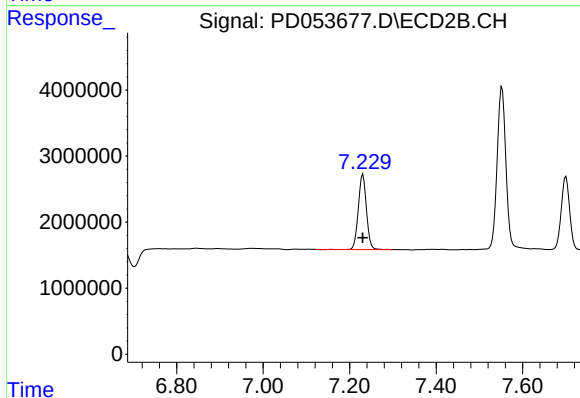


#19 Endosulfan Sulfate

R.T.: 7.231 min
Delta R.T.: 0.000 min
Response: 14888380
Conc: 12.17 ng/ml

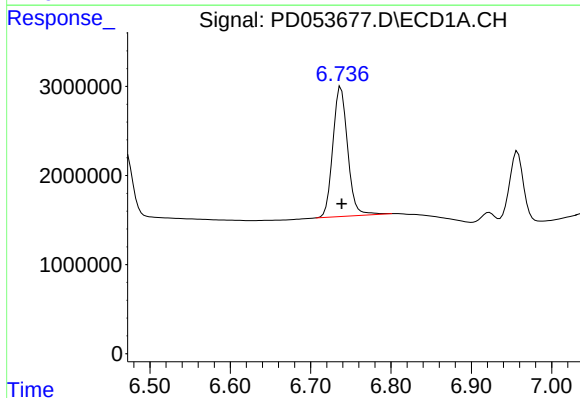


#20 Methoxychlor

R.T.: 6.738 min
Delta R.T.: -0.001 min
Response: 18646819
Conc: 68.65 ng/ml

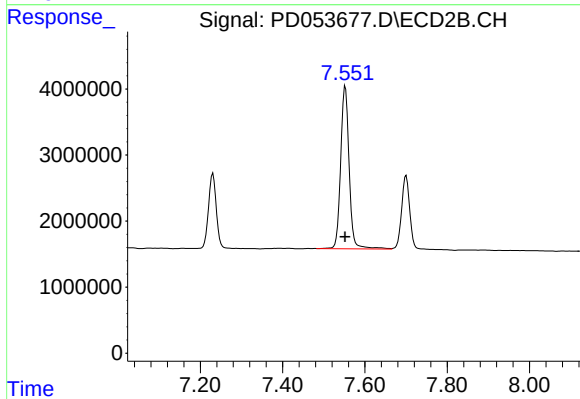

#20 Methoxychlor


R.T.: 7.552 min
Delta R.T.: 0.000 min
Response: 35293321
Conc: 68.74 ng/ml

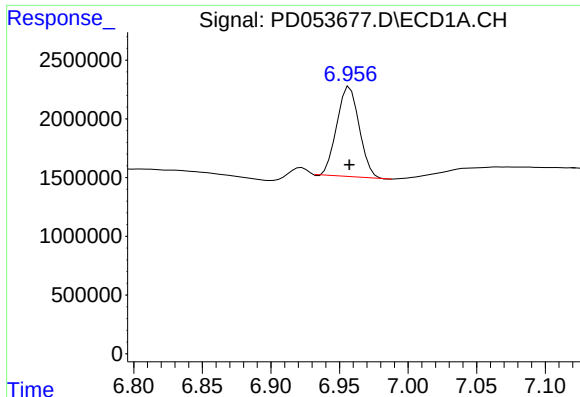

#21 Endrin ketone


R.T.: 6.957 min
Delta R.T.: 0.000 min
Response: 8701656
Conc: 10.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

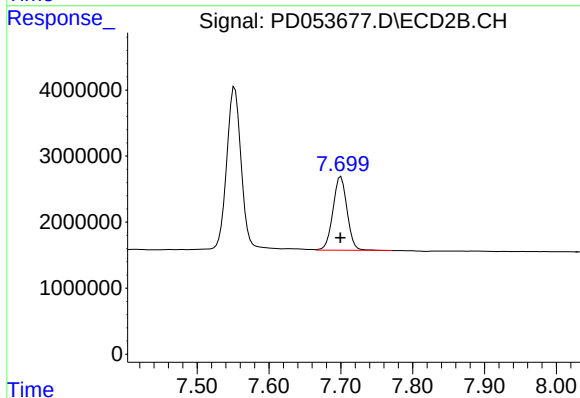


#21 Endrin ketone

R.T.: 7.700 min
Delta R.T.: 0.000 min
Response: 15235235
Conc: 11.12 ng/ml

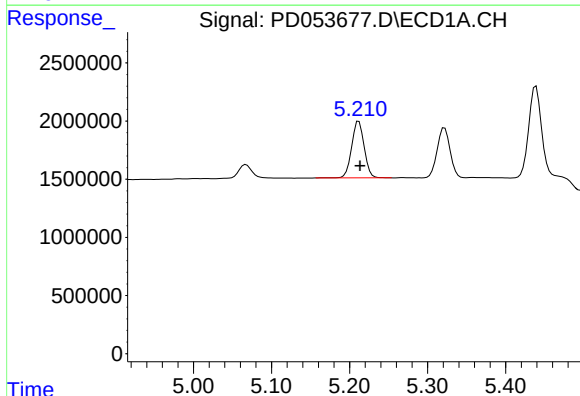


#25 Chlordane-3

R.T.: 5.212 min
Delta R.T.: -0.002 min
Response: 5411714
Conc: 59.56 ng/ml

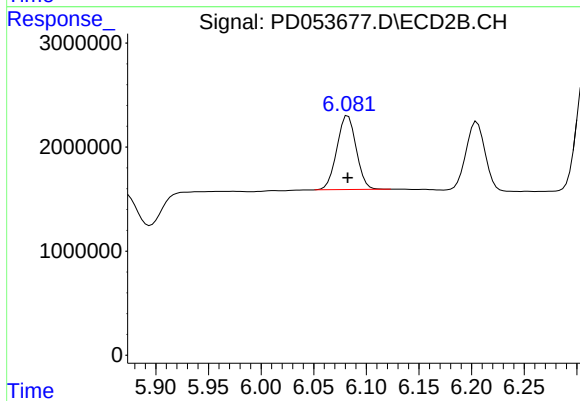

#25 Chlordane-3


R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 9103716
Conc: 45.82 ng/ml

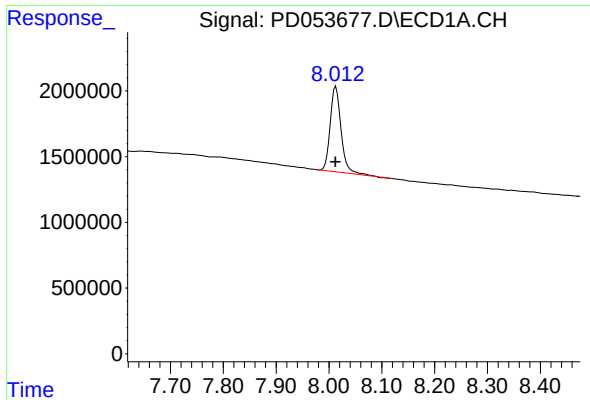

#28 Decachlorobiphenyl

R.T.: 8.013 min
Delta R.T.: 0.000 min
Response: 9232778
Conc: 14.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

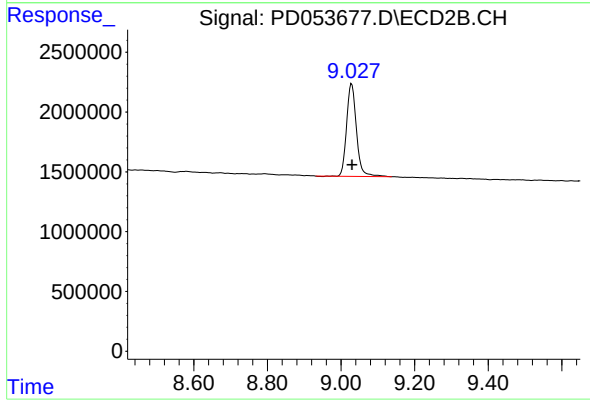

#28 Decachlorobiphenyl

R.T.: 9.029 min
Delta R.T.: 0.000 min
Response: 14440097
Conc: 14.28 ng/ml