

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062119\
 Data File : PD053691.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2019 12:45
 Operator : SM\AJ
 Sample : K3445-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EXT-008-SW116-061719

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 00:37:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 22 00:19:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.984	10397344	16199733	14.711	14.802
28)	SA Decachlor...	8.013	9.028	10212273	15546944	15.708	15.373
Target Compounds							
10)	B gamma-Chl...	5.215	6.082	2485623	7324521	2.775	4.651 #
11)	B alpha-Chl...	5.270	6.156	6498475	19916137	7.340	12.926 #
12)	B 4,4'-DDE	5.440	6.310	2315696	5339272	3.063	3.990 #
15)	B Endosulfa...	6.096	0.000	1557421	0	1.963	N.D. #
17)	MA 4,4'-DDT	6.188	7.096	3496997	6440416	5.704	6.006
25)	Chlordane-3	5.215	6.082	2485623	7324521	27.358	36.863 #
26)	Chlordane-4	5.270	6.156	6498475	19916137	76.310	84.916
27)	Chlordane-5	6.096	6.957	1557421	2970258	54.551	63.764



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062119\
Data File : PD053691.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2019 12:45
Operator : SM\AJ
Sample : K3445-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
EXT-008-SW116-061719

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 00:37:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
Quant Title : GC Extractables
QLast Update : Sat Jun 22 00:19:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

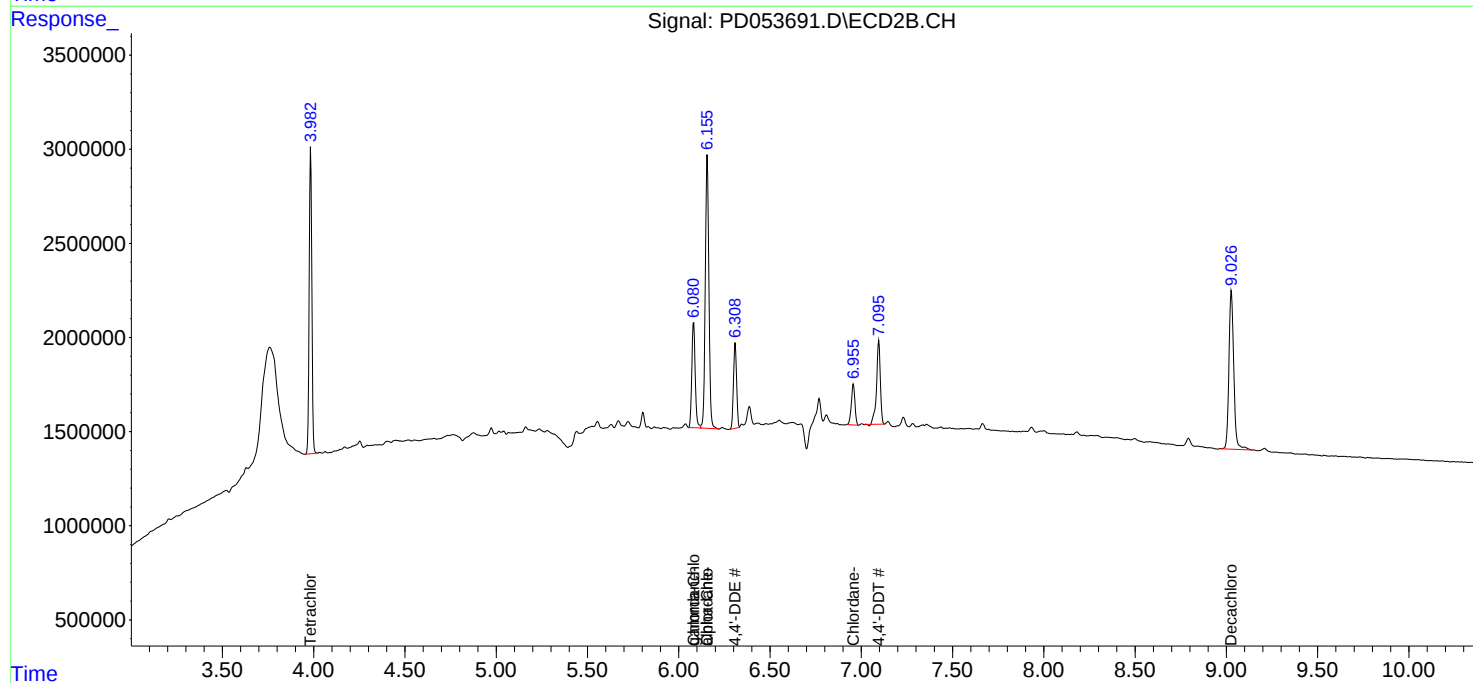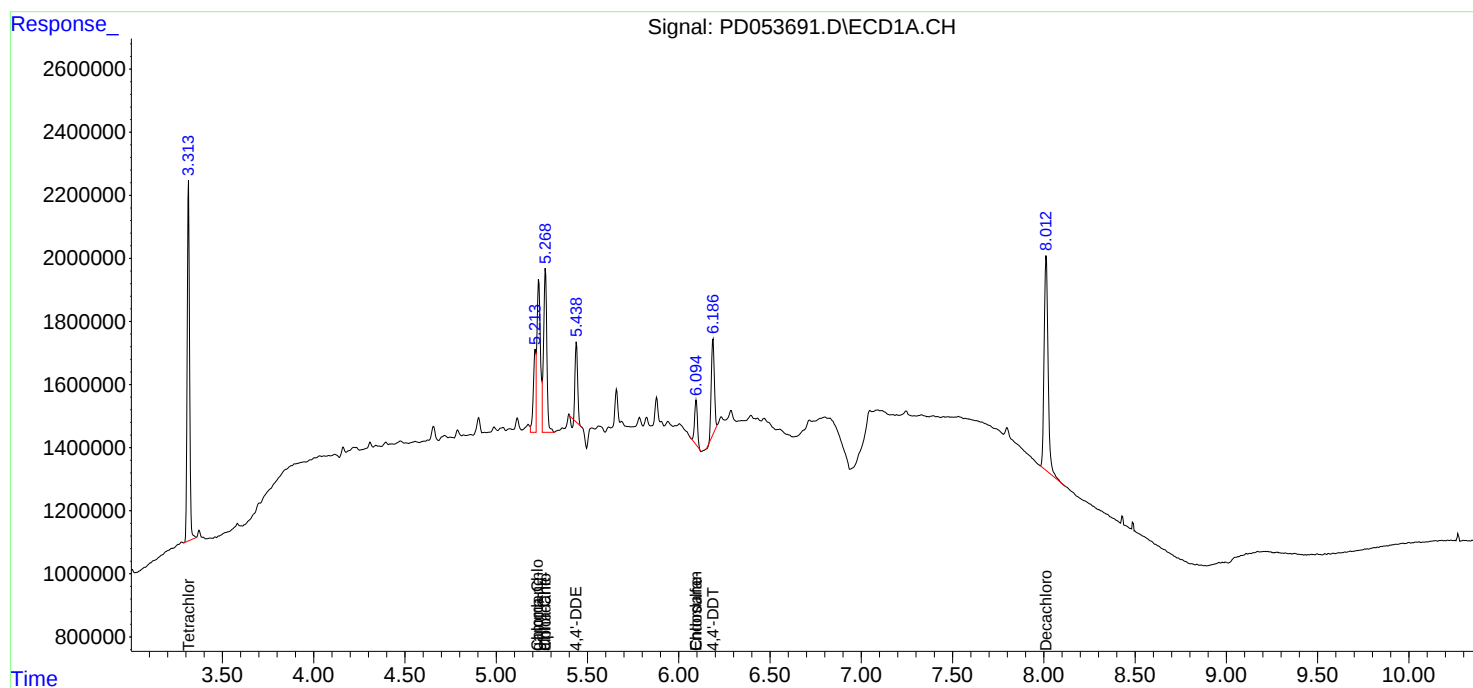


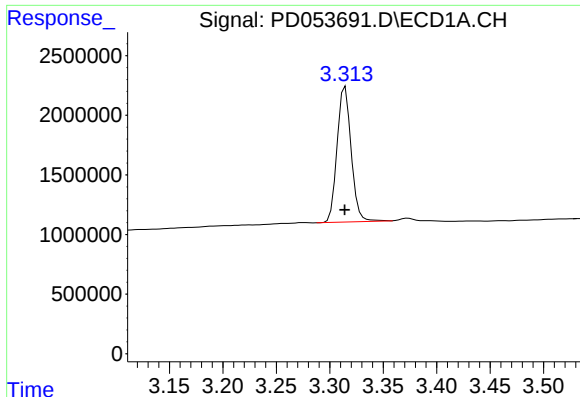

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: 0.000 min
Response: 10397344
Conc: 14.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
EXT-008-SW116-061719

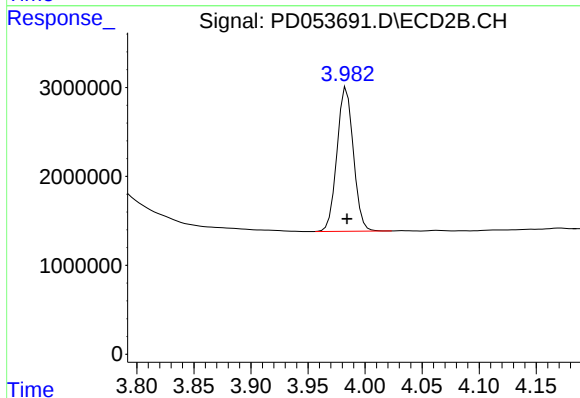


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: 0.000 min
Response: 16199733
Conc: 14.80 ng/ml

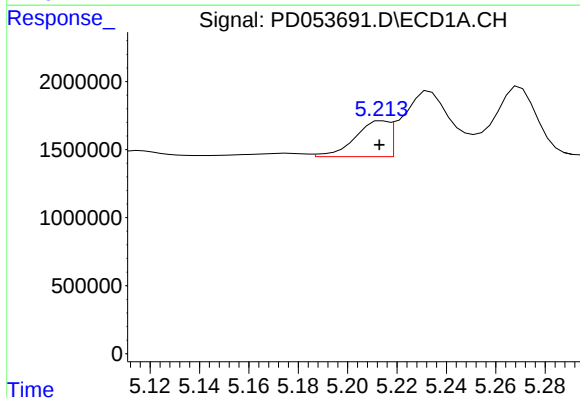


#10 gamma-Chlordane

R.T.: 5.215 min
Delta R.T.: 0.002 min
Response: 2485623
Conc: 2.77 ng/ml

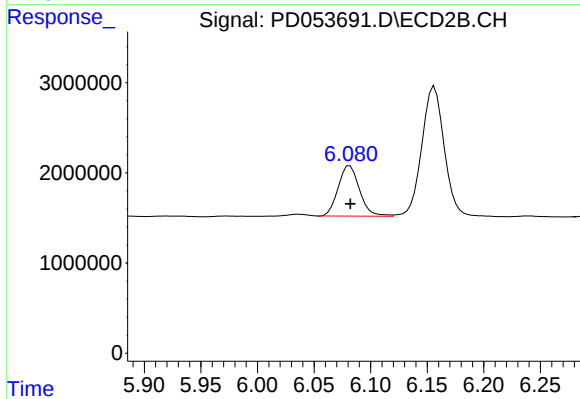

#10 gamma-Chlordane


R.T.: 6.082 min
Delta R.T.: 0.000 min
Response: 7324521
Conc: 4.65 ng/ml

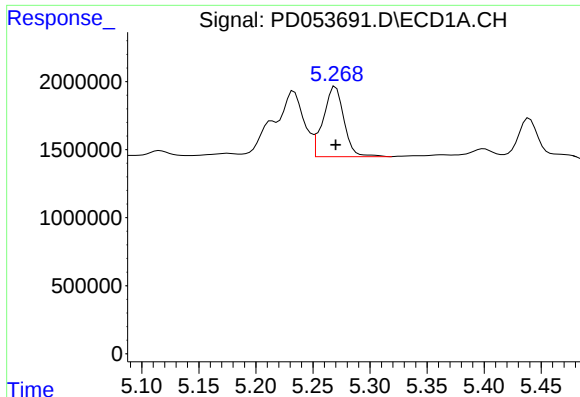

#11 alpha-Chlordane


R.T.: 5.270 min
Delta R.T.: 0.000 min
Response: 6498475
Conc: 7.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
EXT-008-SW116-061719

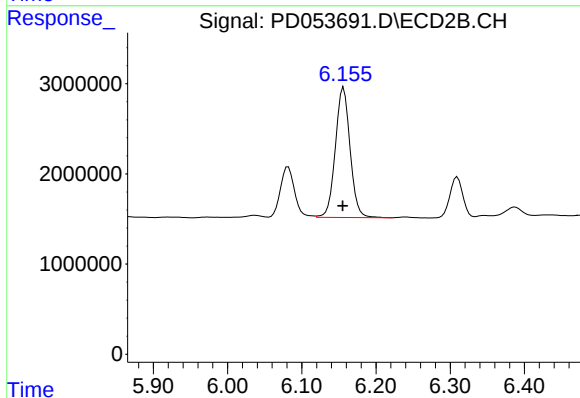


#11 alpha-Chlordane

R.T.: 6.156 min
Delta R.T.: 0.001 min
Response: 19916137
Conc: 12.93 ng/ml

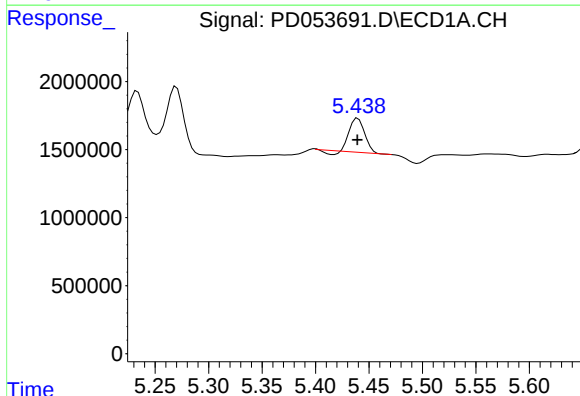


#12 4,4'-DDE

R.T.: 5.440 min
Delta R.T.: 0.000 min
Response: 2315696
Conc: 3.06 ng/ml

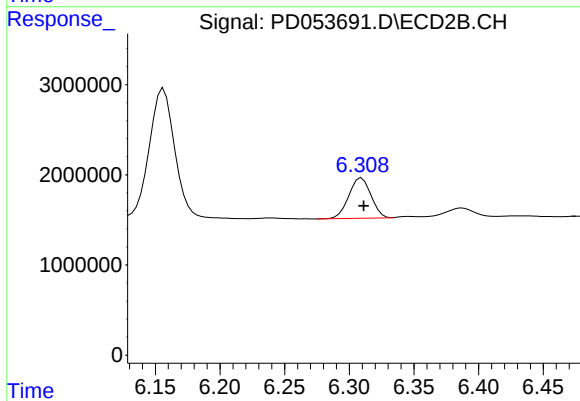

#12 4,4'-DDE


R.T.: 6.310 min
Delta R.T.: -0.002 min
Response: 5339272
Conc: 3.99 ng/ml

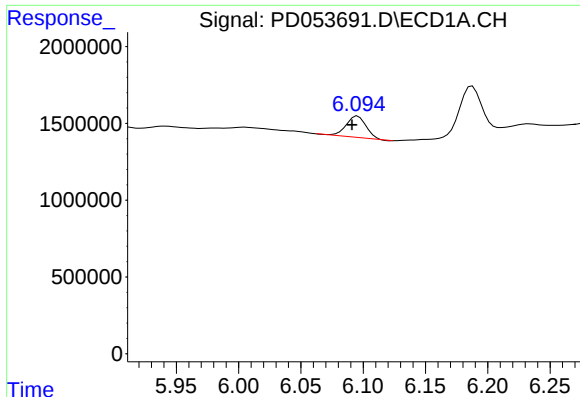

#15 Endosulfan II


R.T.: 6.096 min
Delta R.T.: 0.005 min
Response: 1557421
Conc: 1.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
EXT-008-SW116-061719

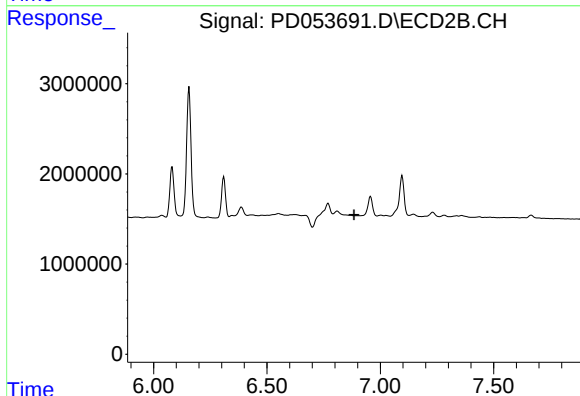


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.885 min
Response: 0
Conc: N.D.

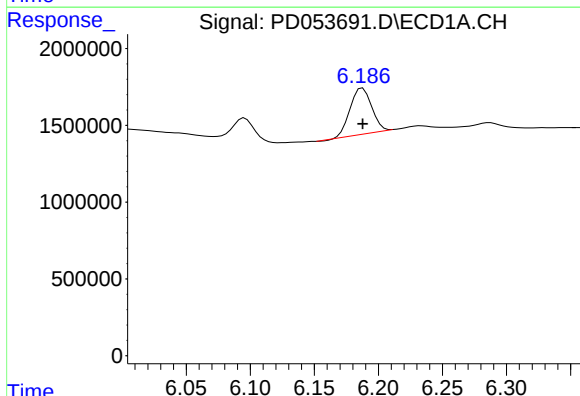


#17 4,4'-DDT

R.T.: 6.188 min
Delta R.T.: 0.000 min
Response: 3496997
Conc: 5.70 ng/ml

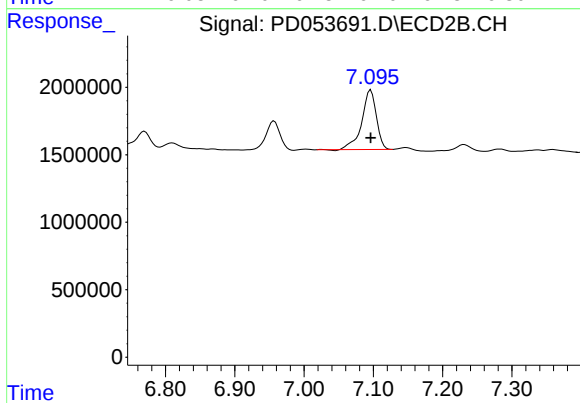

#17 4,4'-DDT


R.T.: 7.096 min
Delta R.T.: 0.000 min
Response: 6440416
Conc: 6.01 ng/ml

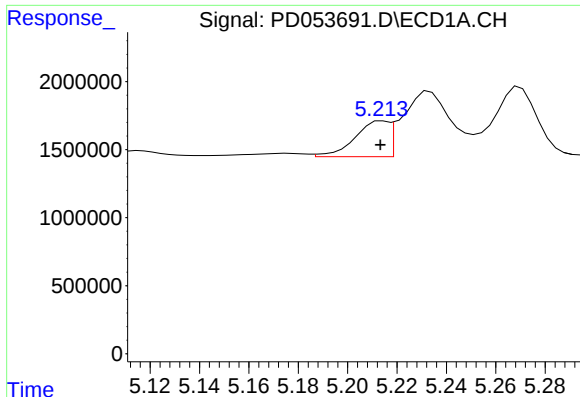

#25 Chlordane-3


R.T.: 5.215 min
Delta R.T.: 0.001 min
Response: 2485623
Conc: 27.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
EXT-008-SW116-061719

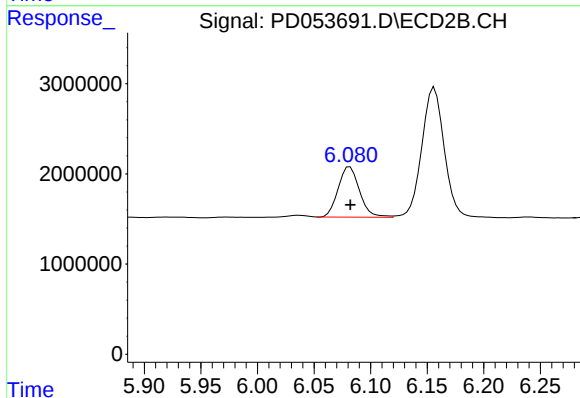


#25 Chlordane-3

R.T.: 6.082 min
Delta R.T.: 0.000 min
Response: 7324521
Conc: 36.86 ng/ml

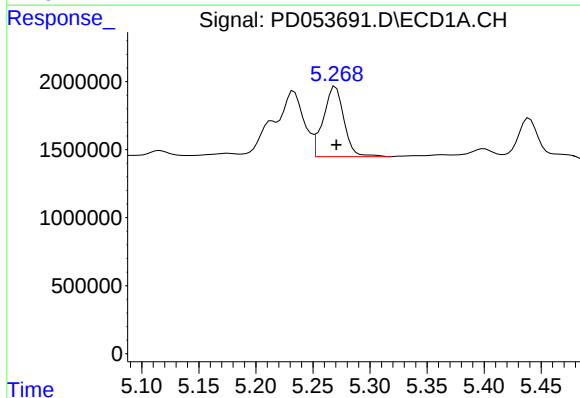


#26 Chlordane-4

R.T.: 5.270 min
Delta R.T.: 0.000 min
Response: 6498475
Conc: 76.31 ng/ml

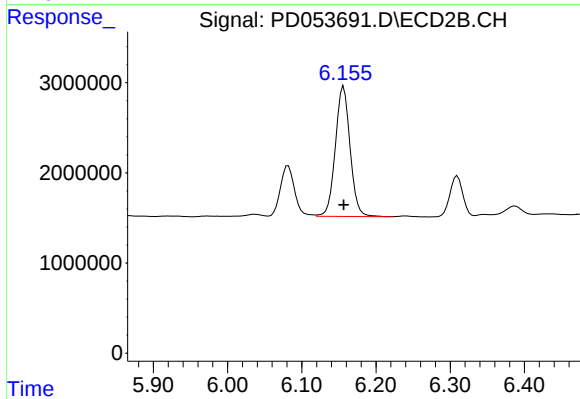

#26 Chlordane-4


R.T.: 6.156 min
Delta R.T.: 0.000 min
Response: 19916137
Conc: 84.92 ng/ml

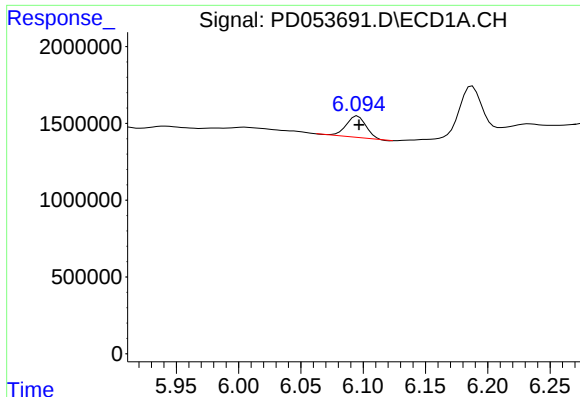

#27 Chlordane-5


R.T.: 6.096 min
Delta R.T.: -0.001 min
Response: 1557421
Conc: 54.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
EXT-008-SW116-061719

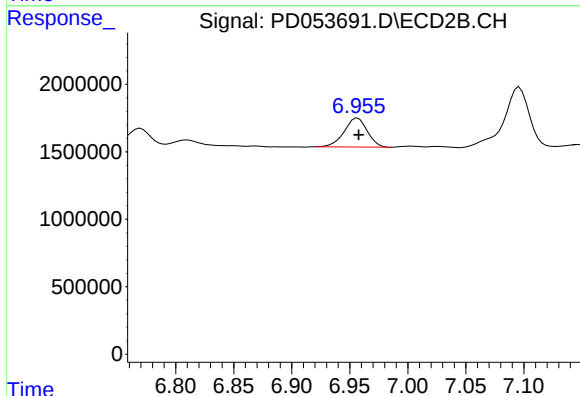


#27 Chlordane-5

R.T.: 6.957 min
Delta R.T.: 0.000 min
Response: 2970258
Conc: 63.76 ng/ml

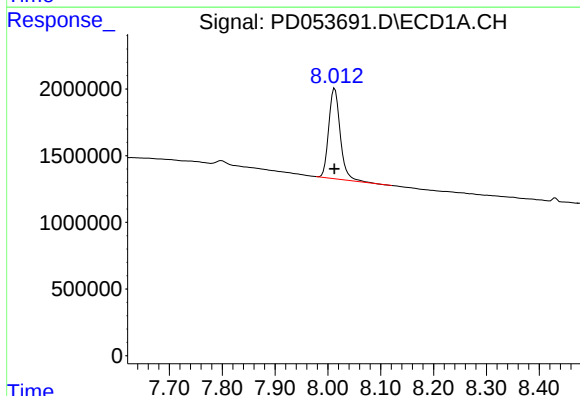

#28 Decachlorobiphenyl

R.T.: 8.013 min
Delta R.T.: 0.000 min
Response: 10212273
Conc: 15.71 ng/ml

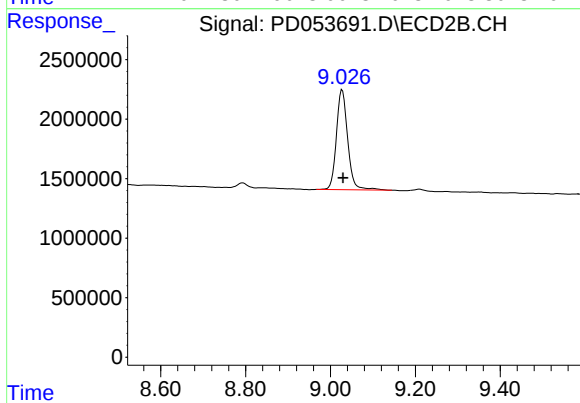

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.002 min
Response: 15546944
Conc: 15.37 ng/ml