

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062119\
 Data File : PD053694.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2019 13:26
 Operator : SM\AJ
 Sample : K3445-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EXT-008-SW112-061719

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 00:37:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 22 00:19:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.984	11052696	17314222	15.638	15.821
28)	SA Decachlor...	8.013	9.028	11191375	16787588	17.214	16.599
Target Compounds							
10)	B gamma-Chl...	5.213	6.082	1972117	4860404	2.202	3.086 #
11)	B alpha-Chl...	5.269	6.157	4053541	10745421	4.578	6.974 #
12)	B 4,4'-DDE	5.439	6.310	1349066	2949767	1.785	2.204
17)	MA 4,4'-DDT	6.187	7.096	2044138	4061062	3.334	3.787
25)	Chlordane-3	5.213	6.082	1972117	4860404	21.706	24.462
26)	Chlordane-4	5.269	6.157	4053541	10745421	47.600	45.815
27)	Chlordane-5	0.000	6.958	0	1550323	N.D.	33.282 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062119\
Data File : PD053694.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2019 13:26
Operator : SM\AJ
Sample : K3445-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
EXT-008-SW112-061719

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 00:37:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
Quant Title : GC Extractables
QLast Update : Sat Jun 22 00:19:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

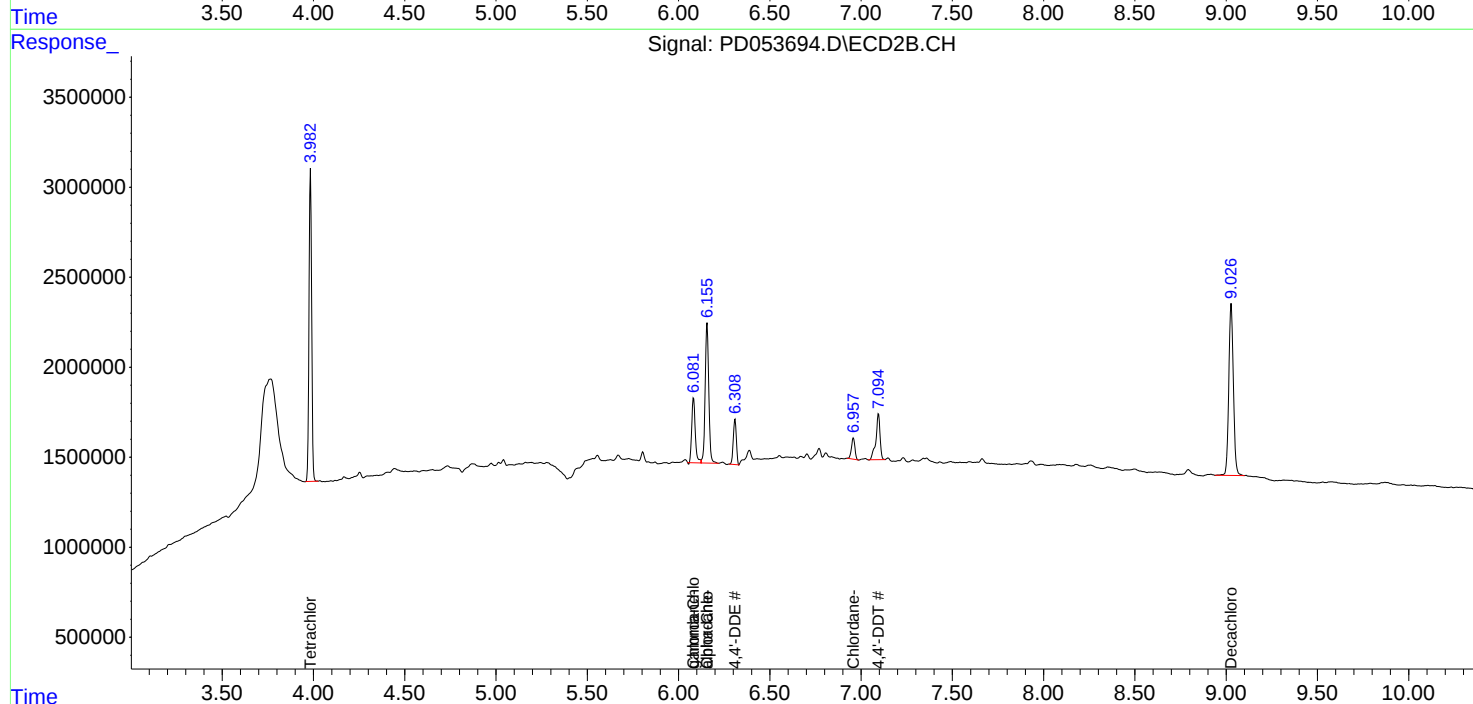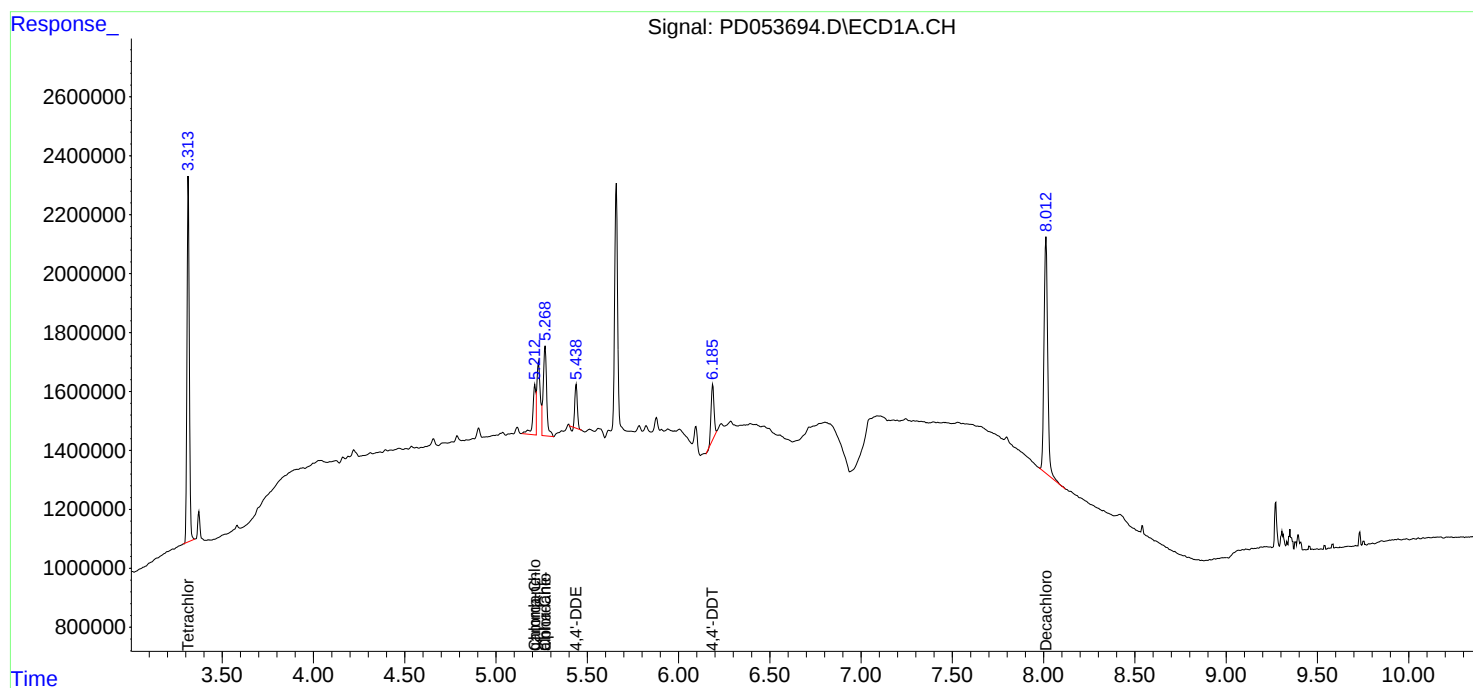


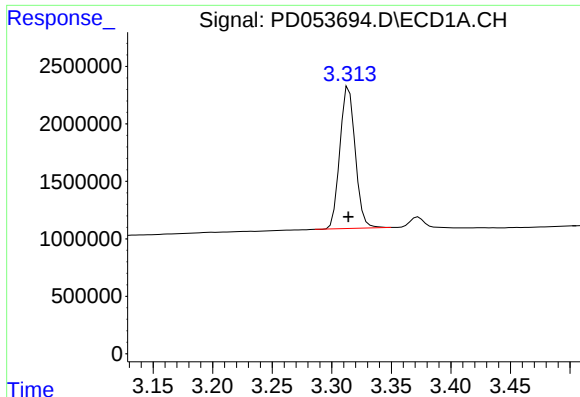

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: 0.000 min
Response: 11052696
Conc: 15.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
EXT-008-SW112-061719

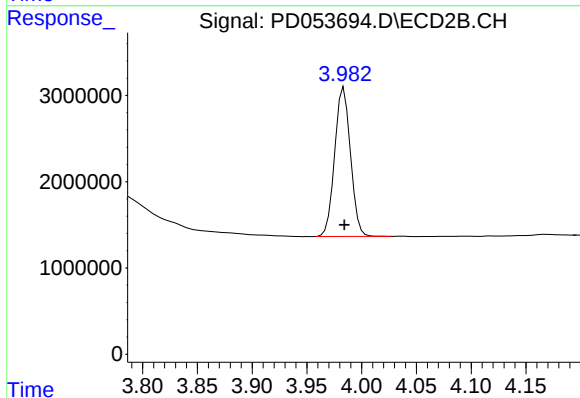


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: 0.000 min
Response: 17314222
Conc: 15.82 ng/ml

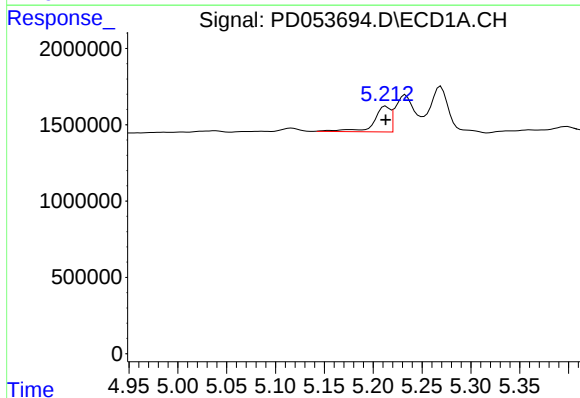


#10 gamma-Chlordane

R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 1972117
Conc: 2.20 ng/ml

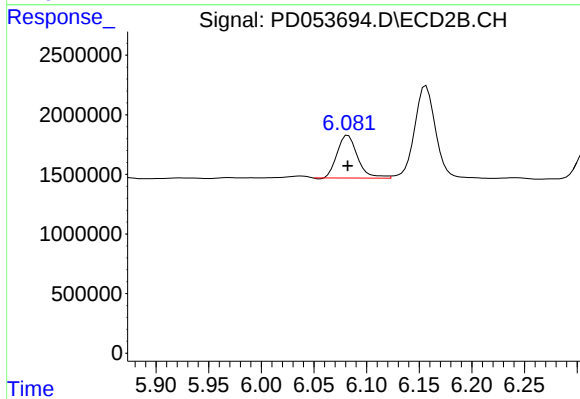

#10 gamma-Chlordane


R.T.: 6.082 min
Delta R.T.: 0.000 min
Response: 4860404
Conc: 3.09 ng/ml

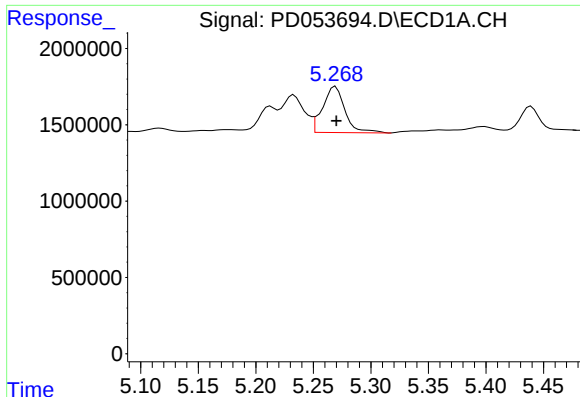

#11 alpha-Chlordane


R.T.: 5.269 min
Delta R.T.: 0.000 min
Response: 4053541
Conc: 4.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
EXT-008-SW112-061719

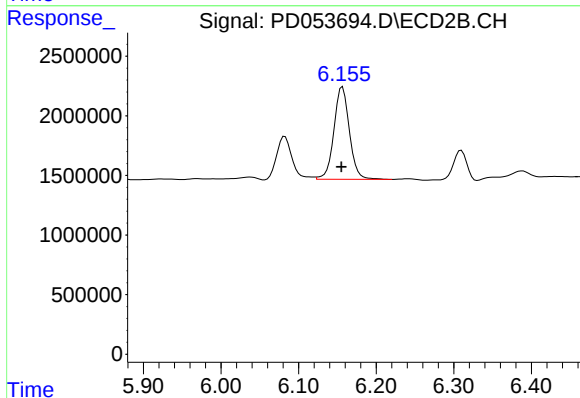


#11 alpha-Chlordane

R.T.: 6.157 min
Delta R.T.: 0.001 min
Response: 10745421
Conc: 6.97 ng/ml

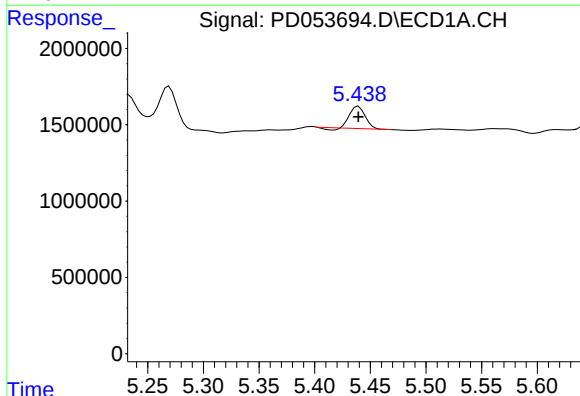


#12 4,4'-DDE

R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 1349066
Conc: 1.78 ng/ml

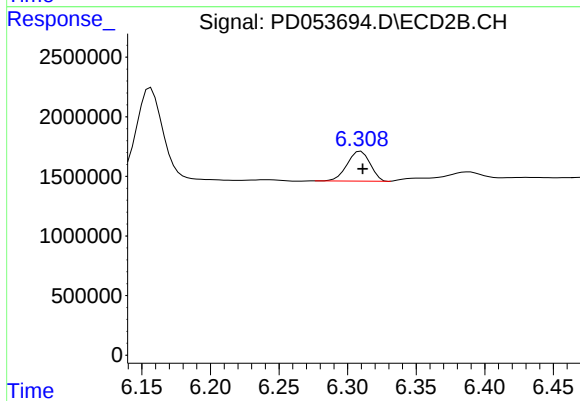

#12 4,4'-DDE


R.T.: 6.310 min
Delta R.T.: -0.001 min
Response: 2949767
Conc: 2.20 ng/ml

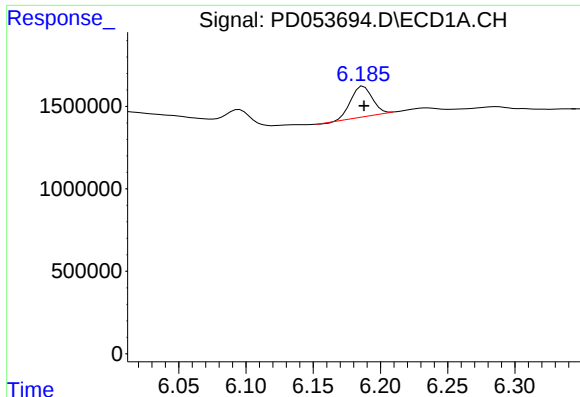

#17 4,4'-DDT


R.T.: 6.187 min
Delta R.T.: 0.000 min
Response: 2044138
Conc: 3.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
EXT-008-SW112-061719

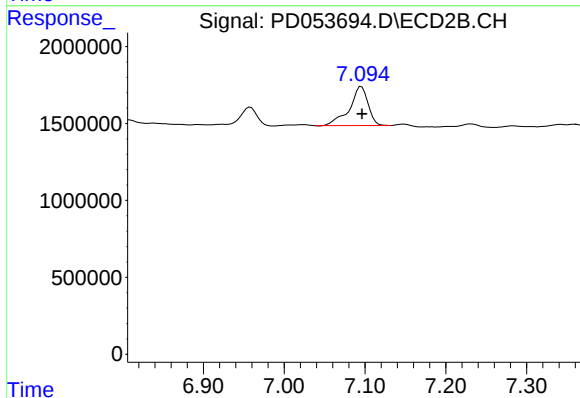


#17 4,4'-DDT

R.T.: 7.096 min
Delta R.T.: 0.000 min
Response: 4061062
Conc: 3.79 ng/ml

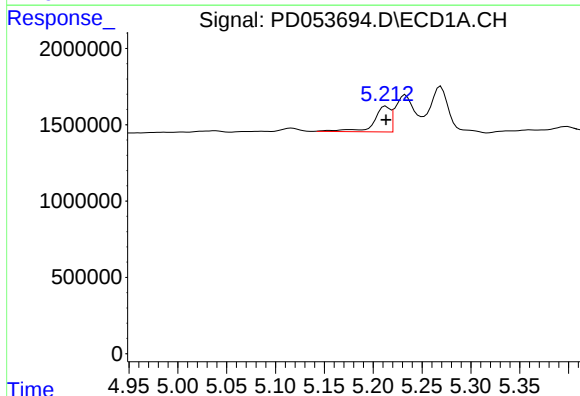


#25 Chlordane-3

R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 1972117
Conc: 21.71 ng/ml

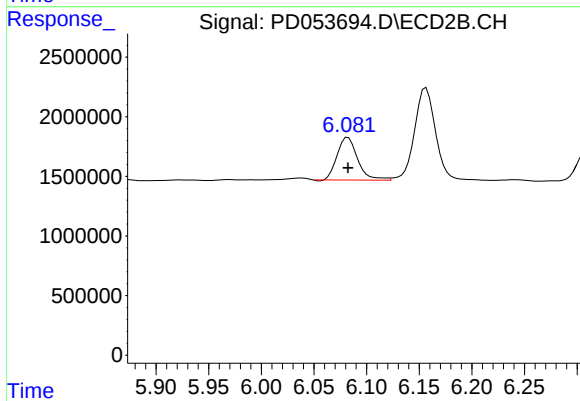

#25 Chlordane-3


R.T.: 6.082 min
Delta R.T.: 0.000 min
Response: 4860404
Conc: 24.46 ng/ml

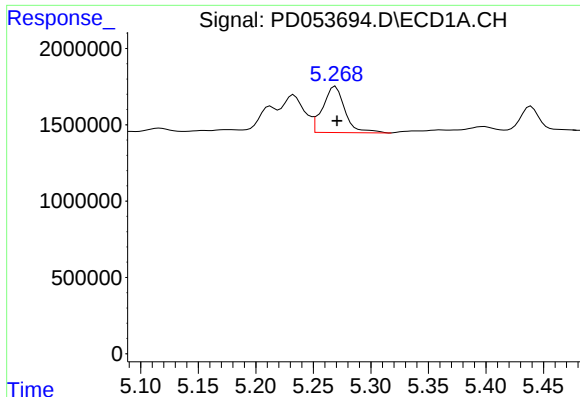

#26 Chlordane-4


R.T.: 5.269 min
Delta R.T.: -0.001 min
Response: 4053541
Conc: 47.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
EXT-008-SW112-061719

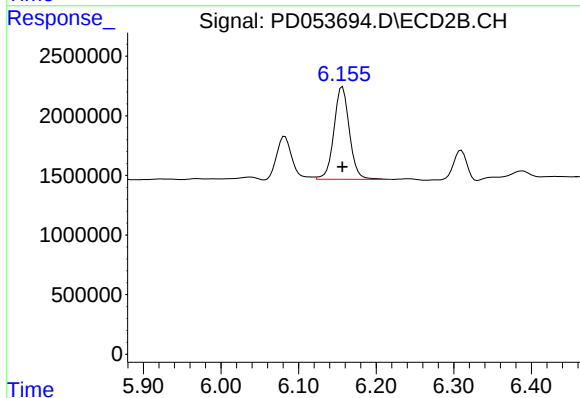


#26 Chlordane-4

R.T.: 6.157 min
Delta R.T.: 0.000 min
Response: 10745421
Conc: 45.81 ng/ml

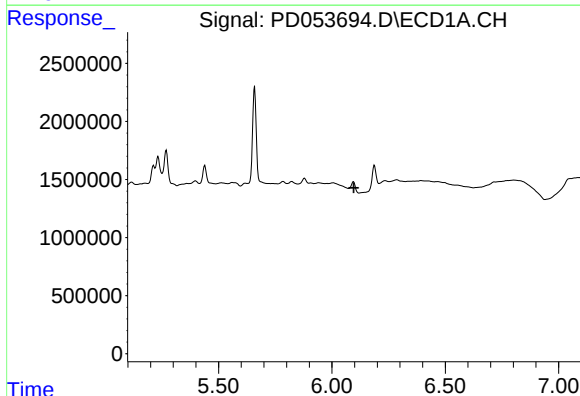


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.097 min
Response: 0
Conc: N.D.

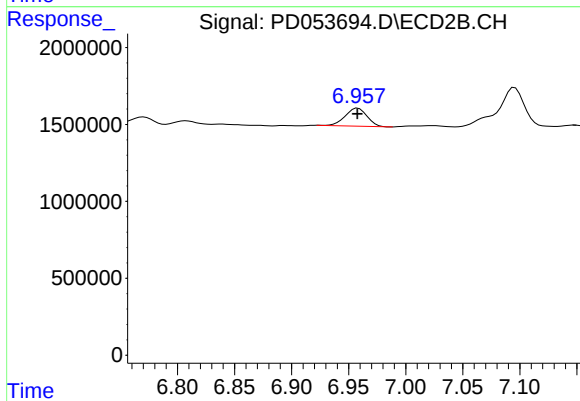

#27 Chlordane-5


R.T.: 6.958 min
Delta R.T.: 0.000 min
Response: 1550323
Conc: 33.28 ng/ml

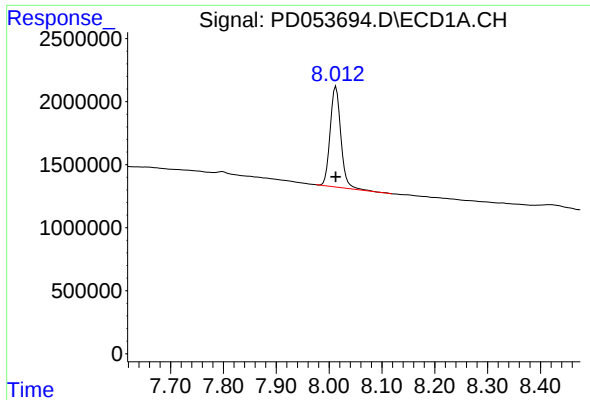

#28 Decachlorobiphenyl

R.T.: 8.013 min
Delta R.T.: 0.000 min
Response: 11191375
Conc: 17.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
EXT-008-SW112-061719

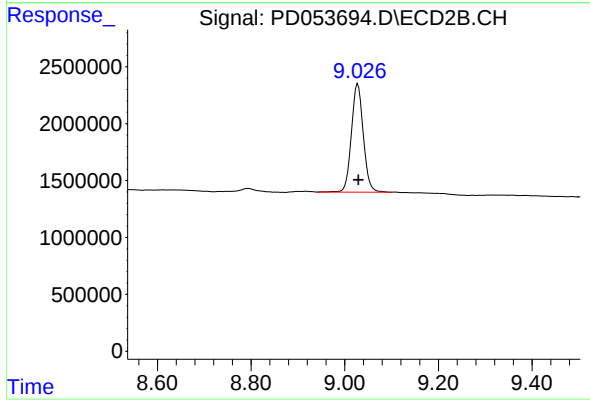

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.002 min
Response: 16787588
Conc: 16.60 ng/ml