

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062119\
 Data File : PD053702.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jun 2019 15:17
 Operator : SM\AJ
 Sample : K3445-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EXT-007-SW124-061819

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 00:38:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
 Quant Title : GC Extractables
 QLast Update : Sat Jun 22 00:19:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.984	13793336	21248783	19.515	19.416
28)	SA Decachlor...	8.011	9.027	10431912	15088322	16.046	14.919
Target Compounds							
9)	A Endosulfan I	5.349f	0.000	1175419	0	1.443	N.D. #
10)	B gamma-Chl...	0.000	6.071	0	1604876	N.D.	1.019 #
12)	B 4,4'-DDE	5.439	6.309	1761950	3080846	2.331	2.302
17)	MA 4,4'-DDT	6.187	7.095	1642887	1840214	2.680	1.716 #
25)	Chlordane-3	0.000	6.071	0	1604876	N.D.	8.077 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062119\
Data File : PD053702.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jun 2019 15:17
Operator : SM\AJ
Sample : K3445-10
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
EXT-007-SW124-061819

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 00:38:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062119.M
Quant Title : GC Extractables
QLast Update : Sat Jun 22 00:19:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

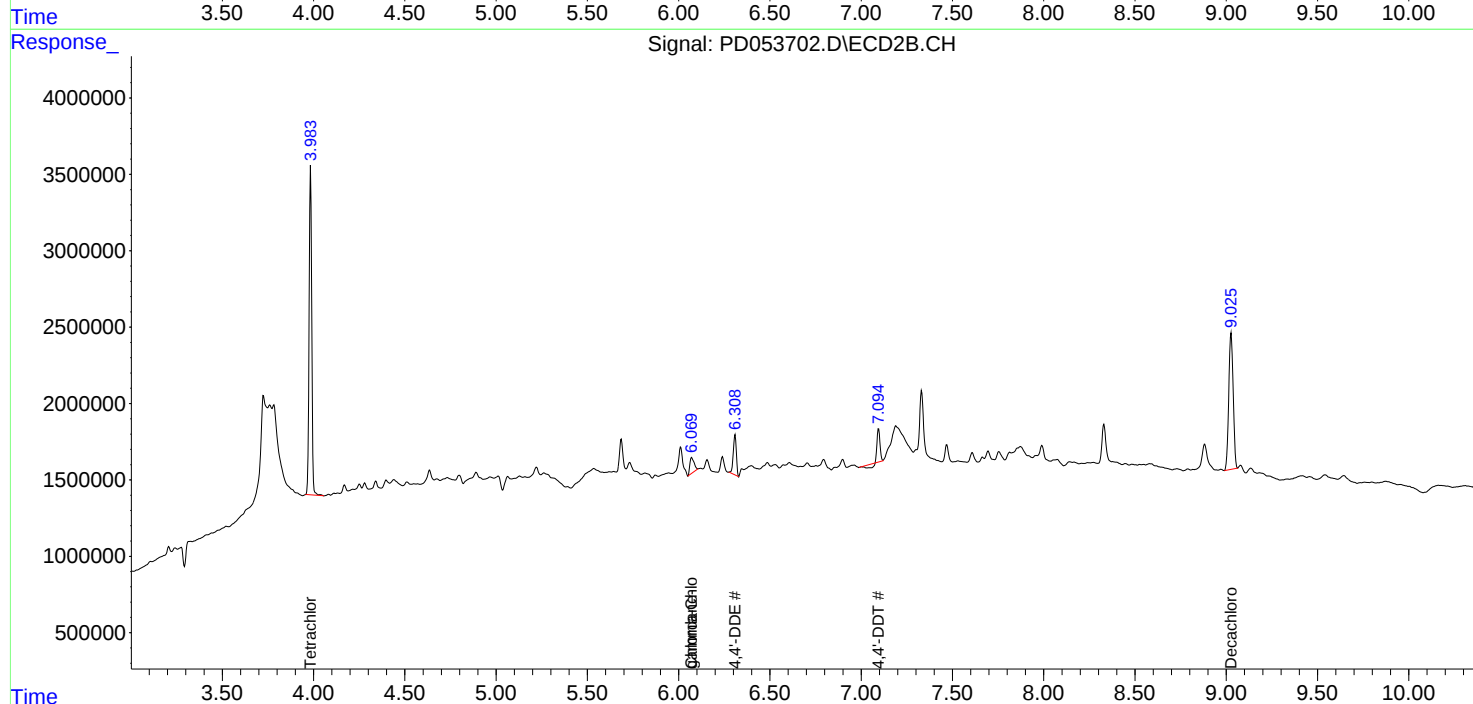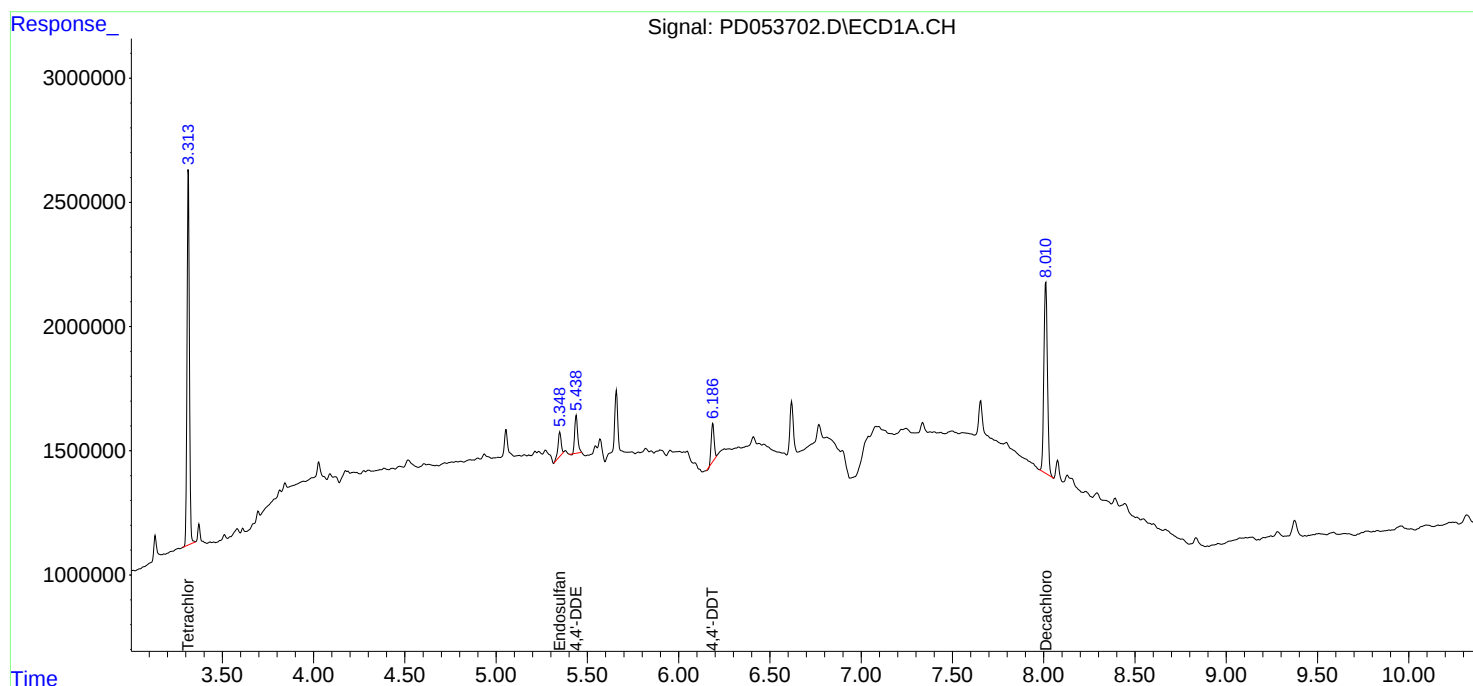


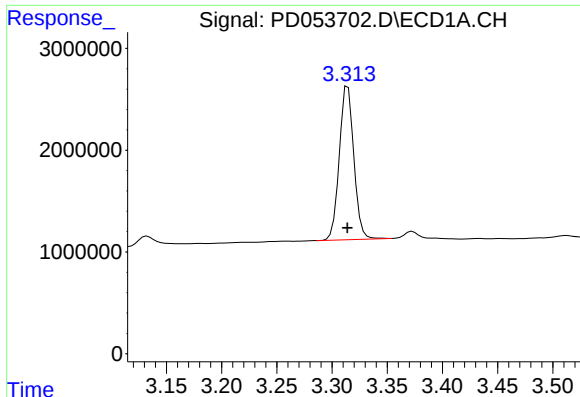

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: 0.000 min
Response: 13793336
Conc: 19.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
EXT-007-SW124-061819

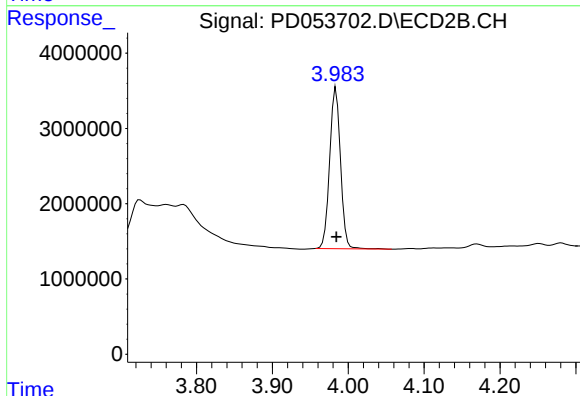


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: 0.000 min
Response: 21248783
Conc: 19.42 ng/ml

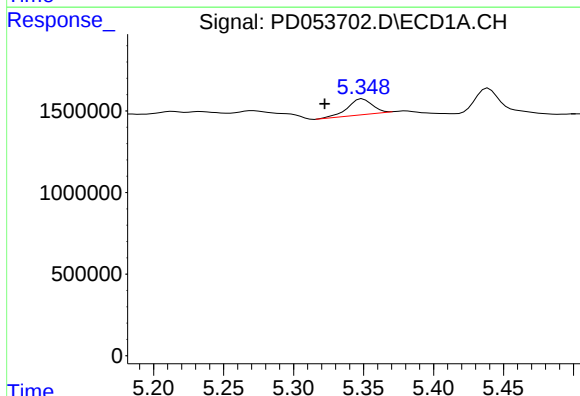


#9 Endosulfan I

R.T.: 5.349 min
Delta R.T.: 0.027 min
Response: 1175419
Conc: 1.44 ng/ml

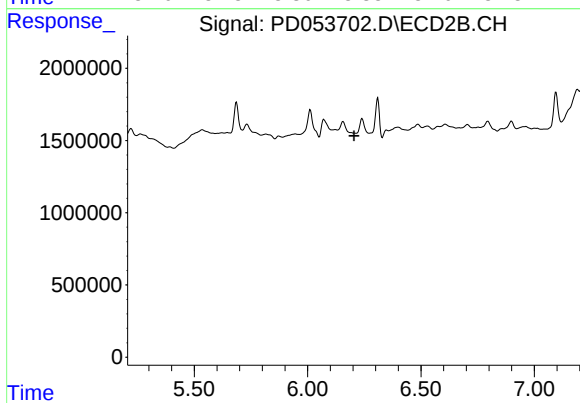

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

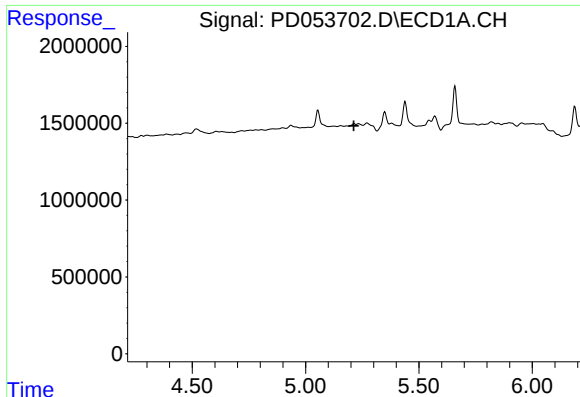

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.213 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
EXT-007-SW124-061819

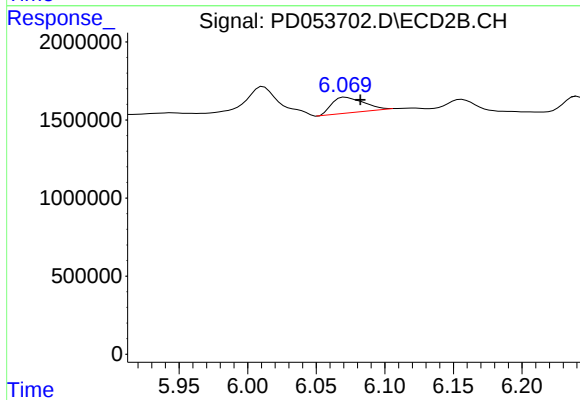


#10 gamma-Chlordane

R.T.: 6.071 min
Delta R.T.: -0.011 min
Response: 1604876
Conc: 1.02 ng/ml

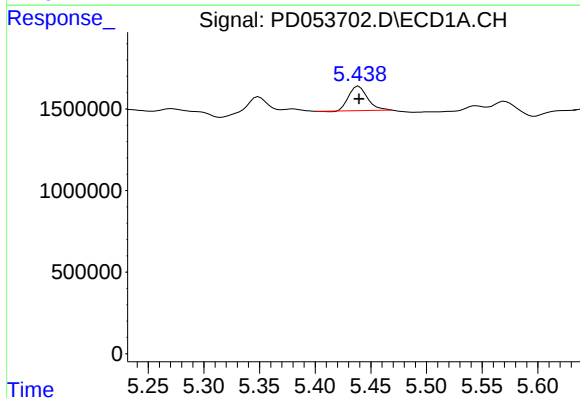


#12 4,4'-DDE

R.T.: 5.439 min
Delta R.T.: 0.000 min
Response: 1761950
Conc: 2.33 ng/ml

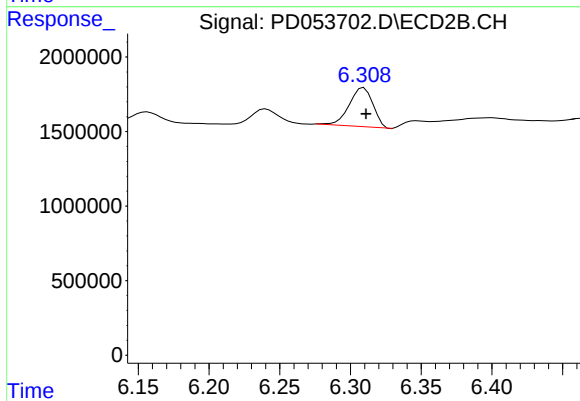

#12 4,4'-DDE


R.T.: 6.309 min
Delta R.T.: -0.002 min
Response: 3080846
Conc: 2.30 ng/ml

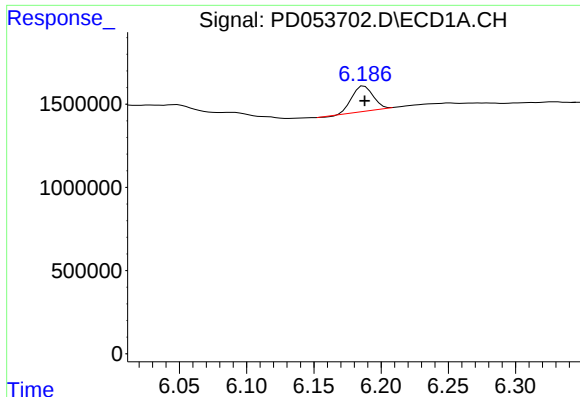

#17 4,4'-DDT


R.T.: 6.187 min
Delta R.T.: 0.000 min
Response: 1642887
Conc: 2.68 ng/ml

Instrument :
ECD_D
ClientSampleId :
EXT-007-SW124-061819

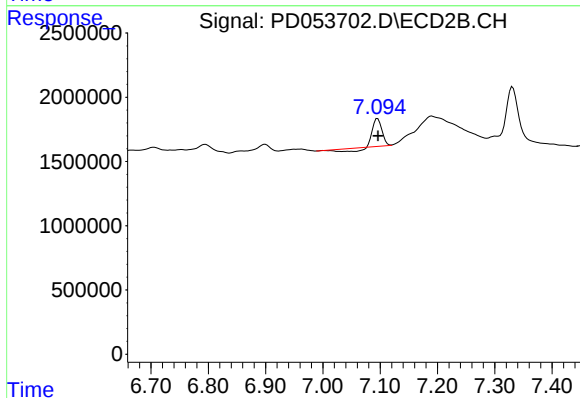


#17 4,4'-DDT

R.T.: 7.095 min
Delta R.T.: 0.000 min
Response: 1840214
Conc: 1.72 ng/ml

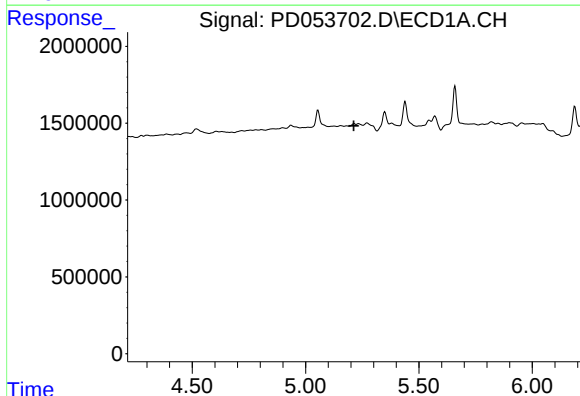


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.213 min
Response: 0
Conc: N.D.

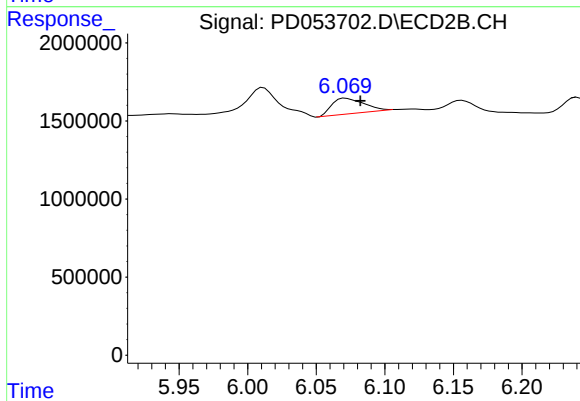

#25 Chlordane-3


R.T.: 6.071 min
Delta R.T.: -0.011 min
Response: 1604876
Conc: 8.08 ng/ml

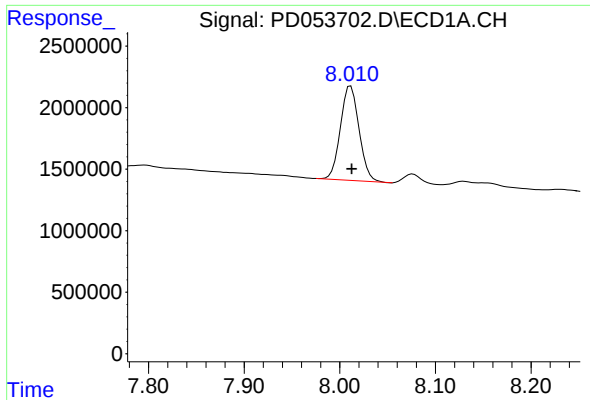

#28 Decachlorobiphenyl

R.T.: 8.011 min
Delta R.T.: -0.001 min
Response: 10431912
Conc: 16.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
EXT-007-SW124-061819

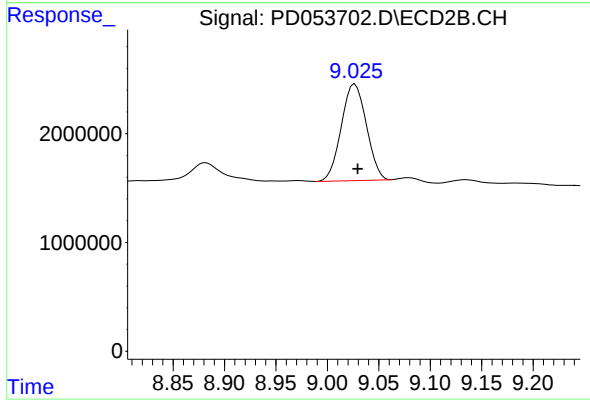

#28 Decachlorobiphenyl

R.T.: 9.027 min
Delta R.T.: -0.003 min
Response: 15088322
Conc: 14.92 ng/ml