

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062122\
 Data File : PD070447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2022 17:07
 Operator : AR\AJ
 Sample : PB145727BS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS727

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/22/2022
 Supervised By : Ankita Jodhani 06/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 02:21:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 16:58:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.399	4.120	28876563	269.0E6	19.910	19.916
27)	SA Decachlor...	8.126	9.276	65999311	308.4E6	41.206	42.731
Target Compounds							
2)	A alpha-BHC	3.834	4.513	9675970	91890983	4.579	4.694
3)	MA gamma-BHC...	4.115	4.801	10534079	95137527	5.246	5.217
4)	MA Heptachlor	4.408	5.324	10097821	96750070	5.131	5.400
5)	MB Aldrin	4.653	5.635	10072647	93454767	5.281	5.623
6)	B beta-BHC	4.364	4.964	4732347	43823070	5.287	5.540m
7)	B delta-BHC	4.565	5.190	7546194	24261654	3.739	1.880 #
8)	B Heptachlo...	5.094	6.021	9676902	48063926	5.524	4.119 #
9)	A Endosulfan I	5.430	6.383	8943279	75971189	5.317	5.634
10)	B trans-Chl...	5.318	6.258	9747579	82645840	5.419	5.718
11)	B cis-Chlor...	5.377	6.332	9639158	81759661	5.450	5.823
12)	B 4,4'-DDE	5.543	6.484	17644777	150.0E6	10.452	11.533
13)	MA Dieldrin	5.672	6.641	19062045	151.4E6	10.049	11.053
14)	MA Endrin	5.929	6.861	17248303	122.4E6	10.135	10.636
15)	B Endosulfa...	6.202	7.066	16691387	126.4E6	10.286	11.490
16)	A 4,4'-DDD	6.058	6.974	15511345	130.1E6	10.245	11.785
17)	MA 4,4'-DDT	6.296	7.276	13254901	109.8E6	9.109	10.680
18)	B Endrin al...	6.371	7.190	15241261	110.3E6	12.252	13.112
19)	B Endosulfa...	6.583	7.414	15336298	104.1E6	9.682	10.528
20)	A Methoxychlor	6.846	7.731	45980538	268.4E6	54.326	56.850
21)	B Endrin ke...	7.074	7.888	19592484	122.1E6	10.987	11.986

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062122\
Data File : PD070447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2022 17:07
Operator : AR\AJ
Sample : PB145727BS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 02:21:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 16:58:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

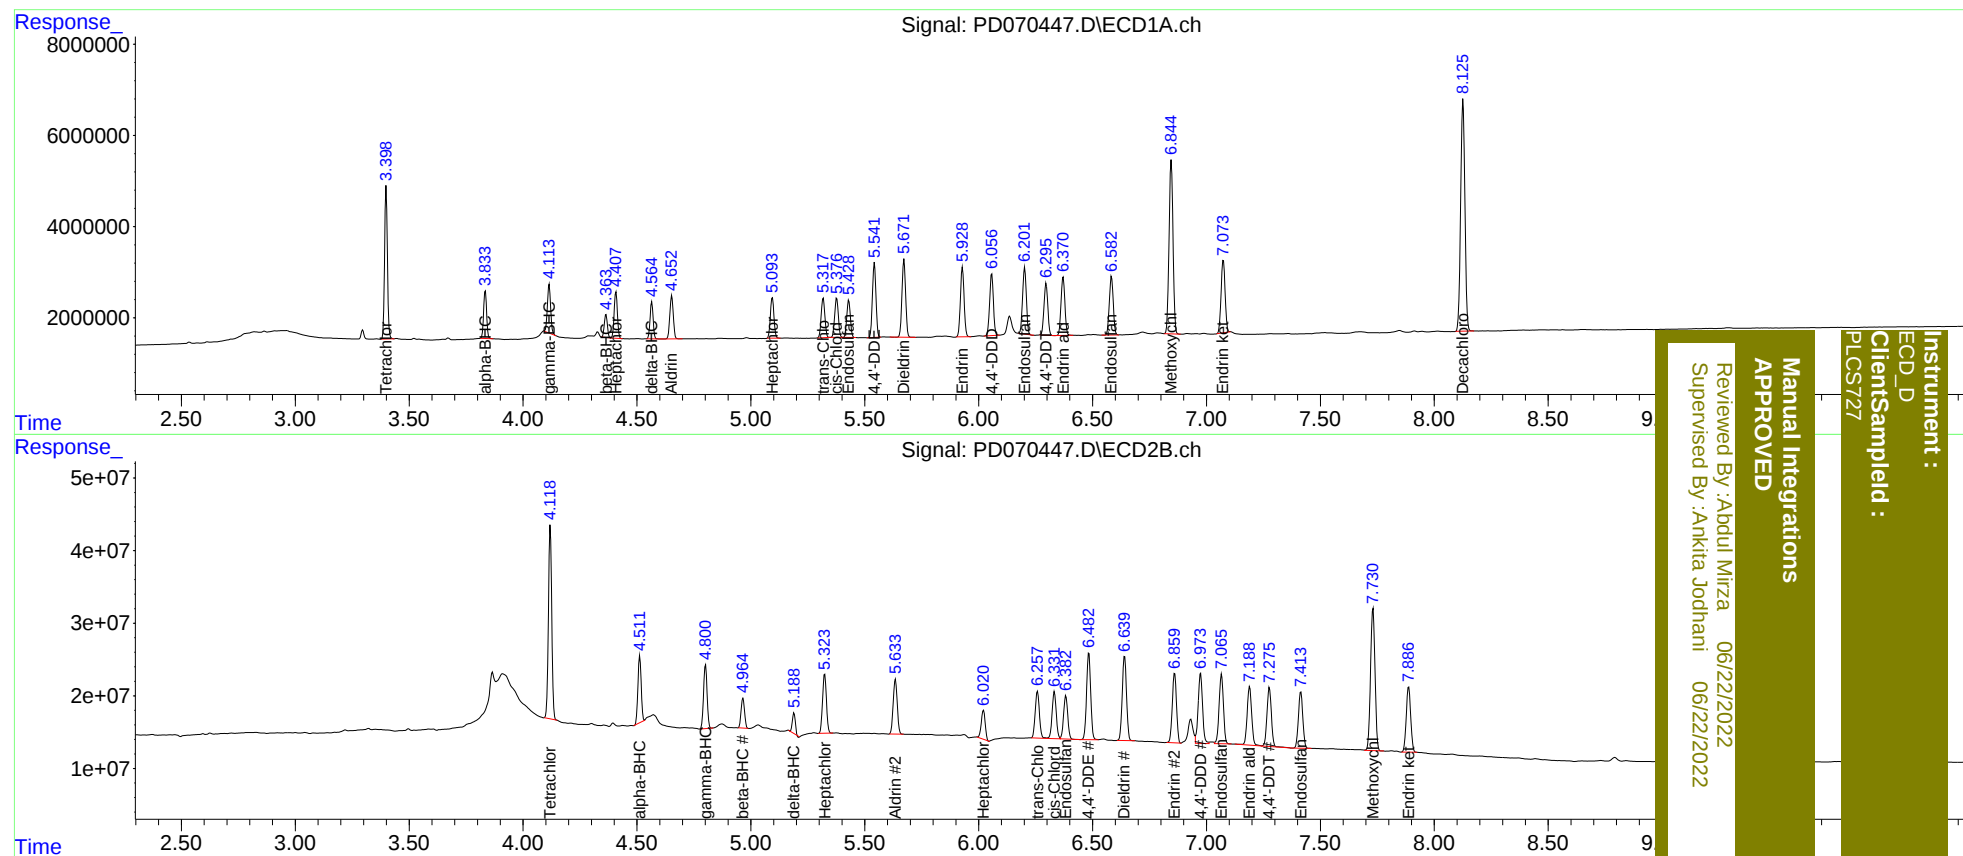

Instrument :
ECD_D
ClientSampled :
PLC5727

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 06/22/2022
Supervised By: Ankita Jodhani 06/22/2022