

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062124\
 Data File : PD083778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2024 12:05
 Operator : AR\AJ
 Sample : P2899-12DL2 50X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AB4DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/24/2024
 Supervised By : Ankita Jodhani 06/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 00:43:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
13) MA	Dieldrin	6.380	5.353	31377865	66670901	15.175m 9.152 #
14) MA	Endrin	6.613	5.632	17073934	43125831	10.107 6.668 #
15) B	Endosulfa...	6.827	5.911	9334893	28155898	5.190m 4.437
17) MA	4,4'-DDT	7.036	6.019	98167202	266.8E6	65.165m 47.130 #
19) B	Endosulfa...	7.179	6.318	25882527	95264246	15.129 15.419

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062124\
Data File : PD083778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2024 12:05
Operator : AR\AJ
Sample : P2899-12DL2 50X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 00:43:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

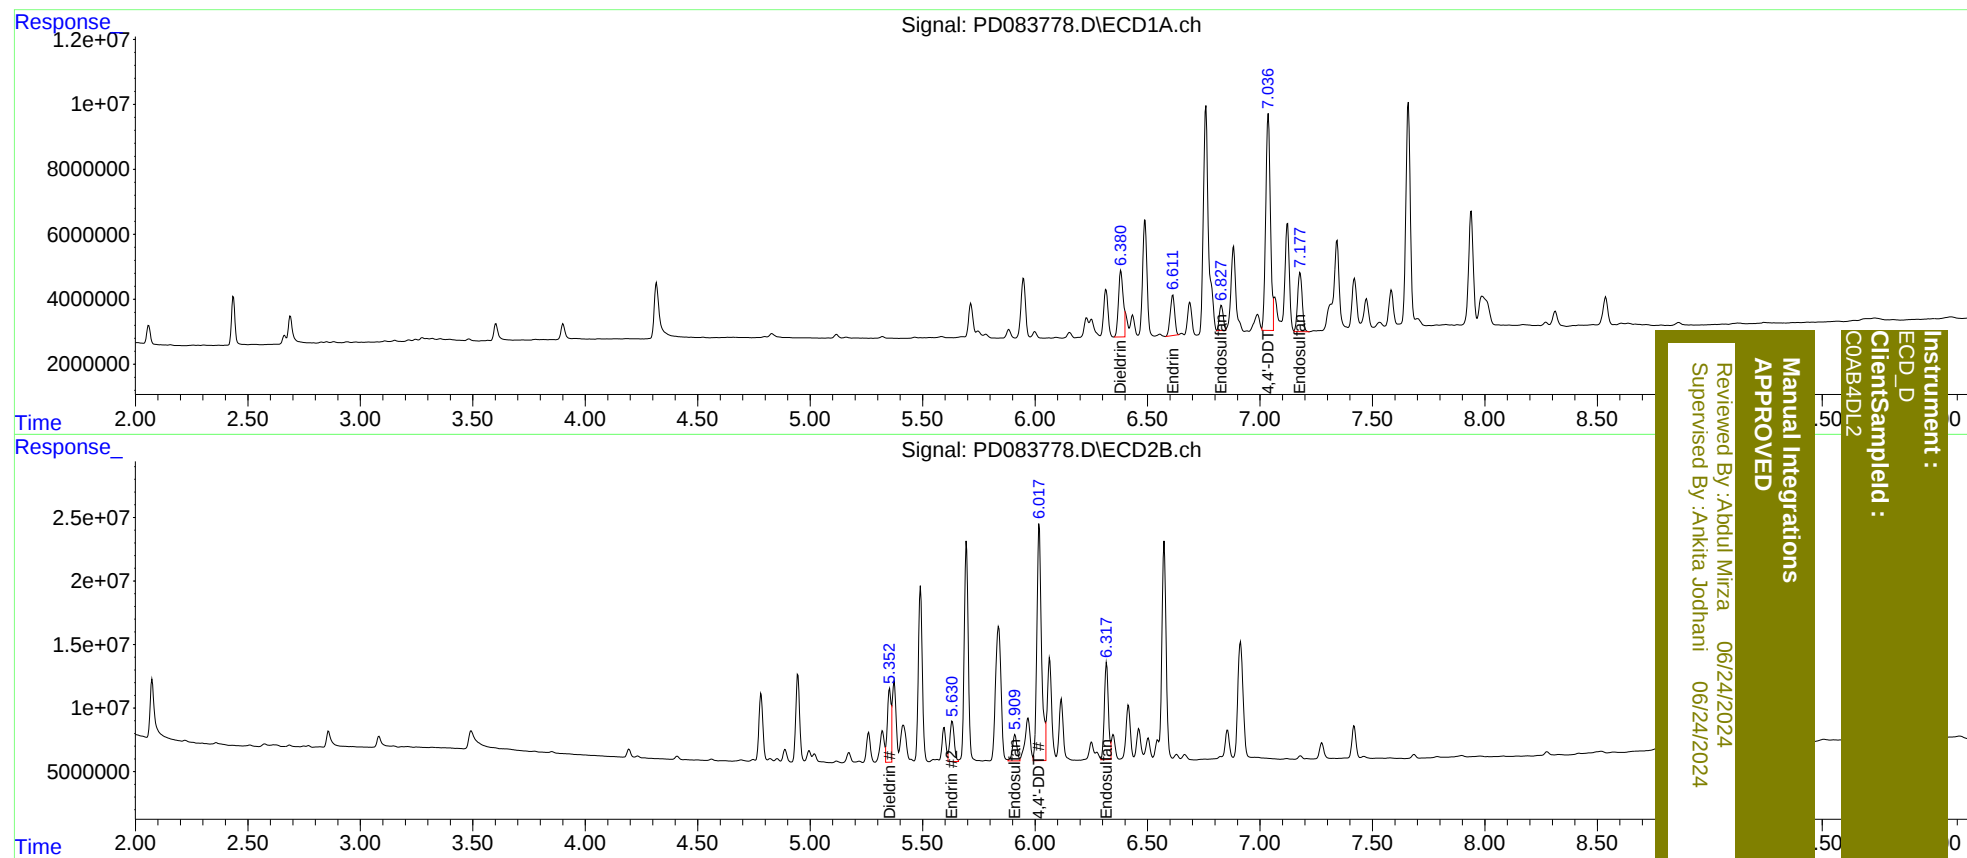

Reviewed By: Abdul Mirza 06/24/2024
Supervised By: Ankita Jodhani 06/24/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
COAB4DL2