

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062124\
 Data File : PD083781.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2024 13:15
 Operator : AR\AJ
 Sample : P2899-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA7

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/24/2024
 Supervised By :Ankita Jodhani 06/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 01:36:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.561	2.772	21018200	90300923	16.102m	16.566m
2) SA Decachlor...	9.114	7.897	40708261	119.5E6	20.935m	19.678
Target Compounds						
3) MA gamma-BHC...	4.350	3.602	1238892	3607719	0.569m	0.462m
12) B 4,4'-DDE	6.222	5.218	1790257	4232914	0.863m	0.596m#
14) MA Endrin	6.607	5.633	2073491	5348889	1.227	0.827m#
17) MA 4,4'-DDT	7.031	6.019	6600261	23183335	4.381m	4.096m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062124\
Data File : PD083781.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2024 13:15
Operator : AR\AJ
Sample : P2899-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 01:36:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

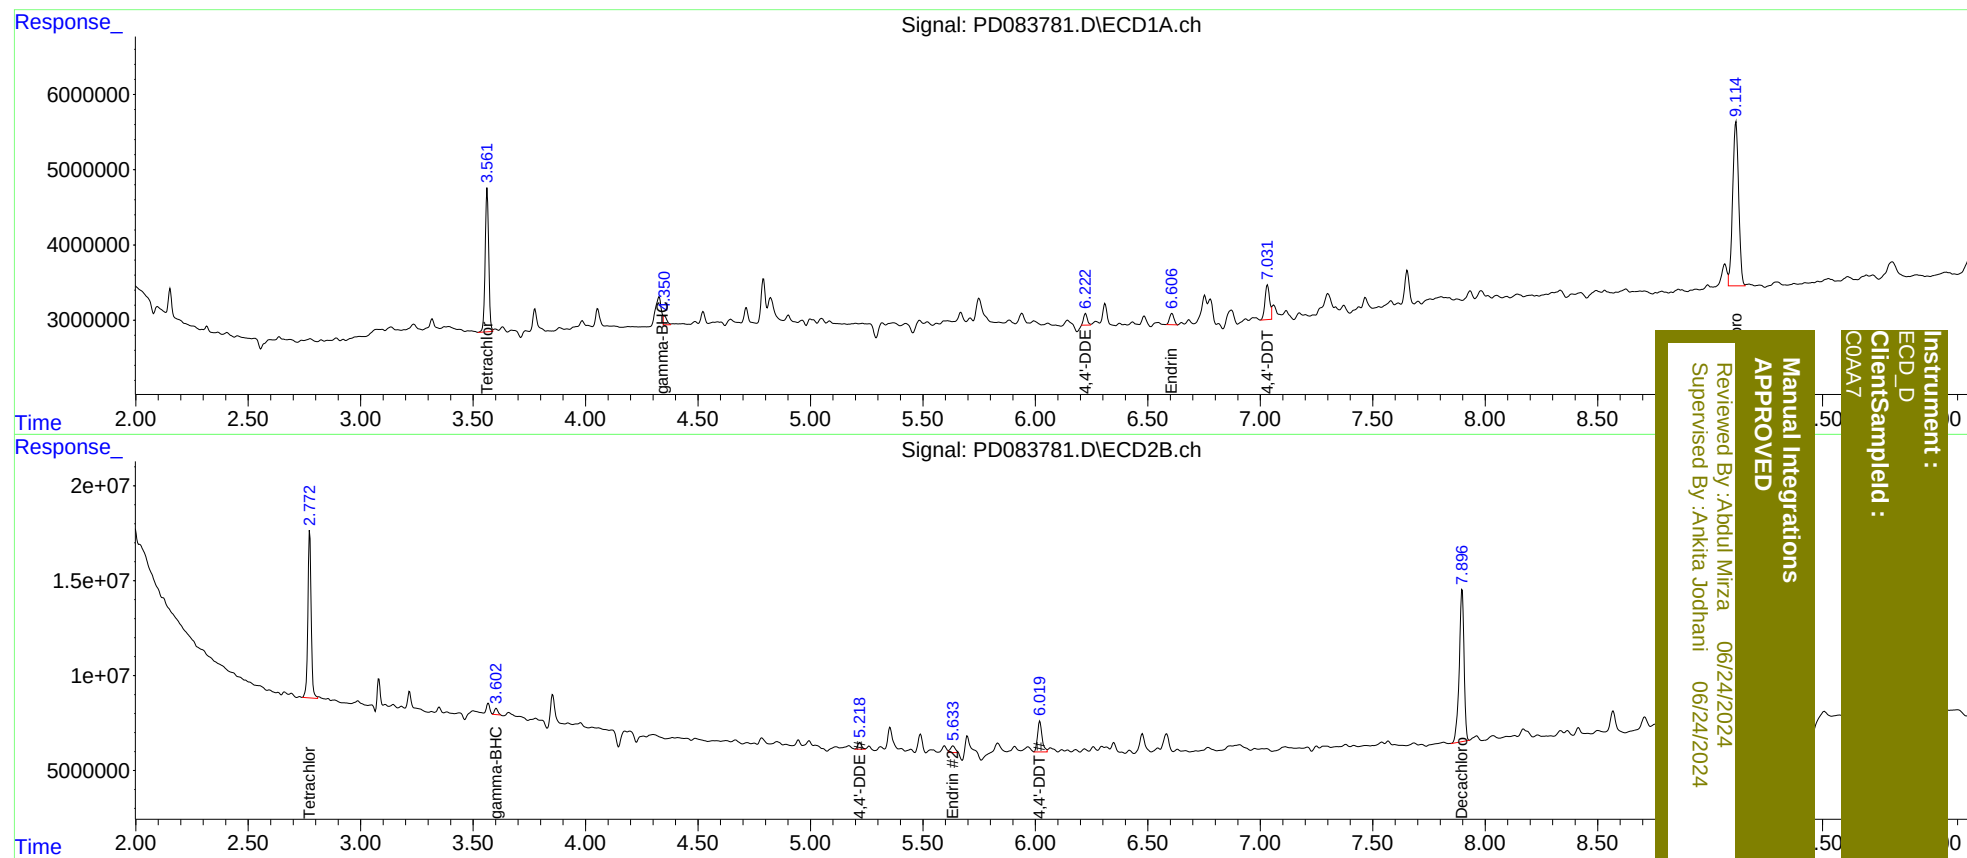

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/24/2024
Supervised By: Ankita Jodhani 06/24/2024

Instrument :
ECD_D
ClientSampled :
COAA7