

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062124\
 Data File : PD083783.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2024 14:09
 Operator : AR\AJ
 Sample : P2899-12DL2 40X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AB4DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/24/2024
 Supervised By : Ankita Jodhani 06/24/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 22 00:44:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
13) MA	Dieldrin	6.374	5.351	35403878	78340575	17.122m 10.753m#
14) MA	Endrin	6.603	5.630	20966078	54587153	12.411m 8.440m#
15) B	Endosulfa...	6.821	5.908	11011499	31053885	6.122m 4.894m
17) MA	4,4'-DDT	7.028	6.016	119.3E6	357.9E6	79.161m 63.227m
19) B	Endosulfa...	7.172	6.316	32531480	131.8E6	19.015 21.335m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062124\
Data File : PD083783.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2024 14:09
Operator : AR\AJ
Sample : P2899-12DL2 40X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 22 00:44:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

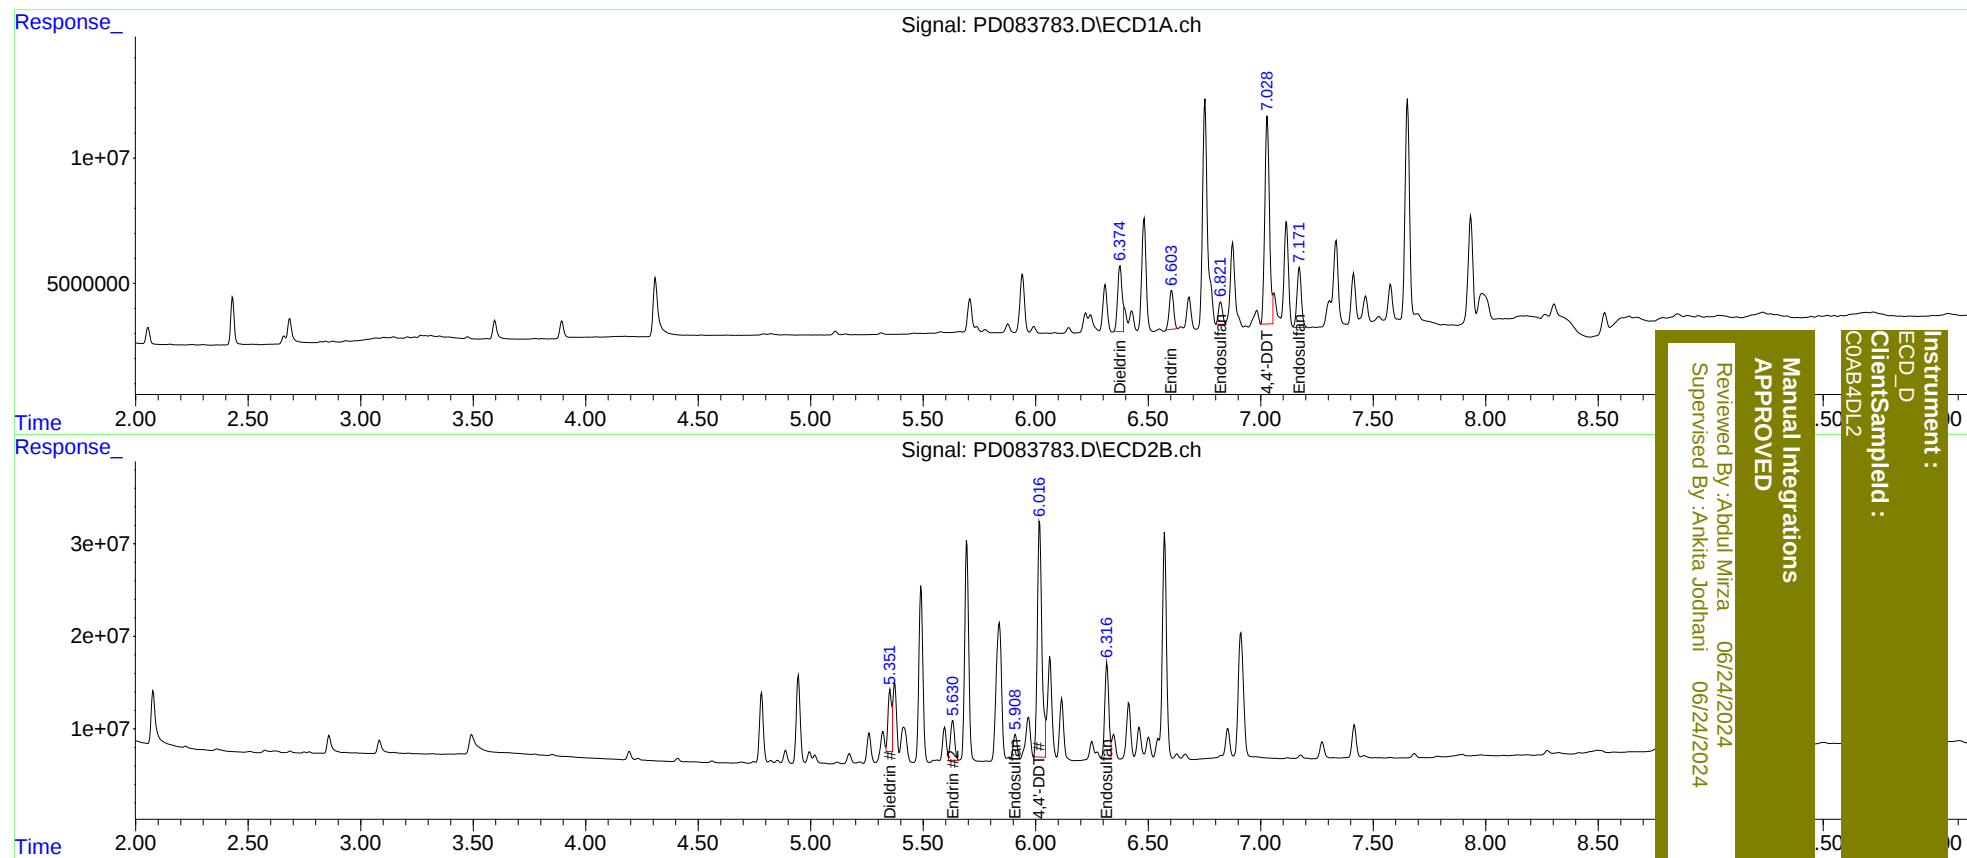

Reviewed By: Abdul Mirza 06/24/2024
Supervised By: Ankita Jodhani 06/24/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
COAB4DL2