

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062220\
 Data File : PD058362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2020 12:44
 Operator : AJ\MA
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA101

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 04:20:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062220CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 23 04:18:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.867	7788771	9831394	4.974	5.024
27)	SA Decachlor...	7.847	8.860	17273818	22079468	10.546	10.726
Target Compounds							
2)	A alpha-BHC	3.632	4.249	9444625	13422111	4.526	4.520
3)	MA gamma-BHC...	3.903	4.529	9373886	13477975	4.748	4.687
4)	MA Heptachlor	4.182	5.029	5914545	11638530	4.924	4.866
9)	A Endosulfan I	5.177	6.065	8070476	11902496	4.796	4.933
13)	MA Dieldrin	5.415	6.321	14215183	25348716	9.468	9.415
14)	MA Endrin	5.666	6.537	12689282	21388656	9.916	9.825
16)	A 4,4'-DDD	5.803	6.665	9142887	19359782	10.041	9.345
17)	MA 4,4'-DDT	6.037	6.961	10959015	19525954	9.216	9.318
20)	A Methoxychlor	6.585	7.422	21190102	51512574	51.851	50.827


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062220\
Data File : PD058362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2020 12:44
Operator : AJ\MA
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
INDA101

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 04:20:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062220CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 23 04:18:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

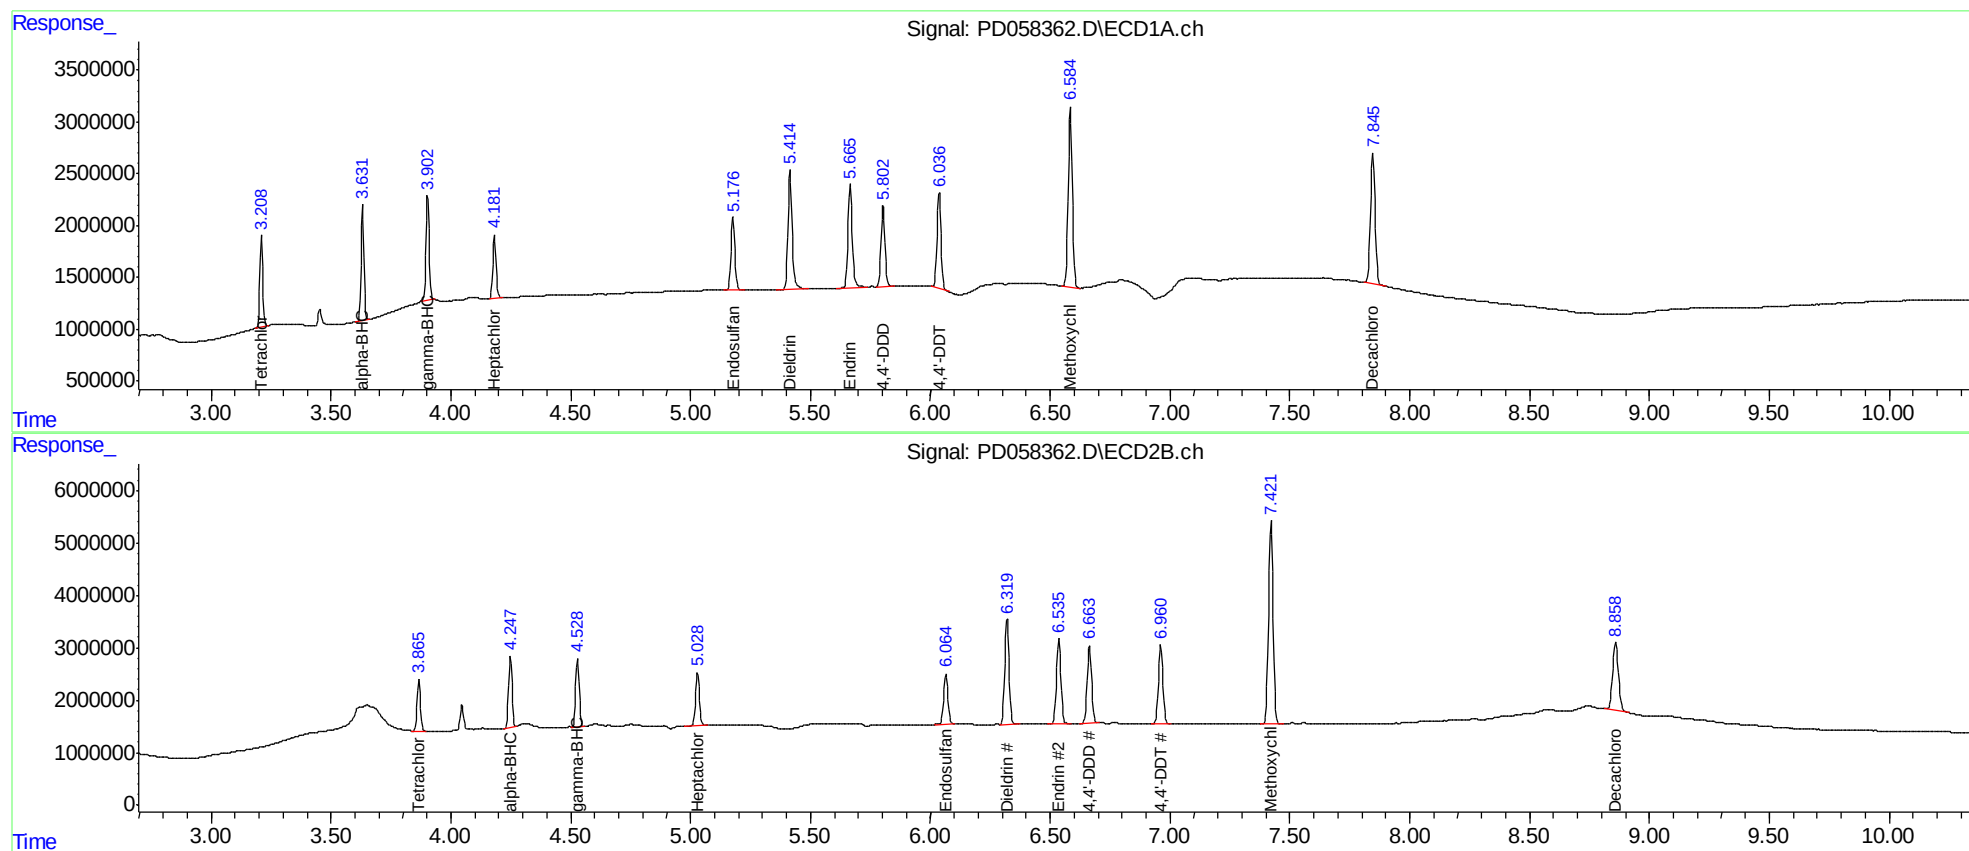


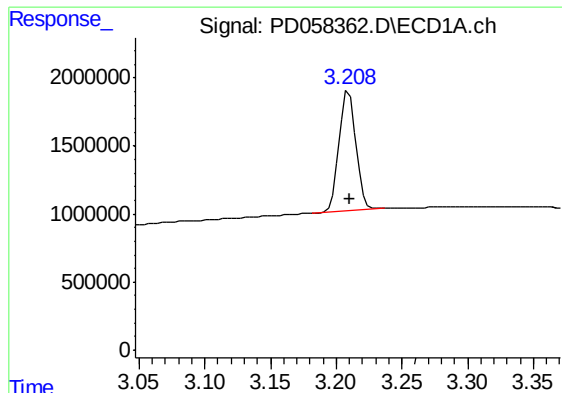

#1 Tetrachloro-m-xylene


R.T.: 3.210 min
Delta R.T.: 0.000 min
Response: 7788771
Conc: 4.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

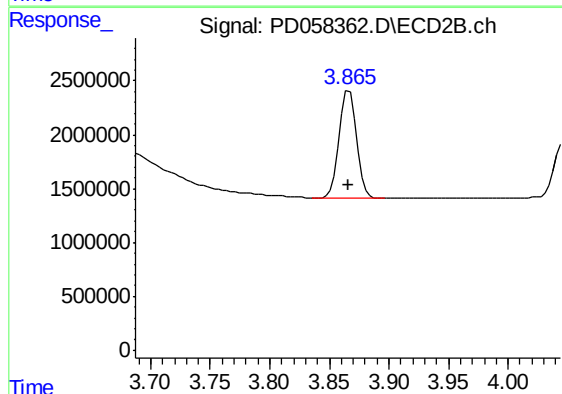


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 9831394
Conc: 5.02 ng/ml

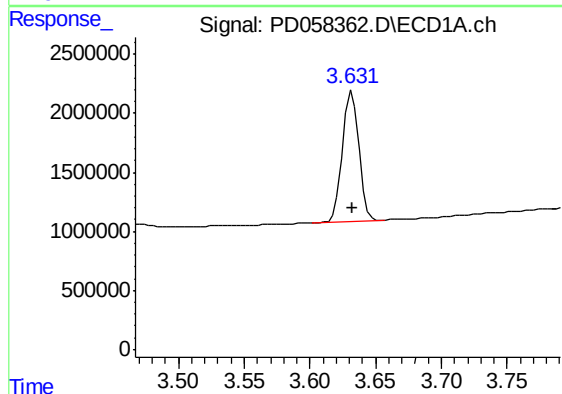


#2 alpha-BHC

R.T.: 3.632 min
Delta R.T.: 0.000 min
Response: 9444625
Conc: 4.53 ng/ml

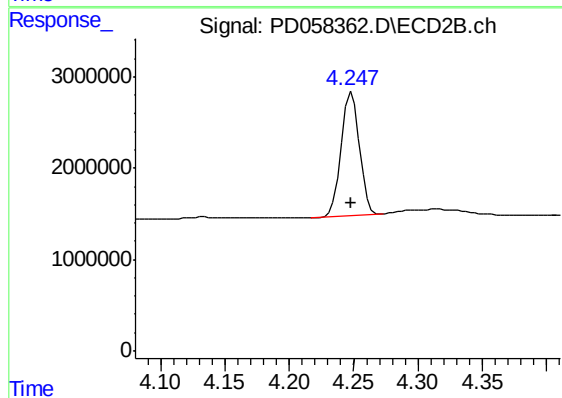

#2 alpha-BHC


R.T.: 4.249 min
Delta R.T.: 0.000 min
Response: 13422111
Conc: 4.52 ng/ml

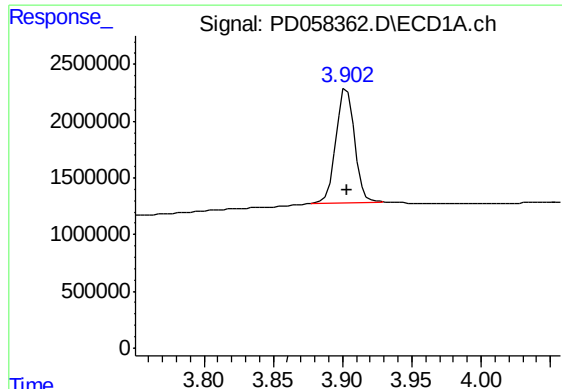

#3 gamma-BHC (Lindane)


R.T.: 3.903 min
Delta R.T.: 0.000 min
Response: 9373886
Conc: 4.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

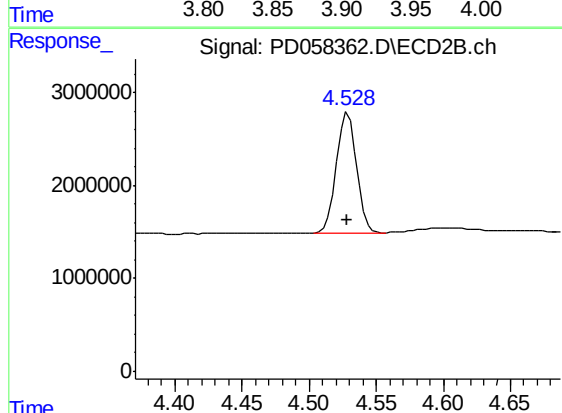


#3 gamma-BHC (Lindane)

R.T.: 4.529 min
Delta R.T.: 0.000 min
Response: 13477975
Conc: 4.69 ng/ml

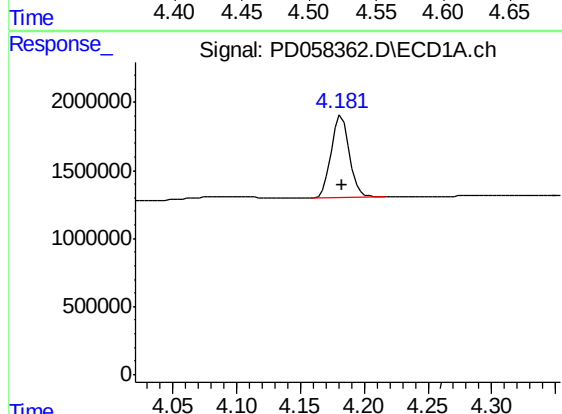


#4 Heptachlor

R.T.: 4.182 min
Delta R.T.: 0.000 min
Response: 5914545
Conc: 4.92 ng/ml

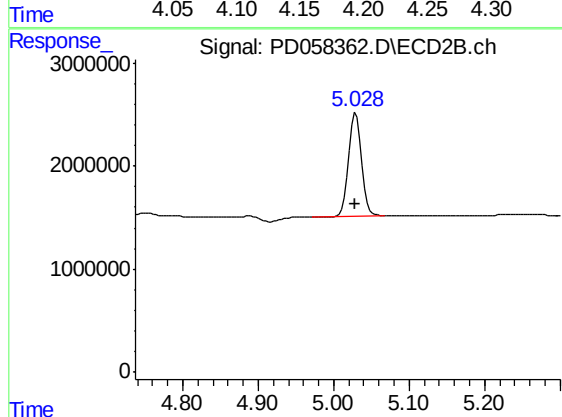

#4 Heptachlor


R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 11638530
Conc: 4.87 ng/ml

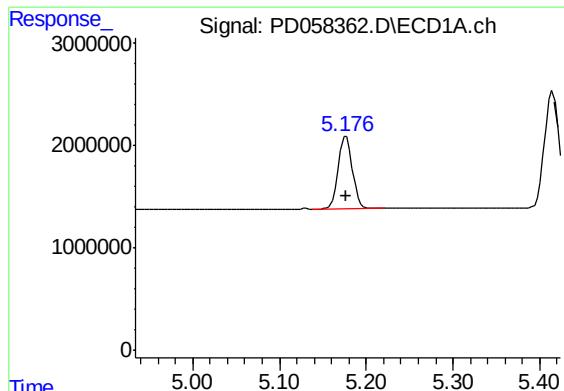

#9 Endosulfan I


R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 8070476
Conc: 4.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

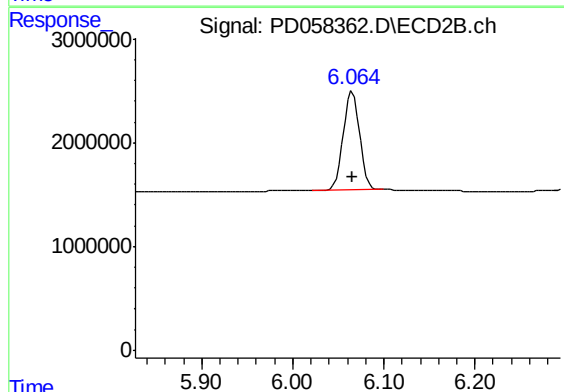


#9 Endosulfan I

R.T.: 6.065 min
Delta R.T.: 0.000 min
Response: 11902496
Conc: 4.93 ng/ml

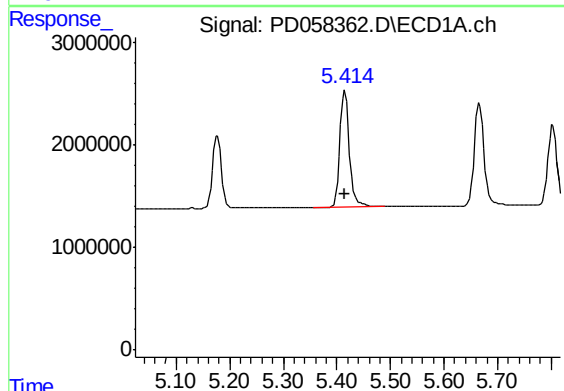


#13 Dieldrin

R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 14215183
Conc: 9.47 ng/ml

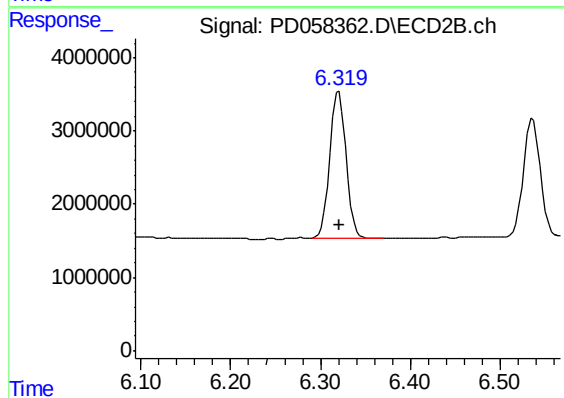

#13 Dieldrin


R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 25348716
Conc: 9.41 ng/ml

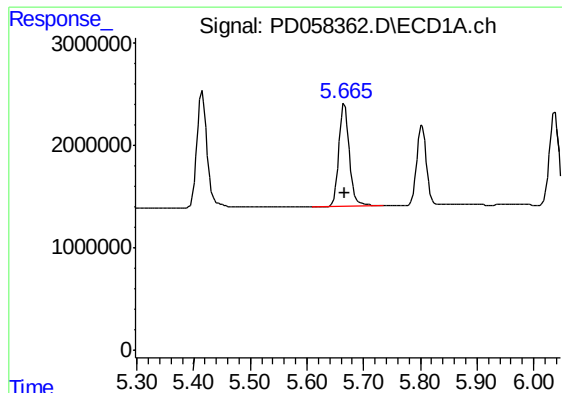

#14 Endrin


R.T.: 5.666 min
Delta R.T.: 0.000 min
Response: 12689282
Conc: 9.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

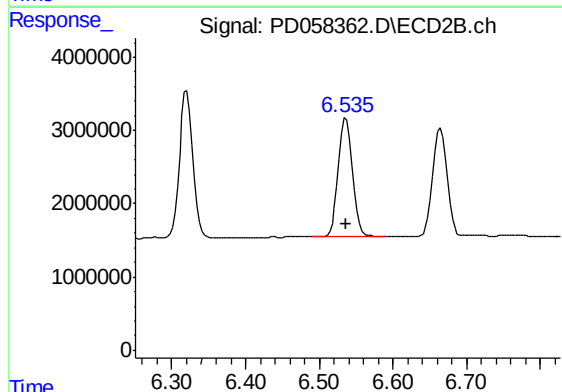


#14 Endrin

R.T.: 6.537 min
Delta R.T.: 0.000 min
Response: 21388656
Conc: 9.82 ng/ml

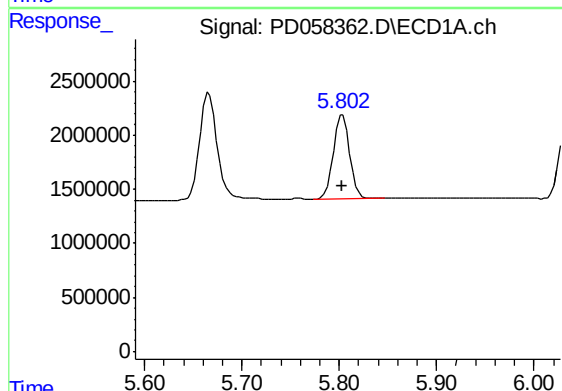


#16 4,4'-DDD

R.T.: 5.803 min
Delta R.T.: 0.000 min
Response: 9142887
Conc: 10.04 ng/ml

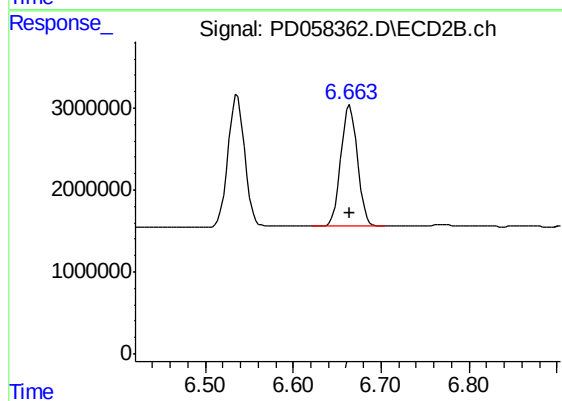

#16 4,4'-DDD


R.T.: 6.665 min
Delta R.T.: 0.000 min
Response: 19359782
Conc: 9.34 ng/ml

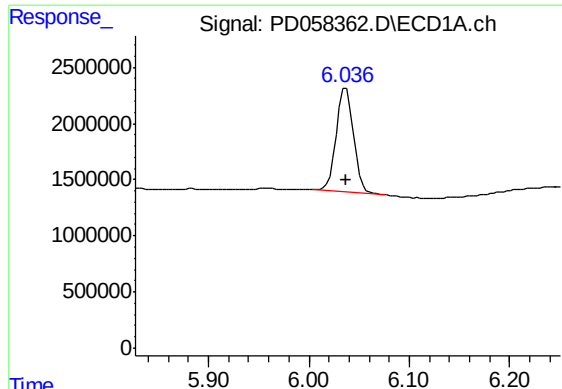

#17 4,4'-DDT


R.T.: 6.037 min
Delta R.T.: 0.000 min
Response: 10959015
Conc: 9.22 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

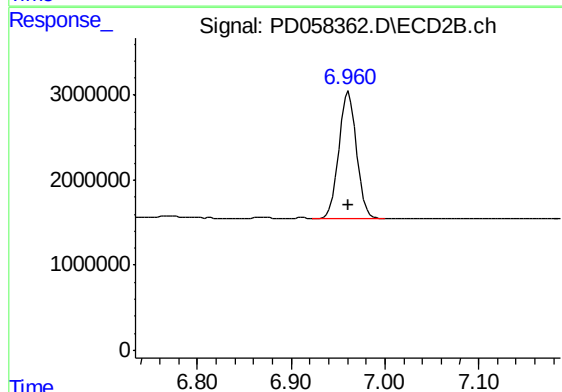


#17 4,4'-DDT

R.T.: 6.961 min
Delta R.T.: 0.000 min
Response: 19525954
Conc: 9.32 ng/ml

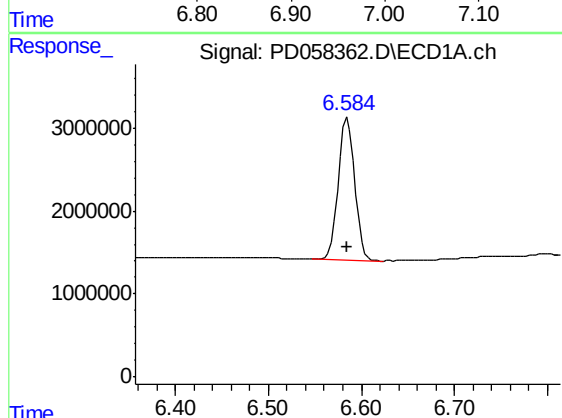


#20 Methoxychlor

R.T.: 6.585 min
Delta R.T.: 0.000 min
Response: 21190102
Conc: 51.85 ng/ml

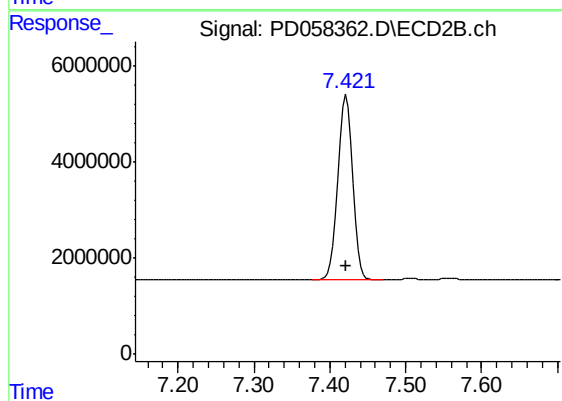

#20 Methoxychlor


R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 51512574
Conc: 50.83 ng/ml

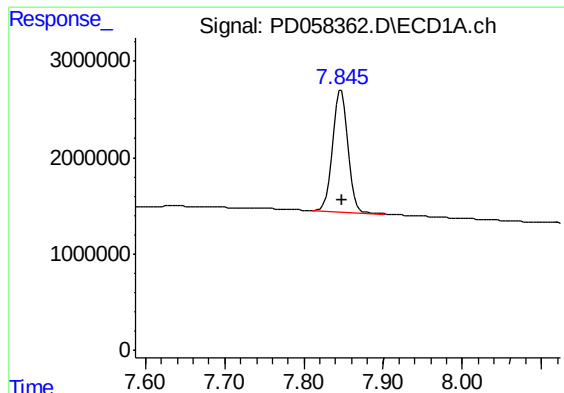

#27 Decachlorobiphenyl

R.T.: 7.847 min
Delta R.T.: 0.000 min
Response: 17273818
Conc: 10.55 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA101

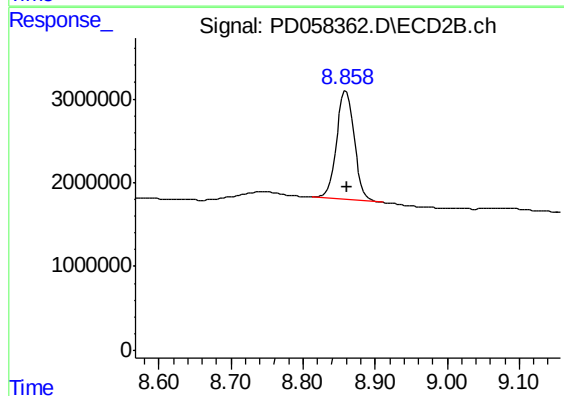

#27 Decachlorobiphenyl

R.T.: 8.860 min
Delta R.T.: 0.000 min
Response: 22079468
Conc: 10.73 ng/ml