

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062220\
 Data File : PD058368.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2020 14:09
 Operator : AJ\MA
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA401

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 04:21:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062220CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 23 04:18:58 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.210	3.867	62503096	77464529	39.918	39.583
27)	SA Decachlor...	7.847	8.860	130.4E6	158.3E6	79.635	76.908
Target Compounds							
2)	A alpha-BHC	3.632	4.249	87644518	122.6E6	41.997	41.287
3)	MA gamma-BHC...	3.904	4.530	81530087	117.3E6	41.293	40.772
4)	MA Heptachlor	4.183	5.030	48226310	96413128	40.146	40.310
9)	A Endosulfan I	5.177	6.066	68325511	96401773	40.601	39.951
13)	MA Dieldrin	5.415	6.321	122.9E6	217.0E6	81.883	80.593
14)	MA Endrin	5.666	6.537	103.6E6	175.8E6	80.954	80.751
16)	A 4,4'-DDD	5.804	6.665	73896159	168.3E6	81.155	81.241
17)	MA 4,4'-DDT	6.037	6.962	100.2E6	172.2E6	84.232	82.194
20)	A Methoxychlor	6.585	7.422	160.0E6	396.6E6	391.542	391.276


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062220\
Data File : PD058368.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2020 14:09
Operator : AJ\MA
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
INDA401

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 04:21:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062220CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 23 04:18:58 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

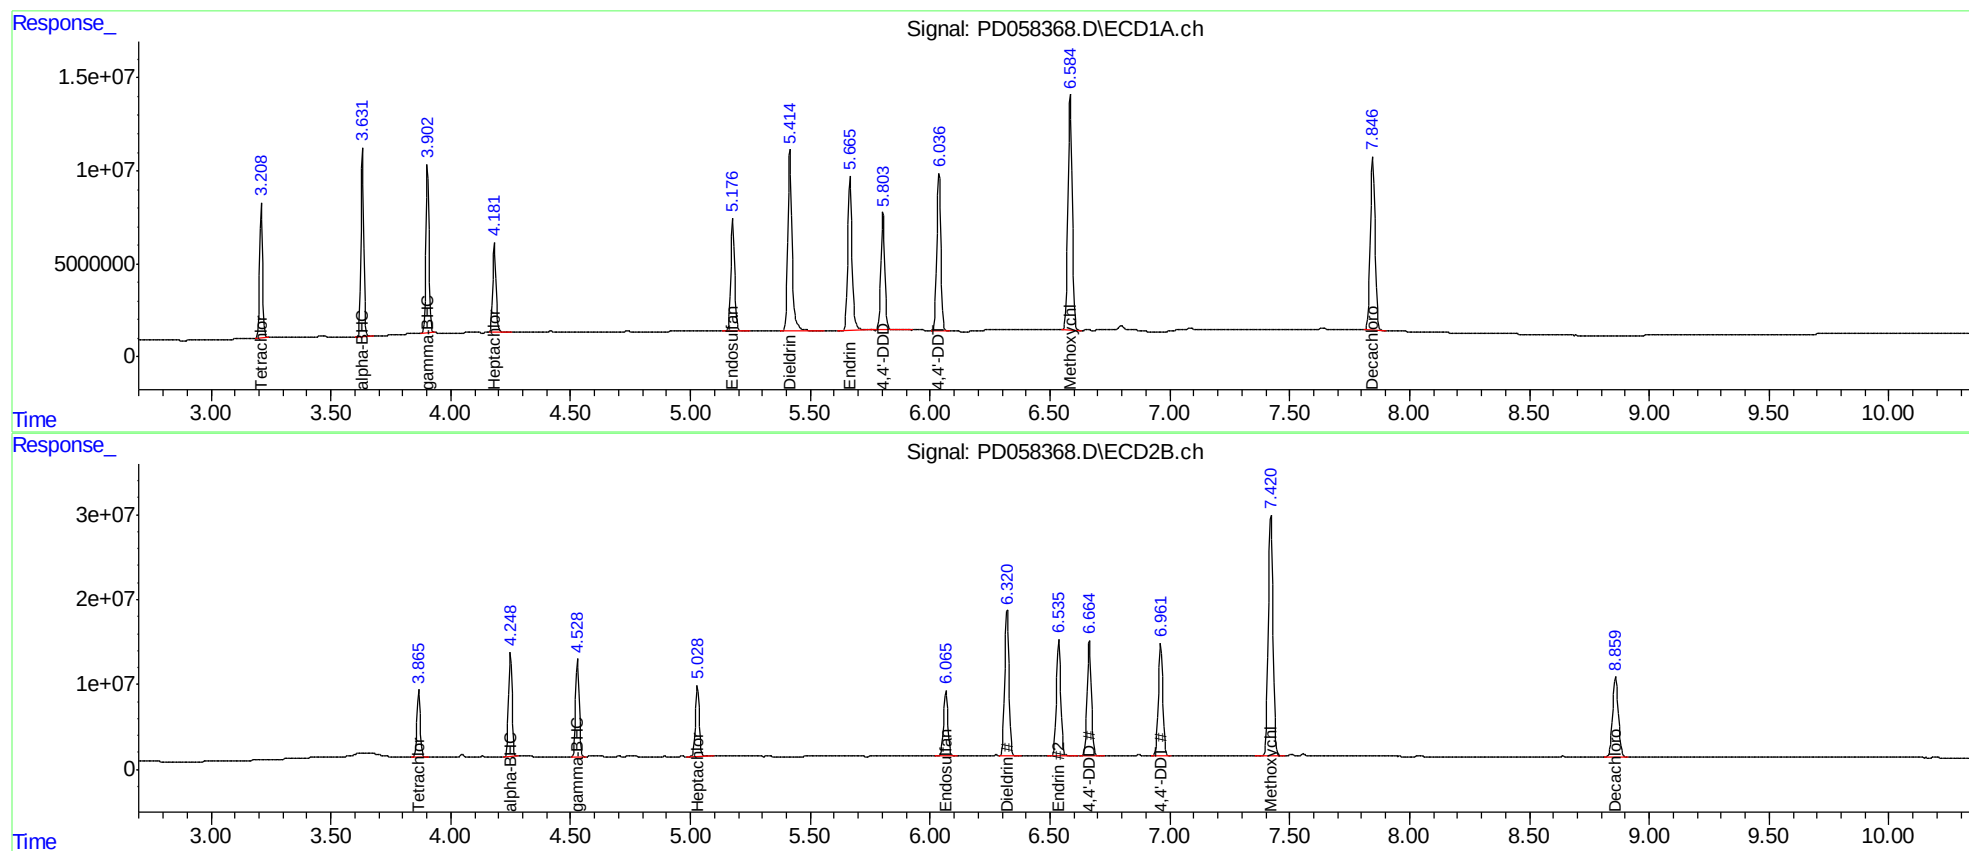


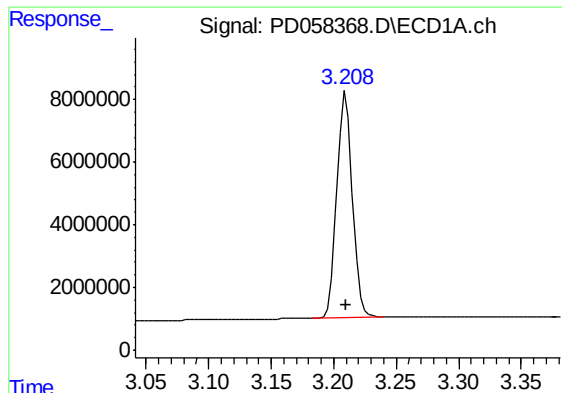

#1 Tetrachloro-m-xylene


R.T.: 3.210 min
Delta R.T.: 0.000 min
Response: 62503096
Conc: 39.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

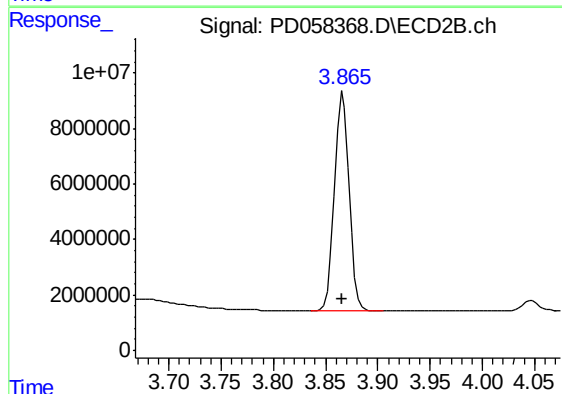


#1 Tetrachloro-m-xylene

R.T.: 3.867 min
Delta R.T.: 0.000 min
Response: 77464529
Conc: 39.58 ng/ml

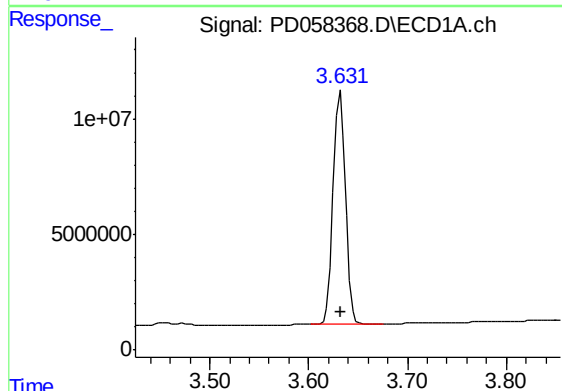


#2 alpha-BHC

R.T.: 3.632 min
Delta R.T.: 0.000 min
Response: 87644518
Conc: 42.00 ng/ml

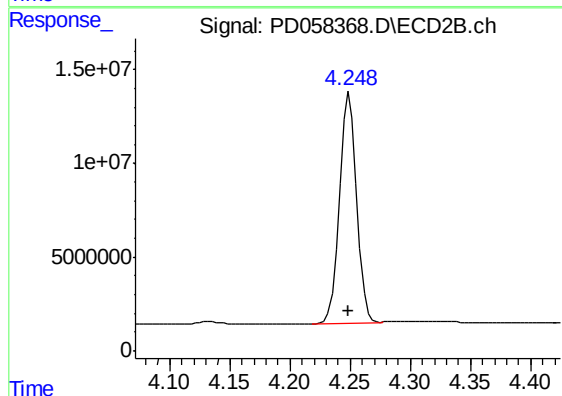

#2 alpha-BHC


R.T.: 4.249 min
Delta R.T.: 0.001 min
Response: 122591145
Conc: 41.29 ng/ml

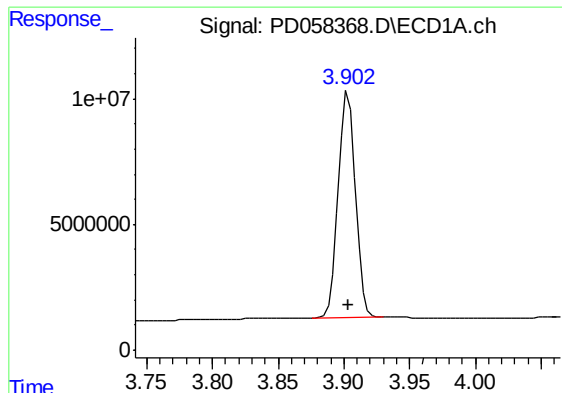

#3 gamma-BHC (Lindane)


R.T.: 3.904 min
Delta R.T.: 0.000 min
Response: 81530087
Conc: 41.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

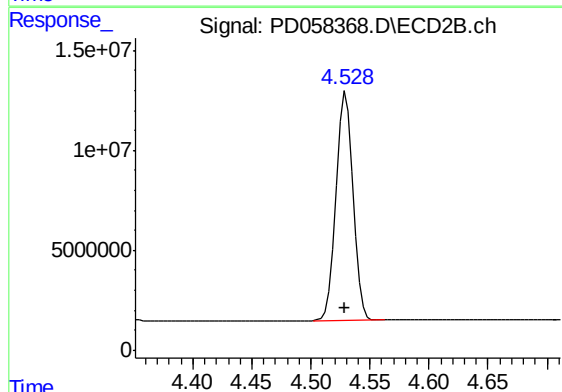


#3 gamma-BHC (Lindane)

R.T.: 4.530 min
Delta R.T.: 0.000 min
Response: 117252760
Conc: 40.77 ng/ml

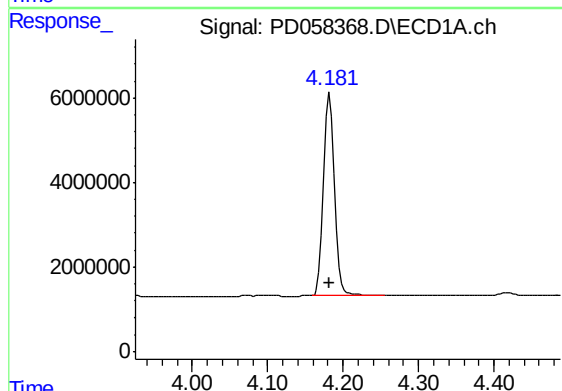


#4 Heptachlor

R.T.: 4.183 min
Delta R.T.: 0.000 min
Response: 48226310
Conc: 40.15 ng/ml

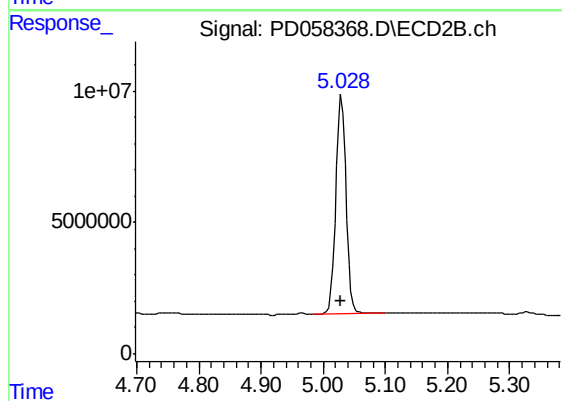

#4 Heptachlor


R.T.: 5.030 min
Delta R.T.: 0.000 min
Response: 96413128
Conc: 40.31 ng/ml

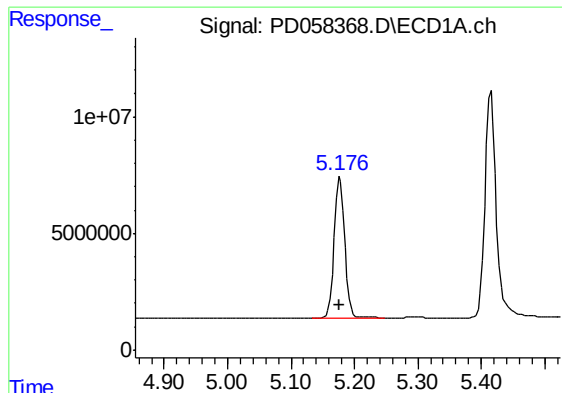

#9 Endosulfan I


R.T.: 5.177 min
Delta R.T.: 0.000 min
Response: 68325511
Conc: 40.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

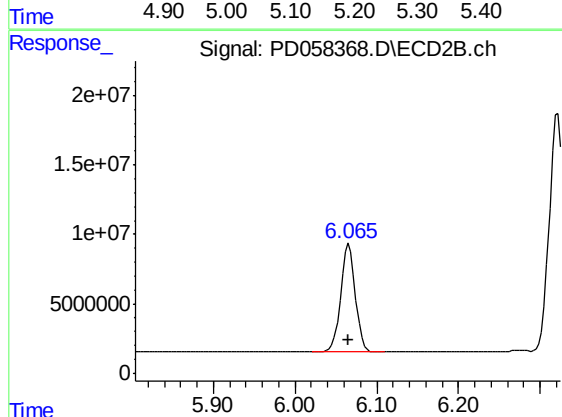


#9 Endosulfan I

R.T.: 6.066 min
Delta R.T.: 0.000 min
Response: 96401773
Conc: 39.95 ng/ml

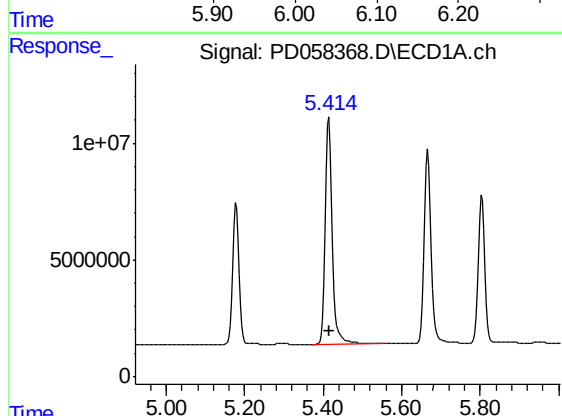


#13 Dieldrin

R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 122934617
Conc: 81.88 ng/ml

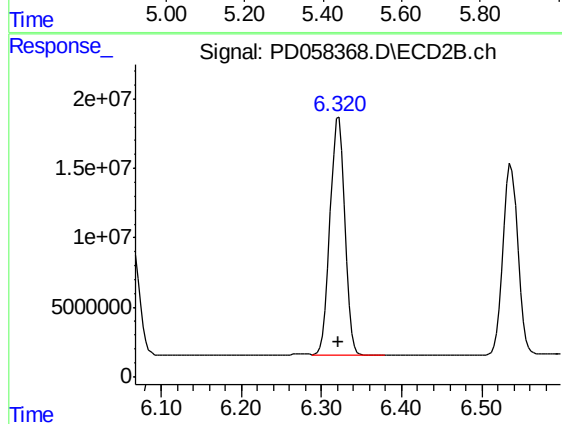

#13 Dieldrin


R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 216997799
Conc: 80.59 ng/ml

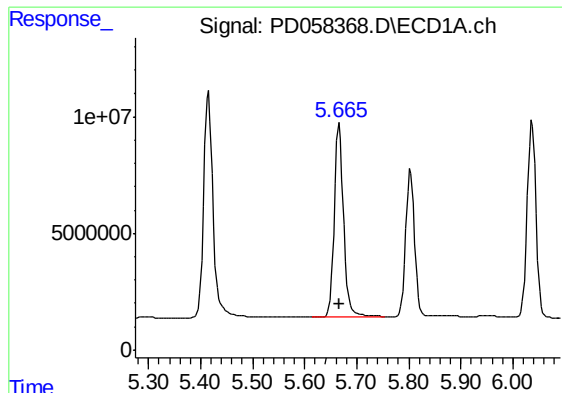

#14 Endrin


R.T.: 5.666 min
Delta R.T.: 0.000 min
Response: 103598369
Conc: 80.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

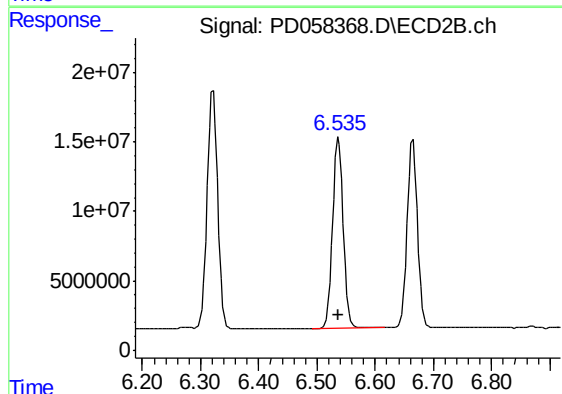


#14 Endrin

R.T.: 6.537 min
Delta R.T.: 0.000 min
Response: 175794188
Conc: 80.75 ng/ml

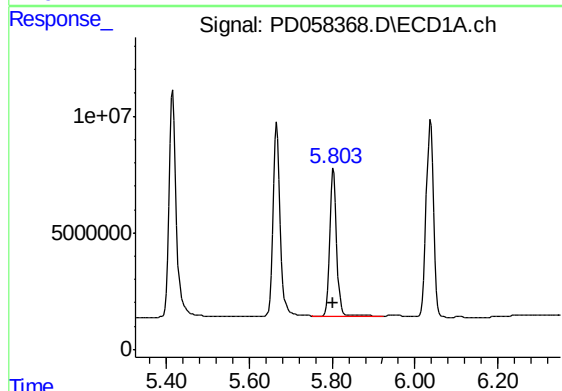


#16 4,4'-DDD

R.T.: 5.804 min
Delta R.T.: 0.000 min
Response: 73896159
Conc: 81.16 ng/ml

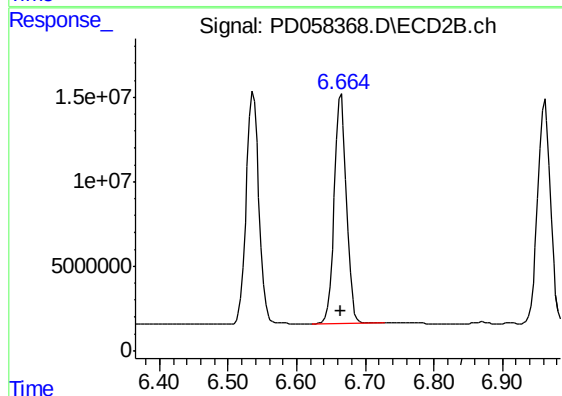

#16 4,4'-DDD


R.T.: 6.665 min
Delta R.T.: 0.000 min
Response: 168310645
Conc: 81.24 ng/ml

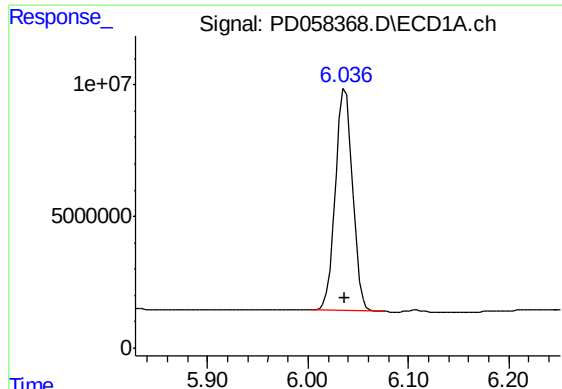

#17 4,4'-DDT


R.T.: 6.037 min
Delta R.T.: 0.000 min
Response: 100161426
Conc: 84.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

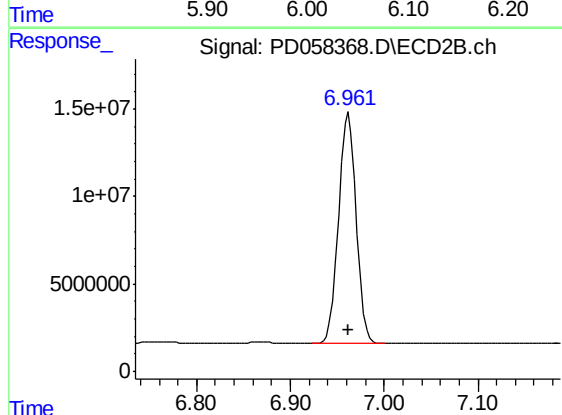


#17 4,4'-DDT

R.T.: 6.962 min
Delta R.T.: 0.000 min
Response: 172236979
Conc: 82.19 ng/ml

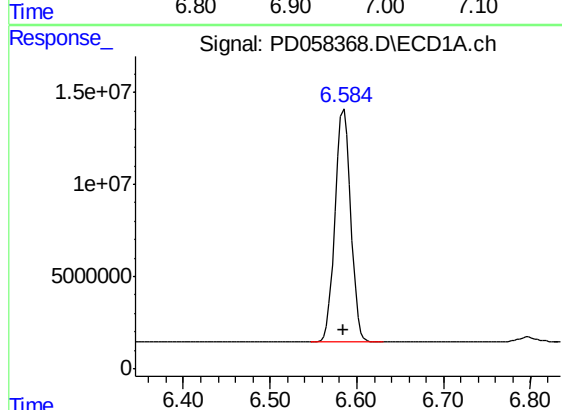


#20 Methoxychlor

R.T.: 6.585 min
Delta R.T.: 0.000 min
Response: 160012327
Conc: 391.54 ng/ml

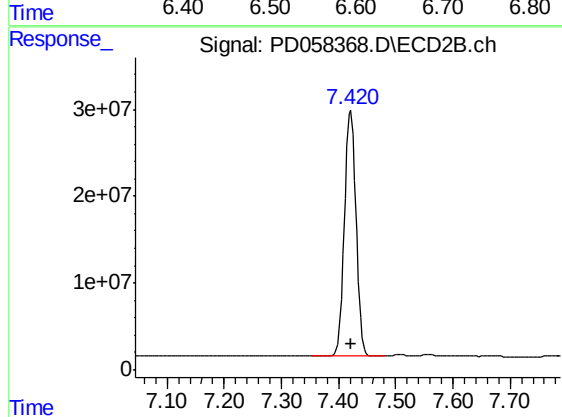

#20 Methoxychlor


R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 396550309
Conc: 391.28 ng/ml

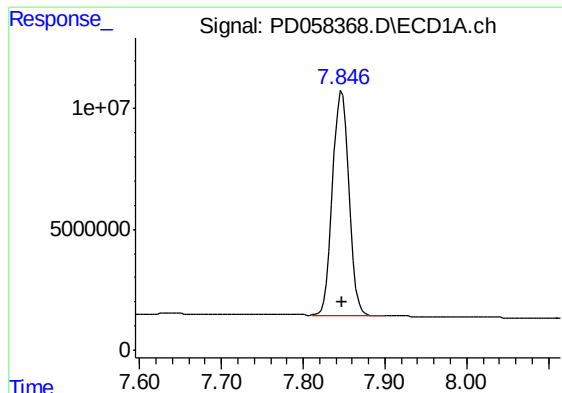

#27 Decachlorobiphenyl

R.T.: 7.847 min
Delta R.T.: 0.000 min
Response: 130432865
Conc: 79.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA401

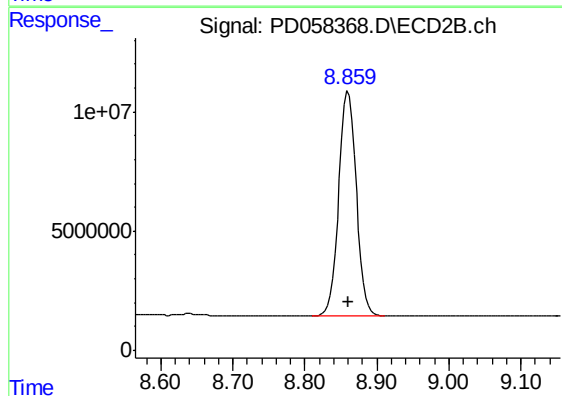

#27 Decachlorobiphenyl

R.T.: 8.860 min
Delta R.T.: 0.000 min
Response: 158317925
Conc: 76.91 ng/ml