

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062222\
 Data File : PL075893.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2022 08:34
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 00:13:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.643	4.638	15679085	36532279	23.232	21.769
28)	SA Decachlor...	11.636	10.379	18248087	25458614	29.806	18.069 #
Target Compounds							
7)	B delta-BHC	0.000	6.402	0	363357	N.D.	0.170 #
8)	B Heptachlo...	8.124	0.000	525457	0	0.680	N.D. #
9)	A Endosulfan I	8.535	0.000	154846	0	0.221	N.D. #
10)	B gamma-Chl...	8.386	0.000	942109	0	1.213	N.D. #
11)	B alpha-Chl...	8.497f	0.000	140710	0	0.185	N.D. #
13)	MA Dieldrin	0.000	7.751	0	149381	N.D.	0.088 #
14)	MA Endrin	0.000	8.063f	0	446334	N.D.	0.326 #
15)	B Endosulfa...	9.305	0.000	339970	0	0.546	N.D. #
21)	B Endrin ke...	10.187f	0.000	495511	0	0.705	N.D. #
24)	Chlordane-2	0.000	6.672f	0	768686	N.D.	11.495 #
25)	Chlordane-3	8.386	0.000	942109	0	9.124	N.D. #
26)	Chlordane-4	8.497f	0.000	140710	0	1.111	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062222\
Data File : PL075893.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2022 08:34
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:13:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

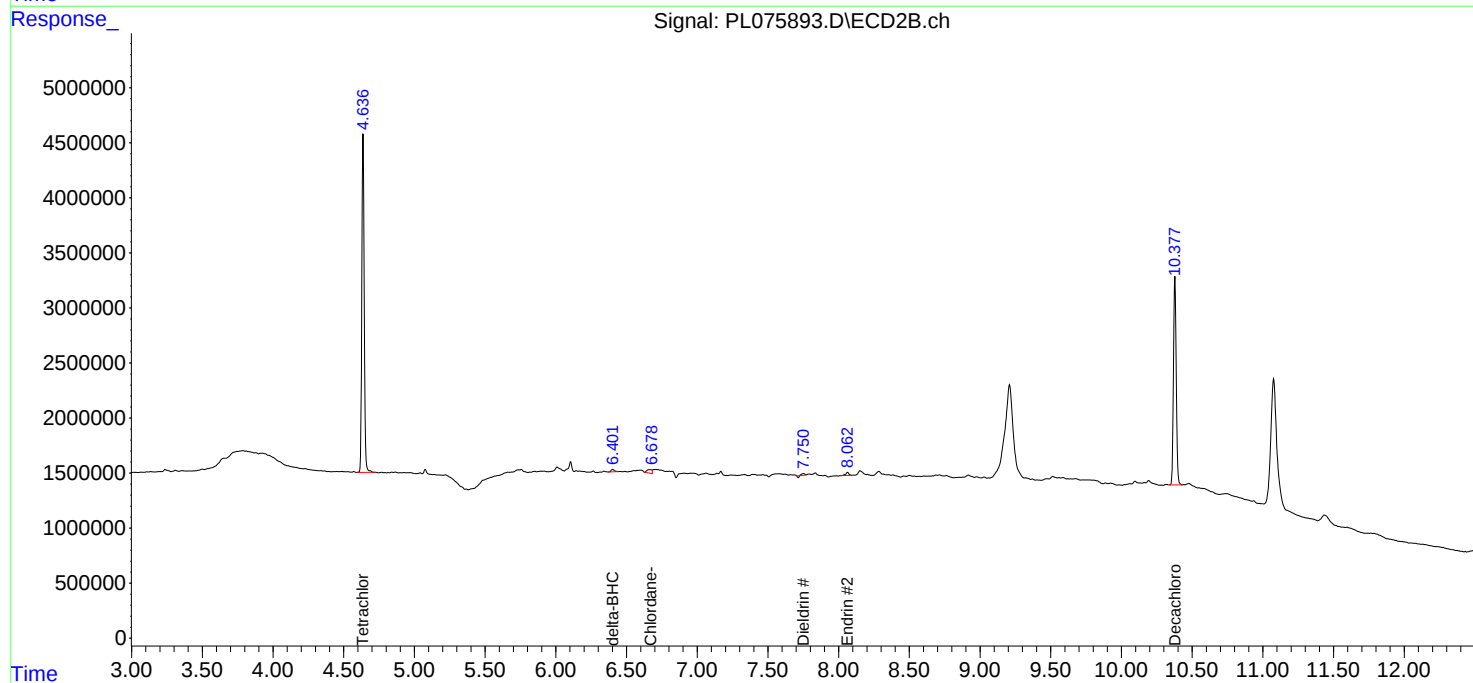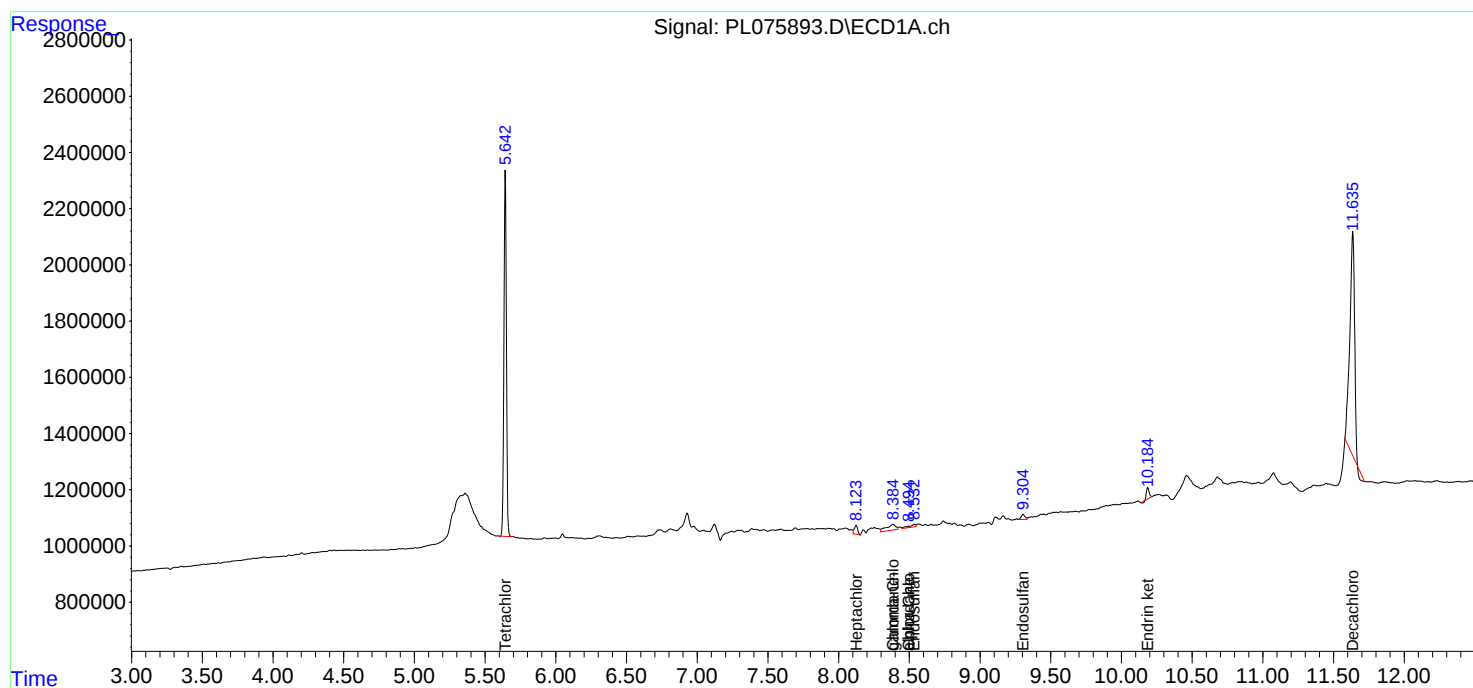


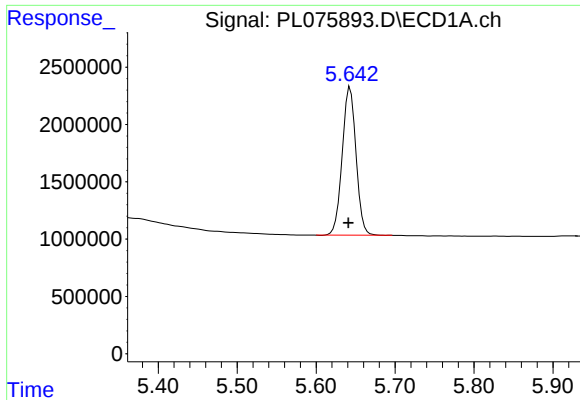

#1 Tetrachloro-m-xylene


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 15679085
Conc: 23.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

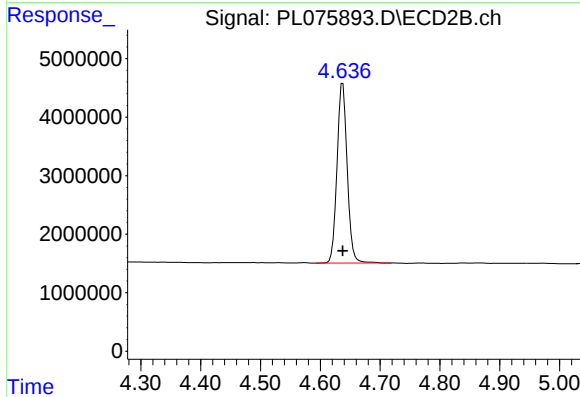


#1 Tetrachloro-m-xylene

R.T.: 4.638 min
Delta R.T.: 0.000 min
Response: 36532279
Conc: 21.77 ng/ml

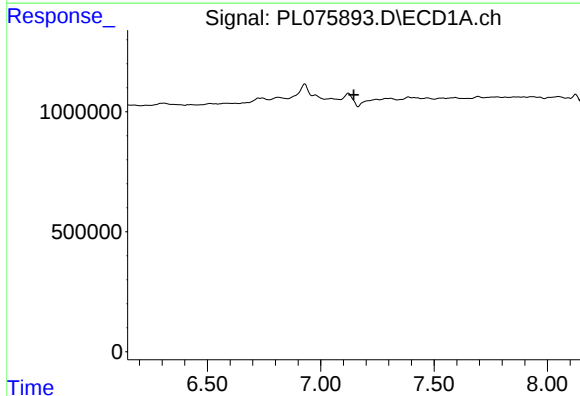


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

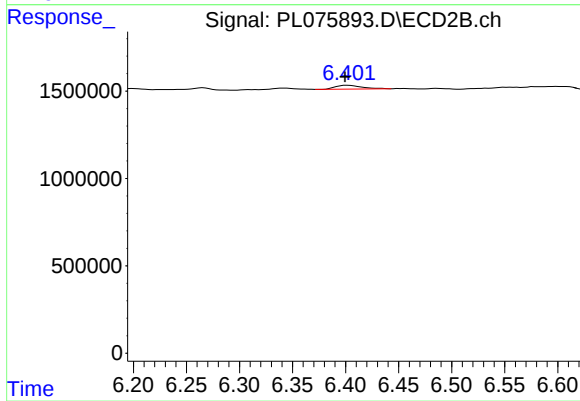

#7 delta-BHC


R.T.: 6.402 min
Delta R.T.: 0.003 min
Response: 363357
Conc: 0.17 ng/ml

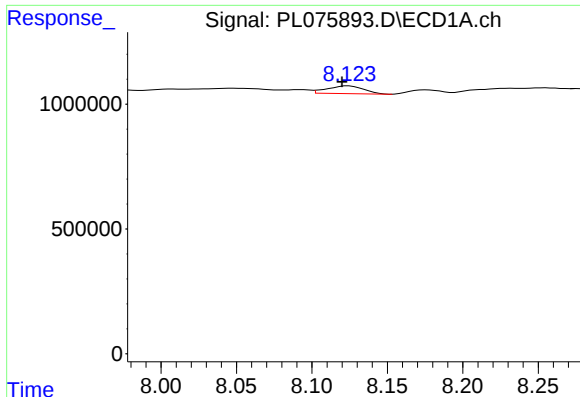

#8 Heptachlor epoxide

R.T.: 8.124 min
Delta R.T.: 0.004 min
Response: 525457
Conc: 0.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

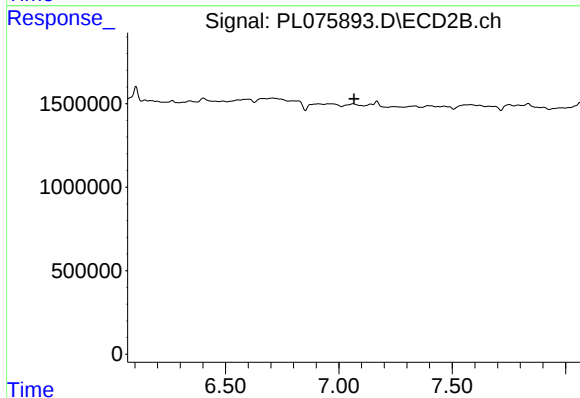


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.067 min
Response: 0
Conc: N.D.


#9 Endosulfan I

R.T.: 8.535 min
Delta R.T.: 0.006 min
Response: 154846
Conc: 0.22 ng/ml

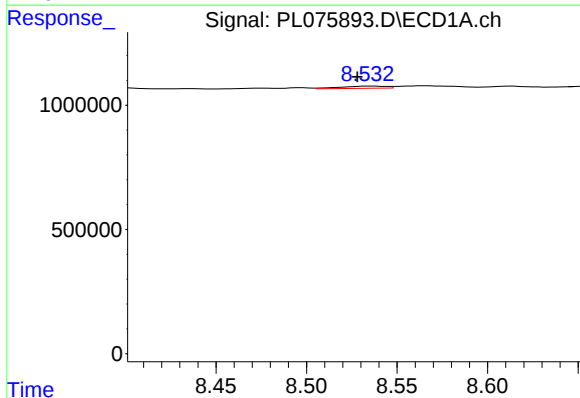

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 7.469 min
Response: 0
Conc: N.D.

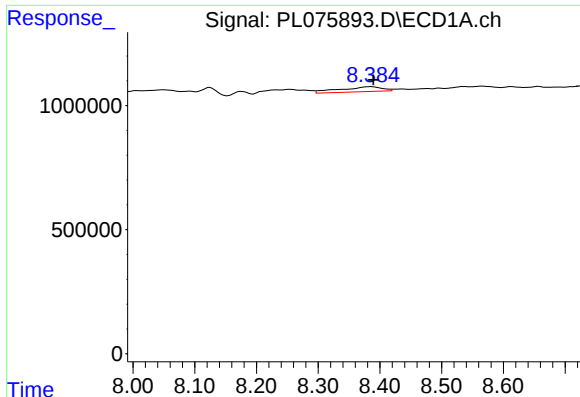

#10 gamma-Chlordane


R.T.: 8.386 min
Delta R.T.: -0.004 min
Response: 942109
Conc: 1.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

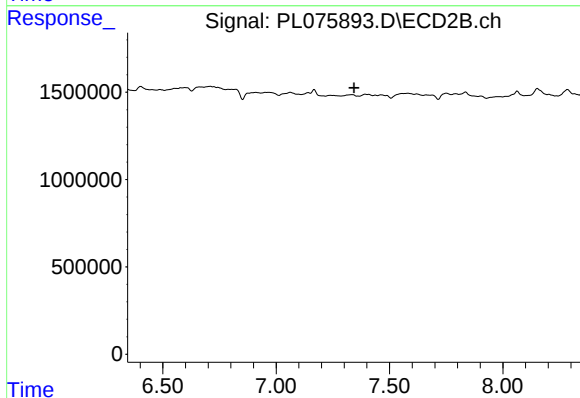


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

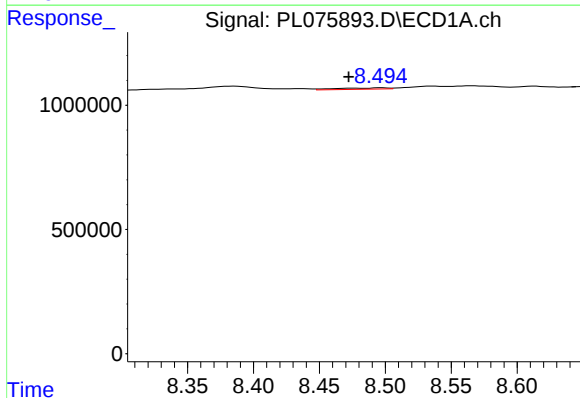


#11 alpha-Chlordane

R.T.: 8.497 min
Delta R.T.: 0.025 min
Response: 140710
Conc: 0.18 ng/ml

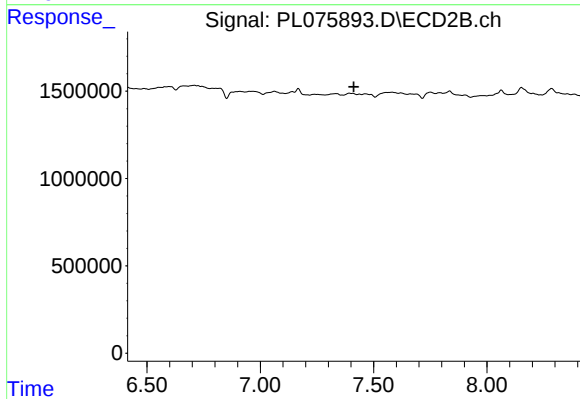

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.412 min
Response: 0
Conc: N.D.

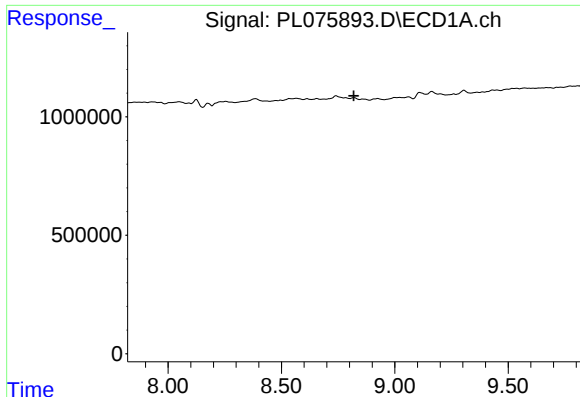

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.819 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

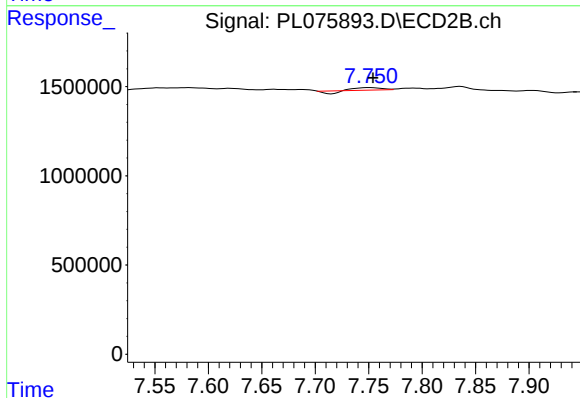


#13 Dieldrin

R.T.: 7.751 min
Delta R.T.: -0.003 min
Response: 149381
Conc: 0.09 ng/ml

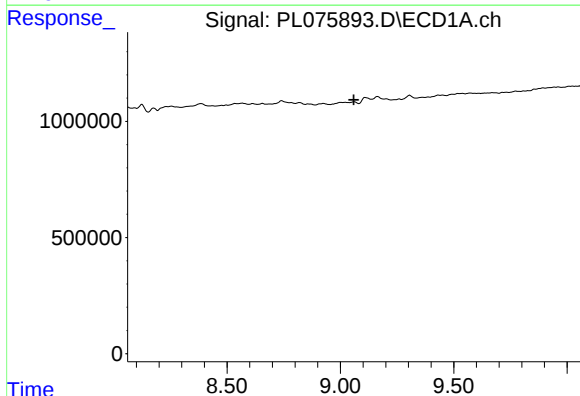


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.059 min
Response: 0
Conc: N.D.

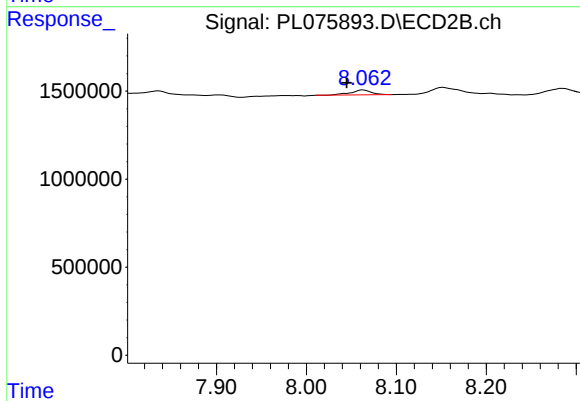

#14 Endrin


R.T.: 8.063 min
Delta R.T.: 0.018 min
Response: 446334
Conc: 0.33 ng/ml

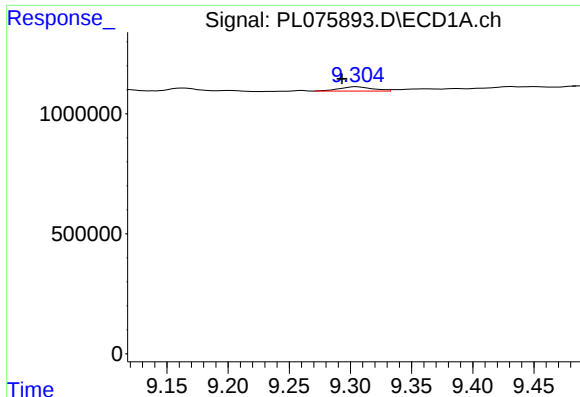

#15 Endosulfan II


R.T.: 9.305 min
Delta R.T.: 0.012 min
Response: 339970
Conc: 0.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

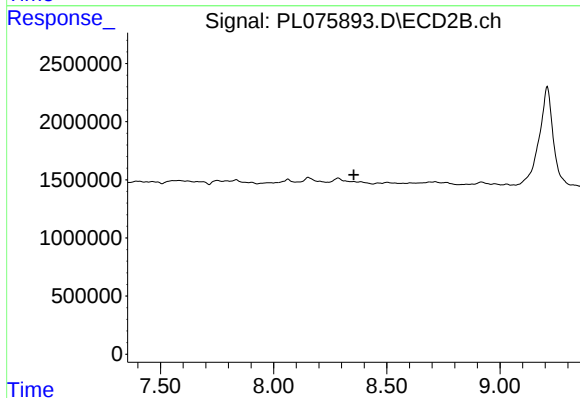


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

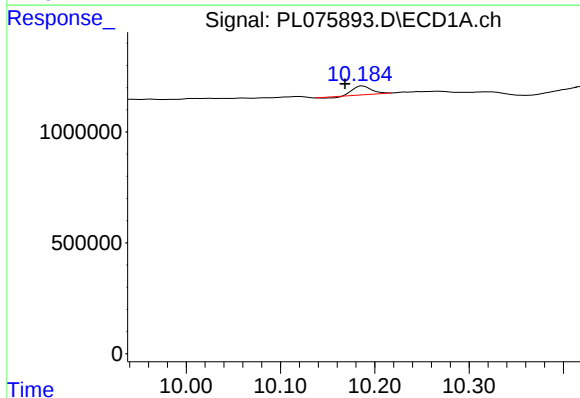


#21 Endrin ketone

R.T.: 10.187 min
Delta R.T.: 0.019 min
Response: 495511
Conc: 0.70 ng/ml

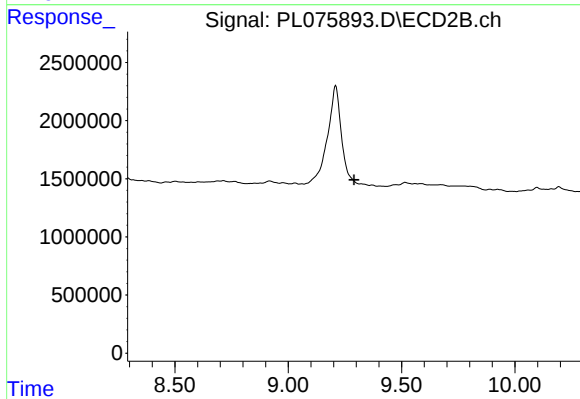

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

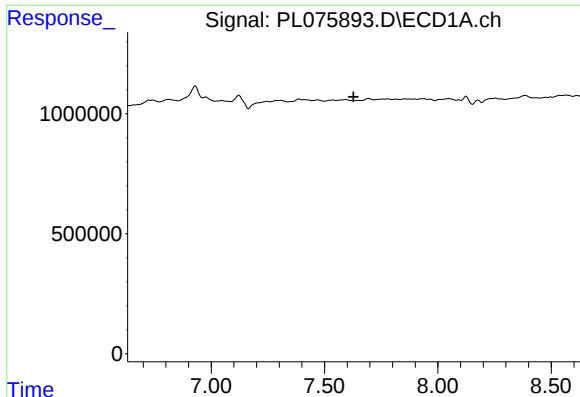

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 7.628 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

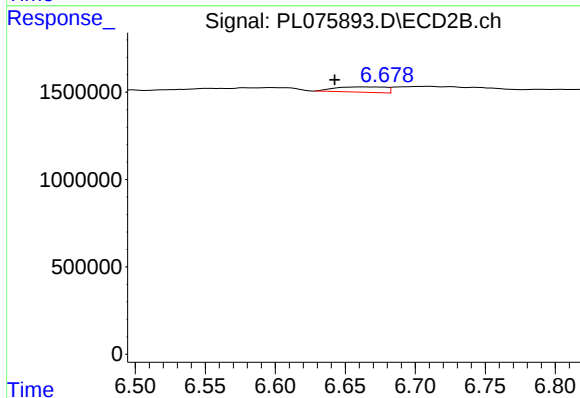


#24 Chlordane-2

R.T.: 6.672 min
Delta R.T.: 0.029 min
Response: 768686
Conc: 11.49 ng/ml

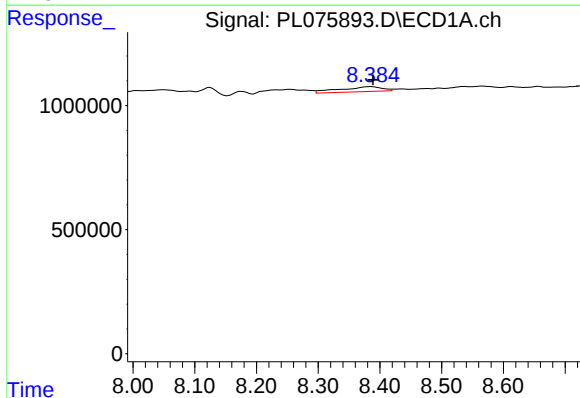


#25 Chlordane-3

R.T.: 8.386 min
Delta R.T.: -0.003 min
Response: 942109
Conc: 9.12 ng/ml

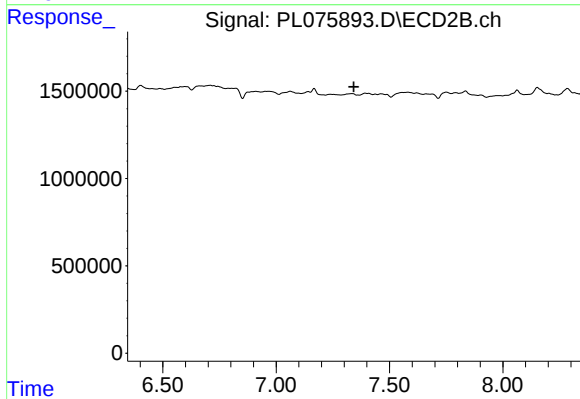

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

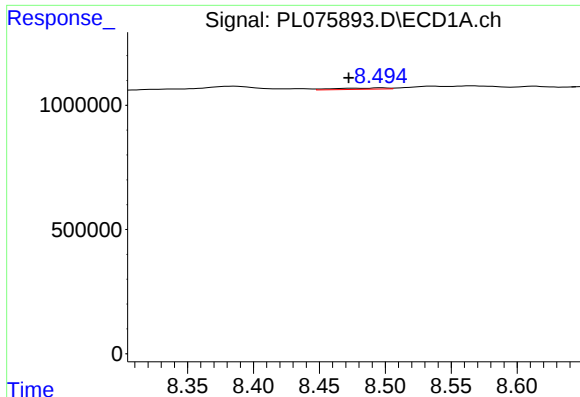

#26 Chlordane-4


R.T.: 8.497 min
Delta R.T.: 0.025 min
Response: 140710
Conc: 1.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

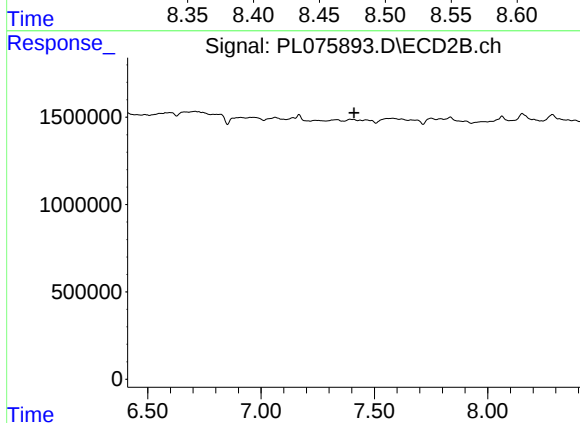


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.411 min
Response: 0
Conc: N.D.

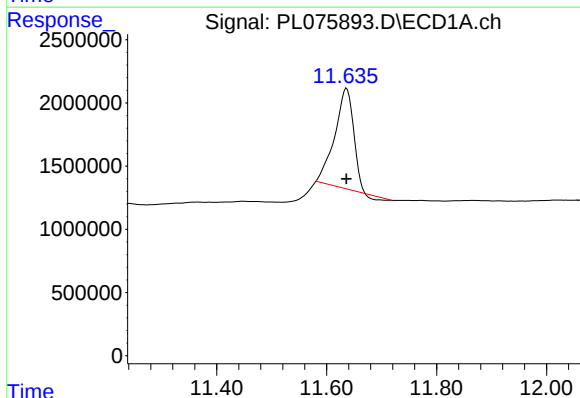

#28 Decachlorobiphenyl

R.T.: 11.636 min
Delta R.T.: 0.000 min
Response: 18248087
Conc: 29.81 ng/ml

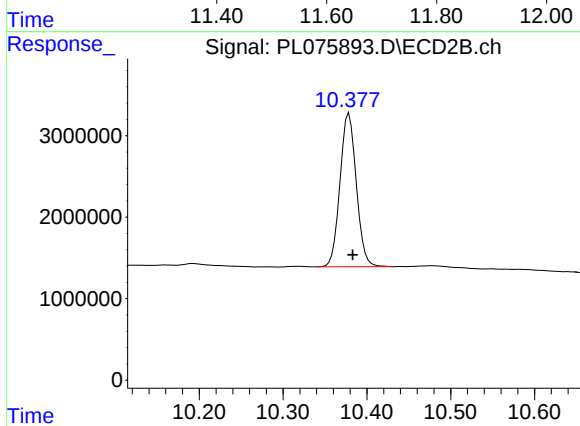

#28 Decachlorobiphenyl

R.T.: 10.379 min
Delta R.T.: -0.004 min
Response: 25458614
Conc: 18.07 ng/ml