

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062222\
 Data File : PL075899.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2022 15:55
 Operator : AR\AJ
 Sample : PB145740BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 00:15:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.635	11657130	27554758	17.273	16.419
28)	SA Decachlor...	11.636	10.376	11133817	22158401	18.186	15.727
Target Compounds							
7)	B delta-BHC	0.000	6.400	0	251039	N.D.	0.117 #
10)	B gamma-Chl...	8.380	0.000	855657	0	1.102	N.D. #
11)	B alpha-Chl...	8.492f	0.000	147981	0	0.194	N.D. #
14)	MA Endrin	0.000	8.061f	0	417936	N.D.	0.306 #
15)	B Endosulfa...	9.303	0.000	200114	0	0.322	N.D. #
21)	B Endrin ke...	10.185f	0.000	628970	0	0.894	N.D. #
25)	Chlordane-3	8.380	0.000	855657	0	8.287	N.D. #
26)	Chlordane-4	8.492f	0.000	147981	0	1.168	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062222\
Data File : PL075899.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2022 15:55
Operator : AR\AJ
Sample : PB145740BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:15:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

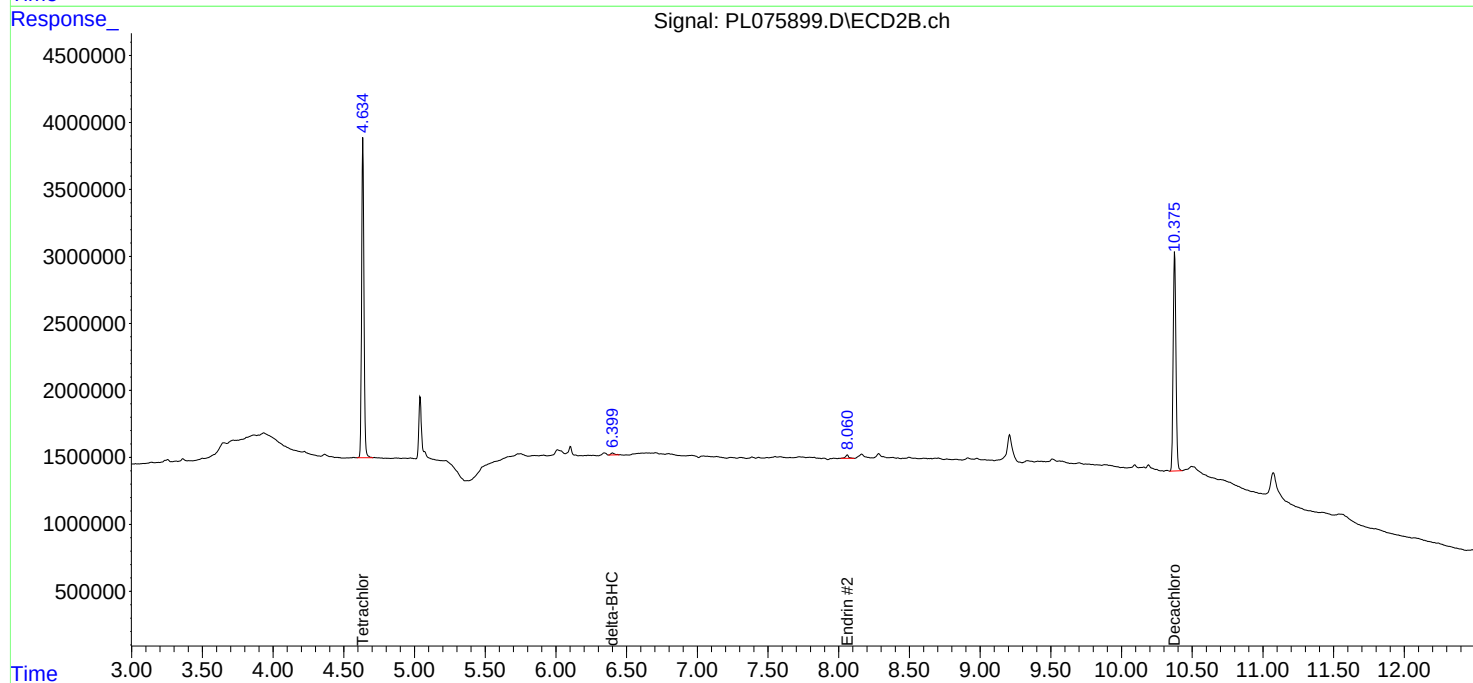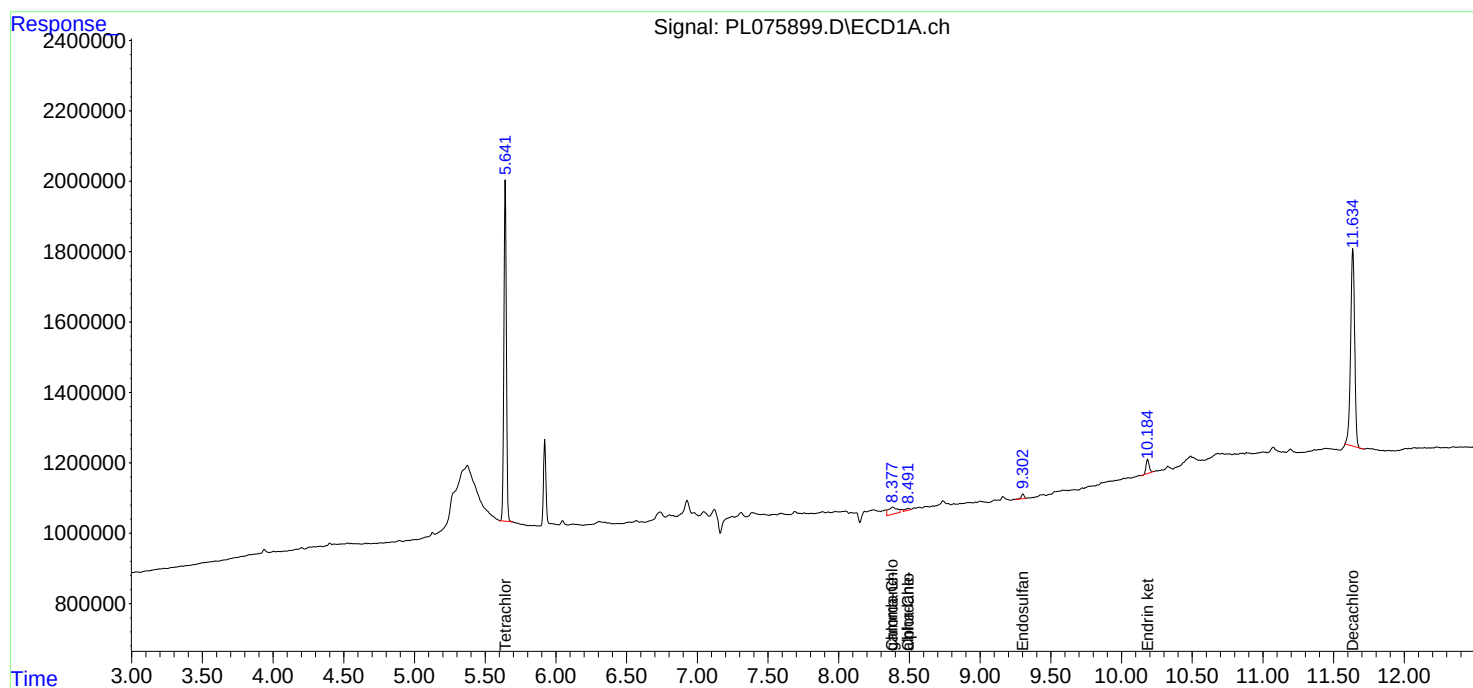


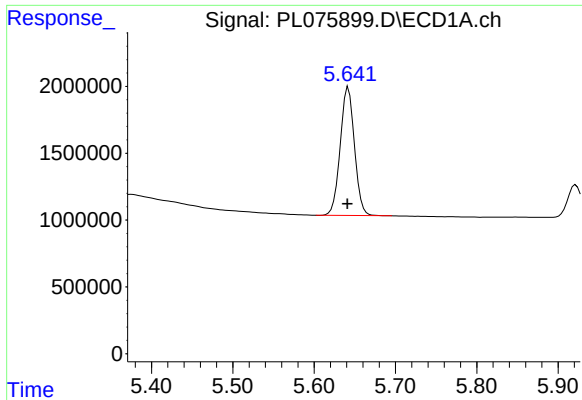

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: 0.001 min
Response: 11657130
Conc: 17.27 ng/ml

Instrument :
ECD_D
ClientSampleId :

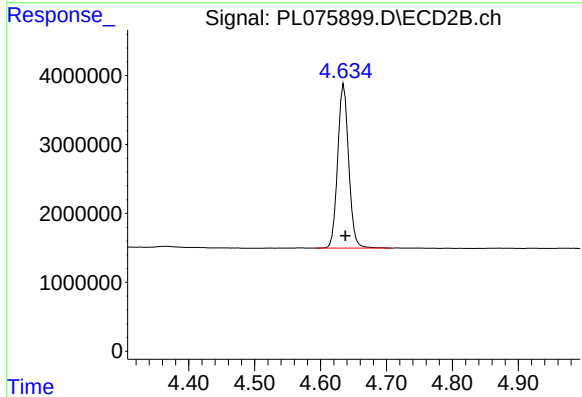


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: -0.002 min
Response: 27554758
Conc: 16.42 ng/ml

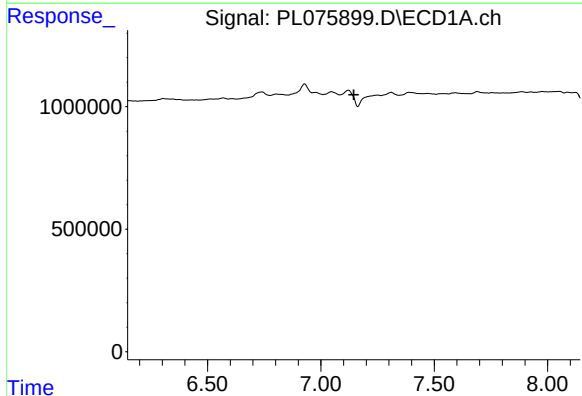


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

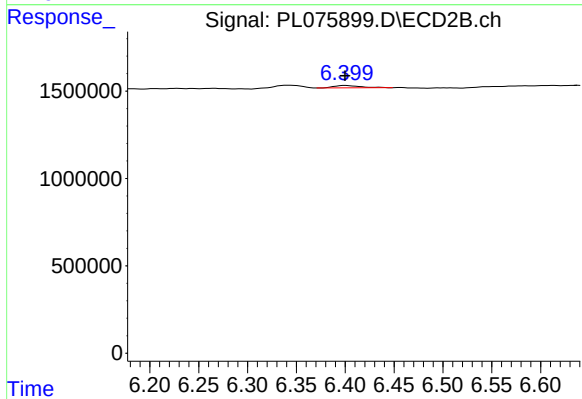

#7 delta-BHC

R.T.: 6.400 min
Delta R.T.: 0.000 min
Response: 251039
Conc: 0.12 ng/ml

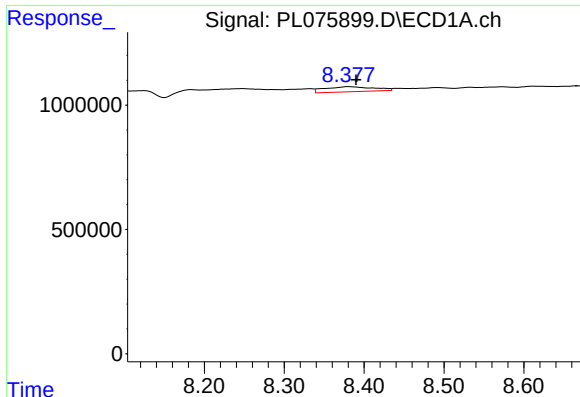

#10 gamma-Chlordane

R.T.: 8.380 min
Delta R.T.: -0.009 min
Response: 855657
Conc: 1.10 ng/ml

Instrument :
ECD_D
ClientSampleId :

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

#11 alpha-Chlordane

R.T.: 8.492 min
Delta R.T.: 0.020 min
Response: 147981
Conc: 0.19 ng/ml

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.412 min
Response: 0
Conc: N.D.

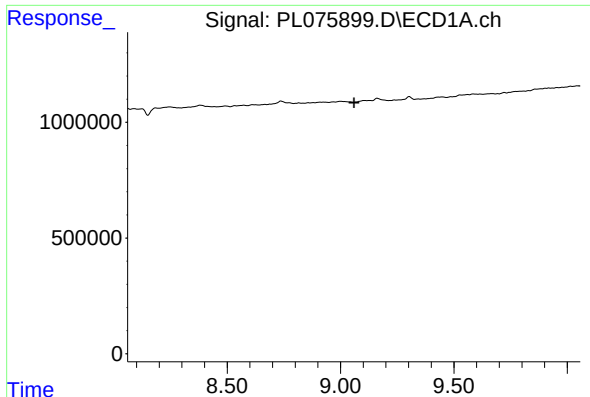

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

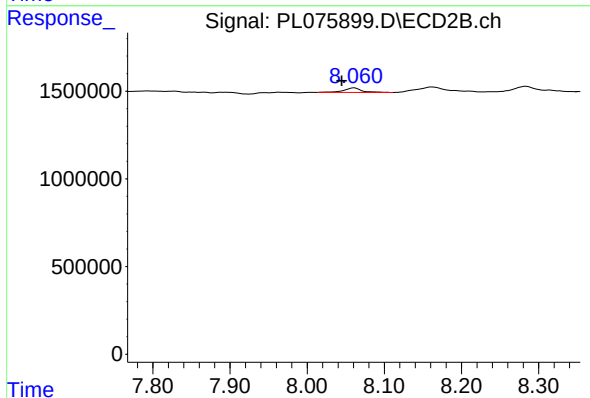


#14 Endrin

R.T.: 8.061 min
Delta R.T.: 0.016 min
Response: 417936
Conc: 0.31 ng/ml

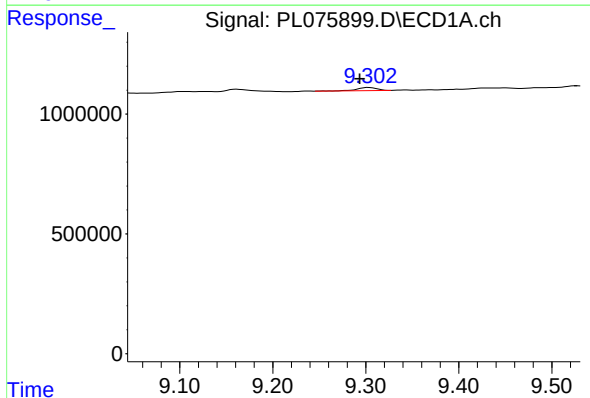


#15 Endosulfan II

R.T.: 9.303 min
Delta R.T.: 0.010 min
Response: 200114
Conc: 0.32 ng/ml

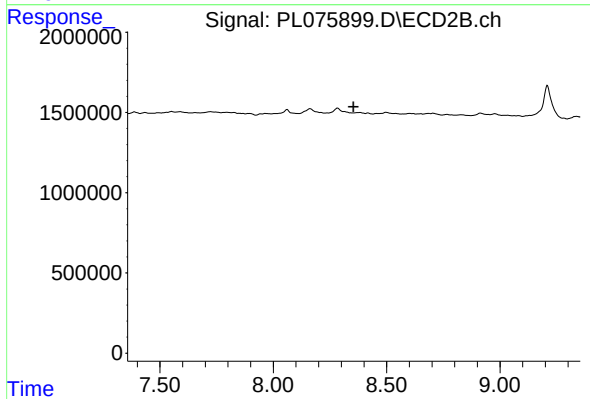

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.354 min
Response: 0
Conc: N.D.

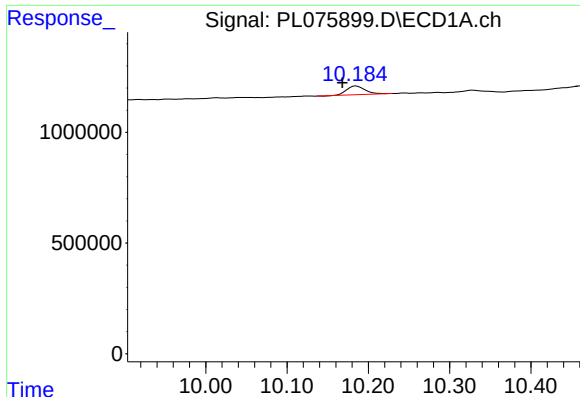

#21 Endrin ketone


R.T.: 10.185 min
Delta R.T.: 0.017 min
Response: 628970
Conc: 0.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

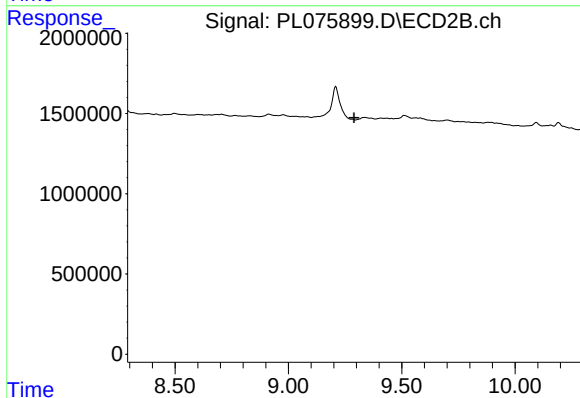


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

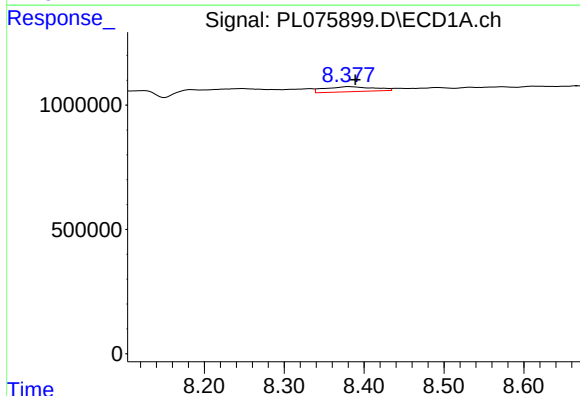


#25 Chlordane-3

R.T.: 8.380 min
Delta R.T.: -0.009 min
Response: 855657
Conc: 8.29 ng/ml

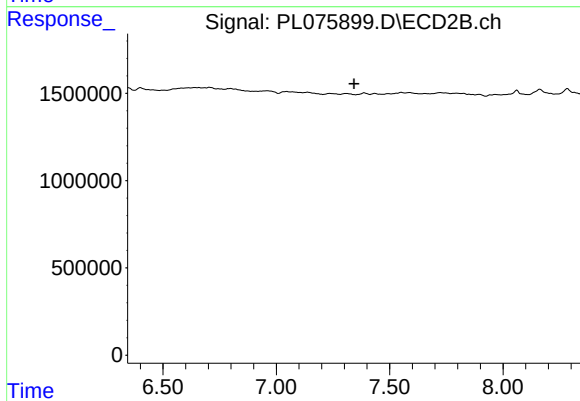

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

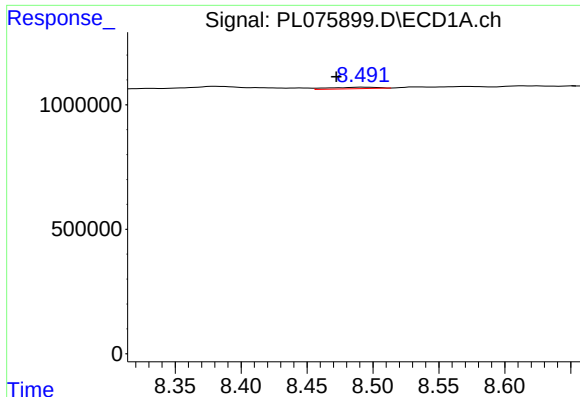

#26 Chlordane-4


R.T.: 8.492 min
Delta R.T.: 0.020 min
Response: 147981
Conc: 1.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

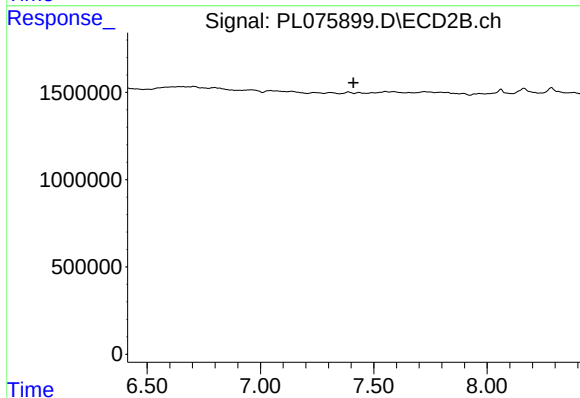


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.411 min
Response: 0
Conc: N.D.

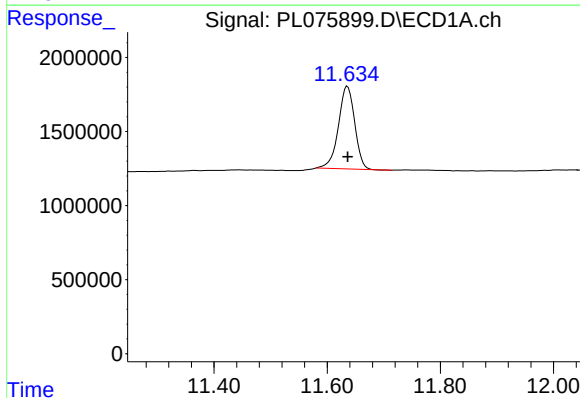

#28 Decachlorobiphenyl

R.T.: 11.636 min
Delta R.T.: 0.000 min
Response: 11133817
Conc: 18.19 ng/ml

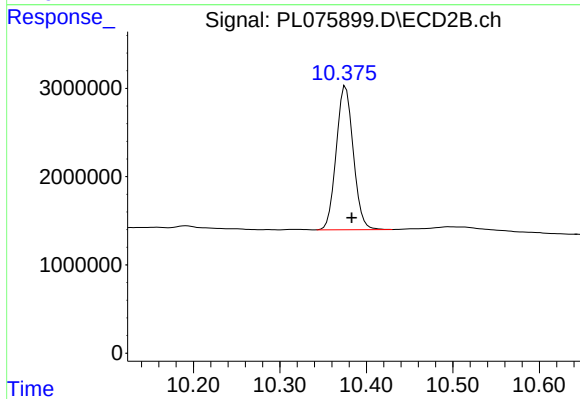

#28 Decachlorobiphenyl

R.T.: 10.376 min
Delta R.T.: -0.007 min
Response: 22158401
Conc: 15.73 ng/ml