

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062222\
 Data File : PL075909.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2022 18:41
 Operator : AR\AJ
 Sample : PB145757BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 00:18:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.642	4.636	10606039	26668259	15.715	15.891
28)	SA Decachlor...	11.635	10.377	8229716	17423730	13.442	12.366
Target Compounds							
5)	MB Aldrin	0.000	6.500	0	374370	N.D.	0.191 #
7)	B delta-BHC	0.000	6.400	0	348930	N.D.	0.163 #
10)	B gamma-Chl...	8.379	0.000	1164234	0	1.499	N.D. #
11)	B alpha-Chl...	8.470	0.000	44700	0	0.059	N.D. #
14)	MA Endrin	0.000	8.061f	0	855898	N.D.	0.626 #
15)	B Endosulfa...	9.303	0.000	257655	0	0.414	N.D. #
17)	MA 4,4'-DDT	9.533	0.000	2189233	0	3.418	N.D. #
19)	B Endosulfa...	9.673	0.000	40259	0	0.064	N.D. #
21)	B Endrin ke...	10.184f	0.000	910768	0	1.295	N.D. #
25)	Chlordane-3	8.379	0.000	1164234	0	11.276	N.D. #
26)	Chlordane-4	8.470	0.000	44700	0	0.353	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062222\
Data File : PL075909.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2022 18:41
Operator : AR\AJ
Sample : PB145757BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:18:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

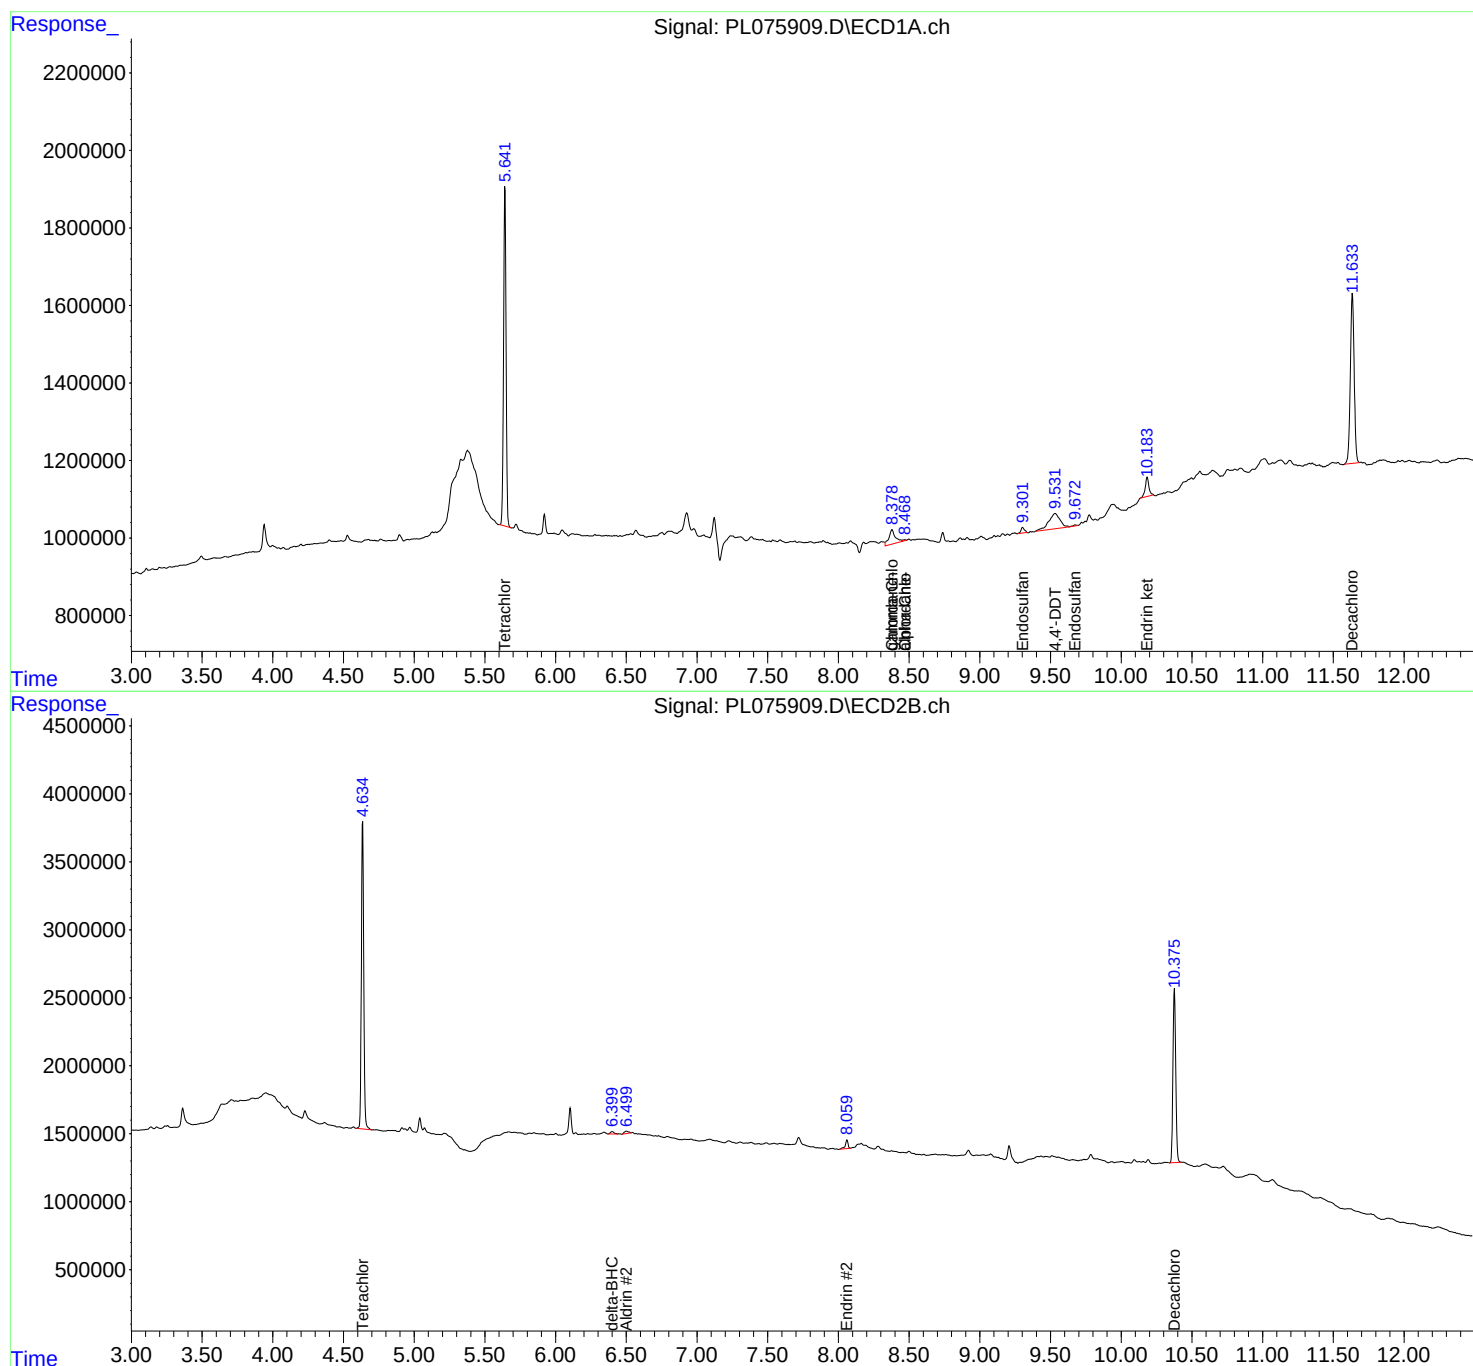


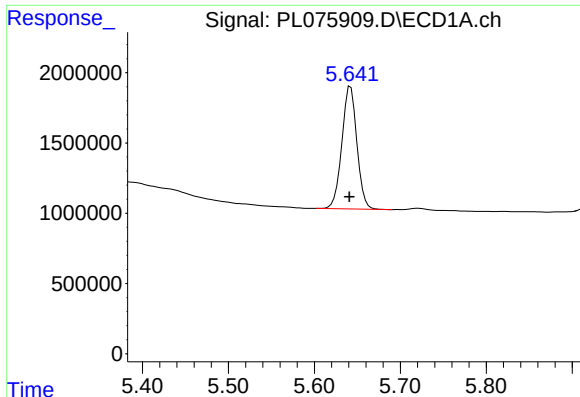

#1 Tetrachloro-m-xylene


R.T.: 5.642 min
Delta R.T.: 0.001 min
Response: 10606039
Conc: 15.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

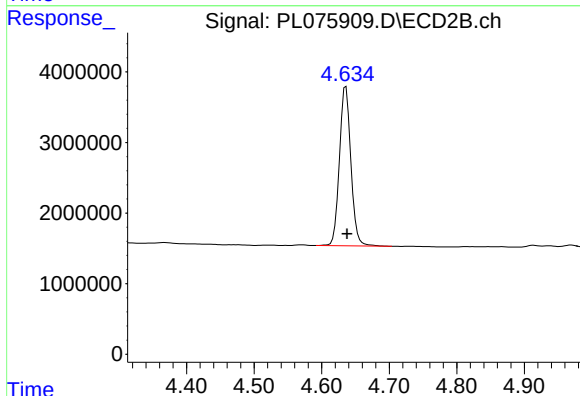


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.002 min
Response: 26668259
Conc: 15.89 ng/ml

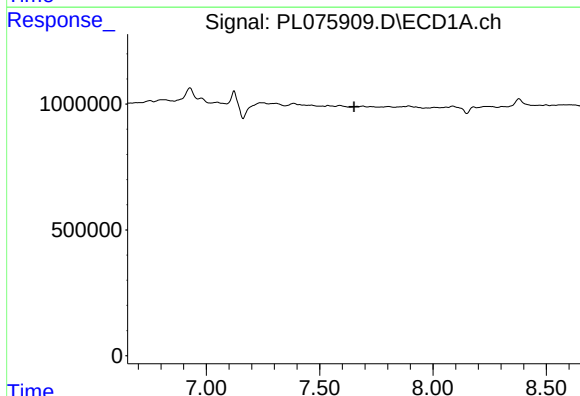


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 7.652 min
Response: 0
Conc: N.D.

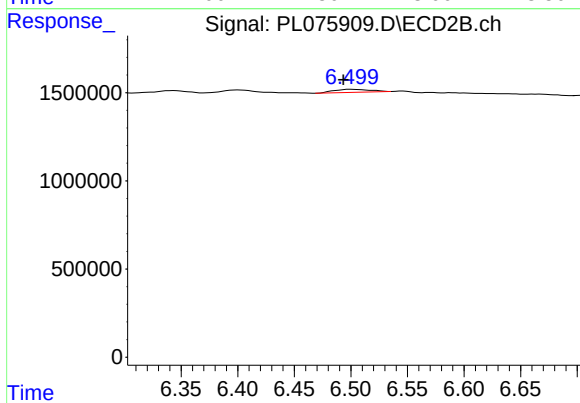

#5 Aldrin


R.T.: 6.500 min
Delta R.T.: 0.007 min
Response: 374370
Conc: 0.19 ng/ml

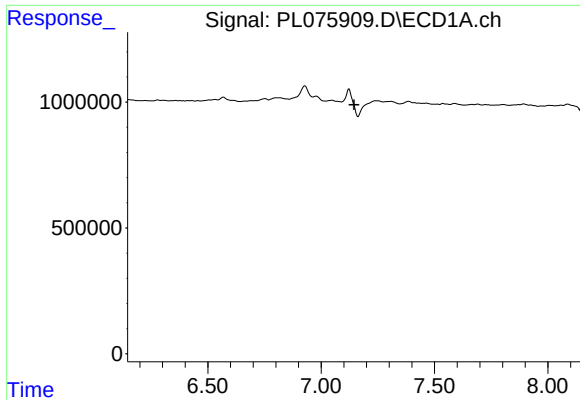

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 7.145 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

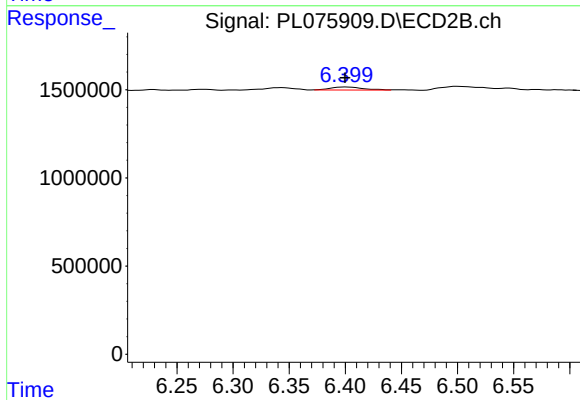


#7 delta-BHC

R.T.: 6.400 min
Delta R.T.: 0.000 min
Response: 348930
Conc: 0.16 ng/ml

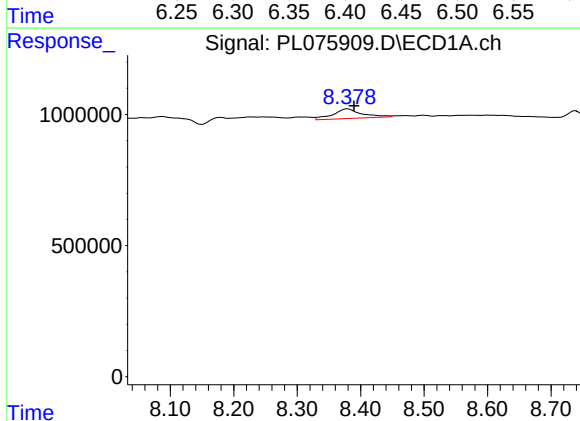


#10 gamma-Chlordane

R.T.: 8.379 min
Delta R.T.: -0.011 min
Response: 1164234
Conc: 1.50 ng/ml

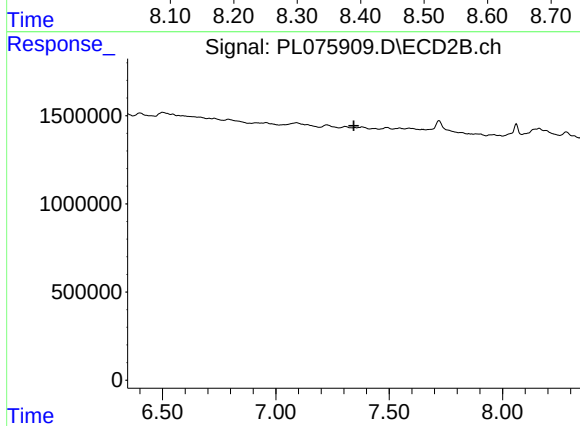

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.344 min
Response: 0
Conc: N.D.

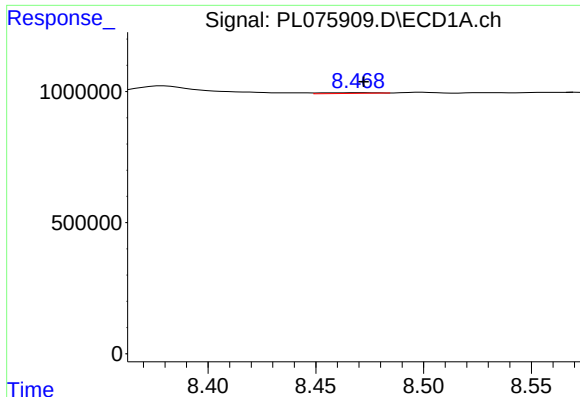

#11 alpha-Chlordane


R.T.: 8.470 min
Delta R.T.: -0.002 min
Response: 44700
Conc: 0.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

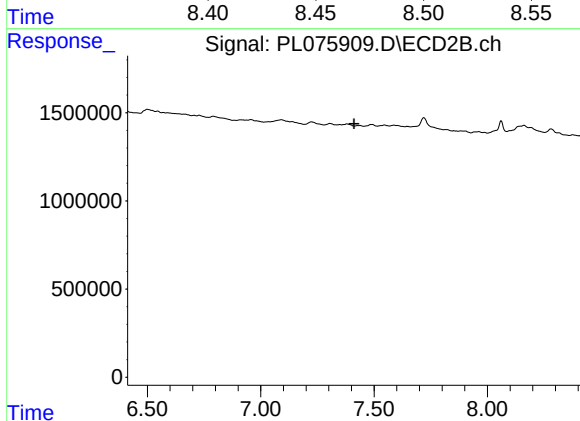


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.412 min
Response: 0
Conc: N.D.

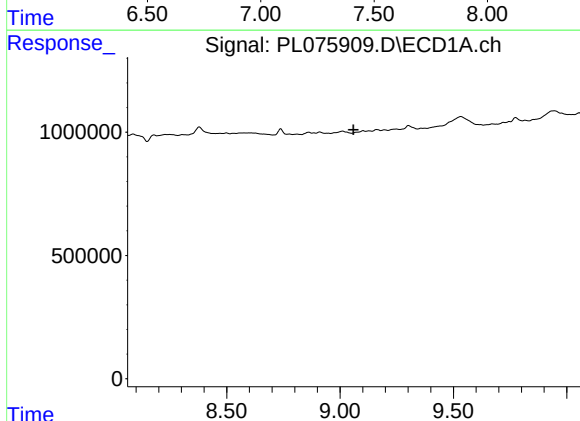


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 9.059 min
Response: 0
Conc: N.D.

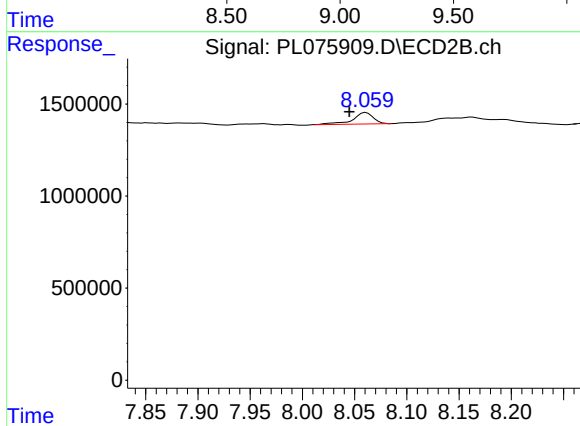

#14 Endrin


R.T.: 8.061 min
Delta R.T.: 0.016 min
Response: 855898
Conc: 0.63 ng/ml

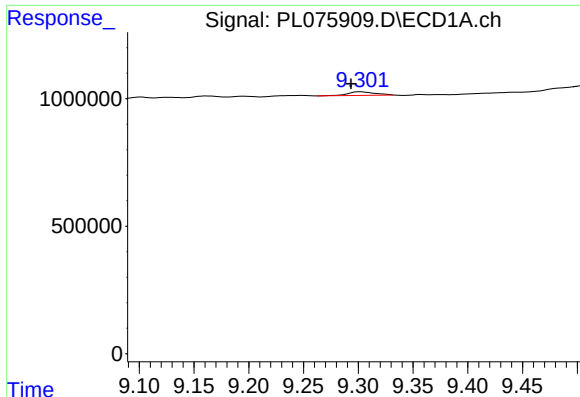

#15 Endosulfan II


R.T.: 9.303 min
Delta R.T.: 0.009 min
Response: 257655
Conc: 0.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

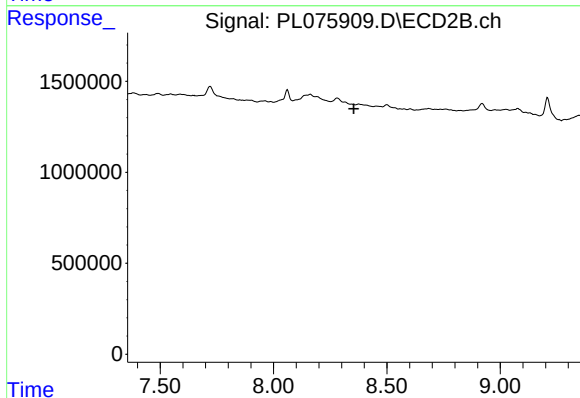


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

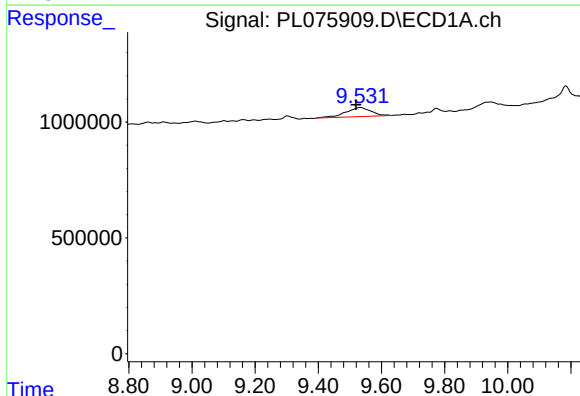


#17 4,4'-DDT

R.T.: 9.533 min
Delta R.T.: 0.014 min
Response: 2189233
Conc: 3.42 ng/ml

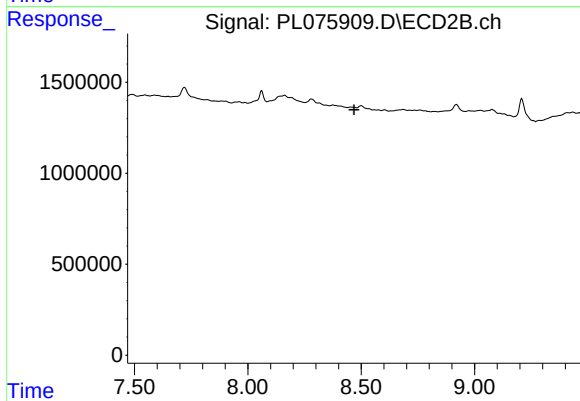

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 8.469 min
Response: 0
Conc: N.D.

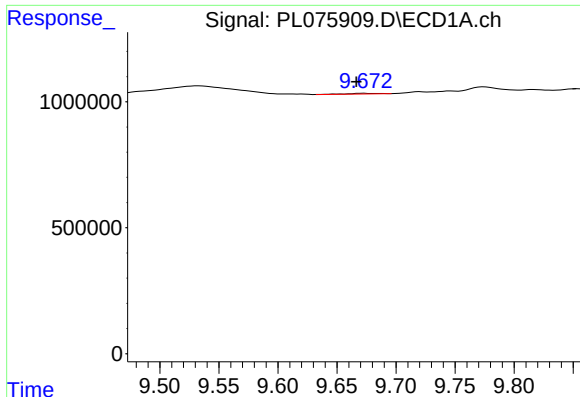

#19 Endosulfan Sulfate


R.T.: 9.673 min
Delta R.T.: 0.007 min
Response: 40259
Conc: 0.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

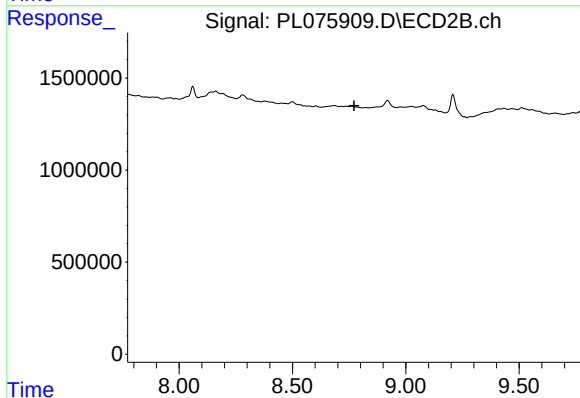


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 8.772 min
Response: 0
Conc: N.D.

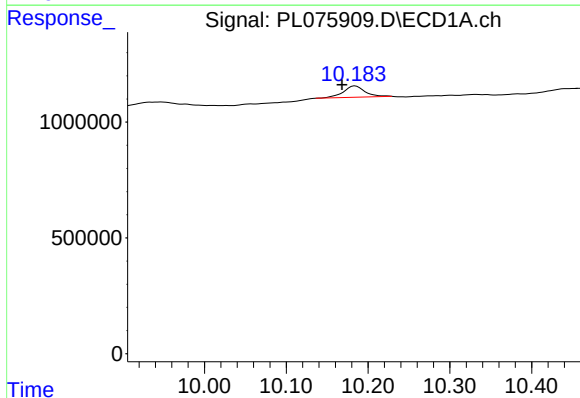


#21 Endrin ketone

R.T.: 10.184 min
Delta R.T.: 0.016 min
Response: 910768
Conc: 1.30 ng/ml

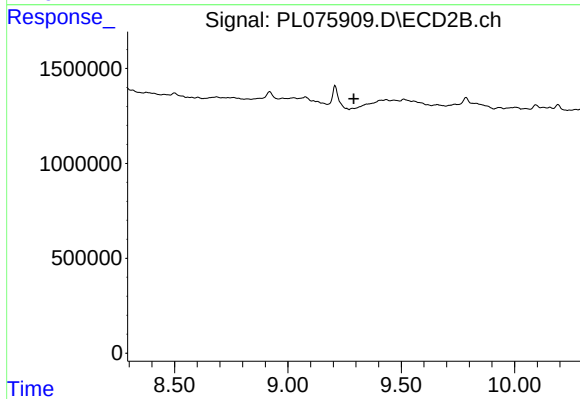

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

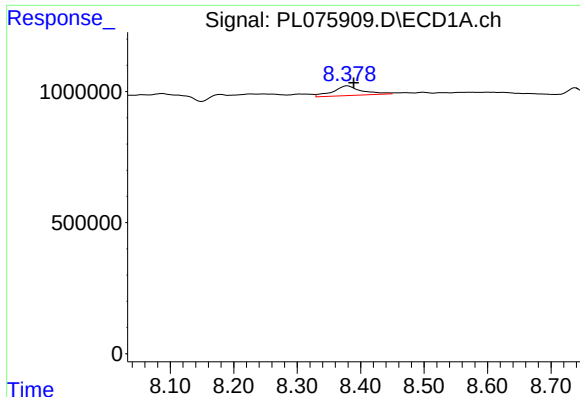

#25 Chlordane-3


R.T.: 8.379 min
Delta R.T.: -0.010 min
Response: 1164234
Conc: 11.28 ng/ml

Instrument :
ECD_D
ClientSampleId :

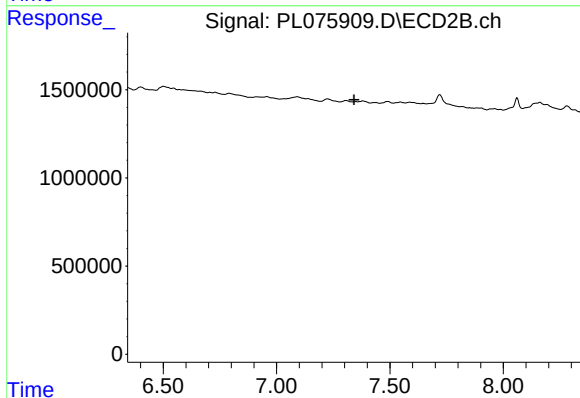


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

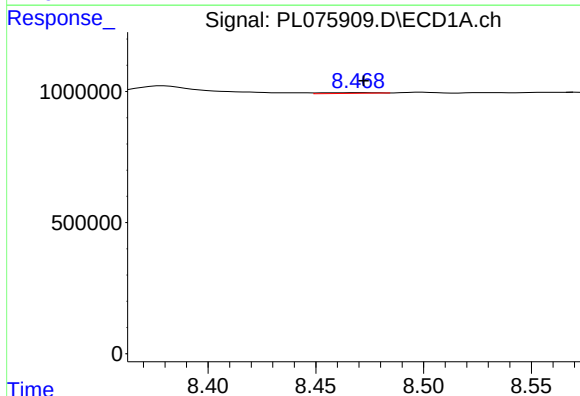


#26 Chlordane-4

R.T.: 8.470 min
Delta R.T.: -0.002 min
Response: 44700
Conc: 0.35 ng/ml

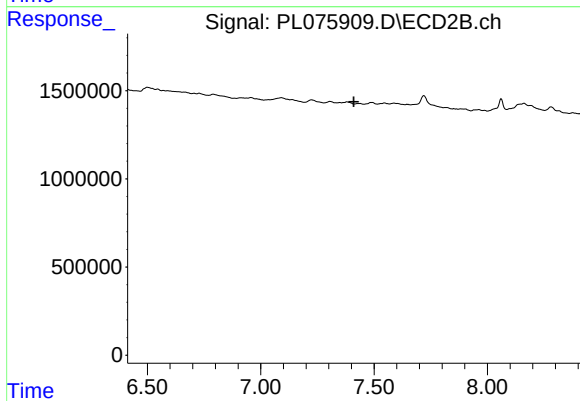

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 7.411 min
Response: 0
Conc: N.D.

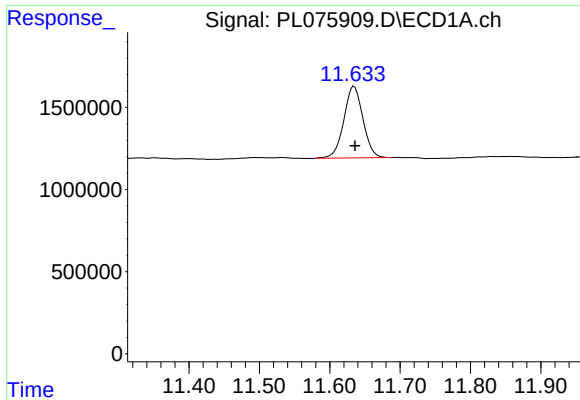

#28 Decachlorobiphenyl

R.T.: 11.635 min
Delta R.T.: -0.002 min
Response: 8229716
Conc: 13.44 ng/ml

Instrument :
ECD_D
ClientSampleId :

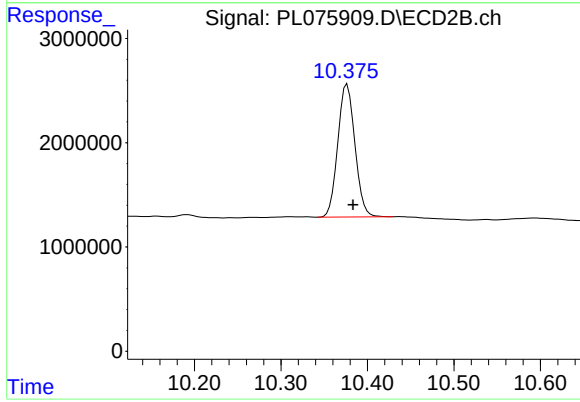

#28 Decachlorobiphenyl

R.T.: 10.377 min
Delta R.T.: -0.007 min
Response: 17423730
Conc: 12.37 ng/ml