

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062222\
 Data File : PL075915.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2022 22:16
 Operator : AR\AJ
 Sample : PB145757BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 00:19:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.635	11472018	28299078	16.998	16.863
28)	SA Decachlor...	11.634	10.375	9776880	22562240	15.969	16.014
Target Compounds							
7)	B delta-BHC	0.000	6.399	0	341070	N.D.	0.159 #
9)	A Endosulfan I	8.533	0.000	140918	0	0.201	N.D. #
10)	B gamma-Chl...	8.376	0.000	1910834	0	2.461	N.D. #
11)	B alpha-Chl...	8.498f	0.000	458375	0	0.601	N.D. #
13)	MA Dieldrin	0.000	7.726f	0	212347	N.D.	0.125 #
14)	MA Endrin	0.000	8.061f	0	1805019	N.D.	1.320 #
15)	B Endosulfa...	9.302	0.000	241011	0	0.387	N.D. #
21)	B Endrin ke...	10.183	0.000	663630	0	0.944	N.D. #
25)	Chlordane-3	8.376	0.000	1910834	0	18.506	N.D. #
26)	Chlordane-4	8.498f	0.000	458375	0	3.619	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062222\
Data File : PL075915.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2022 22:16
Operator : AR\AJ
Sample : PB145757BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:19:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

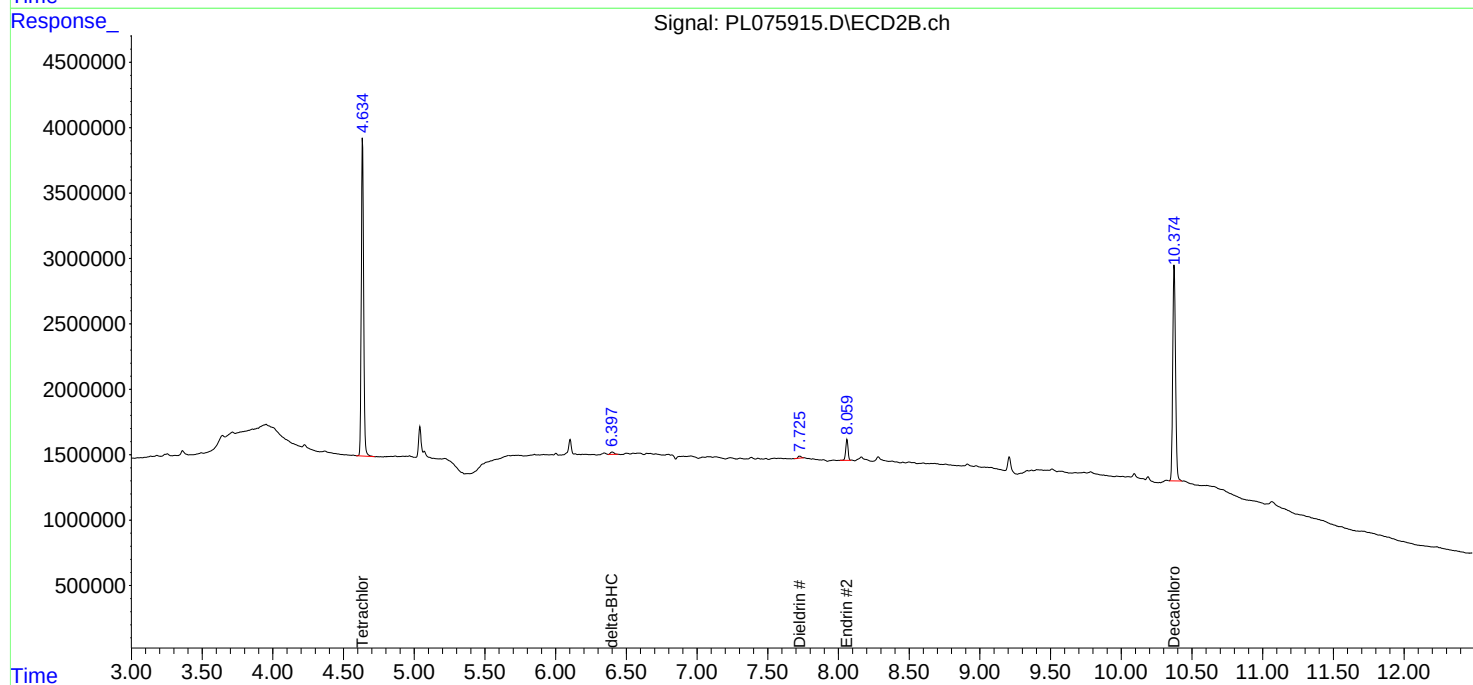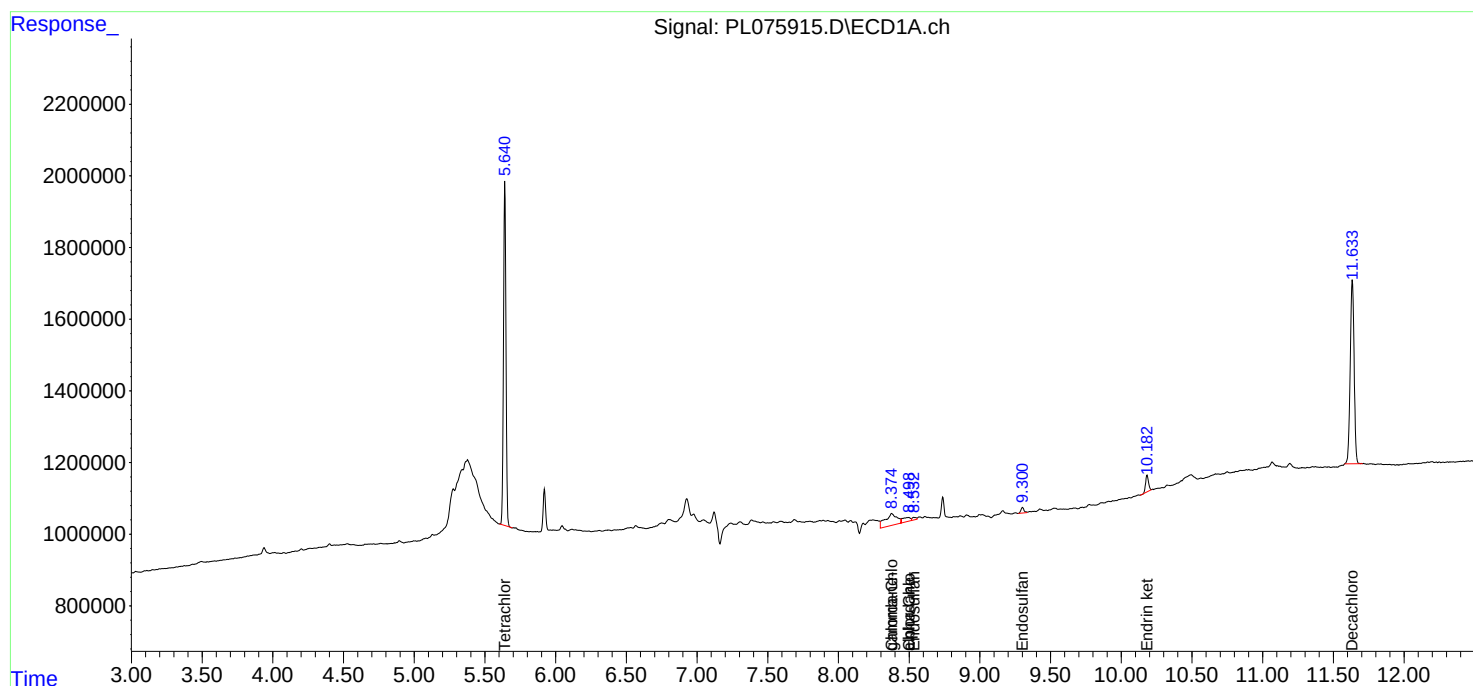


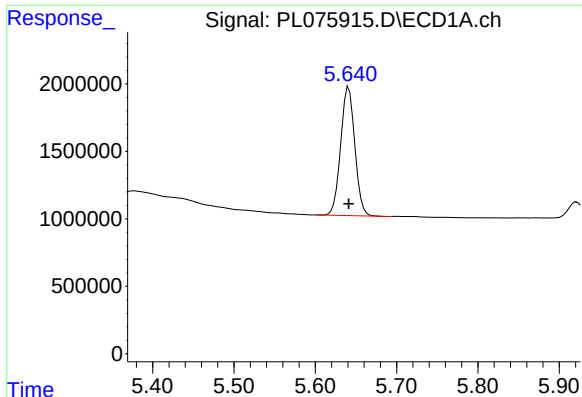

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 11472018
Conc: 17.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

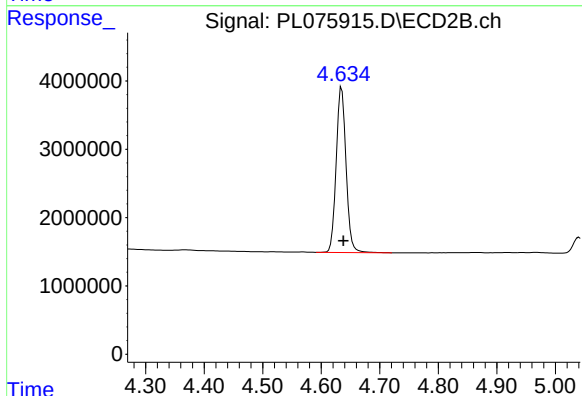


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: -0.003 min
Response: 28299078
Conc: 16.86 ng/ml

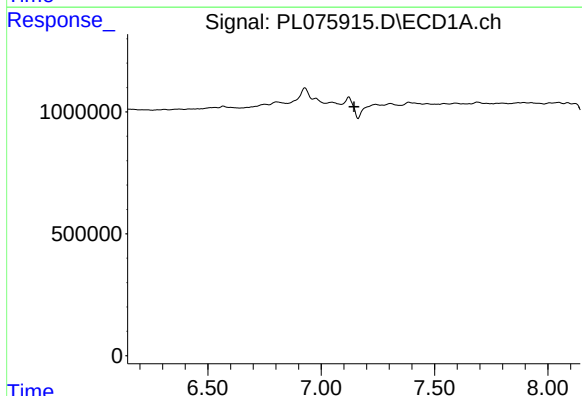


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

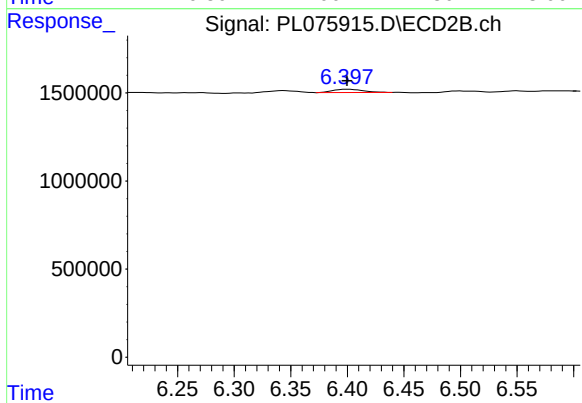

#7 delta-BHC


R.T.: 6.399 min
Delta R.T.: 0.000 min
Response: 341070
Conc: 0.16 ng/ml

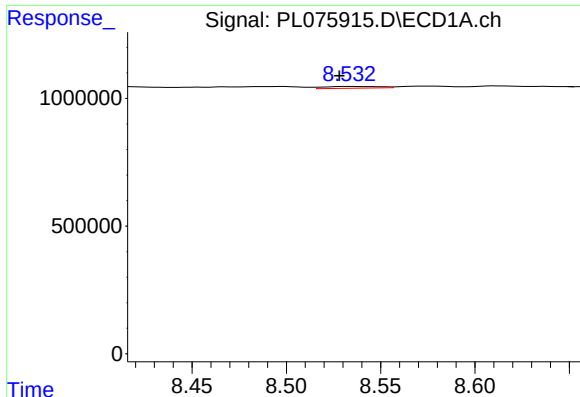

#9 Endosulfan I


R.T.: 8.533 min
Delta R.T.: 0.005 min
Response: 140918
Conc: 0.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

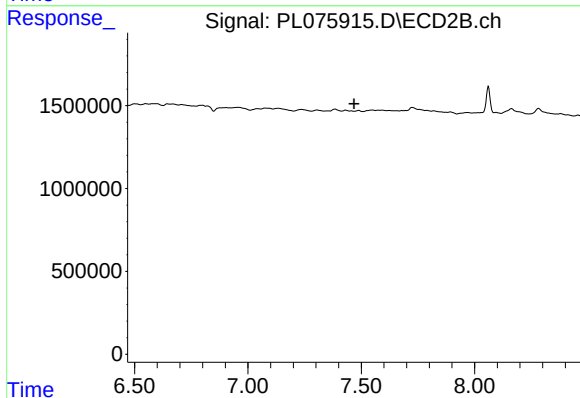


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.469 min
Response: 0
Conc: N.D.

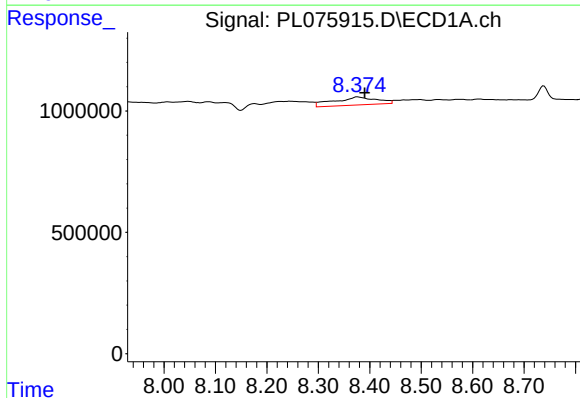


#10 gamma-Chlordane

R.T.: 8.376 min
Delta R.T.: -0.014 min
Response: 1910834
Conc: 2.46 ng/ml

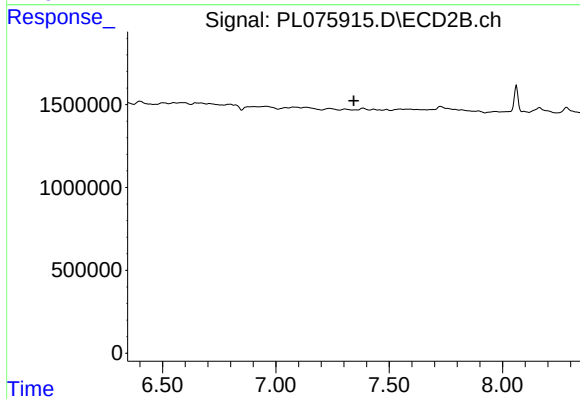

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

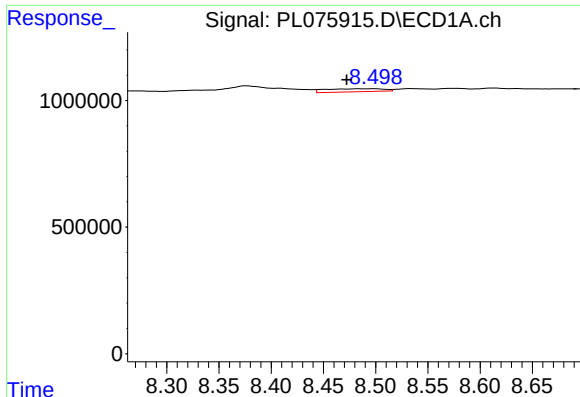

#11 alpha-Chlordane


R.T.: 8.498 min
Delta R.T.: 0.026 min
Response: 458375
Conc: 0.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

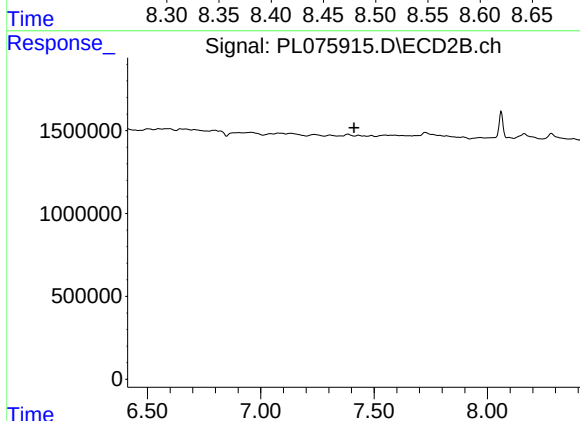


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.412 min
Response: 0
Conc: N.D.

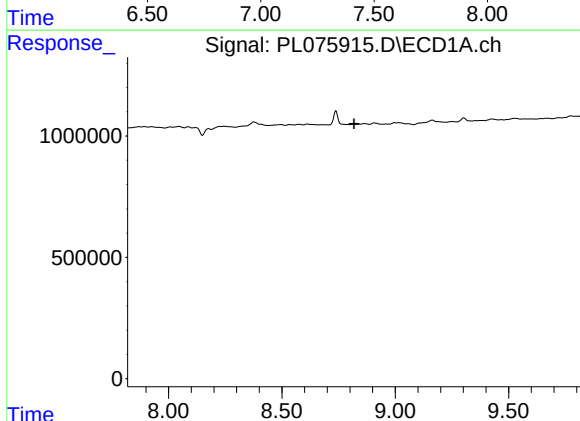


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.819 min
Response: 0
Conc: N.D.

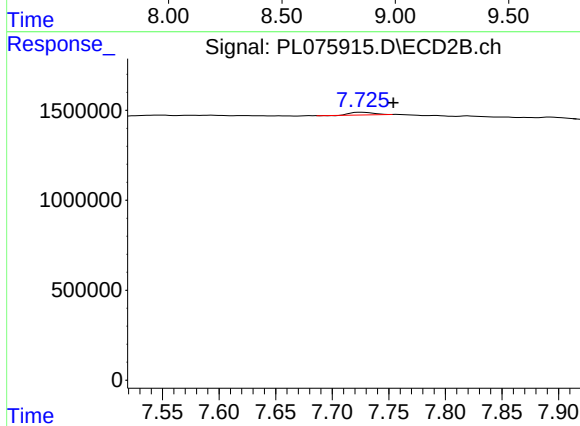

#13 Dieldrin


R.T.: 7.726 min
Delta R.T.: -0.028 min
Response: 212347
Conc: 0.13 ng/ml

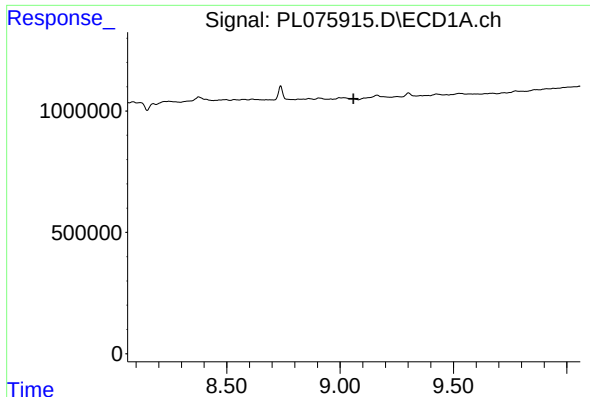

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 9.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

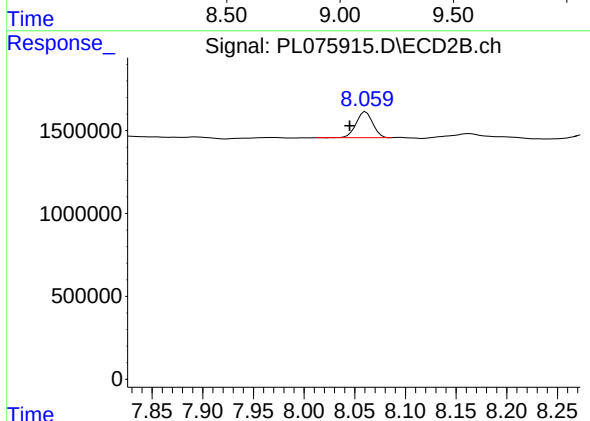


#14 Endrin

R.T.: 8.061 min
Delta R.T.: 0.016 min
Response: 1805019
Conc: 1.32 ng/ml

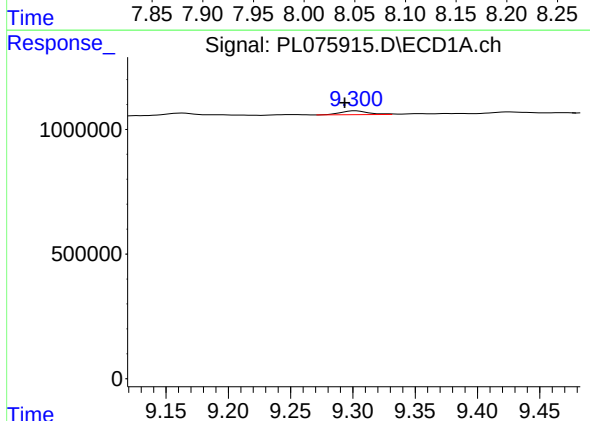


#15 Endosulfan II

R.T.: 9.302 min
Delta R.T.: 0.009 min
Response: 241011
Conc: 0.39 ng/ml

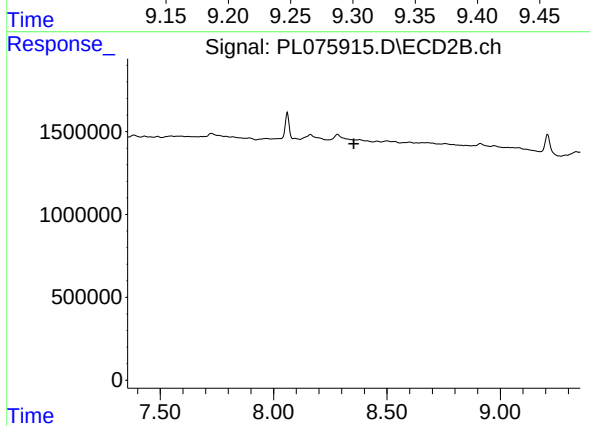

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.354 min
Response: 0
Conc: N.D.

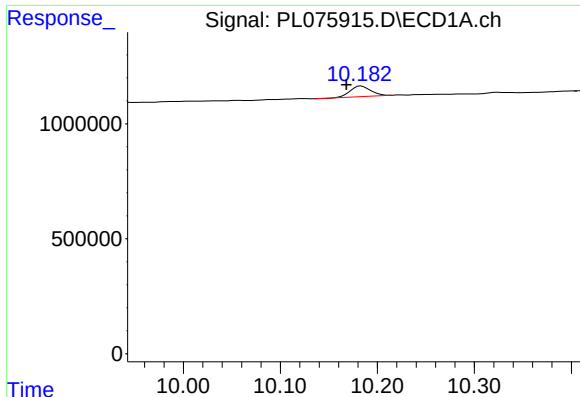

#21 Endrin ketone


R.T.: 10.183 min
Delta R.T.: 0.015 min
Response: 663630
Conc: 0.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

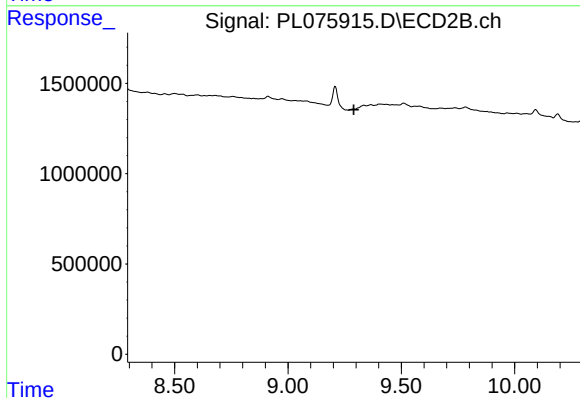


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

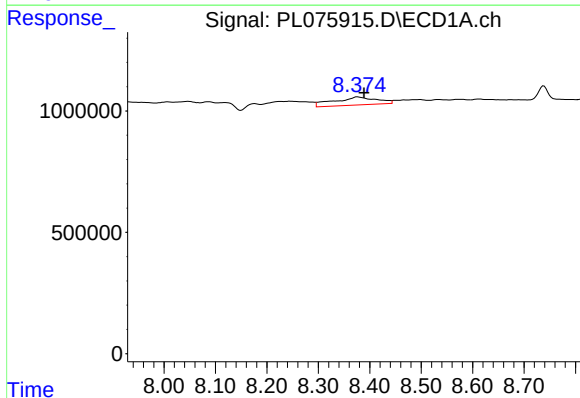


#25 Chlordane-3

R.T.: 8.376 min
Delta R.T.: -0.013 min
Response: 1910834
Conc: 18.51 ng/ml

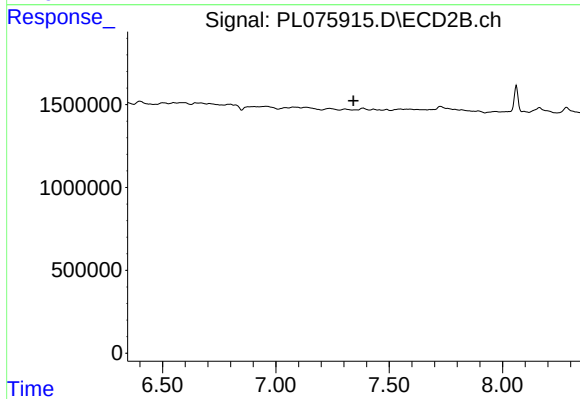

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

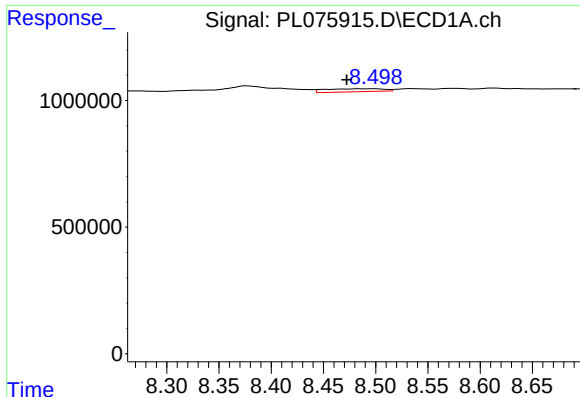

#26 Chlordane-4


R.T.: 8.498 min
Delta R.T.: 0.026 min
Response: 458375
Conc: 3.62 ng/ml

Instrument :
ECD_D
ClientSampleId :

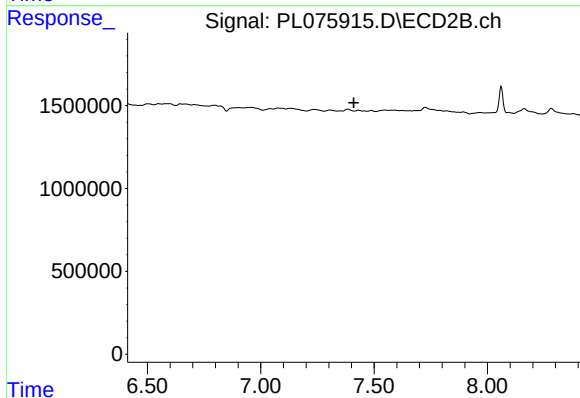


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.411 min
Response: 0
Conc: N.D.

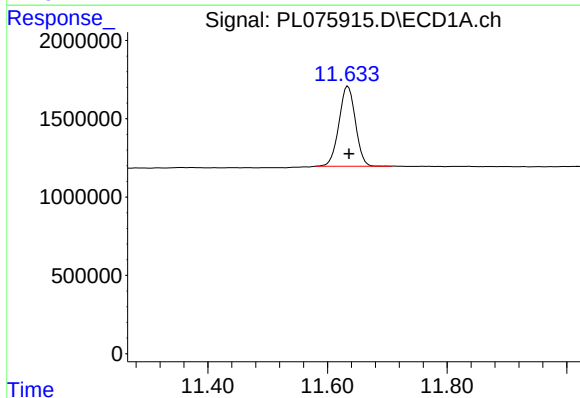

#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: -0.002 min
Response: 9776880
Conc: 15.97 ng/ml

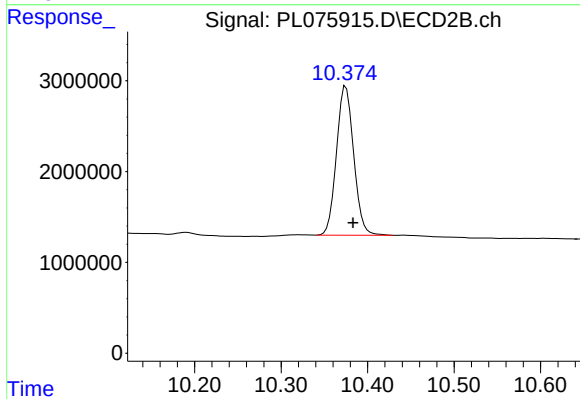

#28 Decachlorobiphenyl

R.T.: 10.375 min
Delta R.T.: -0.008 min
Response: 22562240
Conc: 16.01 ng/ml