

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062222\
 Data File : PL075917.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jun 2022 22:49
 Operator : AR\AJ
 Sample : PB145645TB
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 23 00:20:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 07 02:04:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.641	4.635	12687716	30738596	18.800	18.317
28)	SA Decachlor...	11.634	10.376	10887856	24709358	17.784	17.537
Target Compounds							
7)	B delta-BHC	0.000	6.399	0	262811	N.D.	0.123 #
10)	B gamma-Chl...	8.378	0.000	777234	0	1.001	N.D. #
11)	B alpha-Chl...	8.458	0.000	42944	0	0.056	N.D. #
13)	MA Dieldrin	0.000	7.724f	0	418959	N.D.	0.248 #
14)	MA Endrin	0.000	8.061f	0	642675	N.D.	0.470 #
15)	B Endosulfa...	9.303	0.000	235828	0	0.379	N.D. #
21)	B Endrin ke...	10.185f	0.000	736303	0	1.047	N.D. #
25)	Chlordane-3	8.378	0.000	777234	0	7.527	N.D. #
26)	Chlordane-4	8.458	0.000	42944	0	0.339	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL062222\
Data File : PL075917.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jun 2022 22:49
Operator : AR\AJ
Sample : PB145645TB
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 23 00:20:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL060622.M
Quant Title : GC Extractables
QLast Update : Tue Jun 07 02:04:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

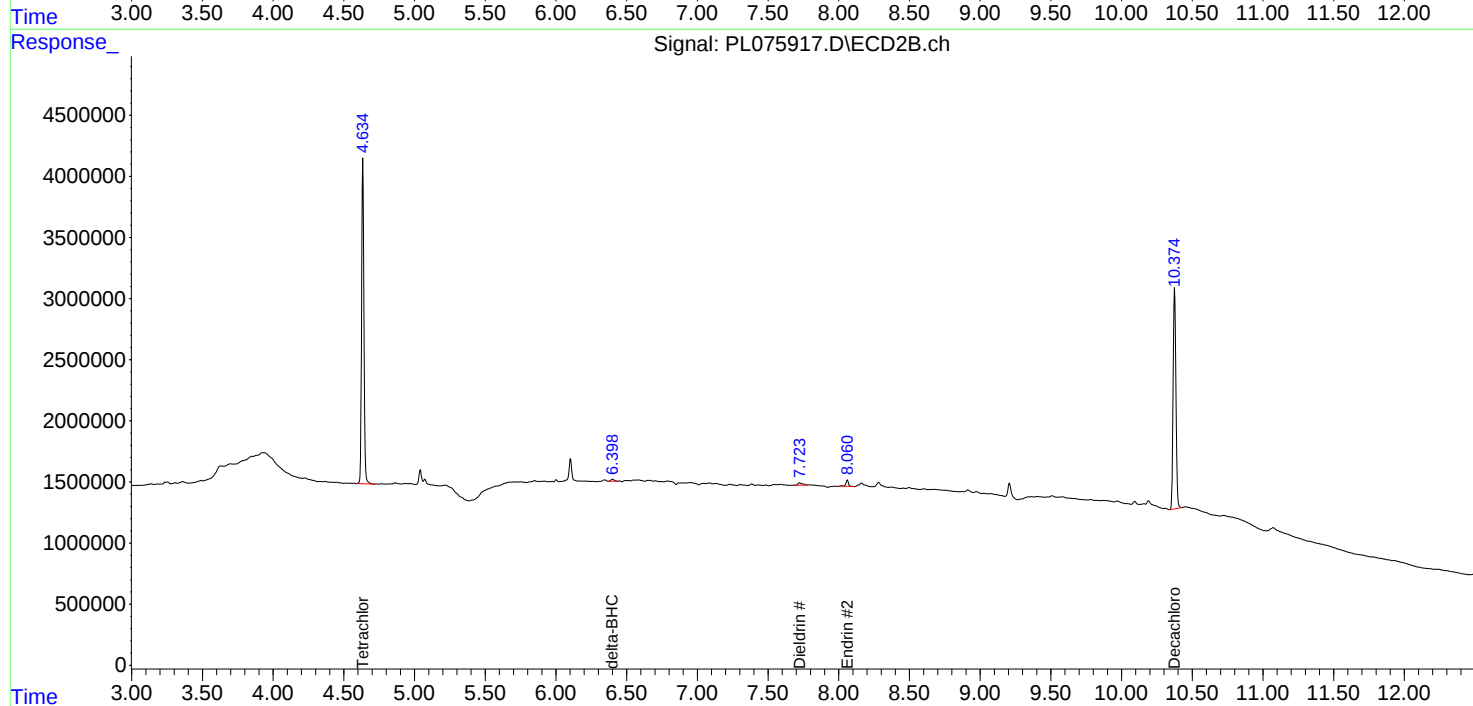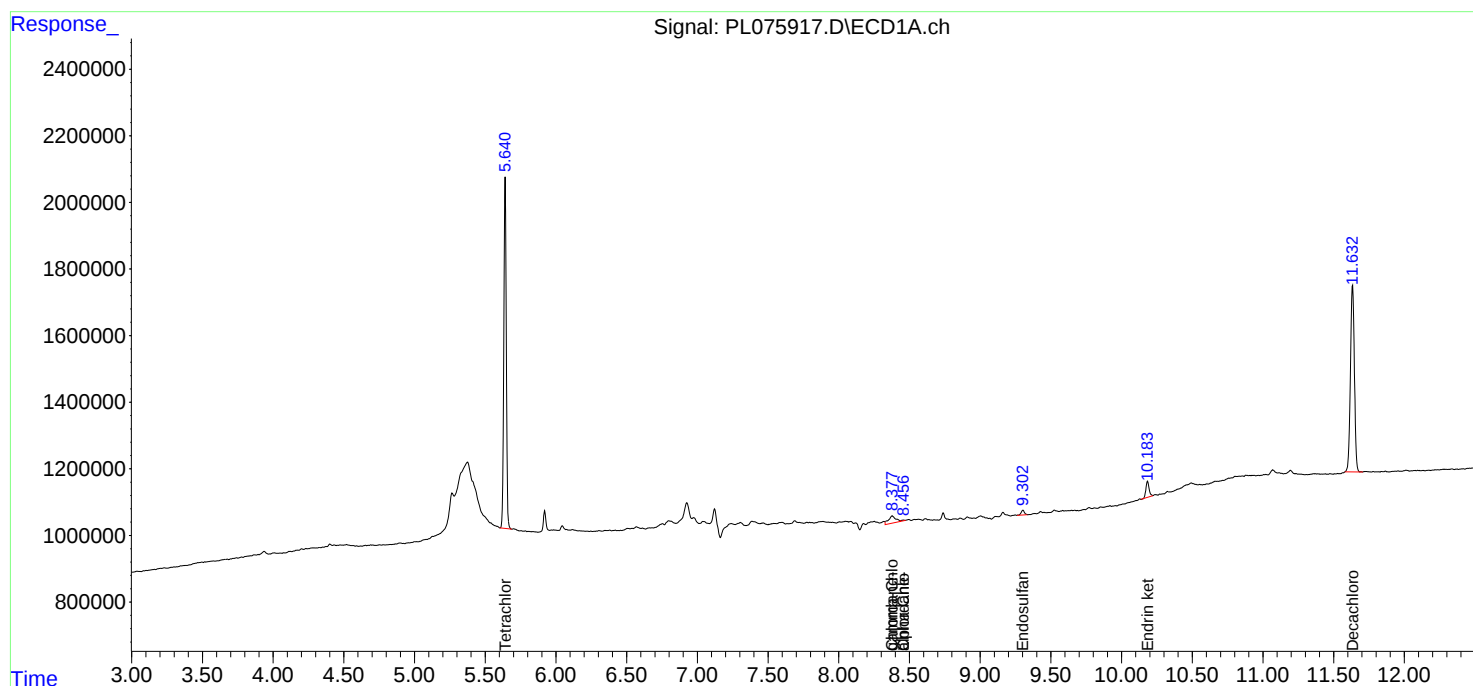


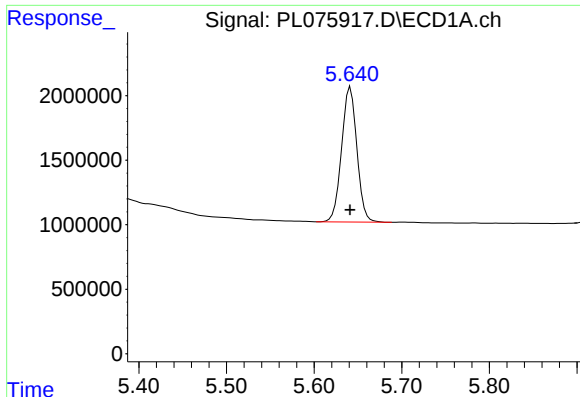

#1 Tetrachloro-m-xylene


R.T.: 5.641 min
Delta R.T.: 0.000 min
Response: 12687716
Conc: 18.80 ng/ml

Instrument :
ECD_D
ClientSampleId :

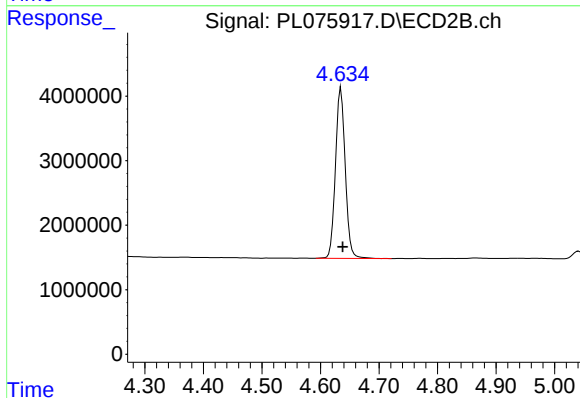


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: -0.003 min
Response: 30738596
Conc: 18.32 ng/ml

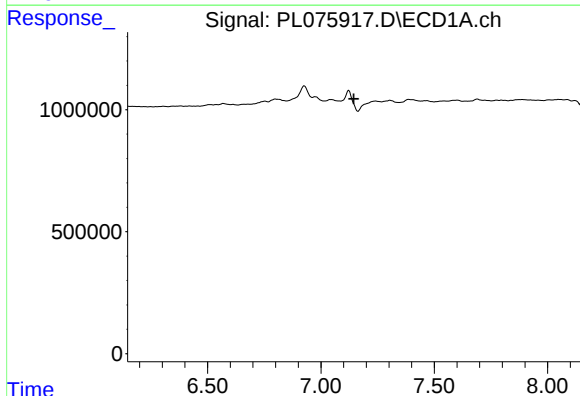


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 7.145 min
Response: 0
Conc: N.D.

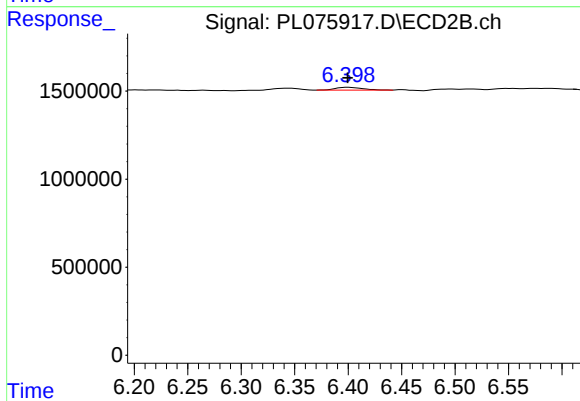

#7 delta-BHC


R.T.: 6.399 min
Delta R.T.: 0.000 min
Response: 262811
Conc: 0.12 ng/ml

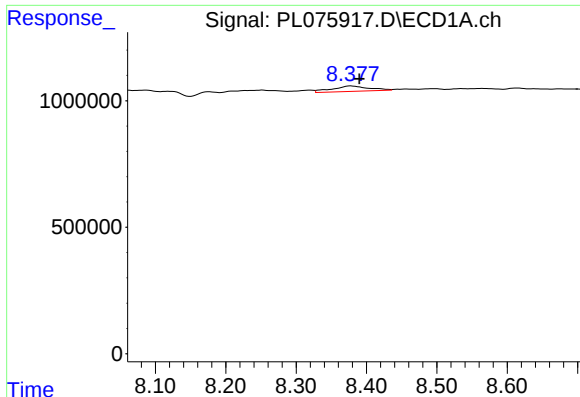

#10 gamma-Chlordane


R.T.: 8.378 min
Delta R.T.: -0.012 min
Response: 777234
Conc: 1.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

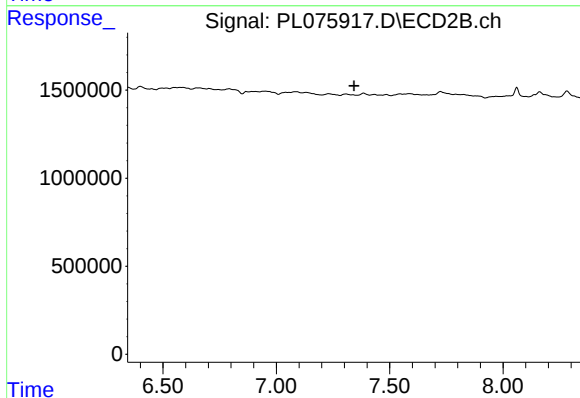


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.344 min
Response: 0
Conc: N.D.

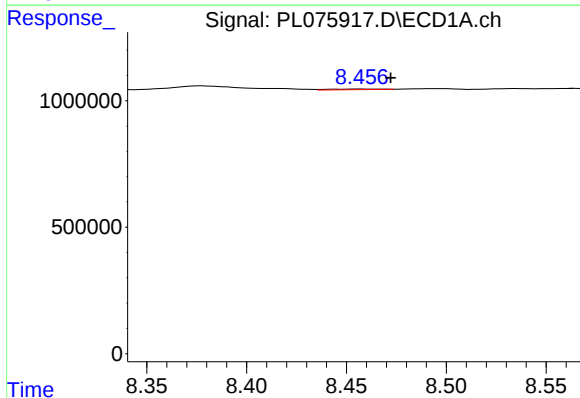


#11 alpha-Chlordane

R.T.: 8.458 min
Delta R.T.: -0.014 min
Response: 42944
Conc: 0.06 ng/ml

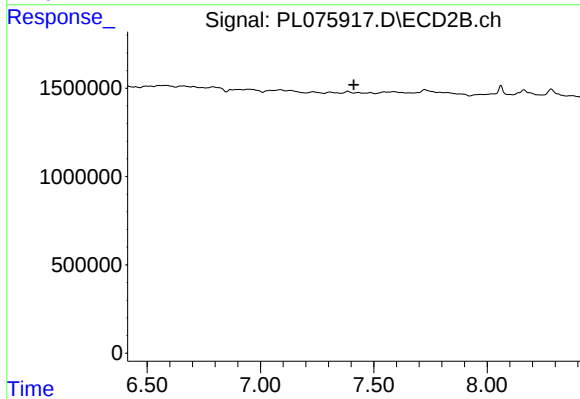

#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.412 min
Response: 0
Conc: N.D.

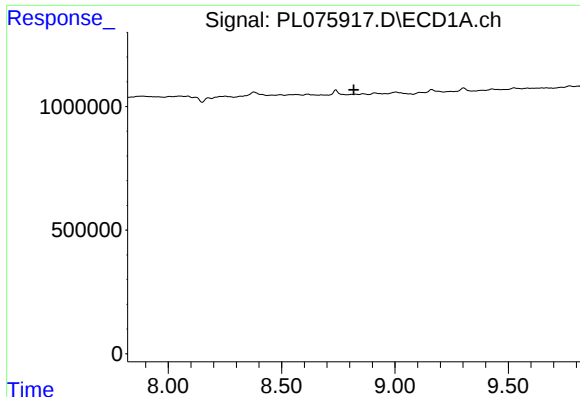

#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 8.819 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

#13 Dieldrin


R.T.: 7.724 min
Delta R.T.: -0.030 min
Response: 418959
Conc: 0.25 ng/ml

#14 Endrin

R.T.: 0.000 min
Exp R.T.: 9.059 min
Response: 0
Conc: N.D.

#14 Endrin


R.T.: 8.061 min
Delta R.T.: 0.016 min
Response: 642675
Conc: 0.47 ng/ml

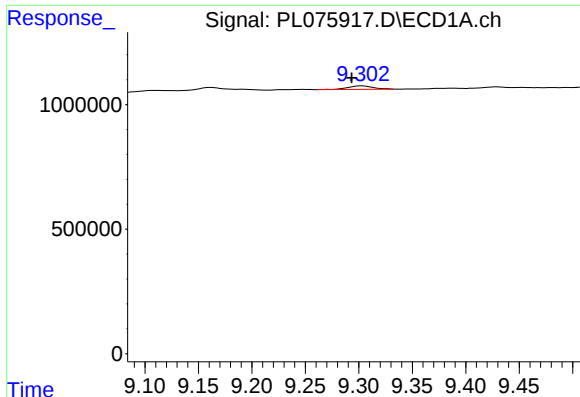

#15 Endosulfan II


R.T.: 9.303 min
Delta R.T.: 0.010 min
Response: 235828
Conc: 0.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

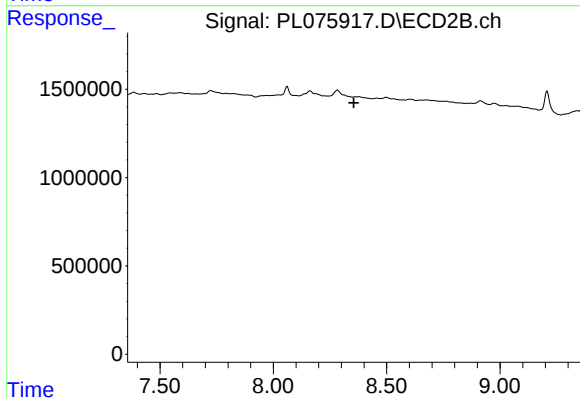


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.354 min
Response: 0
Conc: N.D.

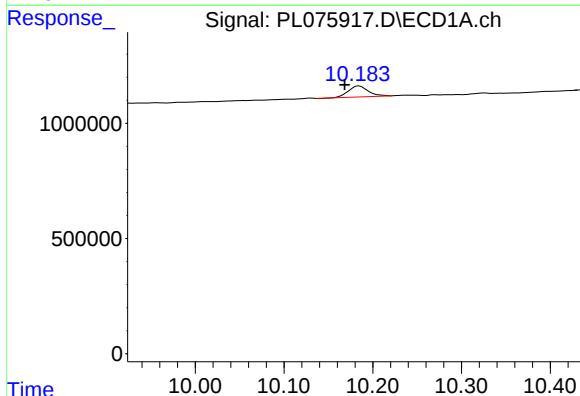


#21 Endrin ketone

R.T.: 10.185 min
Delta R.T.: 0.016 min
Response: 736303
Conc: 1.05 ng/ml

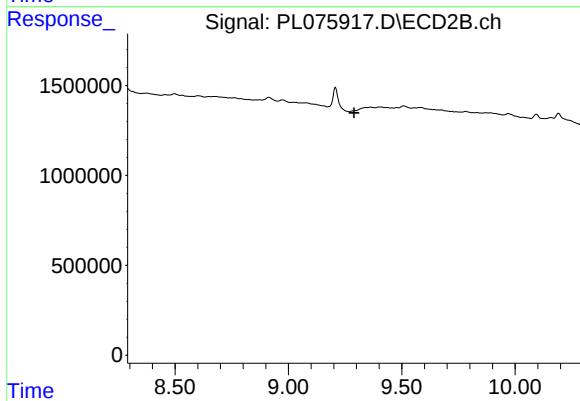

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.290 min
Response: 0
Conc: N.D.

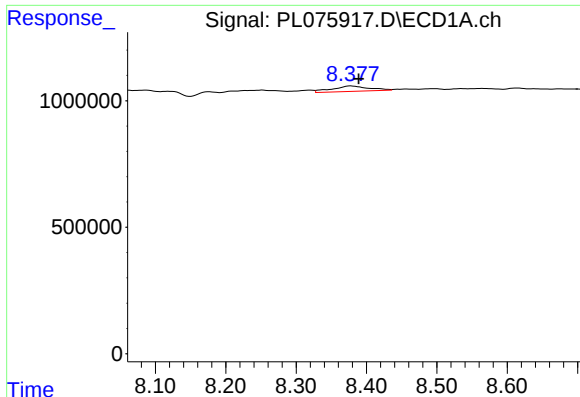

#25 Chlordane-3


R.T.: 8.378 min
Delta R.T.: -0.011 min
Response: 777234
Conc: 7.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

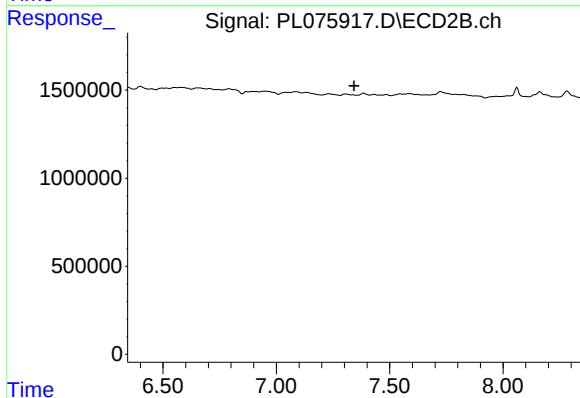


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.343 min
Response: 0
Conc: N.D.

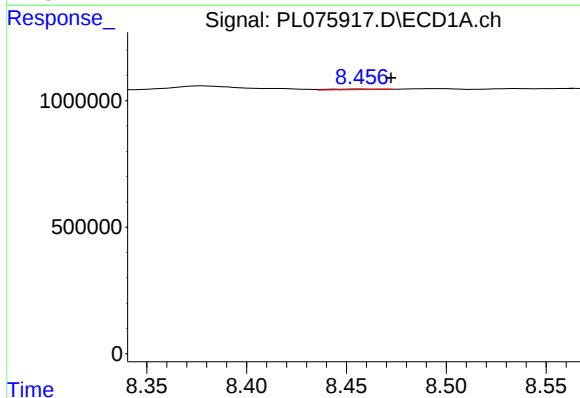


#26 Chlordane-4

R.T.: 8.458 min
Delta R.T.: -0.014 min
Response: 42944
Conc: 0.34 ng/ml

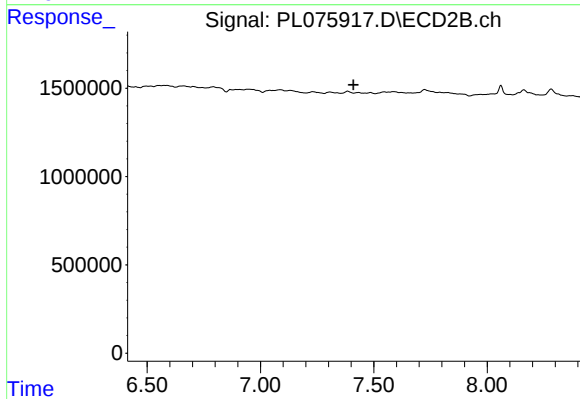

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 7.411 min
Response: 0
Conc: N.D.

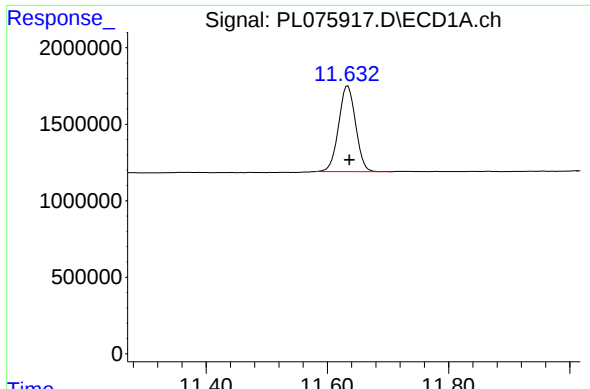

#28 Decachlorobiphenyl

R.T.: 11.634 min
Delta R.T.: -0.003 min
Response: 10887856
Conc: 17.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

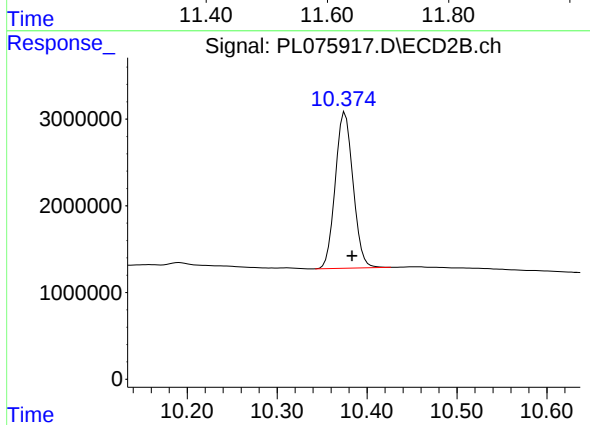

#28 Decachlorobiphenyl

R.T.: 10.376 min
Delta R.T.: -0.008 min
Response: 24709358
Conc: 17.54 ng/ml