

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
 Data File : PD076002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2023 19:00
 Operator : AR\AJ
 Sample : 03121-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 22:27:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 21 16:21:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.767	35887427	18153755	17.119	16.965
2)	SA Decachlor...	9.084	7.909	74490720	31861730	30.990	30.411
Target Compounds							
15)	B Endosulfa...	0.000	5.884f	0	747297	N.D.	0.634


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
Data File : PD076002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2023 19:00
Operator : AR\AJ
Sample : 03121-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 22:27:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 21 16:21:29 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

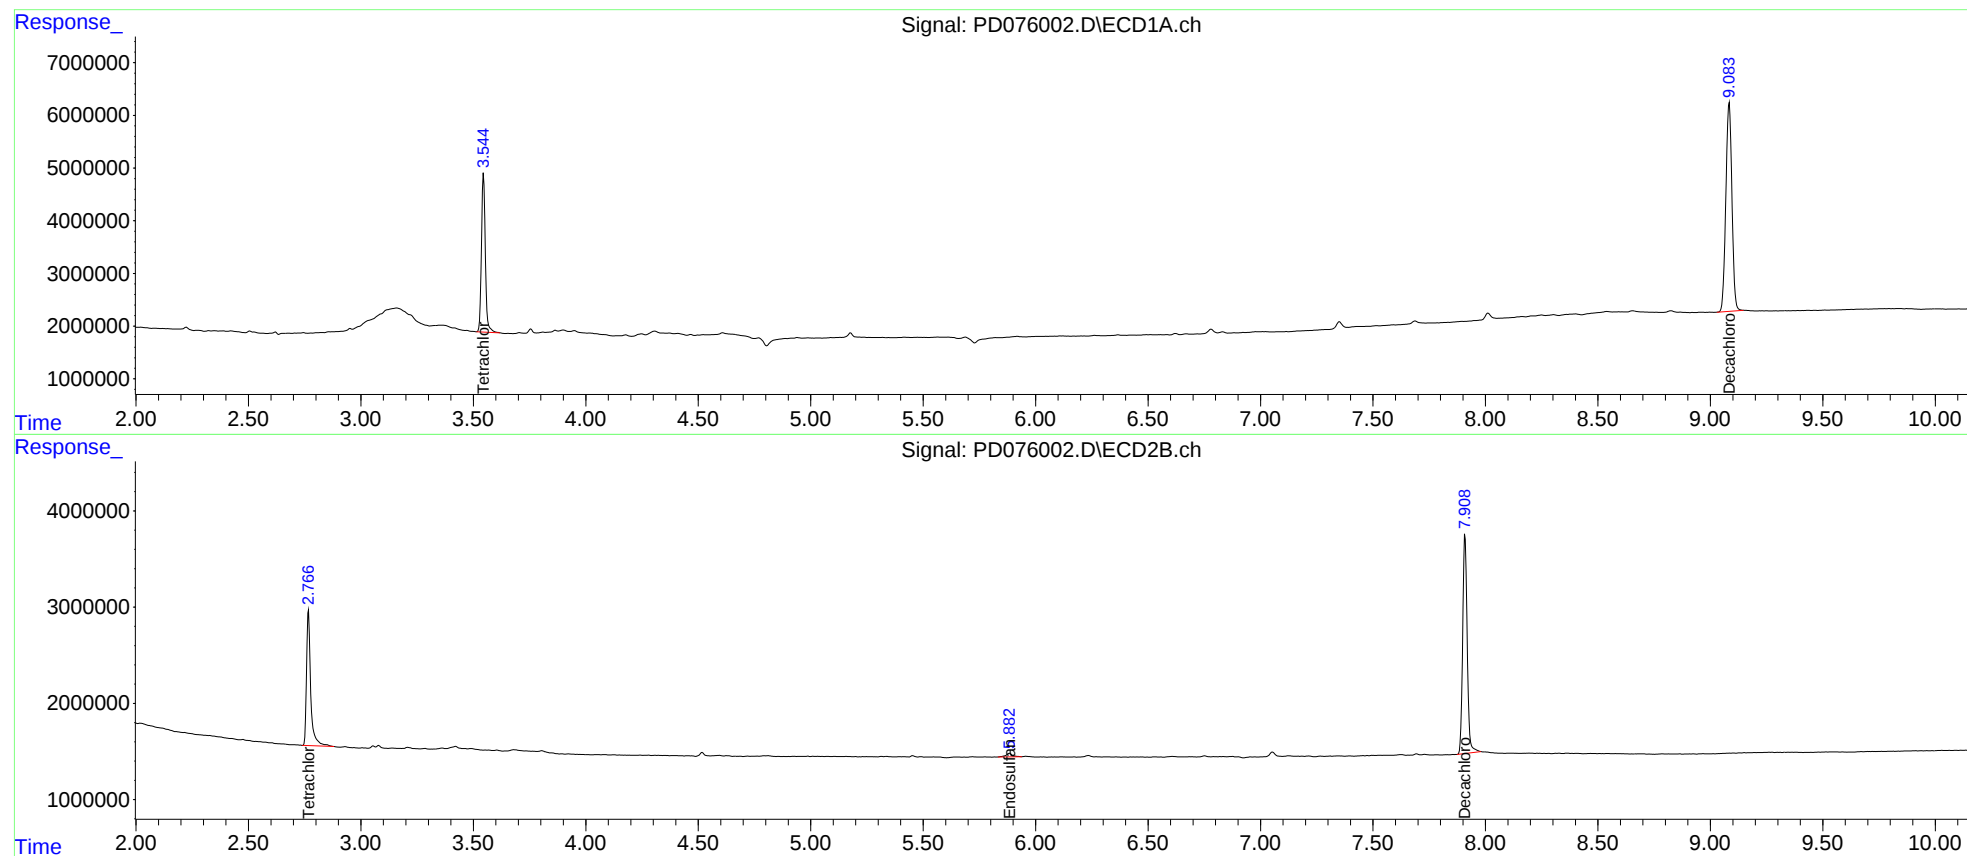

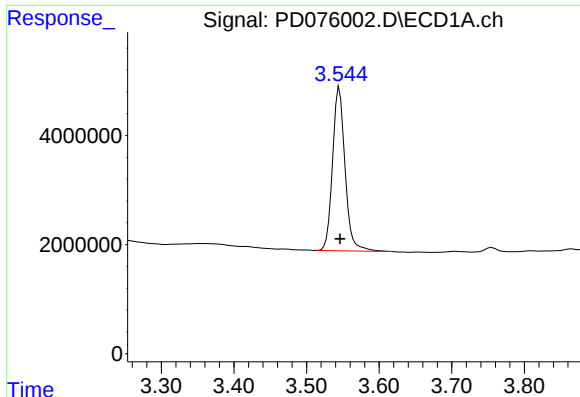


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 35887427
Conc: 17.12 ng/ml

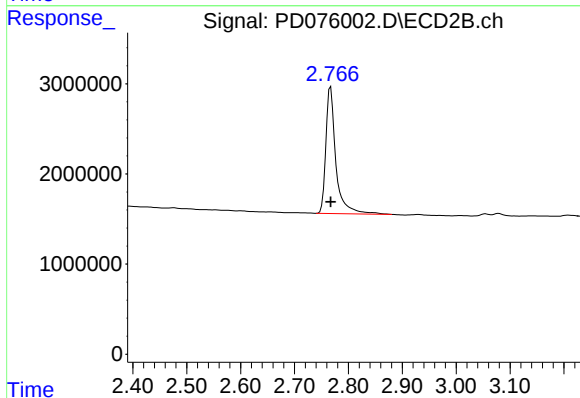


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 18153755
Conc: 16.97 ng/ml

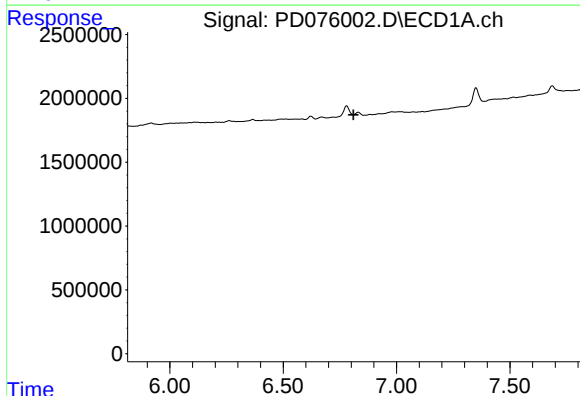


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.810 min
Response: 0
Conc: N.D.

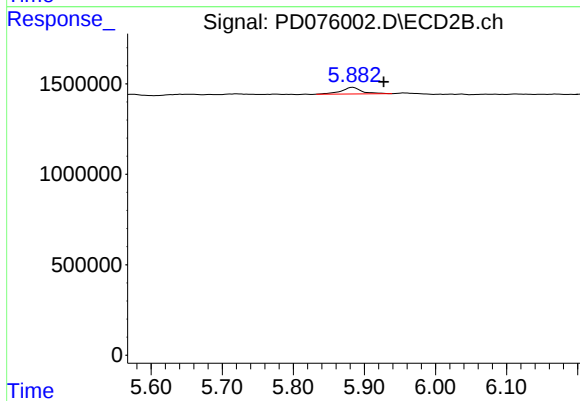


#15 Endosulfan II

R.T.: 5.884 min
Delta R.T.: -0.044 min
Response: 747297
Conc: 0.63 ng/ml

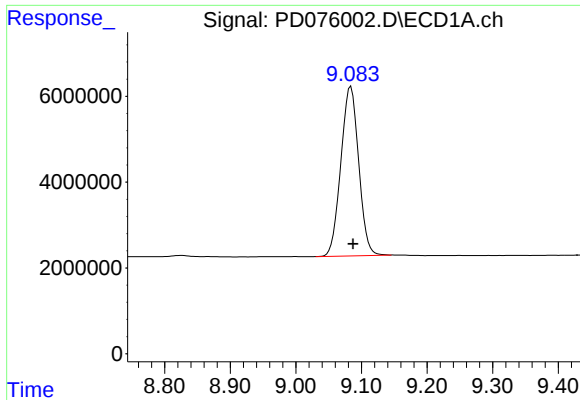

#27 Decachlorobiphenyl

R.T.: 9.084 min
Delta R.T.: -0.004 min
Response: 74490720
Conc: 30.99 ng/ml

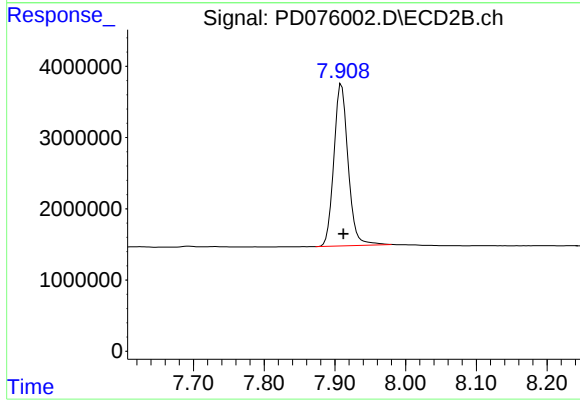

#27 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: -0.003 min
Response: 31861730
Conc: 30.41 ng/ml