

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
 Data File : PD076005.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2023 19:41
 Operator : AR\AJ
 Sample : 03121-07
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 22:28:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 21 16:21:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.767	45579630	22808660	21.742	21.315
27)	SA Decachlor...	9.082	7.910	87204119	36351287	36.279	34.696
Target Compounds							
8)	B Heptachlo...	0.000	4.791f	0	235109	N.D.	0.174
15)	B Endosulfa...	0.000	5.885f	0	650847	N.D.	0.552


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
Data File : PD076005.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2023 19:41
Operator : AR\AJ
Sample : 03121-07
Misc :
ALS Vial : 31 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 22:28:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 21 16:21:29 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

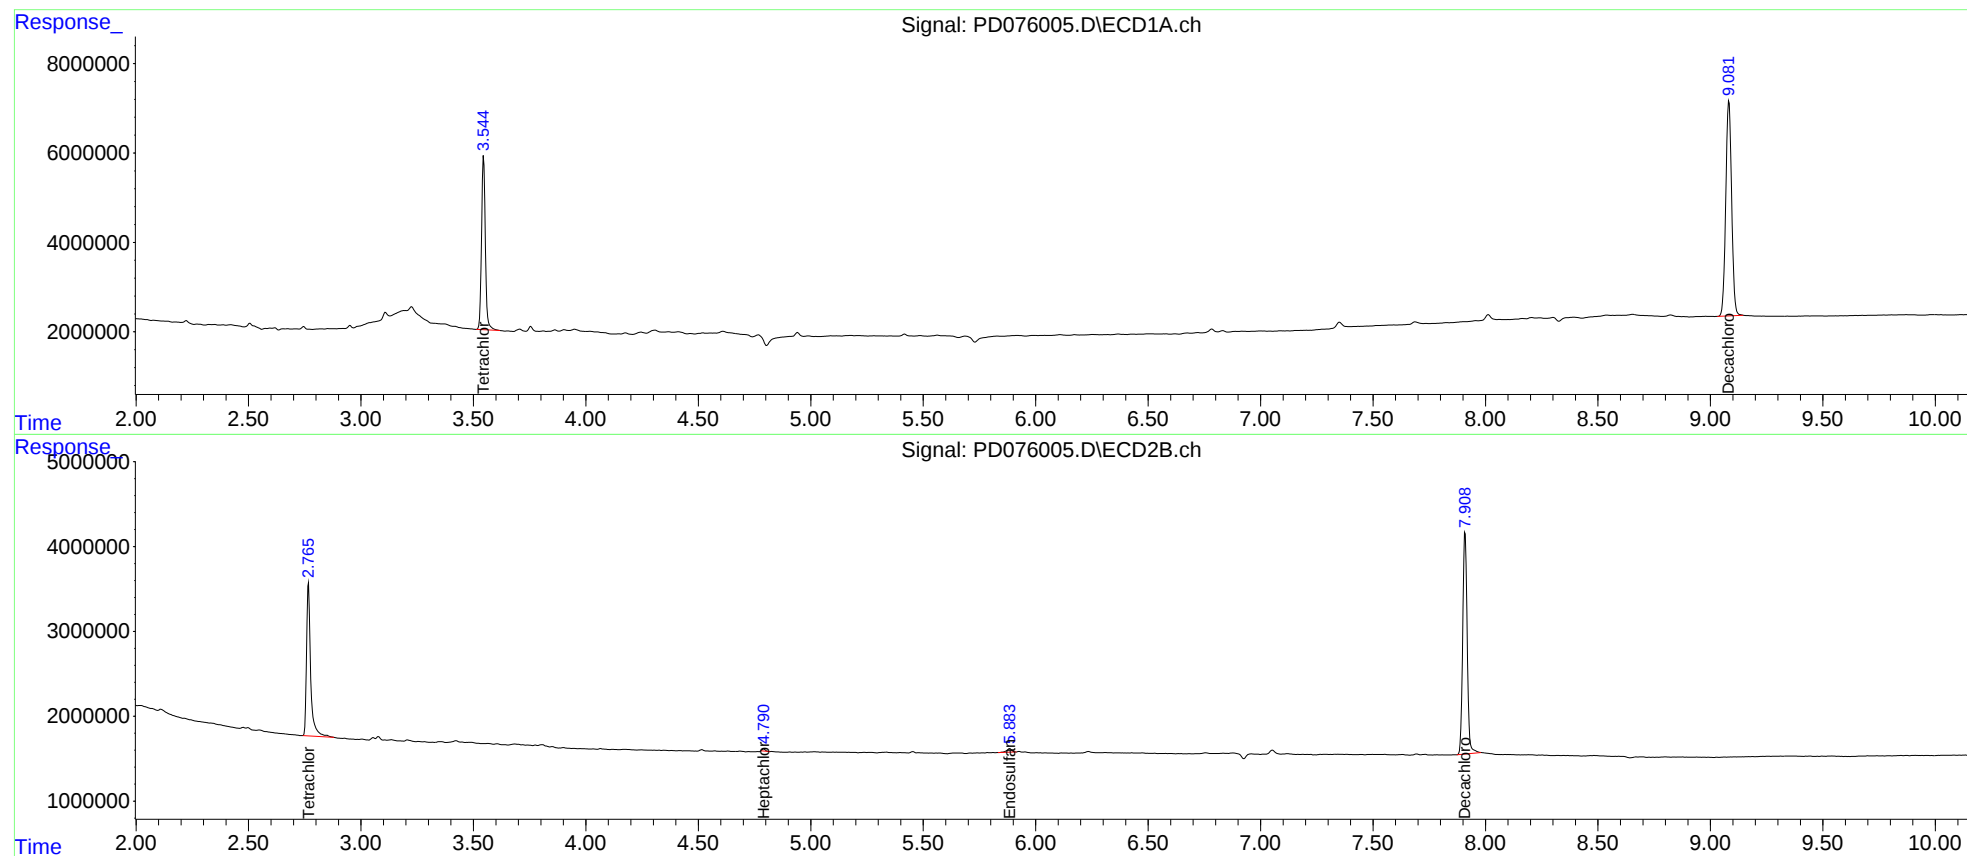

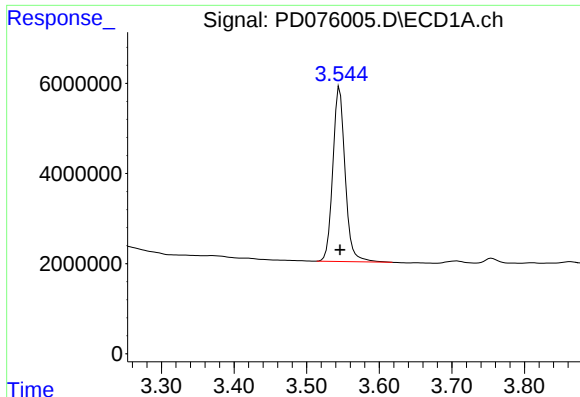


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 45579630
Conc: 21.74 ng/ml

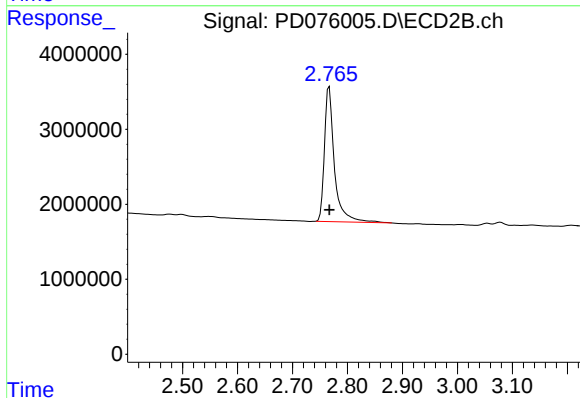


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 22808660
Conc: 21.32 ng/ml

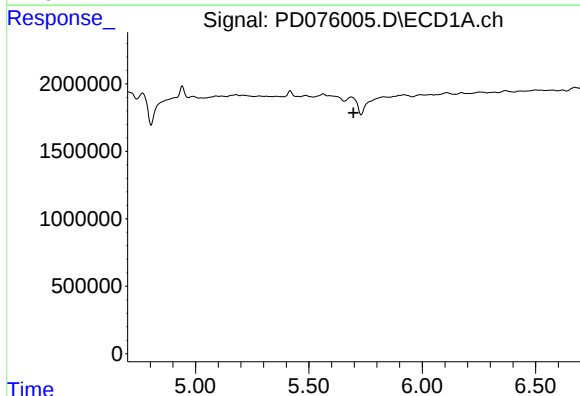


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.697 min
Response: 0
Conc: N.D.

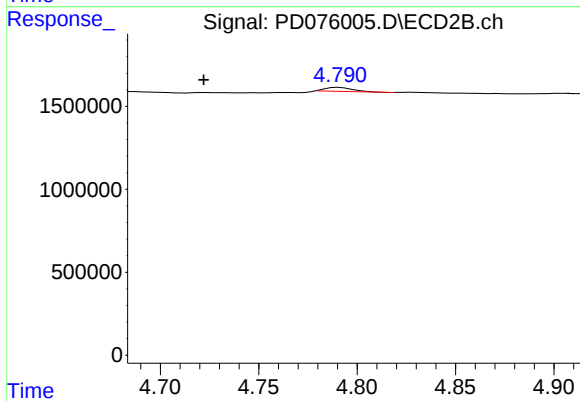


#8 Heptachlor epoxide

R.T.: 4.791 min
Delta R.T.: 0.069 min
Response: 235109
Conc: 0.17 ng/ml

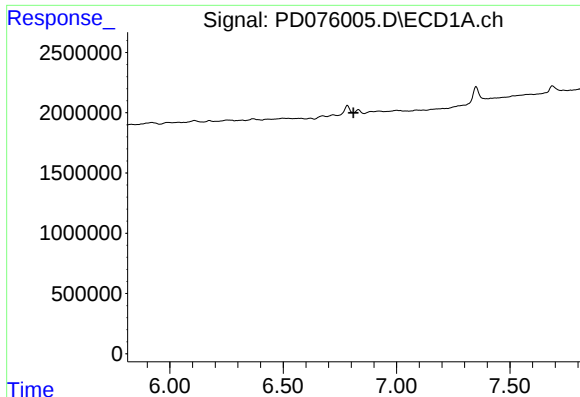


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.810 min
Response: 0
Conc: N.D.

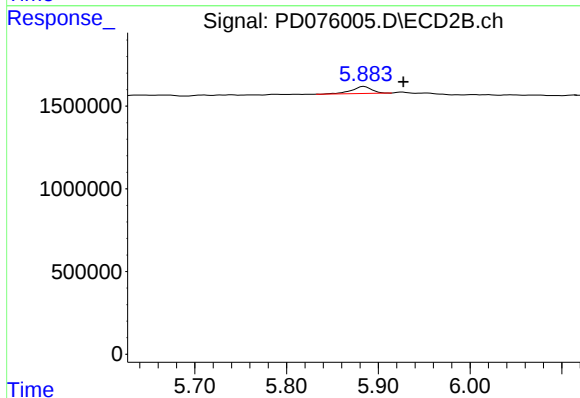


#15 Endosulfan II

R.T.: 5.885 min
Delta R.T.: -0.043 min
Response: 650847
Conc: 0.55 ng/ml

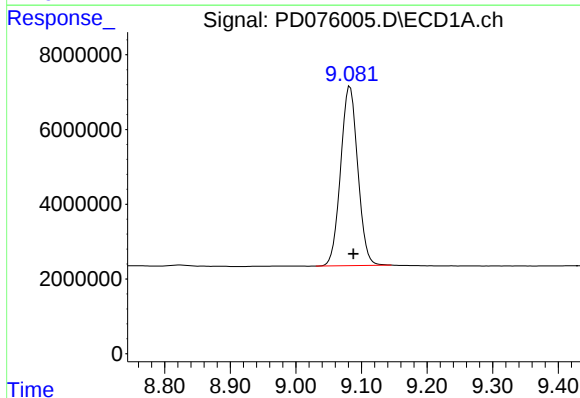

#27 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: -0.005 min
Response: 87204119
Conc: 36.28 ng/ml

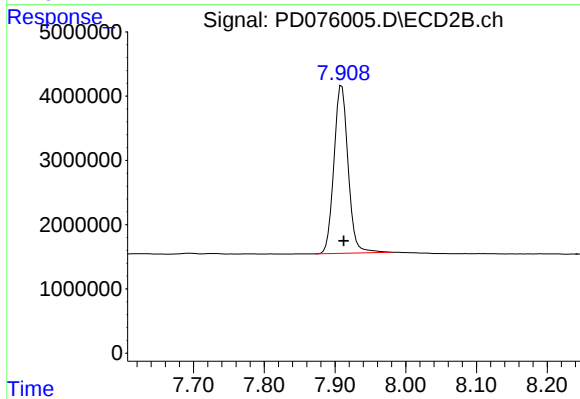

#27 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: -0.003 min
Response: 36351287
Conc: 34.70 ng/ml