

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
 Data File : PD076007.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jun 2023 20:08
 Operator : AR\AJ
 Sample : 03121-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 21 22:28:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 21 16:21:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.767	46222411	22858017	22.049	21.361
2)	SA Decachlor...	9.082	7.909	79720722	33222868	33.166	31.710
Target Compounds							
15)	B Endosulfa...	0.000	5.883f	0	510546	N.D.	0.433


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD062223\
Data File : PD076007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jun 2023 20:08
Operator : AR\AJ
Sample : 03121-09
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 21 22:28:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD062223CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jun 21 16:21:29 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

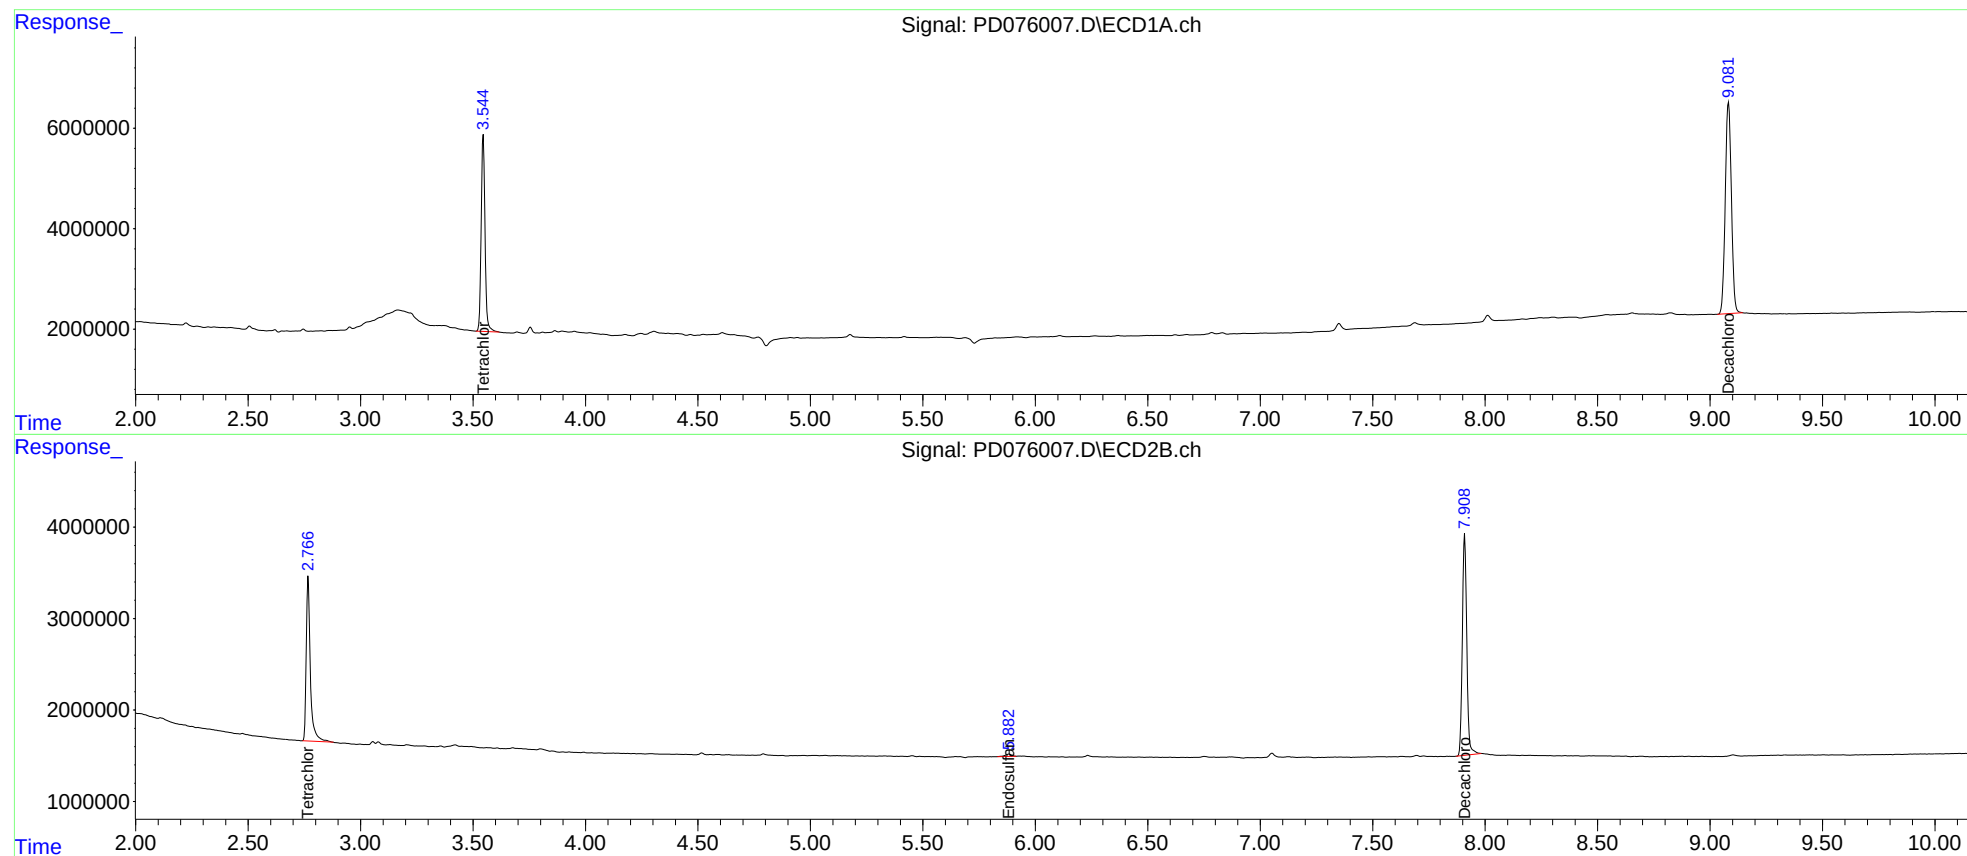

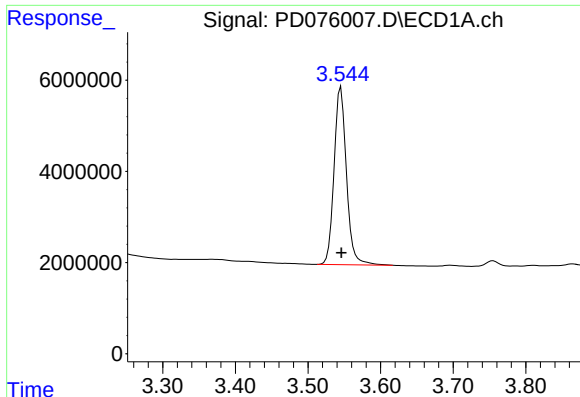


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 46222411
Conc: 22.05 ng/ml

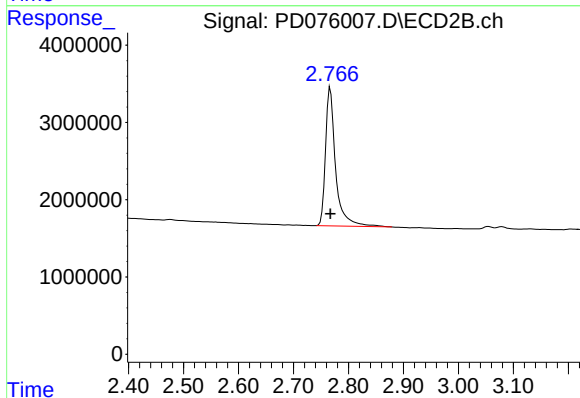


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 22858017
Conc: 21.36 ng/ml

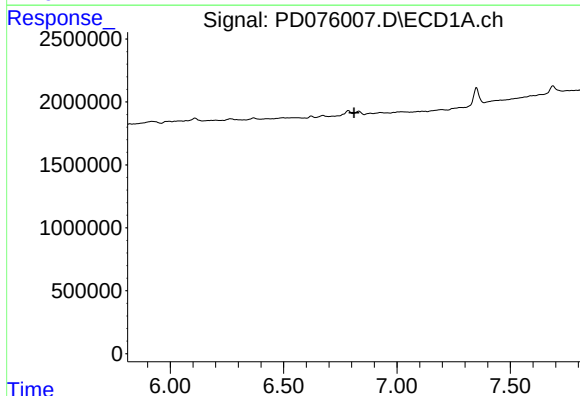


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.810 min
Response: 0
Conc: N.D.

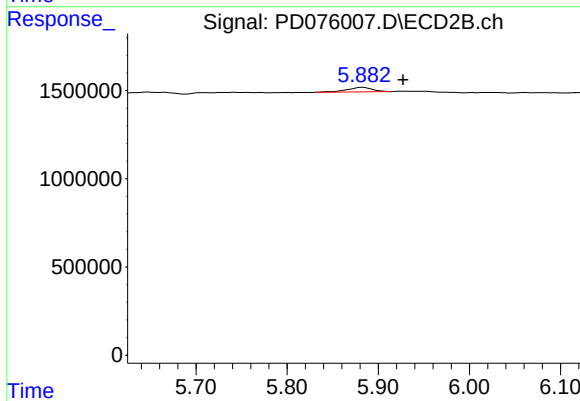


#15 Endosulfan II

R.T.: 5.883 min
Delta R.T.: -0.044 min
Response: 510546
Conc: 0.43 ng/ml

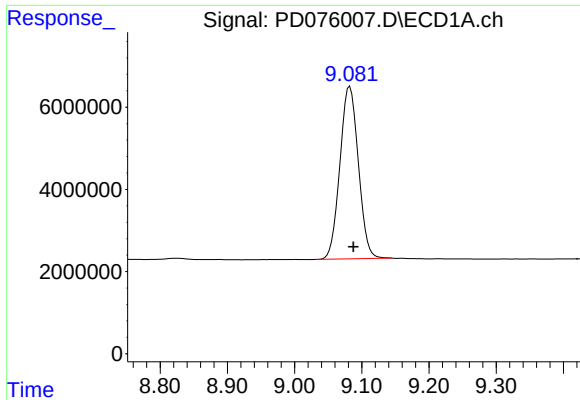

#27 Decachlorobiphenyl

R.T.: 9.082 min
Delta R.T.: -0.005 min
Response: 79720722
Conc: 33.17 ng/ml

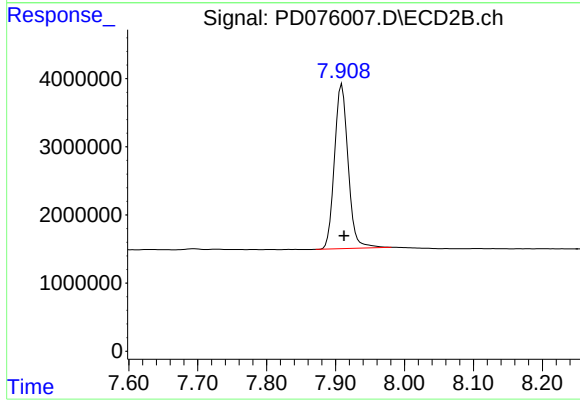

#27 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: -0.003 min
Response: 33222868
Conc: 31.71 ng/ml